



# Problem-Oriented Report

A-79-32

II-A-20

RESPONSE FACTORS OF VOC ANALYZERS  
CALIBRATED WITH METHANE  
FOR SELECTED ORGANIC CHEMICALS

## Prepared for:

OFFICE OF AIR QUALITY PLANNING AND STANDARDS

## Prepared by:

INDUSTRIAL ENVIRONMENTAL RESEARCH LABORATORY-RTP  
OFFICE OF RESEARCH AND DEVELOPMENT

PROBLEM-ORIENTED REPORT:

for: K. C. Hustvedt,  
Office of Air Quality Planning and Standards

RESPONSE FACTORS OF VOC ANALYZERS  
CALIBRATED WITH METHANE  
FOR SELECTED ORGANIC CHEMICALS

SEPTEMBER, 1980

by

G.E. Brown, D.A. DuBose, W.R. Phillips, G.E. Harris

RADIAN CORPORATION  
8501 Mo-Pac Blvd.  
Austin, Texas 78759

EPA Contract No.: 68-02-3171, Task 001  
EPA Program Element No.: LAB604

Project Officer: Dr. B.A. Tichenor

Industrial Environmental Research Laboratory  
Office of Environmental Engineering and Technology  
Research Triangle Park, N.C. 27711

Prepared for:

U.S. ENVIRONMENTAL PROTECTION AGENCY  
Office of Research and Development  
Washington, D.C. 20460

## CONTENTS

<u>Section</u>	<u>Page</u>
Figures.....	v
Tables.....	xv
1. INTRODUCTION.....	1
2. CONCLUSIONS.....	3
2.1 Summary of Results.....	3
2.2 Linearity of OVA Response.....	19
2.3 Conversion of Response Factor Basis.....	24
3. TEST PROCEDURES.....	29
3.1 Description of the Instruments.....	29
3.2 Calibration Procedures.....	30
3.3 Generation of Standard Gases.....	32
3.3.1 Preparation of Sample Bags.....	39
3.3.2 Preparation of Standards from Liquids.....	40
3.3.3 Preparation of Standards from Gases.....	43
3.4 Instrument Sampling Procedures.....	47
3.5 Quality Assurance.....	47
4. DATA ANALYSIS.....	57
5. DETAILED RESULTS.....	63
6. REFERENCES.....	419

## FIGURES

<u>Number</u>		<u>Page</u>
2-1	Fitted response factors - OVA.....	10
2-2	Fitted response factors - TLV.....	13
2-3	Linearity of OVA response to n-hexane.....	20
2-4	Variation of response factor with concentration - n-hexane.....	21
2-5	Linearity of OVA response to benzene.....	22
2-6	Variation of response factor with concentration - benzene.....	23
2-7	Linearity of OVA response to methanol.....	25
2-8	Variation of response factor with concentration - methanol.....	26
3-1	TLV recalibration check - benzene.....	33
3-2	TLV recalibration check - methyl ethyl ketone.....	34
3-3	TLV recalibration check - methanol.....	35
3-4	TLV recalibration check - acetic acid.....	36
3-5	TLV recalibration check - n-hexane.....	37
3-6	TLV recalibration check - chlorobenzene.....	38
3-7	Gas-air mixing apparatus.....	44
5-1	Instrument response vs. concentration - acetic acid.....	65
5-2	Instrument response vs. concentration - acetic anhydride.....	67
5-3	Instrument response vs. concentration - acetone.....	69
5-4	Instrument response vs. concentration - acetone cyanohydrin.....	71
5-5	Instrument response vs. concentration - acetonitrile.....	73



FIGURES (continued)

<u>Number</u>		<u>Page</u>
5-6	Instrument response vs. concentration - acetophenone.....	75
5-7	Instrument response vs. concentration - acetyl chloride.....	77
5-8	Instrument response vs. concentration - acetyl-1-propanol,3-....	79
5-9	Instrument response vs. concentration - acetylene.....	81
5-10	Instrument response vs. concentration - acrylic acid.....	83
5-11	Instrument response vs. concentration - acrylonitrile.....	85
5-12	Instrument response vs. concentration - allene.....	87
5-13	Instrument response vs. concentration - allyl alcohol.....	89
5-14	Instrument response vs. concentration - amyl alcohol,n-.....	91
5-15	Instrument response vs. concentration - amylene.....	93
5-16	Instrument response vs. concentration - anisole.....	95
5-17	Instrument response vs. concentration - benzaldehyde.....	97
5-18	Instrument response vs. concentration - benzene.....	101
5-19	Instrument response vs. concentration - benzonitrile.....	103
5-20	Instrument response vs. concentration - benzoyl chloride.....	105
5-21	Instrument response vs. concentration - benzyl chloride.....	107
5-22	Instrument response vs. concentration - bromobenzene.....	109
5-23	Instrument response vs. concentration - butadiene, 1,3-.....	111
5-24	Instrument response vs. concentration - butane,n-.....	113
5-25	Instrument response vs. concentration - butanol,n.....	115
5-26	Instrument response vs. concentration - butanol,sec-.....	117
5-27	Instrument response vs. concentration - butanol,tert.....	119

FIGURES (continued)

<u>Number</u>		<u>Page</u>
5-28	Instrument response vs. concentration - butene,1-.....	121
5-29	Instrument response vs. concentration - butyl acetate.....	123
5-30	Instrument response vs. concentration - butyl acrylate,n-.....	125
5-31	Instrument response vs. concentration - butyl ether,n-.....	127
5-32	Instrument response vs. concentration - butyl ether,sec.....	129
5-33	Instrument response vs. concentration - butylamine,n-.....	131
5-34	Instrument response vs. concentration - butylamine,sec.....	133
5-35	Instrument response vs. concentration - butylamine,tert-.....	135
5-36	Instrument response vs. concentration - butylbenzene,tert-.....	137
5-37	Instrument response vs. concentration - butyraldehyde n-.....	139
5-38	Instrument response vs. concentration - butyric acid.....	141
5-39	Instrument response vs. concentration - butyronitrile.....	143
5-40	Instrument response vs. concentration - carbon disulfide.....	145
5-41	Instrument response vs. concentration - carbon tetrachloride....	147
5-42	Instrument response vs. concentration - chloroacetaldehyde.....	149
5-43	Instrument response vs. concentration - chlorobenzene.....	151
5-44	Instrument response vs. concentration - chloroethane.....	153
5-45	Instrument response vs. concentration - chloroform.....	155
5-46	Instrument response vs. concentration - chlorophenol,o-.....	157
5-47	Instrument response vs. concentration - chloropropene,1-.....	159
5-48	Instrument response vs. concentration - chloropropene,3-.....	161
5-49	Instrument response vs. concentration - chlorotoluene,m-.....	163

FIGURES (continued)

<u>Number</u>	<u>Page</u>
5-50 Instrument response vs. concentration - chlorotoluene, o- .....	165
5-51 Instrument response vs. concentration - chlorotoluene, p- .....	167
5-52 Instrument response vs. concentration - cresol, o-.....	169
5-53 Instrument response vs. concentration - crotonaldehyde.....	171
5-54 Instrument response vs. concentration - cumene.....	173
5-55 Instrument response vs. concentration - cyclohexane.....	175
5-56 Instrument response vs. concentration - cyclohexanol.....	177
5-57 Instrument response vs. concentration - cyclohexanone.....	179
5-58 Instrument response vs. concentration - cyclohexene.....	181
5-59 Instrument response vs. concentration - cyclohexylamine.....	183
5-60 Instrument response vs. concentration - decane.....	185
5-61 Instrument response vs. concentration - diacetone alcohol.....	187
5-62 Instrument response vs. concentration - diacetyl.....	189
5-63 Instrument response vs. concentration - dichloro-1-propanol, 2,3-.....	191
5-64 Instrument response vs. concentration - dichloro-1-propene, 2,3-.....	193
5-65 Instrument response vs. concentration - dichloro-2-propanol, 1,3-.....	195
5-66 Instrument response vs. concentration - dichlorobenzene, m-.....	197
5-67 Instrument response vs. concentration - dichlorobenzene, o-.....	199
5-68 Instrument response vs. concentration - dichloroethane, 1,1-.....	201
5-69 Instrument response vs. concentration - dichloroethane, 1,2-.....	203



FIGURES (continued)

<u>Number</u>	<u>Page</u>
5-70 Instrument response vs. concentration - dichloroethylene, cis 1,2-.....	205
5-71 Instrument response vs. concentration - dichloroethylene, trans 1,2-.....	207
5-72 Instrument response vs. concentration - dichloromethane.....	209
5-73 Instrument response vs. concentration - dichloropropane,1,2-....	211
5-74 Instrument response vs. concentration - diisobutylene.....	213
5-75 Instrument response vs. concentration - diisopropyl benzene, 1,3-.....	215
5-76 Instrument response vs. concentration - dimethoxy ethane,1,2-...	217
5-77 Instrument response vs. concentration - dimethylformamide, n,n-.....	219
5-78 Instrument response vs. concentration - dimethylhydrazine 1,1-.....	221
5-79 Instrument response vs. concentration - dimethylstyrene, 2,4-.....	223
5-80 Instrument response vs. concentration - dimethylsulfoxide.....	225
5-81 Instrument response vs. concentration - dioxane.....	227
5-82 Instrument response vs. concentration - epichlorohydrin.....	229
5-83 Instrument response vs. concentration - ethane.....	231
5-84 Instrument response vs. concentration - ethanol.....	233
5-85 Instrument response vs. concentration - ethoxy ethanol,2-.....	235
5-86 Instrument response vs. concentration - ethyl acetate.....	237
5-87 Instrument response vs. concentration - ethyl acetoacetate.....	239
5-88 Instrument response vs. concentration - ethyl acrylate.....	241



FIGURES (continued)

<u>Number</u>	<u>Page</u>
5-89 Instrument response vs. concentration - ethyl chloroacetate.....	243
5-90 Instrument response vs. concentration - ethyl ether.....	245
5-91 Instrument response vs. concentration - ethylbenzene.....	247
5-92 Instrument response vs. concentration - ethylene.....	249
5-93 Instrument response vs. concentration - ethylene oxide.....	251
5-94 Instrument response vs. concentration - ethylenediamine.....	253
5-95 Instrument response vs. concentration - formic acid.....	255
5-96 Instrument response vs. concentration - freon 12.....	257
5-97 Instrument response vs. concentration - furfural.....	259
5-98 Instrument response vs. concentration - glycidol.....	261
5-99 Instrument response vs. concentration - heptane.....	263
5-100 Instrument response vs. concentration - hexane,n-.....	267
5-101 Instrument response vs. concentration - hexene,1-.....	269
5-102 Instrument response vs. concentration - hydroxyacetone.....	271
5-103 Instrument response vs. concentration - isobutane.....	273
5-104 Instrument response vs. concentration - isobutylene.....	275
5-105 Instrument response vs. concentration - isoprene.....	277
5-106 Instrument response vs. concentration - isopropanol.....	279
5-107 Instrument response vs. concentration - isopropyl acetate.....	281
5-108 Instrument response vs. concentration - isopropyl chloride.....	283
5-109 Instrument response vs. concentration - isovaleraldehyde.....	285
5-110 Instrument response vs. concentration - mesityl oxide.....	287

FIGURES (continued)

<u>Number</u>	<u>Page</u>
5-111 Instrument response vs. concentration - methacrolein.....	289
5-112 Instrument response vs. concentration - methacrylic acid.....	291
5-113 Instrument response vs. concentration - methanol.....	295
5-114 Instrument response vs. concentration - methoxy-ethanol,2-.....	297
5-115 Instrument response vs. concentration - methyl acetate.....	299
5-116 Instrument response vs. concentration - methyl acetylene.....	301
5-117 Instrument response vs. concentration - methyl chloride.....	303
5-118 Instrument response vs. concentration - methyl ethyl ketone.....	305
5-119 Instrument response vs. concentration - methyl formate.....	307
5-120 Instrument response vs. concentration - methyl methacrylate.....	309
5-121 Instrument response vs. concentration - methyl-2-pentanol,4-....	311
5-122 Instrument response vs. concentration - methyl-2-pentanone,4-....	313
5-123 Instrument response vs. concentration - methyl-2,4- pentanediol,2-.....	315
5-124 Instrument response vs. concentration - methyl-3-butyn-2- OL,2.....	317
5-125 Instrument response vs. concentration - methylal.....	319
5-126 Instrument response vs. concentration - methylaniline,n-.....	321
5-127 Instrument response vs. concentration - methylcyclohexane.....	323
5-128 Instrument response vs. concentration - methylcyclohexene,1-....	325
5-129 Instrument response vs. concentration - methylpentynol.....	327
5-130 Instrument response vs. concentration - methylstyrene,a-.....	329
5-131 Instrument response vs. concentration - monoethanolamine.....	331

FIGURES (continued)

<u>Number</u>	<u>Page</u>
5-132 Instrument response vs. concentration - morpholine.....	333
5-133 Instrument response vs. concentration - nitrobenzene.....	335
5-134 Instrument response vs. concentration - nitroethane.....	337
5-135 Instrument response vs. concentration - nitromethane.....	339
5-136 Instrument response vs. concentration - nitropropane.....	341
5-137 Instrument response vs. concentration - nonane-n.....	343
5-138 Instrument response vs. concentration - octane.....	345
5-139 Instrument response vs. concentration - pentane.....	347
5-140 Instrument response vs. concentration - phenol.....	349
5-141 Instrument response vs. concentration - phenyl-2-propanol,2-....	351
5-142 Instrument response vs. concentration - picoline,2-.....	353
5-143 Instrument response vs. concentration - propane.....	355
5-144 Instrument response vs. concentration - propionaldehyde.....	357
5-145 Instrument response vs. concentration - propionic acid.....	359
5-146 Instrument response vs. concentration - propyl alcohol.....	361
5-147 Instrument response vs. concentration - propylbenzene,n-.....	363
5-148 Instrument response vs. concentration - propylene.....	365
5-149 Instrument response vs. concentration - propylene oxide.....	367
5-150 Instrument response vs. concentration - pyridine.....	369
5-151 Instrument response vs. concentration - styrene.....	371
5-152 Instrument response vs. concentration - tetrachloroethane, 1,1,1,2.....	373



FIGURES (continued)

<u>Number</u>		<u>Page</u>
5-153	Instrument response vs. concentration - tetrachloroethane, 1,1,2,2.....	375
5-154	Instrument response vs. concentration - tetrachloroethylene.....	377
5-155	Instrument response vs. concentration - toluene.....	379
5-156	Instrument response vs. concentration - trichlorobenzene, 1,2,4-.....	381
5-157	Instrument response vs. concentration - trichloroethane, 1,1,1-.....	383
5-158	Instrument response vs. concentration - trichloroethane, 1,1,2-.....	385
5-159	Instrument response vs. concentration - trichloroethylene.....	387
5-160	Instrument response vs. concentration - trichloropropane, 1,2,3-.....	389
5-161	Instrument response vs. concentration - triethylamine.....	391
5-162	Instrument response vs. concentration - vinyl acetate.....	393
5-163	Instrument response vs. concentration - vinyl chloride.....	395
5-164	Instrument response vs. concentration - vinyl propionate.....	397
5-165	Instrument response vs. concentration - vinylidene chloride.....	399
5-166	Instrument response vs. concentration - xylene,p-.....	401
5-167	Instrument response vs. concentration - xylene,m-.....	403
5-168	Instrument response vs. concentration - xylene,o-.....	405



TABLES

<u>Number</u>		<u>Page</u>
2-1	Fitted Response Factors with 95% Confidence Intervals.....	4
2-2	Comparison of Response Factors from this Study to Previously Published Values.....	17
3-1	Liquid Response Factor Data Sheet.....	42
3-2	Gas Response Factor Data Sheet.....	46
3-3	Summary of Random Calibration Checks Used for Quality Assurance.	48
5-1	Response Factor Summary - Acetic Acid.....	64
5-2	Response Factor Summary - Acetic Anhydride.....	66
5-3	Response Factor Summary - Acetone.....	68
5-4	Response Factor Summary - Acetone Cyanohydrin.....	70
5-5	Response Factor Summary - Acetonitrile.....	72
5-6	Response Factor Summary - Acetophenone.....	74
5-7	Response Factor Summary - Acetyl Chloride.....	76
5-8	Response Factor Summary - Acetyl-1-Propanol,3-.....	78
5-9	Response Factor Summary - Acetylene.....	80
5-10	Response Factor Summary - Acrylic Acid.....	82
5-11	Response Factor Summary - Acrylonitrile.....	84
5-12	Response Factor Summary - Allene.....	86
5-13	Response Factor Summary - Allyl Alcohol.....	88
5-14	Response Factor Summary - Amyl Alcohol,N-.....	90
5-15	Response Factor Summary - Amylene.....	92

TABLES (continued)

<u>Number</u>		<u>Page</u>
5-16	Response Factor Summary - Anisole.....	94
5-17	Response Factor Summary - Benzaldehyde.....	96
5-18	Response Factor Summary - Benzene.....	98
5-19	Response Factor Summary - Benzonitrile.....	102
5-20	Response Factor Summary - Benzoyl Chloride.....	104
5-21	Response Factor Summary - Benzyl Chloride.....	106
5-22	Response Factor Summary - Bromobenzene.....	108
5-23	Response Factor Summary - Butadiene,1,3-.....	110
5-24	Response Factor Summary - Butane,N-.....	112
5-25	Response Factor Summary - Butanol, N.....	114
5-26	Response Factor Summary - Butanol, Sec.....	116
5-27	Response Factor Summary - Butanol,Tert.....	118
5-28	Response Factor Summary - Butene,1-.....	120
5-29	Response Factor Summary - Butyl Acetate.....	122
5-30	Response Factor Summary - Butyl Acrylate,N.....	124
5-31	Response Factor Summary - Butyl Ether,N.....	126
5-32	Response Factor Summary - Butyl Ether,Sec.....	128
5-33	Response Factor Summary - Butylamine,N.....	130
5-34	Response Factor Summary - Butylamine, Sec.....	132
5-35	Response Factor Summary - Butylamine,Tert.....	134
5-36	Response Factor Summary - Butylbenzene,Tert.....	136
5-37	Response Factor Summary - Butyraldehyde N.....	138
5-38	Response Factor Summary - Butyric Acid.....	140

TABLES (continued)

<u>Number</u>		<u>Page</u>
5-39	Response Factor Summary - Butyronitrile.....	142
5-40	Response Factor Summary - Carbon Disulfide.....	144
5-41	Response Factor Summary - Carbon Tetrachloride.....	146
5-42	Response Factor Summary - Chloroacetaldehyde.....	148
5-43	Response Factor Summary - Chlorobenzene.....	150
5-44	Response Factor Summary - Chloroethane.....	152
5-45	Response Factor Summary - Chloroform.....	154
5-46	Response Factor Summary - Chlorophenol, O-.....	156
5-47	Response Factor Summary - Chloropropene, 1-.....	158
5-48	Response Factor Summary - Chloropropene, 3-.....	160
5-49	Response Factor Summary - Chlorotoluene, M-.....	162
5-50	Response Factor Summary - Chlorotoluene, O-.....	164
5-51	Response Factor Summary - Chlorotoluene, P-.....	166
5-52	Response Factor Summary - Cresol, O-.....	168
5-53	Response Factor Summary - Crotonaldehyde.....	170
5-54	Response Factor Summary - Cumene.....	172
5-55	Response Factor Summary - Cyclohexane.....	174
5-56	Response Factor Summary - Cyclohexanol.....	176
5-57	Response Factor Summary - Cyclohexanone.....	178
5-58	Response Factor Summary - Cyclohexene.....	180
5-59	Response Factor Summary - Cyclohexylamine.....	182
5-60	Response Factor Summary - Decane.....	184
5-61	Response Factor Summary - Diacetone Alcohol.....	186



TABLES (continued)

<u>Number</u>	<u>Page</u>
5-62 Response Factor Summary - Diacetyl.....	188
5-63 Response Factor Summary - Dichloro-1-Propanol,2,3-.....	190
5-64 Response Factor Summary - Dichloro-1-Propene,2,3-.....	192
5-65 Response Factor Summary - Dichloro-2-Propanol,1,3-.....	194
5-66 Response Factor Summary - Dichlorobenzene,M-.....	196
5-67 Response Factor Summary - Dichlorobenzene,O-.....	198
5-68 Response Factor Summary - Dichloroethane,1,1-.....	200
5-69 Response Factor Summary - Dichloroethane,1,2-.....	202
5-70 Response Factor Summary - Dichloroethylene,cis 1,2-.....	204
5-71 Response Factor Summary - Dichloroethylene,trans 1,2.....	206
5-72 Response Factor Summary - Dichloromethane.....	208
5-73 Response Factor Summary - Dichloropropane,1,2-.....	210
5-74 Response Factor Summary - Diisobutylene.....	212
5-75 Response Factor Summary - Diisopropyl Benzen,1,3-.....	214
5-76 Response Factor Summary - Dimethoxy Ethane, 1,2-.....	216
5-77 Response Factor Summary - Dimethylformamide,N,N-.....	218
5-78 Response Factor Summary - Dimethylhydrazine 1,1-.....	220
5-79 Response Factor Summary - Dimethylstyrene,2,4-.....	222
5-80 Response Factor Summary - Dimethylsulfoxide.....	224
5-81 Response Factor Summary - Dioxane.....	226
5-82 Response Factor Summary - Epichlorohydrin.....	228
5-83 Response Factor Summary - Ethane.....	230



TABLES (continued)

<u>Number</u>	<u>Page</u>
5-84 Response Factor Summary - Ethanol.....	232
5-85 Response Factor Summary - Ethoxy Ethanol,2-.....	234
5-86 Response Factor Summary - Ethyl Acetate.....	236
5-87 Response Factor Summary - Ethyl Acetoacetate.....	238
5-88 Response Factor Summary - Ethyl Acrylate.....	240
5-89 Response Factor Summary - Ethyl Chloroacetate.....	242
5-90 Response Factor Summary - Ethyl Ether.....	244
5-91 Response Factor Summary - Ethylbenzene.....	246
5-92 Response Factor Summary - Ethylene.....	248
5-93 Response Factor Summary - Ethylene Oxide.....	250
5-94 Response Factor Summary - Ethylenediamine.....	252
5-95 Response Factor Summary - Formic Acid.....	254
5-96 Response Factor Summary - Freon 12.....	256
5-97 Response Factor Summary - Furfural.....	258
5-98 Response Factor Summary - Glycidol.....	260
5-99 Response Factor Summary - Heptane.....	262
5-100 Response Factor Summary - Hexane,N-.....	264
5-101 Response Factor Summary - Hexene,1-.....	268
5-102 Response Factor Summary - Hydroxyacetone.....	270
5-103 Response Factor Summary - Isobutane.....	272
5-104 Response Factor Summary - Isobutylene.....	274
5-105 Response Factor Summary - Isoprene.....	276

TABLES (continued)

<u>Number</u>	<u>Page</u>
5-106 Response Factor Summary - Isopropanol.....	278
5-107 Response Factor Summary - Isopropyl Acetate.....	280
5-108 Response Factor Summary - Isopropyl Chloride.....	282
5-109 Response Factor Summary - Isovaleraldehyde.....	284
5-110 Response Factor Summary - Mesityl Oxide.....	286
5-111 Response Factor Summary - Methacrolein.....	288
5-112 Response Factor Summary - Methacrylic Acid.....	290
5-113 Response Factor Summary - Methanol.....	292
5-114 Response Factor Summary - Methoxy-Ethanol, 2-.....	296
5-115 Response Factor Summary - Methyl Acetate.....	298
5-116 Response Factor Summary - Methyl Acetylene.....	300
5-117 Response Factor Summary - Methyl Chloride.....	302
5-118 Response Factor Summary - Methyl Ethyl Ketone.....	304
5-119 Response Factor Summary - Methyl Formate.....	306
5-120 Response Factor Summary - Methyl Methacrylate.....	308
5-121 Response Factor Summary - Methyl-2-Pentanol, 4-.....	310
5-122 Response Factor Summary - Methyl-2-Pentanone, 4-.....	312
5-123 Response Factor Summary - Methyl-2,4-Pentanediol, 2-.....	314
5-124 Response Factor Summary - Methyl-3-Butyn-2-OL, 2.....	316
5-125 Response Factor Summary - Methylal.....	318
5-126 Response Factor Summary - Methylaniline, N-.....	320
5-127 Response Factor Summary - Methylcyclohexane.....	322

TABLES (continued)

<u>Number</u>	<u>Page</u>
5-128 Response Factor Summary - Methylcyclohexene,1-.....	324
5-129 Response Factor Summary - Methylpentynol.....	326
5-130 Response Factor Summary - Methylstyrene,A- .....	328
5-131 Response Factor Summary - Monoethanolamine.....	330
5-132 Response Factor Summary - Morpholine.....	332
5-133 Response Factor Summary - Nitrobenzene.....	334
5-134 Response Factor Summary - Nitroethane.....	336
5-135 Response Factor Summary - Nitromethane.....	338
5-136 Response Factor Summary - Nitropropane.....	340
5-137 Response Factor Summary - Nonane-N.....	342
5-138 Response Factor Summary - Octane.....	344
5-139 Response Factor Summary - Pentane.....	346
5-140 Response Factor Summary - Phenol.....	348
5-141 Response Factor Summary - Phenyl-2-Propanol,2-.....	350
5-142 Response Factor Summary - Picoline,2-.....	352
5-143 Response Factor Summary - Propane.....	354
5-144 Response Factor Summary - Propionaldehyde.....	356
5-145 Response Factor Summary - Propionic Acid.....	358
5-146 Response Factor Summary - Propyl Alcohol.....	360
5-147 Response Factor Summary - Propylbenzene,N-.....	362
5-148 Response Factor Summary - Propylene.....	364
5-149 Response Factor Summary - Propylene Oxide.....	366

TABLES (continued)

<u>Number</u>	<u>Page</u>
5-150 Response Factor Summary - Pyridine.....	368
5-151 Response Factor Summary - Styrene.....	370
5-152 Response Factor Summary - Tetrachloroethane,1,1,1,2.....	372
5-153 Response Factor Summary - Tetrachloroethane,1,1,2,2.....	374
5-154 Response Factor Summary - Tetrachloroethylene.....	376
5-155 Response Factor Summary - Toluene.....	378
5-156 Response Factor Summary - Trichlorobenzene;1,2,4-.....	380
5-157 Response Factor Summary - Trichloroethane,1,1,1-.....	382
5-158 Response Factor Summary - Trichloroethane,1,1,2-.....	384
5-159 Response Factor Summary - Trichloroethylene.....	386
5-160 Response Factor Summary - Trichloropropane,1,2,3-.....	388
5-161 Response Factor Summary - Triethylamine.....	390
5-162 Response Factor Summary - Vinyl Acetate.....	392
5-163 Response Factor Summary - Vinyl Chloride.....	394
5-164 Response Factor Summary - Vinyl Propionate.....	396
5-165 Response Factor Summary - Vinylidene Chloride.....	398
5-166 Response Factor Summary - Xylene,P-.....	400
5-167 Response Factor Summary - Xylene,M-.....	402
5-168 Response Factor Summary - Xylene,O-.....	404
5-169 Statistics for Computing Estimates and Confidence Intervals (OVA).....	407
5-170 Statistics for Computing Estimates and Confidence Intervals (TLV).....	413



## SECTION 1

### INTRODUCTION

This report presents the results of a laboratory study of the sensitivity of two types of portable hydrocarbon detectors to a variety of organic chemicals. This work was funded by the EPA as part of contract number 68-02-3171, Task 4. This introductory section will briefly discuss the background, objectives, and procedures used in the project.

The study of fugitive Volatile Organic Compound (VOC) emissions has rapidly gained emphasis over the past several years. Several research efforts designed to measure fugitive emission levels and to assess the effectiveness of proposed control schemes are in various stages of completion. The development of regulations to control fugitive emissions has begun at both the state and Federal level.

As a result of this research, a roughly quantitative method for leak detection has been developed which is commonly called "screening". The screening process is simply the measurement of the VOC concentration at a point close to the potential leak site (valve stem, pump seal, etc.). The measurement is made with a portable hydrocarbon detector. While many instruments could potentially be used for this service, the bulk of the existing data has been taken using either the J. W. Bacharach "TLV Sniffer" or the Century Systems "OVA-108".

While these instruments will respond to almost any combustible material, they exhibit different sensitivities to various types of hydrocarbons and substituted organic chemicals. The "response factor" is a correction factor which quantifies these differences in sensitivity.

The primary objective of this work is to experimentally determine the response factors for a large number of commonly encountered chemical species. Such response factors are presented here for both the OVA and the TLV. Two instruments of each type (one old and one new) were tested to check for instrument-to-instrument variations. Each chemical was tested at several concentrations to assess variations in the response factor over the range of interest.

The experimental determination of a response factor simply requires reading the observed concentration on the instrument when testing a gas sample of known concentration. Such standard gas samples were prepared by introducing a measured quantity of the subject chemical into a Tedlar bag containing a measured quantity of pure air. The response factor was then calculated by:

$$\text{Response Factor (RF)} = \frac{\text{Actual Concentration}}{\text{Observed Concentration}}$$

## SECTION 2

### CONCLUSIONS

This report presents data on the sensitivity of two types of portable hydrocarbon analyzers, the "OVA-108" and the "TLV Sniffer", to 168 different chemical compounds. This sensitivity is expressed as a response factor for each chemical based on a calibration to methane. The response factor is defined as the ratio of the actual concentration to the observed concentration (or response).

#### 2.1 SUMMARY OF RESULTS

One of the major conclusions of this work is that response factors vary with concentration, which makes it difficult to characterize a given chemical's response with a single number. Attempts to characterize the entire concentration range with a mean value (or other similar statistical parameters) have proved unsuccessful.

The estimated response factor at an actual concentration of 10,000 ppw has been chosen as the most desirable single point mode of expression. Table 2-1 presents these estimated response factors for all 168 chemicals on both types of instruments and the 95 percent confidence intervals which bound the estimates. Figures 2-1 and 2-2 are graphical representations of the same data for the OVA and TLV, respectively.

The choice of an estimated response factor at 10,000 ppw actual concentration is based on the need to provide meaningful input to the regulation and control of fugitive emissions from the SOCNI. The Background Information Document on fugitives from SOCNI<sup>(1)</sup> recommends an action level of 10,000 ppw



TABLE 2-1  
 FITTED RESPONSE FACTORS  
 WITH 95 % CONFIDENCE INTERVALS  
 ESTIMATED AT 10,000 PPMV

DEPOB* ID NO	COMPOUND NAME	VOLATILITY CLASS**	OVA		FLV	
			RESPONSE FACTOR	CONFIDENCE INTERVALS	RESPONSE FACTOR	CONFIDENCE INTERVALS
70	ACETIC ACID	LL	1.83	( 1.17- 2.87)	9.70	( 4.16- 17.81)
80	ACETIC ANHYDRIDE	LL	1.36	( 1.12- 1.65)	2.89	( 1.62- 5.14)
90	ACETONE	LL	0.79	( 0.53- 1.10)	1.22	( 0.81- 1.83)
100	ACETONE CYANHYDRIN	ML	2.42	( 0.70- 16.83)	7.84	( 1.40- 43.78)
110	ACETONITRILE	LL	0.94	( 0.89- 1.05)	1.17	( 0.98- 1.42)
120	ACETOPHENONE	HL	10.98	( 0.98- 21.68)	54.86	( 38.35- 78.48)
125	ACETYL CHLORIDE	LL	1.89	( 1.76- 2.26)	2.59	( 1.81- 3.71)
	ACETYL-1-PROPANOL, 3-	LL	10.87	( 6.98- 17.90)	25.81	( 13.70- 48.03)
130	ACETYLENE	G	0.37	( 0.32- 0.43)	11.95	( 10.41- 13.73)
160	ACRYLIC ACID	LL	4.65	( 3.85- 5.51)	36.95	( 5.34- 255.00)
170	ACRYLONITRILE	LL	0.98	( 0.79- 1.17)	2.70	( 0.44- 18.30)
	ALLENE	G	0.55	( 0.49- 0.61)	5.78	( 5.38- 6.24)
200	ALLYL ALCOHOL	LL	0.94	( 0.69- 1.30)		
250	AMYL ALCOHOL, N-	HL	0.60	( 0.47- 1.00)	1.78	( 1.19- 2.65)
2855	AMYLENE	LL	0.31	( 0.19- 0.51)	1.03	( 0.46- 2.32)
330	ANISOLE	LL	0.92	( 0.64- 1.32)	2.69	( 1.69- 4.71)
360	BENZALDEHYDE	HL	2.30	( 1.52- 3.68)	0.20	( 5.77- 8.88)
380	BENZENE	LL	0.21	( 0.19- 0.24)	1.07	( 0.97- 1.19)
450	BENZONITRILE	ML	2.24	( 1.18- 4.24)	9.13	( 2.82- 29.62)
490	BENZOYL CHLORIDE	HL	6.40	( 3.70- 12.80)	6.60	( 3.61- 12.79)
510	BENZYL CHLORIDE	HL	4.22	( 2.74- 5.52)	4.87	( 2.50- 9.48)
570	BROMBENZENE	LL	0.36	( 0.28- 0.46)	1.16	( 0.69- 1.94)
590	BUTADIENE, 1,3-	G	0.37	( 0.34- 0.42)	6.00	( 5.64- 6.39)
	BUTANE, N-	G	0.36	( 0.31- 0.46)	0.88	( 0.61- 0.75)
640	BUTANOL, N	LL	1.42	( 0.66- 3.13)	2.80	( 1.49- 5.27)
650	BUTANOL, SEC-	LL	0.70	( 0.63- 0.78)	1.20	( 1.00- 1.57)
660	BUTANOL, TERT	S	0.44	( 0.26- 0.74)	2.19	( 1.54- 3.11)
592	BUTENE, 1-	G	0.51	( 0.45- 0.58)	2.97	( 2.73- 3.24)
600	BUTYL ACETATE, N-	LL	0.60	( 0.48- 0.78)	1.30	( 1.18- 1.42)
630	BUTYL ACRYLATE, N-	LL	0.64	( 0.58- 0.74)	1.98	( 0.89- 4.43)
	BUTYL ETHER, N	LL	2.70	( 1.85- 3.73)	2.66	( 1.42- 4.95)

\* ORGANIC CHEMICAL PRODUCERS DATA BASE.

\*\* G = GAS; LL = LIGHT LIQUID; HL = HEAVY LIQUID.

TABLE 2-1 (continued)

FITTED RESPONSE FACTORS  
WITH 95 % CONFIDENCE INTERVALS  
ESTIMATED AT 10,000 PPMV

DCPDB ID NO	COMPOUND NAME	VOLATILITY CLASS**	GVA		TLV	
			RESPONSE FACTOR	CONFIDENCE INTERVALS	RESPONSE FACTOR	CONFIDENCE INTERVALS
670	BUTYL ETHER, SEC	LL	0.25	( 0.11- 0.60)	1.13	( 0.78- 1.64)
680	BUTYLAMINE, N-	LL	0.63	( 0.43- 0.82)	1.91	( 1.38- 2.65)
690	BUTYLAMINE, SEC-	LL	0.67	( 0.52- 0.84)	1.90	( 1.26- 2.79)
	BUTYLAMINE, TERT-	LL	0.98	( 0.82- 0.65)	1.80	( 1.53- 2.11)
	BUTYLBENZENE, TERT-	HL	1.27	( 0.94- 1.73)	6.42	( 1.82- 22.07)
750	BUTYRALDEHYDE, N-	LL	1.39	( 1.12- 1.71)	1.89	( 1.50- 2.27)
760	BUTYRIC ACID	HL	0.74	( 0.22- 2.52)	4.58	( 2.39- 8.78)
780	BUTYRONITRILE	LL	0.40	( 0.31- 0.70)	1.33	( 0.44- 3.99)
790	CARBON DISULFIDE	LL	571.92	( 279.65-1169.7)	2.95	( 2.82- 3.34)
810	CARBON TETRACHLORIDE	LL	21.28	( 10.95- 41.36)	30.52	( 8.98-103.88)
830	CHLORACETALDEHYDE	LL	13.40	( 9.85- 18.24)	5.07	( 3.65- 7.06)
890	CHLOROBENZENE	LL	0.36	( 0.28- 0.48)	0.88	( 0.77- 1.00)
1740	CHLOROETHANE	G	0.87	( 0.02- 22.84)	2.18	( 0.31- 14.93)
930	CHLOROFORM	LL	4.48	( 3.60- 5.98)	8.77	( 6.65- 13.84)
960	CHLOROPHENOL, O-	HL	3.33	( 1.88- 5.92)	5.87	( 2.45- 14.08)
	CHLOROPROPENE, 1-	LL	0.59	( 0.53- 0.66)	0.84	( 0.54- 1.19)
710	CHLOROPROPENE, 2-	LL	0.75	( 0.65- 0.87)	1.24	( 1.09- 1.41)
970	CHLOROTOLUENE, M-	LL	0.43	( 0.38- 0.47)	0.82	( 0.70- 1.21)
980	CHLOROTOLUENE, O-	LL	0.45	( 0.38- 0.54)	1.05	( 0.62- 2.12)
990	CHLOROTOLUENE, P-	LL	0.52	( 0.47- 0.58)	1.15	( 0.62- 2.12)
1010	CRESOL, O-	S	0.95	( 0.59- 1.52)	3.98	( 0.22- 72.91)
1040	CROTOMALDEHYDE	LL	1.32	( 0.78- 2.23)	8.64	( 2.53- 31.38)
1060	CUMENE	LL	1.92	( 1.13- 3.28)	12.49	( 5.62- 27.74)
1120	CYCLOHEXANE	LL	0.82	( 0.58- 1.17)	4.92	( 1.18- 20.48)
1130	CYCLOHEXANOL	HL	1.50	( 1.01- 2.22)	3.99	( 1.79- 8.91)
1140	CYCLOHEXANONE	LL	0.40	( 0.32- 0.51)	1.84	( 1.65- 2.05)
1150	CYCLOHEXENE	LL	0.47	( 0.28- 0.78)	1.38	( 1.31- 1.45)
1160	CYCLOHEXYLAMINE	LL	0.00	( 0.00- 3.31)	0.20	( 0.00- 31.01)
	DECANE	HL	1.53	( 1.01- 2.31)	0.98	( 0.29- 3.38)
1190	DIACETONE ALCOHOL	HL	1.81	( 1.31- 1.99)	2.81	( 2.15- 3.87)
	DIACETYL	LL				

\* ORGANIC CHEMICAL PRODUCERS DATA BASE

\*\* G = GAS; LL = LIGHT LIQUID; HL = HEAVY LIQUID.

TABLE 2-1 (continued)

FITTED RESPONSE FACTORS  
WITH 95 % CONFIDENCE INTERVALS  
ESTIMATED AT 10,000 PPBY

OCFDB* 10 NO	COMPOUND NAME	VOLATILITY CLASS**	OVA		FLV	
			RESPONSE FACTOR	CONFIDENCE INTERVALS	RESPONSE FACTOR	CONFIDENCE INTERVALS
1270	DICHLOR-1-PROPANOL, 2,3-	LL	81.81	( 30.13-125.55)	34.34	( 1.22-49.55)
-	DICHLOR-1-PROPENE, 2,3-	LL	0.70	( 0.47-1.05)	1.82	( 1.23-2.14)
-	DICHLOR-2-PROPANOL, 1,3-	LL	29.34	( 17.42-49.40)	18.62	( 12.95-26.82)
1215	DICHLOROBENZENE, N-	HL	0.68	( 0.56-0.78)	1.89	( 1.37-2.60)
1216	DICHLOROBENZENE, O-	HL	0.70	( 0.48-1.02)	1.72	( 0.80-1.80)
-	DICHLOROTRIANE, 1,1-	LL	0.77	( 0.50-0.98)	1.80	( 1.58-2.06)
1244	DICHLOROTRIANE, 1,2-	LL	0.95	( 0.77-1.18)	2.08	( 1.73-2.51)
1235	DICHLOROTRIETHYLENE, CIS, 1,2-	LL	1.31	( 1.08-1.58)	1.93	( 1.02-3.06)
1236	DICHLOROTRIETHYLENE, TRANS, 1,2-	LL	1.13	( 0.99-1.20)	1.88	( 0.55-6.29)
2620	DICHLOROTRIETHYLENE, TRANS, 1,2-	LL	2.26	( 1.94-2.64)	3.63	( 2.72-4.84)
3110	DICHLOROPROPANE, 1,2-	LL	1.03	( 0.82-1.29)	1.80	( 1.12-2.89)
1440	DIBROMOTRIETHYLENE	LL	0.74	( 0.17-0.30)	1.79	( 0.97-2.01)
-	DIBROMOPROPANE, 1,2-	LL	0.42	( 3.68-24.18)	24.96	( 6.07-102.87)
1870	DIMETHYL BENZENE, 1,3-	LL	1.28	( 0.97-2.00)	1.42	( 1.16-1.75)
1490	DIMETHOXY ETHANE, 1,2-	LL	3.89	( 3.11-4.85)	2.95	( 2.88-3.03)
1495	DIMETHYLHYDRAZINE, 1,1-	LL	1.04	( 0.71-1.52)	2.74	( 1.61-4.87)
-	DIMETHYLSTYRENE, 2,4-	LL	37.09	( 28.75-53.42)	78.06	( 38.51-158.23)
1520	DIMETHYLSULFOXIDE	HL	0.00	( 0.00-4300.81)	4.88	( 1.41-16.92)
1480	DIOXANE	LL	1.58	( 1.10-2.28)	1.23	( 1.07-1.41)
1650	EPICHLOROHYDRIN	LL	1.72	( 1.51-1.82)	2.02	( 1.84-2.22)
-	ETHANE	G	0.97	( 0.20-1.26)	0.72	( 0.21-2.52)
1680	ETHANOL	LL	2.04	( 1.62-2.78)	-	-
1910	ETHOXY ETHANOL, 2-	LL	1.68	( 1.28-2.06)	1.81	( 1.42-1.84)
1670	ETHYL ACETATE	LL	0.84	( 0.74-0.94)	1.37	( 1.08-1.74)
1680	ETHYL ACRYLATE	HL	3.02	( 1.98-4.82)	3.12	( 2.71-3.62)
1690	ETHYL ACRYLATE	LL	0.72	( 0.55-0.92)	-	-
1750	ETHYL CHLOROACETATE	LL	1.97	( 1.70-2.21)	1.47	( 0.97-2.20)
1990	ETHYL ETHER	LL	0.97	( 0.73-1.28)	1.11	( 1.01-1.23)
1710	ETHYLBENZENE	LL	0.70	( 0.45-1.09)	3.14	( 1.42-8.92)
1770	ETHYLENE	G	0.82	( 0.39-0.88)	1.49	( 1.27-1.74)
1880	ETHYLENE OXIDE	G	2.72	( 2.31-3.20)	2.43	( 1.92-3.02)

\* ORGANIC CHEMICAL PRODUCERS DATA BASE.

\*\* G - GAS; LL - LIGHT LIQUID; HL - HEAVY LIQUID.

TABLE 2-1 (continued)



TABLE 2-1 (continued)

FITTED RESPONSE FACTORS  
WITH 95 % CONFIDENCE INTERVALS

ESTIMATED AT 10,000 PPBV

COPD ID NO	COMPOUND NAME	VOLATILITY CLASS**	OVA		FLY	
			RESPONSE FACTOR	CONFIDENCE INTERVALS	RESPONSE FACTOR	CONFIDENCE INTERVALS
1800	ETHYLENEDIAMINE	LL	1.78	( 1.39 - 2.38)	2.40	( 1.83 - 3.21)
2060	FORMIC ACID	LL	34.87	( 29.00 - 41.94)	33.21	( 16.78 - 65.73)
1721	FREON 12	G	9.55	( 6.99 - 13.32)	11.83	( 3.63 - 38.59)
2073	FURFURAL	HL	7.96	( 3.69 - 13.15)	10.01	( 9.72 - 10.31)
2105	GLYCIDOL	LL	8.42	( 5.14 - 13.83)	5.23	( 2.68 - 10.23)
-	HEPTANE	LL	0.30	( 0.12 - 0.75)	0.79	( 0.56 - 1.08)
-	HEXANE, N-	LL	0.31	( 0.20 - 0.38)	0.72	( 0.65 - 0.79)
-	HEXANE, 1-	LL	0.39	( 0.20 - 0.81)	2.52	( 0.85 - 9.09)
-	HYDROXYACETONE	LL	8.70	( 6.91 - 11.84)	9.34	( 6.21 - 14.06)
2200	ISOBUTANE	G	0.30	( 0.09 - 0.95)	0.61	( 0.44 - 0.66)
2350	ISOBUTYLENE	G	2.42	( 1.01 - 5.84)	8.23	( 0.09 - 46.41)
2160	ISOPRENE	LL	0.48	( 0.22 - 0.72)	-	-
2370	ISOPROPANOL	LL	0.80	( 0.88 - 1.48)	1.35	( 0.78 - 1.96)
2390	ISOPROPYL ACETATE	LL	0.68	( 0.58 - 0.80)	1.75	( 1.11 - 1.40)
-	ISOPROPYL CHLORIDE	LL	0.62	( 0.52 - 0.73)	0.99	( 0.81 - 1.19)
-	ISOVALERALDEHYDE	LL	0.55	( 0.40 - 0.66)	2.04	( 1.19 - 3.51)
2450	METHYL OXIDE	LL	1.12	( 0.94 - 1.33)	3.12	( 1.68 - 5.19)
-	METHACROLEIN	LL	1.27	( 0.91 - 1.77)	3.10	( 1.65 - 5.83)
2460	METHACRYLIC ACID	HL	0.71	( 0.06 - 7.84)	0.61	( 0.37 - 1.16)
2500	METHANOL	LL	5.69	( 4.00 - 8.27)	1.88	( 1.52 - 2.18)
1930	METHOXY-ETHANOL, 2-	LL	2.70	( 1.95 - 3.67)	3.19	( 1.85 - 5.03)
2510	METHYL ACETATE	LL	1.80	( 1.55 - 2.08)	1.76	( 1.47 - 2.12)
-	METHYL ACETYLENE	G	0.53	( 0.50 - 0.51)	3.92	( 3.59 - 4.29)
2500	METHYL CHLORIDE	G	1.75	( 1.44 - 2.14)	2.95	( 1.62 - 3.13)
2640	METHYL ETHYL KETONE	LL	0.57	( 0.40 - 0.81)	1.12	( 0.93 - 1.35)
2645	METHYL FORMATE	LL	3.42	( 2.87 - 4.19)	1.93	( 1.76 - 2.11)
2655	METHYL METHACRYLATE	LL	0.99	( 0.89 - 1.10)	2.36	( 1.54 - 3.62)
2650	METHYL-2-PENTANOL, 4-	LL	1.70	( 1.33 - 2.17)	1.94	( 1.46 - 2.58)
2080	METHYL-2-PENTANONE, 4-	LL	0.49	( 0.28 - 0.64)	1.54	( 1.22 - 1.94)
-	METHYL-2,4-PENTANEDIOL, 3-	LL	0.34	( 0.23 - 0.40)	0.77	( 0.36 - 1.23)
2550	METHYL-2-BUTYN-2-OL, 2-	LL	0.51	( 0.32 - 0.78)	-	-

\* ORGANIC CHEMICAL PRODUCERS DATA BASE.

\*\* G = GAS; LL = LIGHT LIQUID; HL = HEAVY LIQUID.

TABLE 2-3 (cont. Inued)  
 FITTED RESPONSE FACTORS  
 WITH 95 % CONFIDENCE INTERVALS  
 ESTIMATED AT 10,000 PPBV

OCPOB* ID NO	COMPOUND NAME	VOLATILITY CLASS**	OVA		TLV	
			RESPONSE FACTOR	CONFIDENCE INTERVALS	RESPONSE FACTOR	CONFIDENCE INTERVALS
	METHYLAL	LL	1.46	( 1.09 - 1.81)	1.41	( 1.23 - 1.62)
2540	METHYLANILINE, N-	HL	4.13	( 3.75 - 4.54)	5.75	( 0.99 - 27.84)
2570	METHYLCYCLOHEXANE	LL	0.38	( 0.12 - 1.18)	0.85	( 0.67 - 1.07)
	METHYLCYCLOHEXENE, 1-	LL	0.33	( 0.24 - 0.48)	2.22	( 1.70 - 2.91)
	METHYL PENTANOL	LL	1.17	( 0.71 - 1.92)	2.82	( 1.92 - 4.14)
2670	METHYLSTYRENE, 4-	LL	10.24	( 8.30 - 12.63)	31.46	( 16.08 - 61.53)
1660	MORCETHANOLAMINE	LL	28.04	( 8.79 - 123.04)	25.83	( 11.83 - 56.44)
2700	MORPHOLINE	LL	0.92	( 0.84 - 1.22)	1.93	( 0.26 - 10.40)
2770	NIROBENZENE	HL	29.77	( 2.92 - 228.03)	40.81	( 4.68 - 352.81)
2790	NIROETHANE	LL	1.40	( 1.23 - 1.59)	2.54	( 1.60 - 4.04)
2791	NIROMETHANE	LL	3.32	( 3.03 - 3.64)	5.25	( 2.72 - 11.81)
2795	NIROPROPANE	LL	1.06	( 0.79 - 1.47)	1.77	( 1.22 - 2.57)
	NONANE - N	LL	1.62	( 0.93 - 2.81)	5.54	( 2.82 - 10.49)
	OCTANE	LL	1.04	( 0.88 - 1.22)	3.08	( 1.78 - 2.46)
2851	PENTANE	LL	0.42	( 0.30 - 0.58)	0.62	( 0.55 - 0.69)
2910	PHENOL	LL	11.75	( 7.55 - 18.29)	12.01	( 3.57 - 40.43)
2973	PHENYL-2-PROPANOLS, 2-	LL	89.50	( 69.84 - 114.87)	76.57	( 46.78 - 126.42)
	PICOLINE, 2	LL	0.34	( 0.27 - 0.41)	1.17	( 1.10 - 1.25)
	PROPANE	G	0.88	( 0.10 - 7.54)	0.67	( 0.24 - 1.64)
3063	PROPIONALDEHYDE	LL	1.14	( 1.02 - 1.30)	1.65	( 1.16 - 2.36)
3066	PROPIONIC ACID	LL	1.34	( 1.06 - 1.69)	3.51	( 0.90 - 13.02)
3070	PROPYL ALCOHOL	LL	0.91	( 0.72 - 1.13)	1.55	( 1.41 - 1.71)
	PROPYLBENZENE, N	LL	0.44	( 0.37 - 0.53)	5.97	( 0.33 - 108.14)
3090	PROPYLENE	G	0.78	( 0.30 - 1.97)	2.83	( 0.96 - 8.20)
3120	PROPYLENE OXIDE	LL	0.80	( 0.69 - 0.93)	1.15	( 0.68 - 1.93)
3130	PYRIDINE	LL	0.41	( 0.30 - 0.51)	1.17	( 1.03 - 1.32)
3230	STYRENE	LL	4.16	( 3.68 - 4.71)	26.83	( 7.32 - 985.28)
3290	TETRACHLOROETHANE, 1,1,1,2	LL	3.00	( 1.27 - 1.07)	6.52	( 2.82 - 11.11)
3291	TETRACHLOROETHANE, 1,1,2,2	LL	6.06	( 4.78 - 1.88)	14.14	( 8.51 - 23.51)
2760	TETRACHLOROETHYLENE	LL	3.16	( 1.92 - 5.21)	11.46	( 6.64 - 15.20)
3349	TOLUENE	LL	0.33	( 0.29 - 0.38)	1.32	( 0.79 - 6.82)

\* ORGANIC CHEMICAL PRODUCERS DATA BASE

\*\* CAS - GAS, LL - LIGHT LIQUID, HL - HEAVY LIQUID

TABLE 2-1 (continued)  
 FITTED RESPONSE FACTORS  
 WITH 95 % CONFIDENCE INTERVALS  
 ESTIMATED AT 10,000 PPMV

DCPDB* ID NO	COMPOUND NAME	VOLATILITY CLASS**	OVA		FLV	
			RESPONSE FACTOR	CONFIDENCE INTERVALS	RESPONSE FACTOR	CONFIDENCE INTERVALS
3393	TRICHLOROBENZENE, 1,2,4-	HL	1.75	( 0.13- 14.00)	0.39	( 0.10- 1.57)
3395	TRICHLOROETHANE, 1,1,1-	LL	0.79	( 0.70- 0.89)	2.41	( 1.98- 2.96)
3400	TRICHLOROETHANE, 1,1,2-	LL	1.26	( 1.08- 1.47)	3.68	( 3.00- 4.43)
3410	TRICHLOROETHYLENE	LL	0.94	( 0.81- 1.08)	3.35	( 2.88- 4.19)
3420	TRICHLOROPROPANE, 1,2,3-	LL	0.95	( 0.54- 1.69)	2.23	( 1.47- 3.40)
3450	TRIMETHYLAMINE	LL	0.40	( 0.32- 0.67)	1.41	( 1.03- 1.92)
3480	VINYL ACETATE	LL	1.31	( 0.97- 1.76)	3.99	( 1.49- 10.69)
3520	VINYL CHLORIDE	G	0.65	( 0.50- 0.84)	1.10	( 0.79- 1.51)
3530	VINYLDENE CHLORIDE	LL	0.94	( 0.40- 2.23)	0.70	( 0.02- 22.87)
3570	XYLENE, P-	LL	1.19	( 0.88- 1.84)	3.38	( 1.95- 2.90)
3550	XYLENE, M-	LL	2.27	( 1.87- 2.76)	0.35	( 0.34- 0.58)
3560	XYLENE, O-	LL	0.30	( 0.20- 0.37)	3.56	( 0.93- 13.64)
		LL	0.36	( 0.16- 0.77)	1.40	( 0.73- 2.70)


\* ORGANIC CHEMICAL PRODUCERS DATA BASE.

\*\* G = GAS; LL = LIGHT LIQUID; HL = HEAVY LIQUID.





Figure 2-1 (continued)  
 SITES ADJACENT TO RIVER  
 WITH THE GREATEST INCREASE  
 BY 1988 FROM 1981

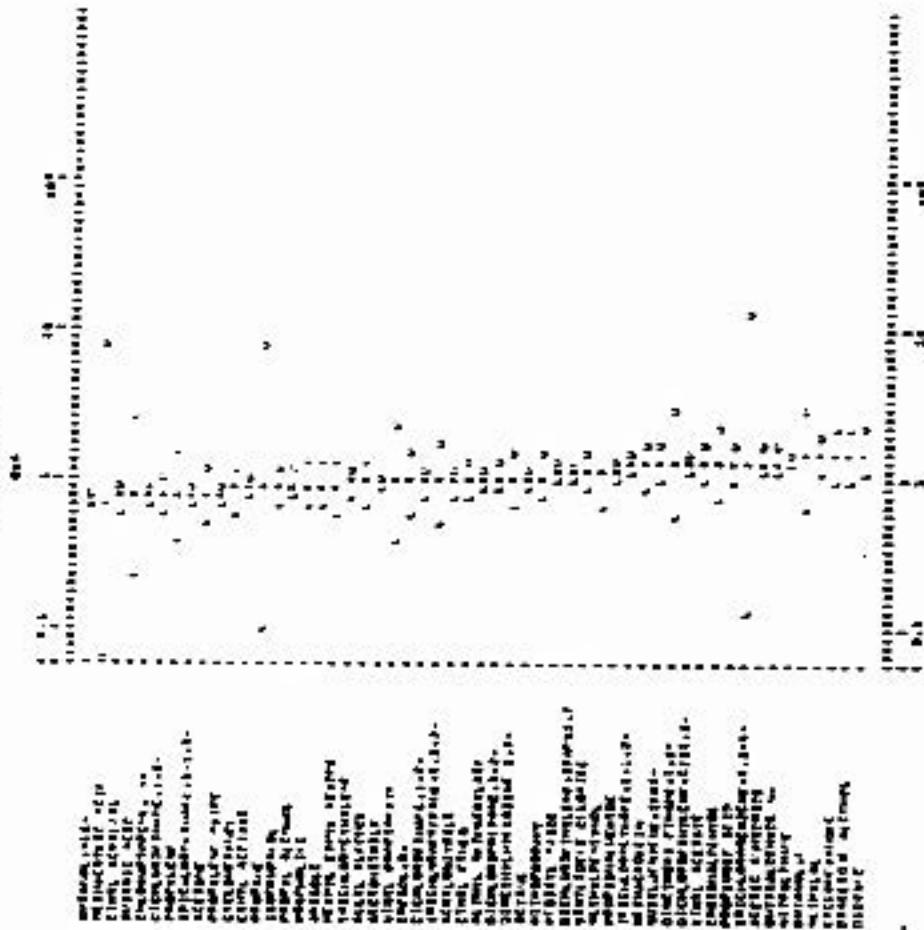











as read directly on the OVA. Response factors are estimated at 10,000 ppmv actual concentration rather than 10,000 ppmv meter response because the experimental design and the statistical interpretation of the data are cleaner and more straightforward when the response factor is estimated in terms of an independent variable (actual concentration) rather than a dependent variable (instrument response).

Table 2-2 presents a comparison of these response factor estimates to previously published data. All previous studies on the TLV are based on hexane calibration, so a column is added giving the response factors from this study converted to a hexane basis. Even with this adjustment, there remains considerable variation between the values obtained in this study and those from literature. The primary cause of this variation is believed to be the change of response factor with concentration. Although the detailed methodology used in determining the previously published response factors is not known, it is likely that they were determined at low concentrations (in the range of 50 to 500 ppmv). This comparison adds emphasis to the dangers involved in the single point expression of response factors. If accurate results are desired for concentrations other than 10,000 ppmv, the detailed results in Section 5.0 should be used to generate an estimated response factor at the concentrations of interest.

The response factor estimates discussed above were based on data taken at three different concentrations. The target values for response factor determinations were set at 200, 1500, and 8000 ppmv. Of the 168 chemicals tested, 79 of them (or 46 percent) were able to achieve these levels.

The maximum concentration on many chemicals was limited by either volatility, instrument response, or explosivity. About 40 chemicals (or 24 percent) were not volatile enough to be prepared at 8000 ppmv at laboratory temperature. These chemicals were prepared at a maximum of 90 percent of their saturated concentration to prevent condensation in the bag and resulting inaccuracies in calculating the actual concentration.



TABLE 2-2. COMPARISON OF RESPONSE FACTORS FROM THIS STUDY TO PREVIOUSLY PUBLISHED VALUES

Vibration Type	Vibration Name	V1		V2	
		Min. Range (G)	Maximum Response (G)	Min. Range (G)	Maximum Response (G)
70	Steel to Steel	1.41	-	1.70	1.41
80	Concrete	2.74	1.47 <sup>(1)</sup>	1.12	1.47
90	Welded Steel	2.11	4.56 <sup>(2)</sup>	1.77	14.17
100	Cast-in-place	2.76	9.44 <sup>(3)</sup>	-	1.70
110	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
120	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
130	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
140	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
150	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
160	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
170	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
180	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
190	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
200	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
210	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
220	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
230	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
240	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
250	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
260	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
270	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
280	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
290	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
300	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
310	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
320	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
330	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
340	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
350	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
360	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
370	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
380	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
390	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
400	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
410	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
420	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
430	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
440	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
450	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
460	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
470	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
480	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56
490	Steel Deck	2.21	4.17 <sup>(1)</sup>	-	1.56
500	Concrete	2.21	4.17 <sup>(1)</sup>	-	1.56

About 49 chemicals (or 29 percent) achieved an instrument response over 10,000 ppmv prior to reaching the 8000 ppmv actual concentration. A trial and error process was used to get a readable response value at the top end of the scale (i.e., if the 8000 ppmv bag went off scale, a 6000 ppmv bag was tested, and then a 4000 ppmv, and so on until a readable response was achieved).

Only two chemicals (or about one percent) were limited by explosivity. In such cases, the maximum concentration was set at 70 percent of the Lower Explosive Limit (LEL) for obvious safety reasons.

One of the objectives of this work was to provide information to judge the suitability of these instruments to monitoring for fugitive VOC emissions in the SOCHI. Although no attempt at a final judgment will be made here, one obvious criterion of suitability can be examined. Any compound with a response factor greater than 100 will indicate less than a 10,000 ppmv action level even in pure form. But for the OVA this is complicated by flameout. The OVA depends on the sample gas flow for combustion air. When VOC concentrations in the sample gas get too high, the flame in the flame ionization detector (FID) is extinguished and the instrument ceases to respond. This will usually occur anywhere from 60,000 ppmv to 300,000 ppmv, depending on the specific compounds in the sample gas. Based on these figures, any chemical with a response factor greater than 30 would not be likely to exceed 10,000 ppmv before flame-out occurs. It can also be said that those chemicals with response factors between 6 and 30 are questionable as to whether a 10,000 ppmv reading would be noted before flameout. Of the 168 chemicals tested, only 6 have response factors greater than 30 and only 20 have response factors greater than 6. Since most of these will seldom occur in pure form, but rather in mixtures with more responsive chemicals, this should not prove to be a serious problem.


## 2.2 LINEARITY OF OVA RESPONSE

As explained in the previous subsection, most of the response factors were based on data taken at three concentrations. A three point data set will allow an evaluation of the overall linearity of response, but it has been suggested that the response may be linear only up to some critical concentration at which point it diverges. It has also been theorized that this critical concentration may be related to the Lower Explosive Limit (LEL) of the subject chemical. To test these theories, three chemicals were tested at ten or more concentrations. The selected chemicals (n-hexane, benzene, and methanol) were chosen to provide a range of organic functional groups, volatilities, LEL's, and response factors.

The data on n-hexane is presented in Figures 2-3 and 2-4. The first plot shows OVA response vs. actual concentration. This could be interpreted as a single linear data set if one is willing to accept a moderate degree of scatter. There do appear to be some break points with more linear segments between them, but no clear definition is evident. Figure 2-4 presents the same data, but it is plotted as actual concentration vs. response factor. This type of presentation accentuates the break points which would seem to occur at about 500 ppmv and 2000 ppmv. Both of these are well below hexane's LEL of 11,000 ppmv.<sup>(5)</sup> The instrument response reaches full scale at an actual concentration of about 3700 ppmv, so no meaningful data could be taken beyond that point.

The data on benzene are presented in similar fashion in Figures 2-5 and 2-6. The first plot appears to be quite linear throughout the concentration range, but a slight break point can be identified in the response factor plot. This break occurs at about 1400 ppmv, or ten percent of the benzene LEL (14,000 ppmv).<sup>(5)</sup>

WVA Response: Uprated

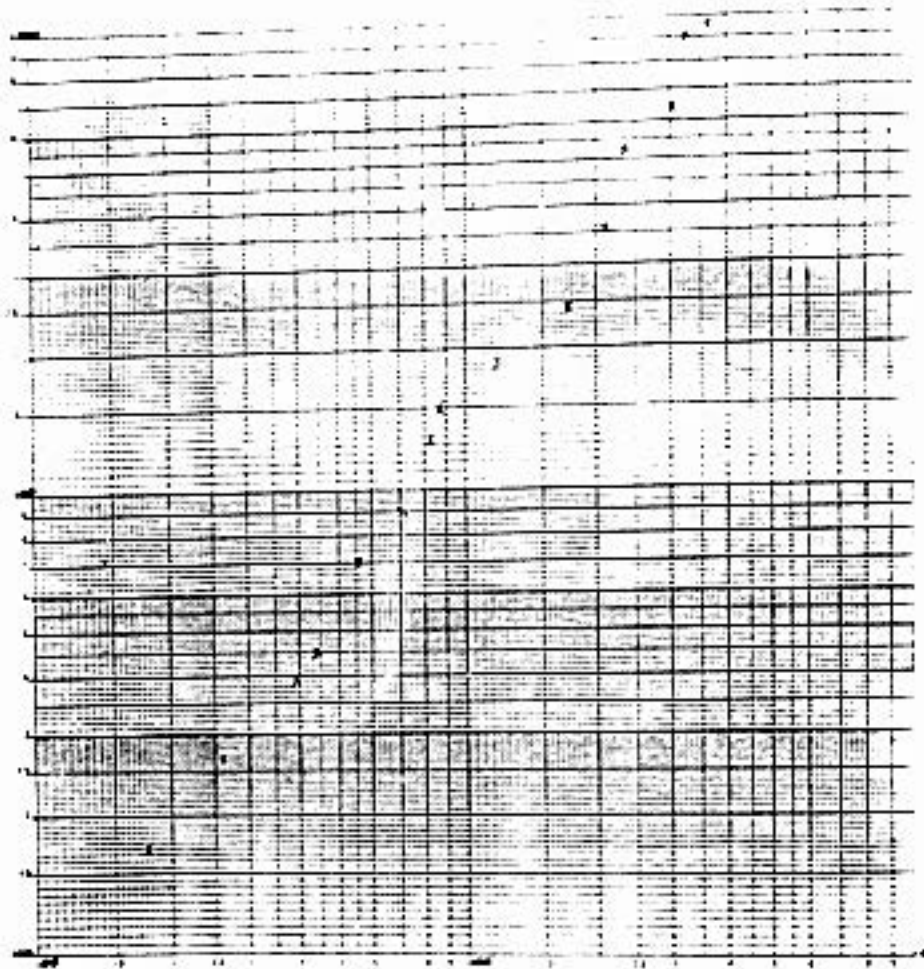

Actual Concentration (ppm)

Figure 1. Comparison of WVA results for hexane.



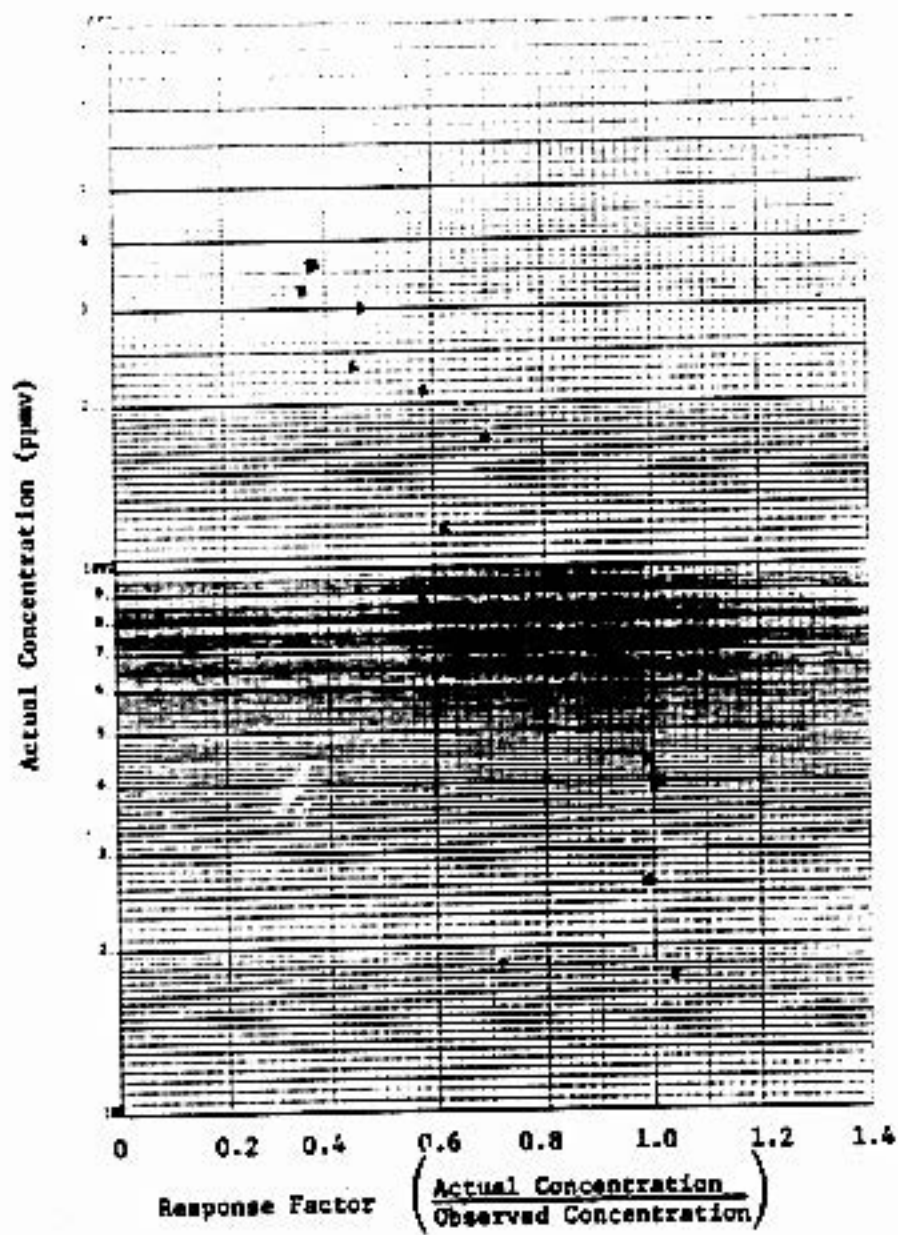


Figure 2-4. Variation of response factor with concentration - n-hexane.

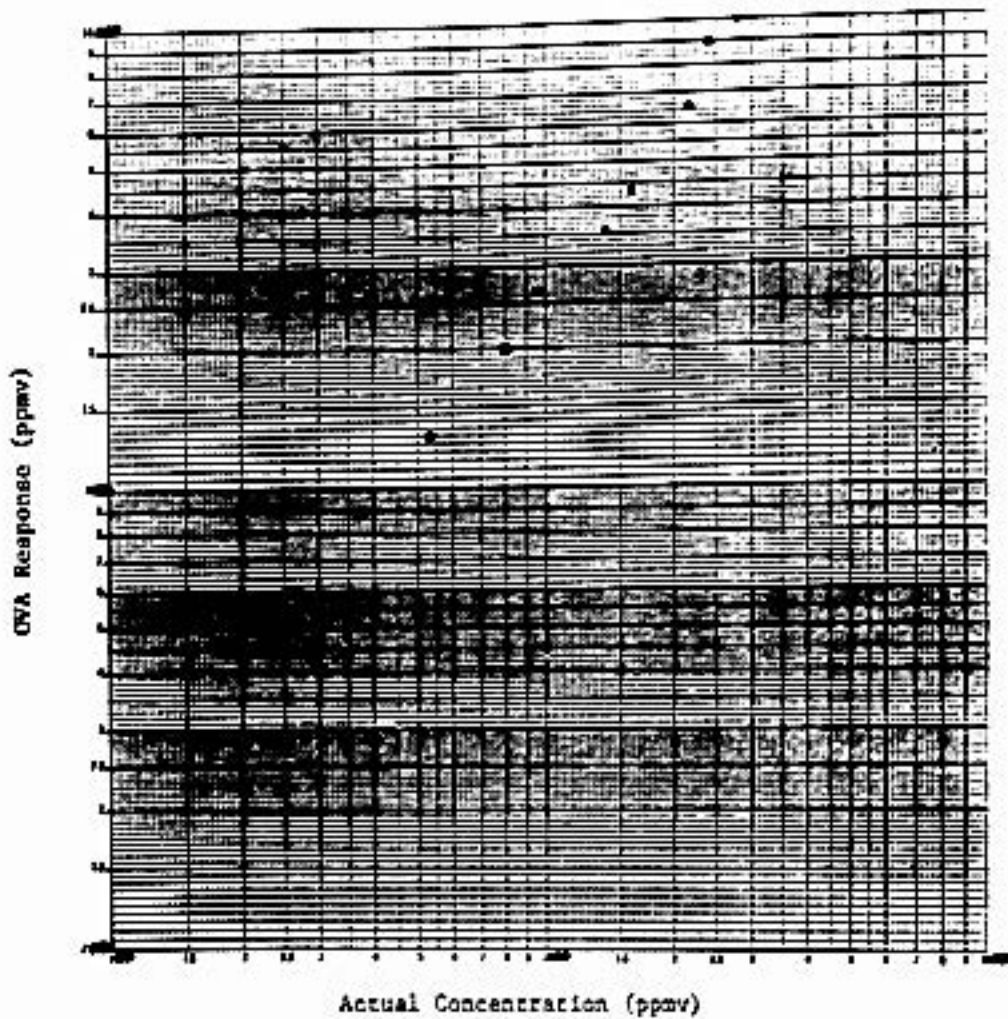


Figure 2-5. Linearity of OVA response to benzene.

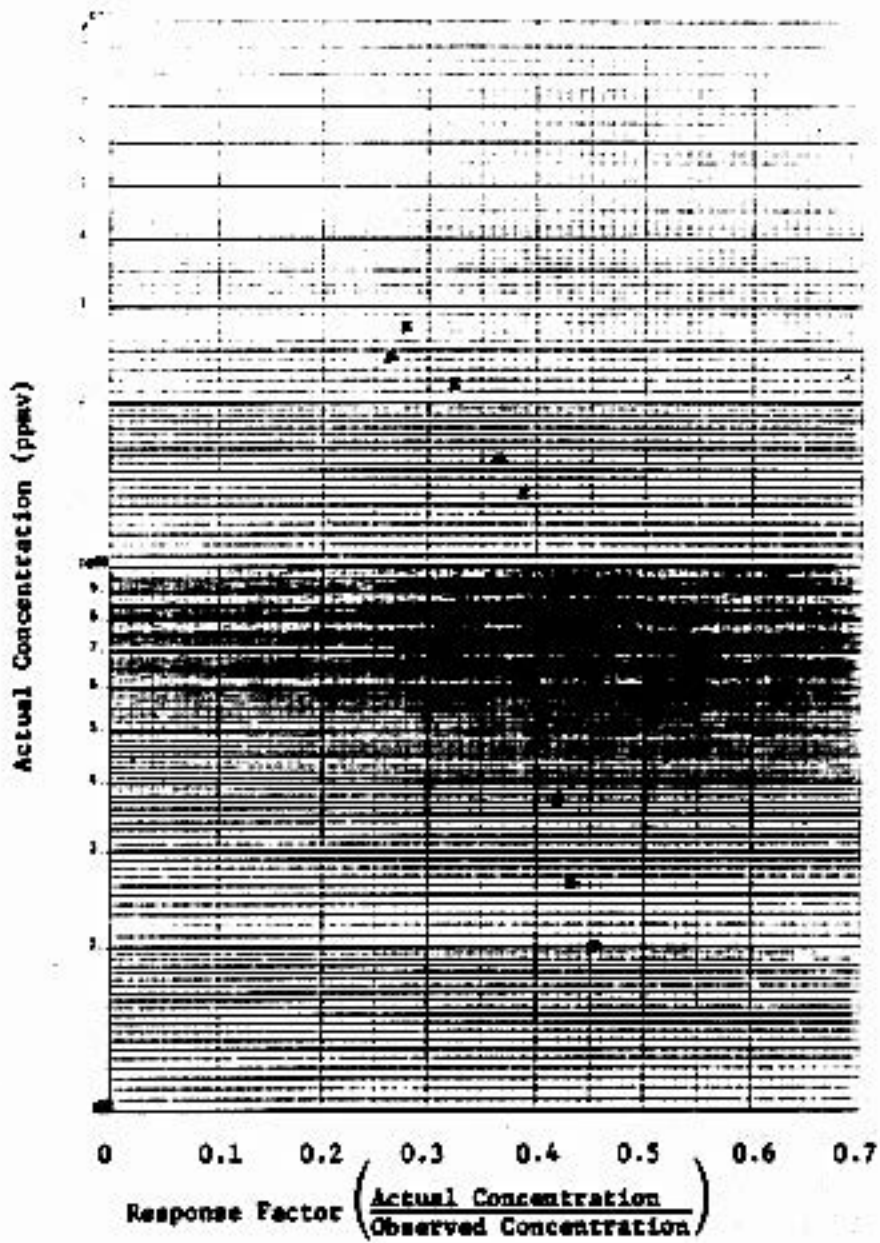


Figure 2-6. Variation of response factor with concentration - benzene.

Similar data on methanol are presented in Figures 2-7 and 2-8. The first plot would suggest a gently ascending curve, but it could be roughly fit with two linear segments intersecting at about 1600 ppmv. This inflection point would be quite low compared to the methanol LEL of 67,200 ppmv. (5) An examination of Figure 2-8 reveals a parabolic curve in the relationship between response factor and actual concentration, with a maximum response factor of about 7 exhibited in the concentration range of 2000 to 8000 ppmv. A second inflection point is noted around 8000 ppmv or 12 percent of the LEL.

All of these data would seem to indicate that the relationship between instrument response and concentration is a complex one. The scatter in the experimental data makes it difficult to state with confidence that any segment of the response is truly linear. There appear to be inflection points in the data, but there are not enough data to assess the relationship of these points to the LEL. These examples do clearly illustrate the large degree of variability in the response factors with concentration and should, therefore, demonstrate the need for care in applying a response factor calculated for one specific concentration.

### 2.3 CONVERSION OF RESPONSE FACTOR BASIS

The data presented in this report base all response factors on calibration to methane. Methane was chosen because of its ease of availability, its volatility (sufficient to prepare standards in the range of the proposed action level of 10,000 ppmv), and its use as the factory calibration standard for the OVA. For one reason or another, it may be more convenient for any given operator to calibrate with some other chemical and to convert the response factors to that calibration basis.

It has been theorized that this conversion can be accomplished in the following manner:



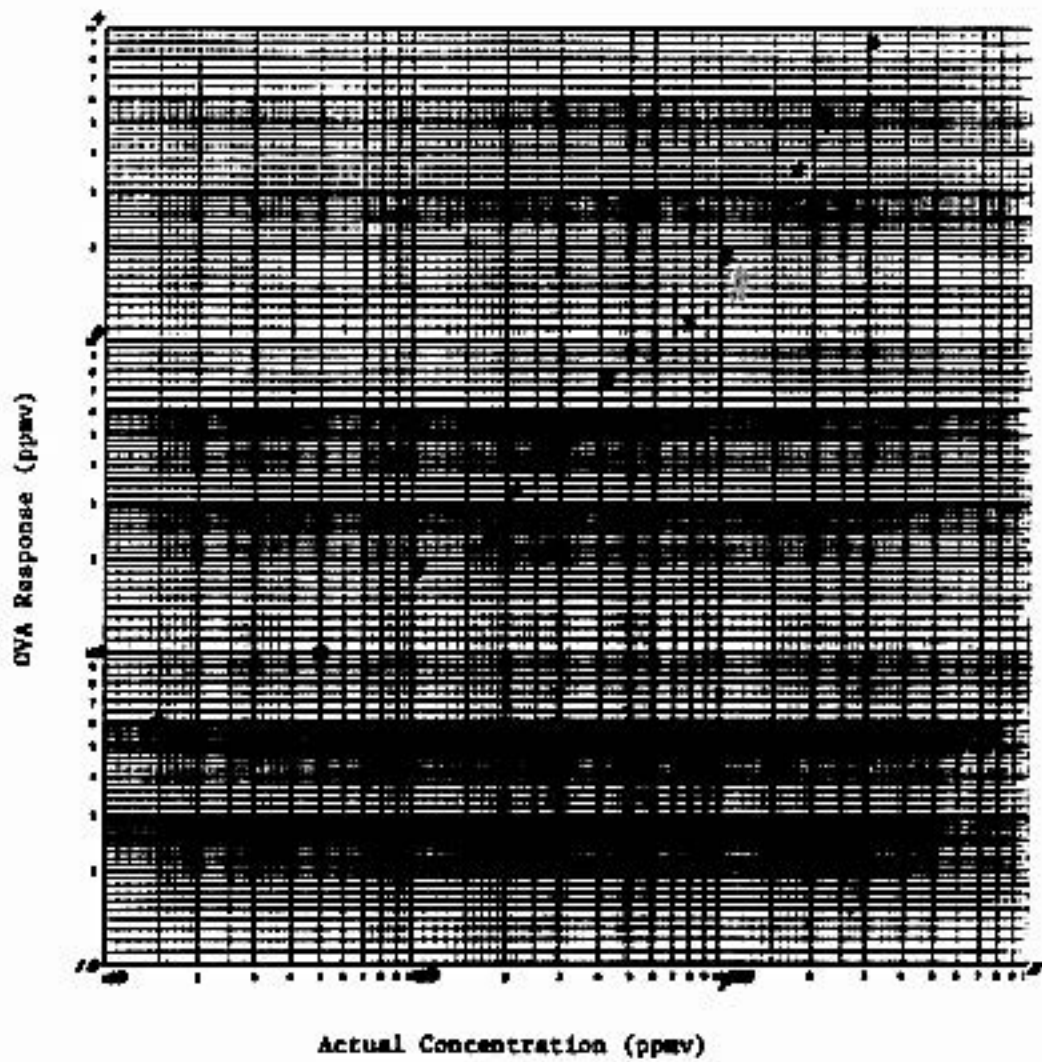


Figure 2-7. Linearity of OVA response to methanol.

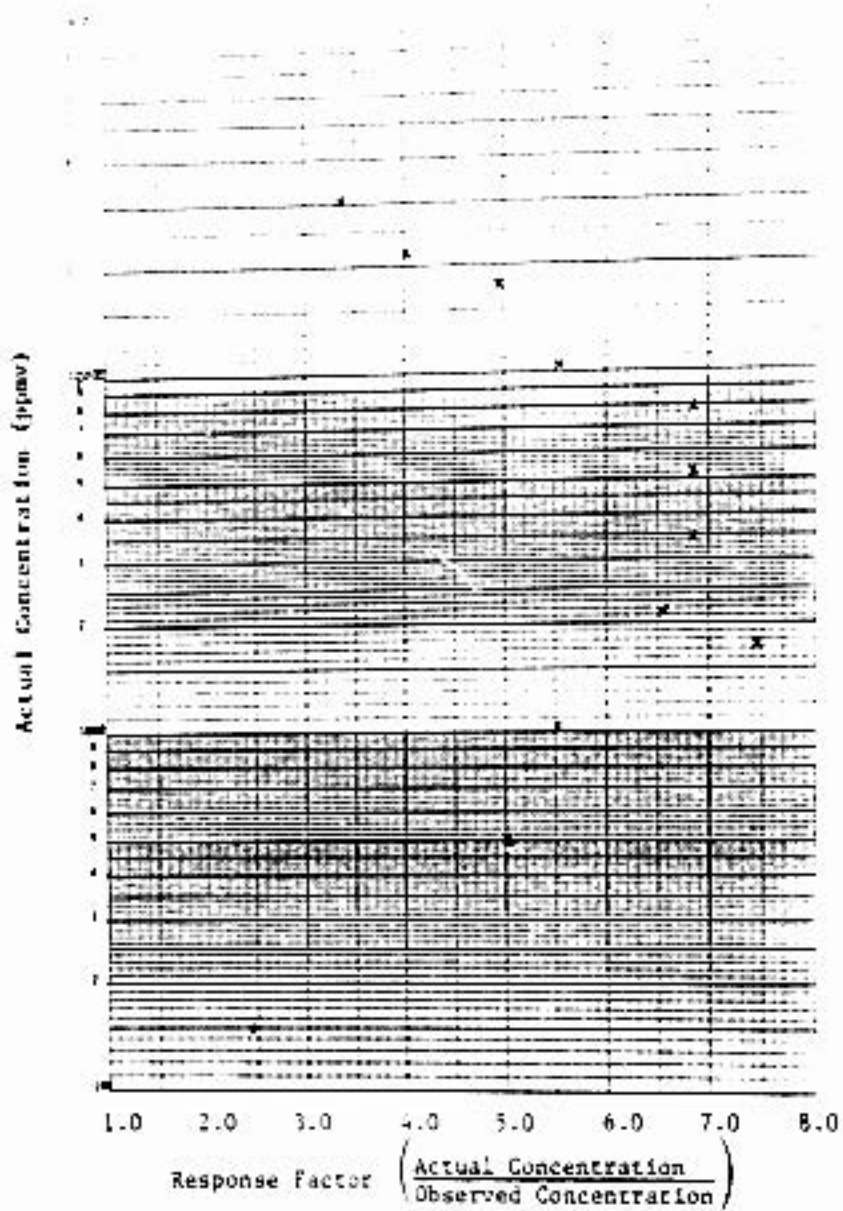


Figure 2-8. Variation of response factor with concentration - methanol.

$$RF_{AX} = \frac{RF_{AM}}{RF_{XM}}$$

where  $RF_{AX}$  is the response factor of chemical "A" as calibrated to chemical "X",

$RF_{AM}$  is the response factor of chemical "A" as calibrated to methane, and

$RF_{XM}$  is the response factor of chemical "X" as calibrated to methane.

In order to test this theory, the instruments were calibrated to n-hexane and the methane standards were run.

The data from these tests show that such a procedure works well on the TLV, where a predicted response factor of methane based on hexane of 1.50 compares favorably with the observed values of 1.56 at 533 ppmv and 1.50 at 8000 ppmv. The OVA results were not so conclusive, however, with a predicted value of 2.77 varying significantly from the observed values of 5.16 and 4.32 at 8000 and 533 ppmv respectively. It is possible that the variation of response factor with concentration is the cause of this discrepancy. The estimated response factor at 10,000 ppmv of hexane relative to methane is used to predict the response with reverse calibration. The OVA is calibrated on methane at 8000 ppmv in one case and on hexane at 5500 ppmv in the other case (because that is the highest stable concentration achievable at laboratory conditions). All these factors make the comparison difficult and much more extensive work would be required to confirm or reject the conversion procedure for the OVA.

## SECTION 3

### TEST PROCEDURES

The experimental procedures used to determine response factors are quite simple in theory, merely requiring that a calibrated instrument be used to sample a gas of known concentration. The response factor is then defined as the ratio of the actual concentration to the concentration indicated on the meter. The following subsections will present the detailed procedures involved in calibration, preparation of standard gases, instrument sampling, and quality control.

#### 3.1 DESCRIPTION OF THE INSTRUMENTS

Two types of instruments were used in the laboratory study, the Century Systems "OVA-108" and the J. W. Bacharach "TLV Sniffer". These particular instruments were chosen because they had both been successfully used in previous fugitive emission studies. Two instruments of each type were tested to check for normal variance between individual instruments and to check for any operating problems. One old and one new instrument of each type were selected to determine if there were any variances in response with detector age.

The Century Systems "OVA-108" is a portable flame ionization detector (FID) with a gas chromatograph option. In the total hydrocarbon mode used for fugitive emission screening, the chromatograph column is bypassed and the sample gas is introduced directly to the detector. The unit is battery powered and has its own hydrogen cylinder with enough fuel for 8 to 10 hours of continuous operation. The unit is certified to be intrinsically safe for operation in explosive atmospheres by Factory Mutual.



The readout on the OVA-108 is logarithmic and has a range from 1 to 10,000 ppmv. The range can be extended by the use of a dilution probe, but this feature was not used in the response factor study. Since the sample is diluted before it reaches the detector, no new response data would be gained by sampling higher concentrations with the dilution probe.

There are some important differences between the construction of the OVA and that of a "standard" laboratory FID. In the laboratory version, the hydrogen is mixed with the sample gas before combustion, and the flame is supported by an independent air supply. The OVA draws its combustion air through the sample probe, which is thus mixed with the sample gas. The OVA flame will, therefore, be extinguished if the VOC concentration gets too high or if a standard in N<sub>2</sub> is used instead of one in air. More importantly, there seem to be differences in the degree of ionization achieved with the OVA style FID as compared to the standard laboratory FID.

The J.W. Bacharach "TLV Sniffer" is a combustible gas detector. The sample gas is passed across a wire coated with oxidation promoting catalyst. Any combustible material is oxidized and the heat released causes the resistance of the coated wire to change. Half of the sample gas is routed through a comparison cell with an identical wire that has no catalyst coating. Both wires are set in a bridge network and the comparative resistance change is read out on a galvanometer. The face of the meter readout is marked directly in ppmv as factory calibrated to hexane. The response of the TLV thus depends on the heat of combustion and heat capacity of the sample gas.

### 3.2 CALIBRATION PROCEDURES

All instruments were checked for calibration at the start of each day, after any prolonged shutdown, and at any other time that the operator suspected that the calibration had drifted. Two "Class A" standards were purchased from Scientific Gas Products in Pasadena, Texas, for use in the calibration checks. The instruments were actually calibrated to the 7993 ppmv

methane-in-air standard (certified to  $\pm 10$  ppmv). The 533 ppmv methane-in-air standard (certified to  $\pm 1$  ppmv) was used to check the linearity of the OVA calibration and, thereby, to detect any instrument malfunctions.

The OVA calibration procedure was initiated with a 20 to 30 minute warm-up period. The instrument was then checked against and reset to its internal electronic standards. The flame was ignited and stabilized, and a bag of the 7993 ppmv standard was sampled. The instrument response was recorded, and the reading adjusted (if necessary) using the "calibrate" knob. The flame was extinguished, and the internal standards checked and readjusted using the "gas select" knob. This procedure was repeated until the instrument responded properly to both the primary methane standard and the internal electronic standards. A bag of the 533 ppmv standard was then sampled and the result recorded. No adjustments were made based on the lower calibration check since the OVA is set up for a single point external calibration. Its span is set by the high and low electronic standards. This lower calibration check was only intended to detect equipment malfunctions, such as preamplifier failure.

During the latter stages of the program, the TLV calibration procedure was quite similar. The instrument was warmed up and zeroed on hydrocarbon-free (zero-grade) air. The 7993 ppmv methane standard was sampled, the result recorded, and the response adjusted (if necessary). The 533 ppmv standard was also read, recorded, and adjusted (the TLV has a separate potentiometer for calibrating each decade of readout response).


During the early stages of the program, the TLV's were mistakenly assumed to be permanently calibrated at the factory to n-hexane. The methane standards were read daily and the results recorded, but the instrument response was not adjusted to read exactly the standard value. It was necessary, therefore, to develop a numerical correction factor to convert the indicated response from a hexane to a methane basis. For instance, if TLV #7C read 300 ppmv when it

was checked on the 533 ppmv standard, then its readings were multiplied by the factor 1.403 (which is 533 divided by 380). In order to test this correction procedure, six chemicals (which had been run in the early part of the program) were rerun under the proper calibration procedure. Figures 3-1 through 3-6 show a graphical comparison of the corrected original response and the response during the recalibrated runs. While there is certainly some scatter among these data points, there is no perceptible bias between the corrected and recalibrated data sets. The magnitude of random variance in the corrected data appears to be only slightly greater than that of the recalibrated data. Based on these observations, it can be stated that the correction procedure is valid and that it should not have a significant negative effect on the overall precision of the TLV response data. All response factors for TLV's presented in this report are either corrected or recalibrated values.

### 3.3 GENERATION OF STANDARD GASES


The determination of instrument response factors requires that gas samples of known concentration be prepared. Concentrations of chemicals which are liquids at room temperature are calculated gravimetrically, from a measured weight of the liquid injected into a measured volume of "zero-grade" (hydrocarbon free) air. Concentrations of chemicals which are gases at room temperature are calculated volumetrically. The details of sample preparation follow in three parts:

- preparation of bags,
- preparation of standards from liquids, and
- preparation of standards from gases.

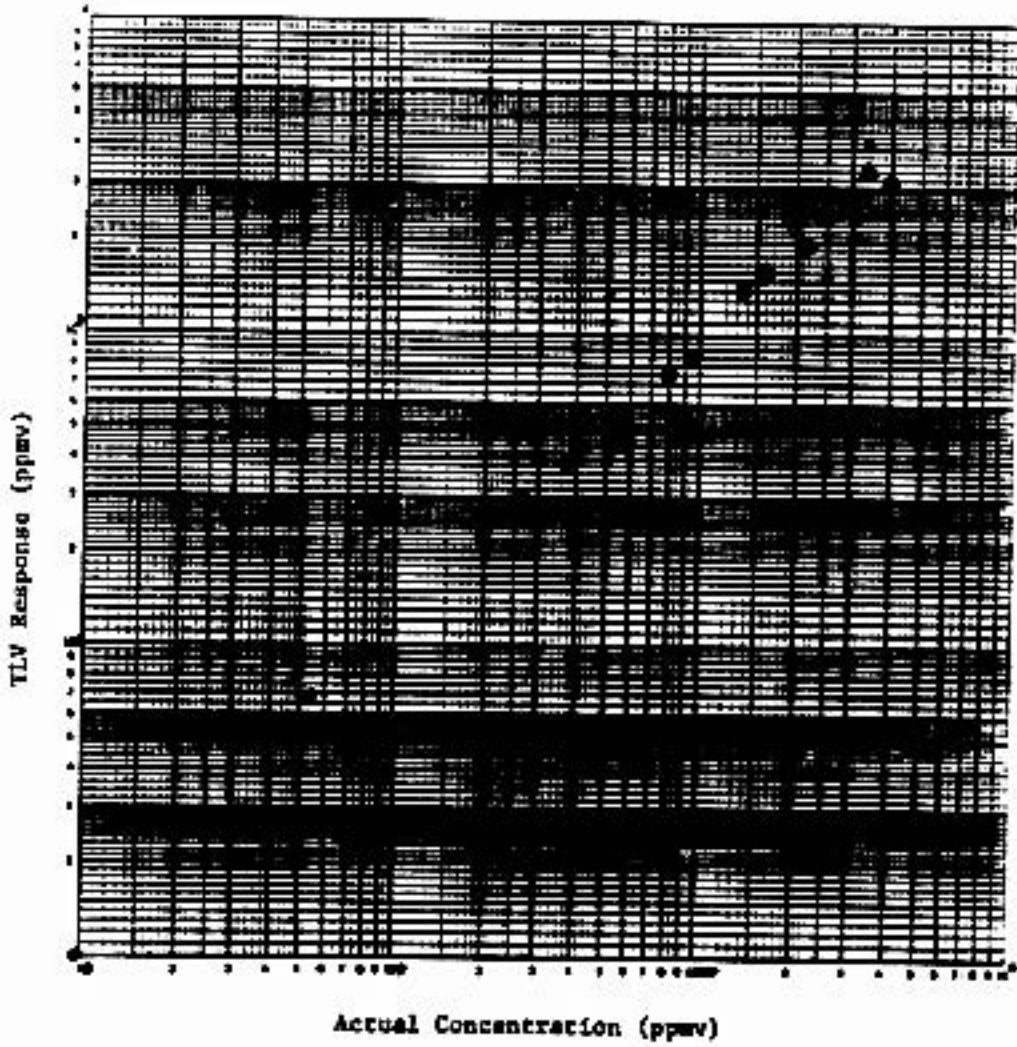

- ⊙⊙⊙      Recalibrated Response
- x x x      Corrected Response (TLV 7C)
- ▲▲▲      Corrected Response (TLV 7E)


Figure 3-1. TLV recalibration check - benzene.

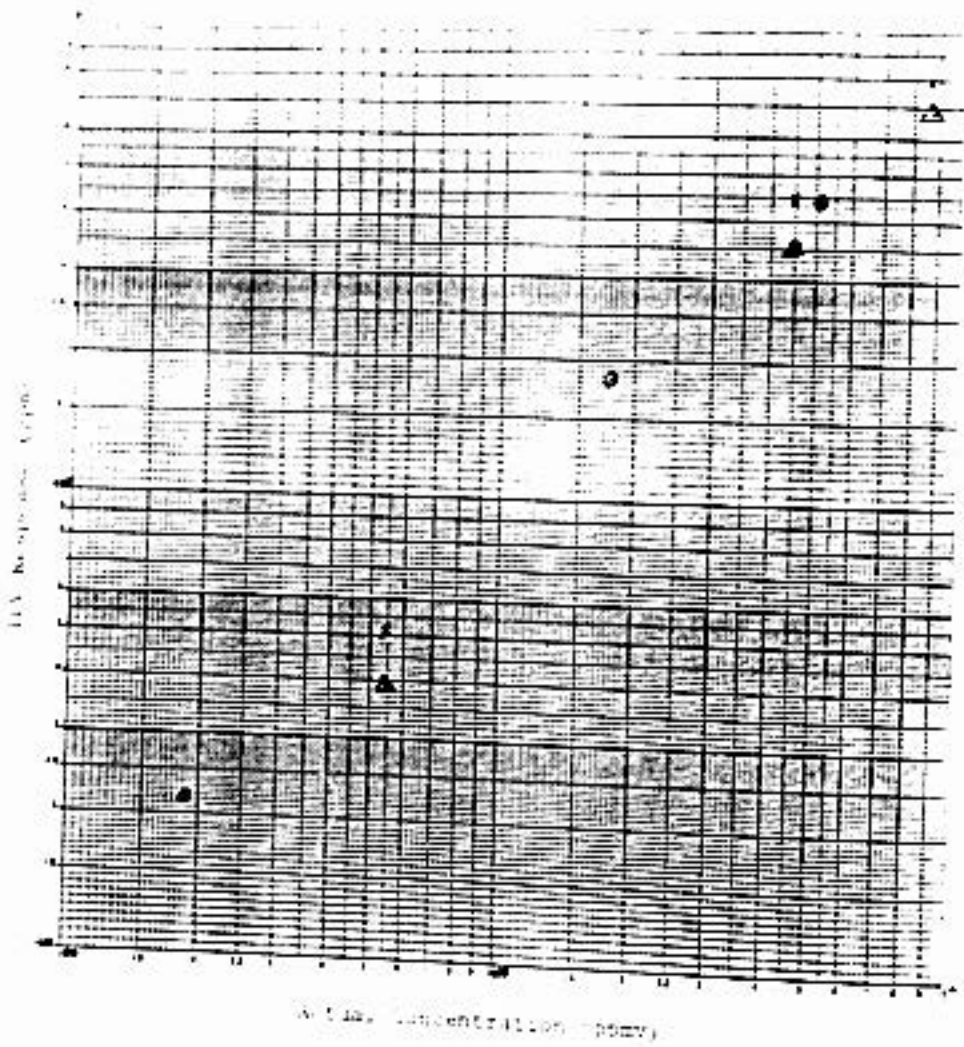

○○○○ Recalibrated Response  
 x x x Corrected Response (TUV TC)  
 ▲▲▲ Corrected Response (TUV TE)


Figure 1-2. TUV recalibration check - methyl ethyl ketone



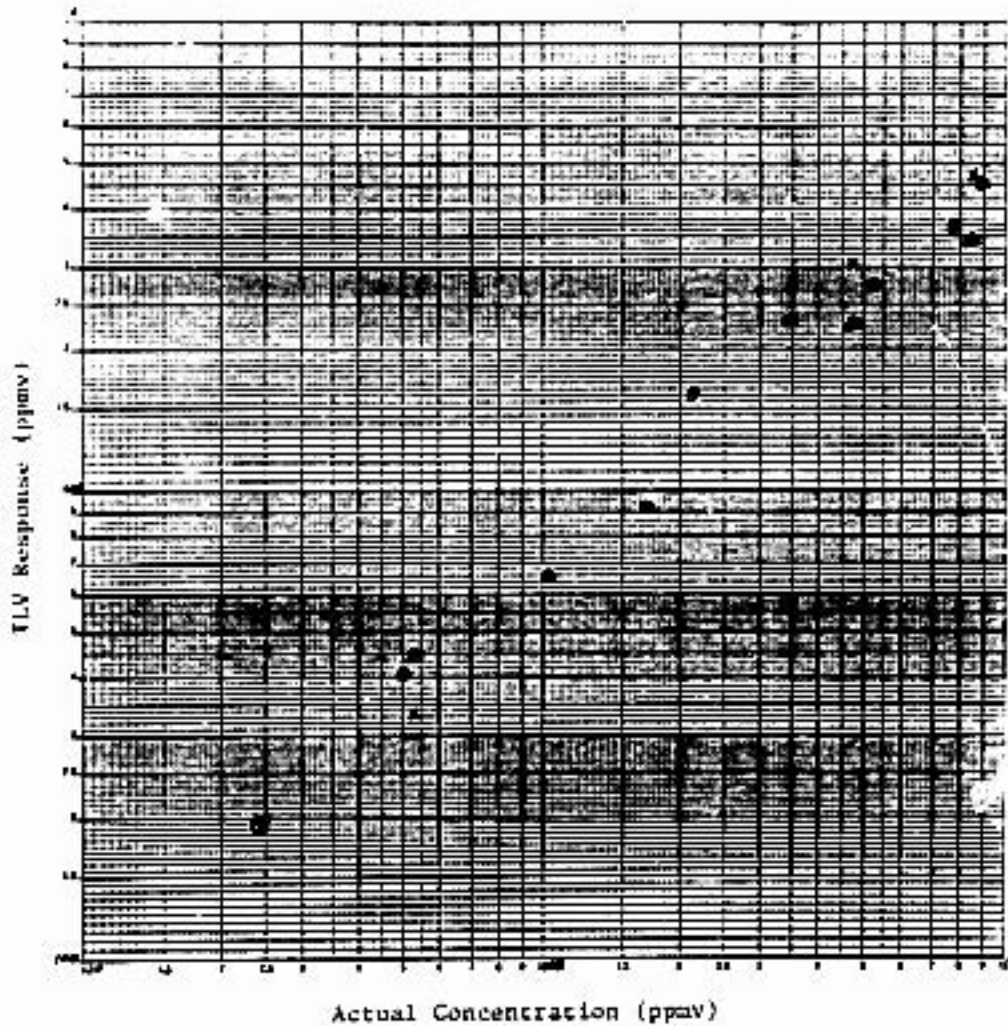


⊙ ⊙ ⊙      Recalibrated Response  
 x x x      Corrected Response (TLV 7C)  
 △ △ △      Corrected Response (TLV 7E)

Figure J-3. TLV recalibration check - methanol.

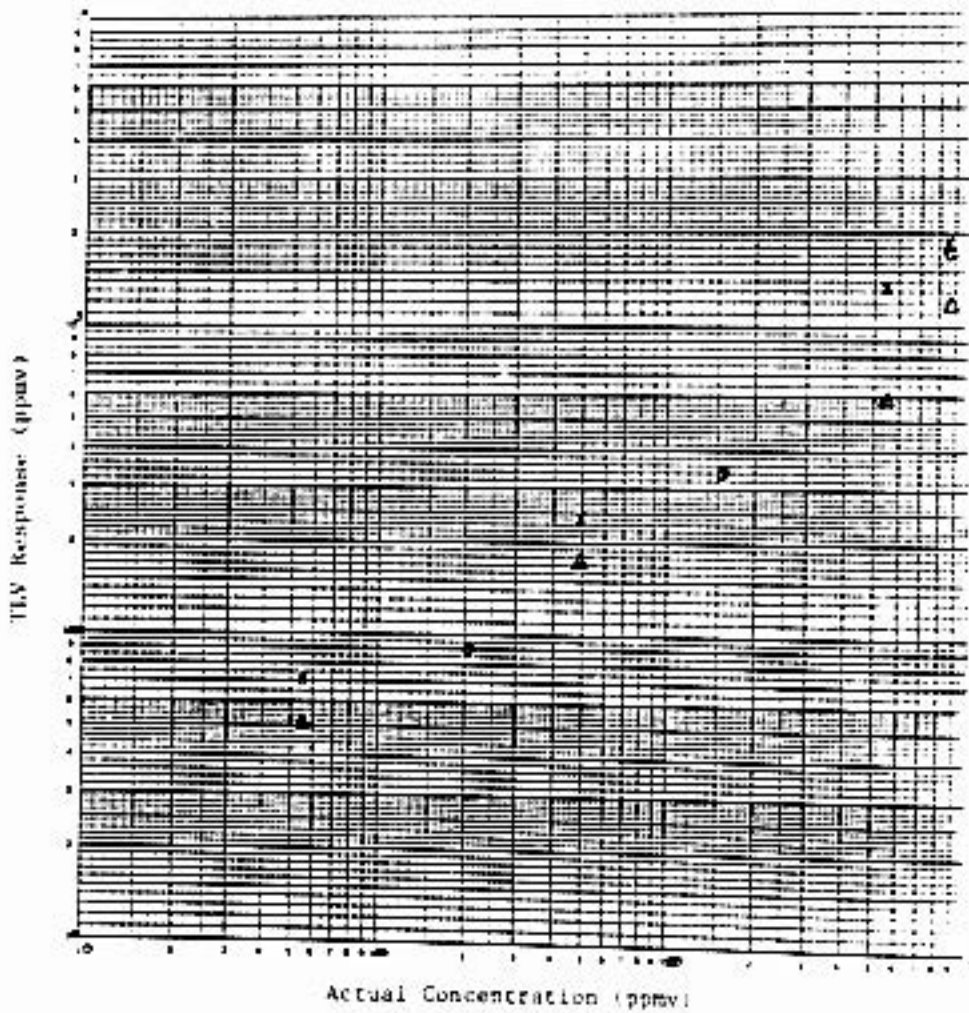

- ○ ○      Recalibrated Response
- x x x      Corrected Response (TLV 70)
- △ △ △      Corrected Response (TLV 7E)

Figure 3-4. TLV recalibration check - acetic acid.

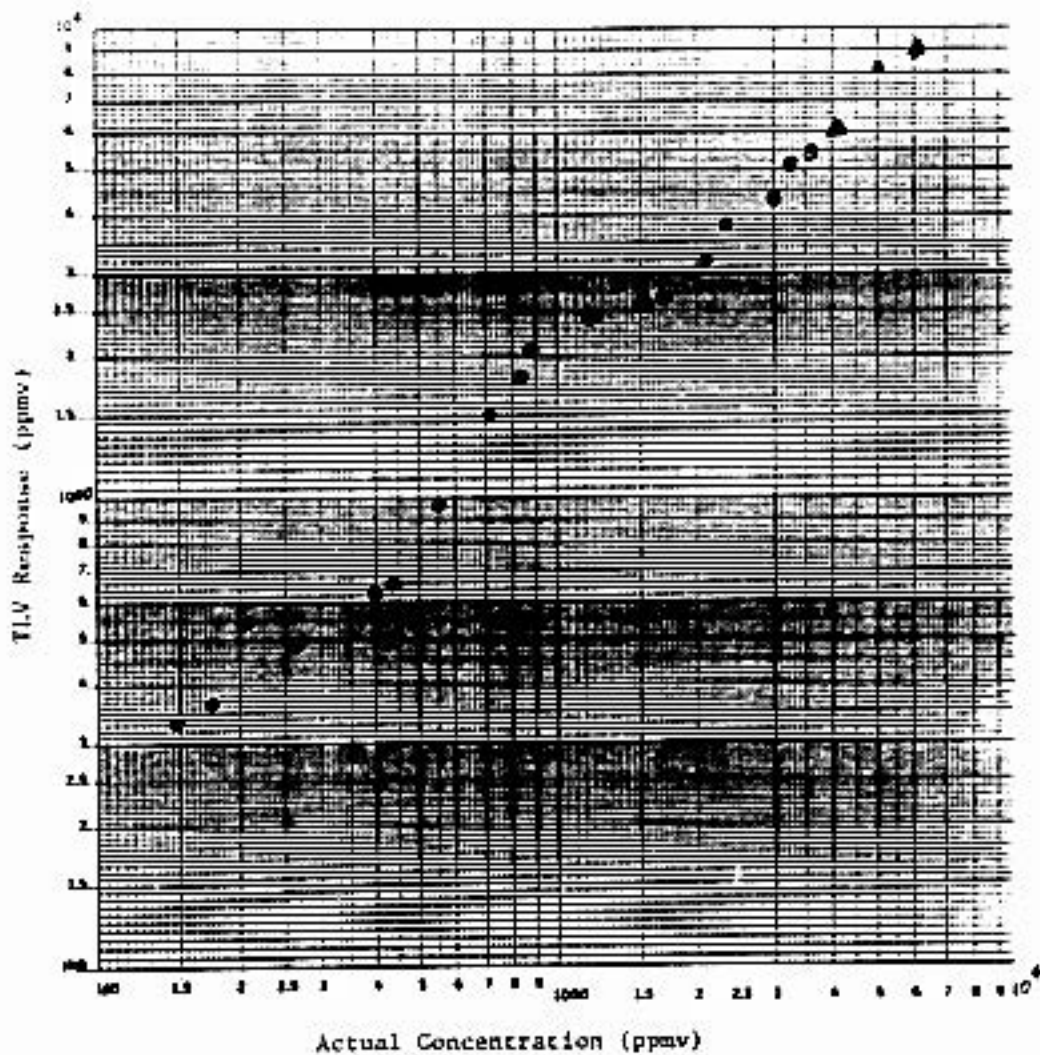

- ⊙⊙⊙ Recalibrated Response
- x x x Corrected Response (TLV 7Q)
- △△△ Corrected Response (TLV 7N)

Figure 3-5. TLV recalibration check - n-hexane.

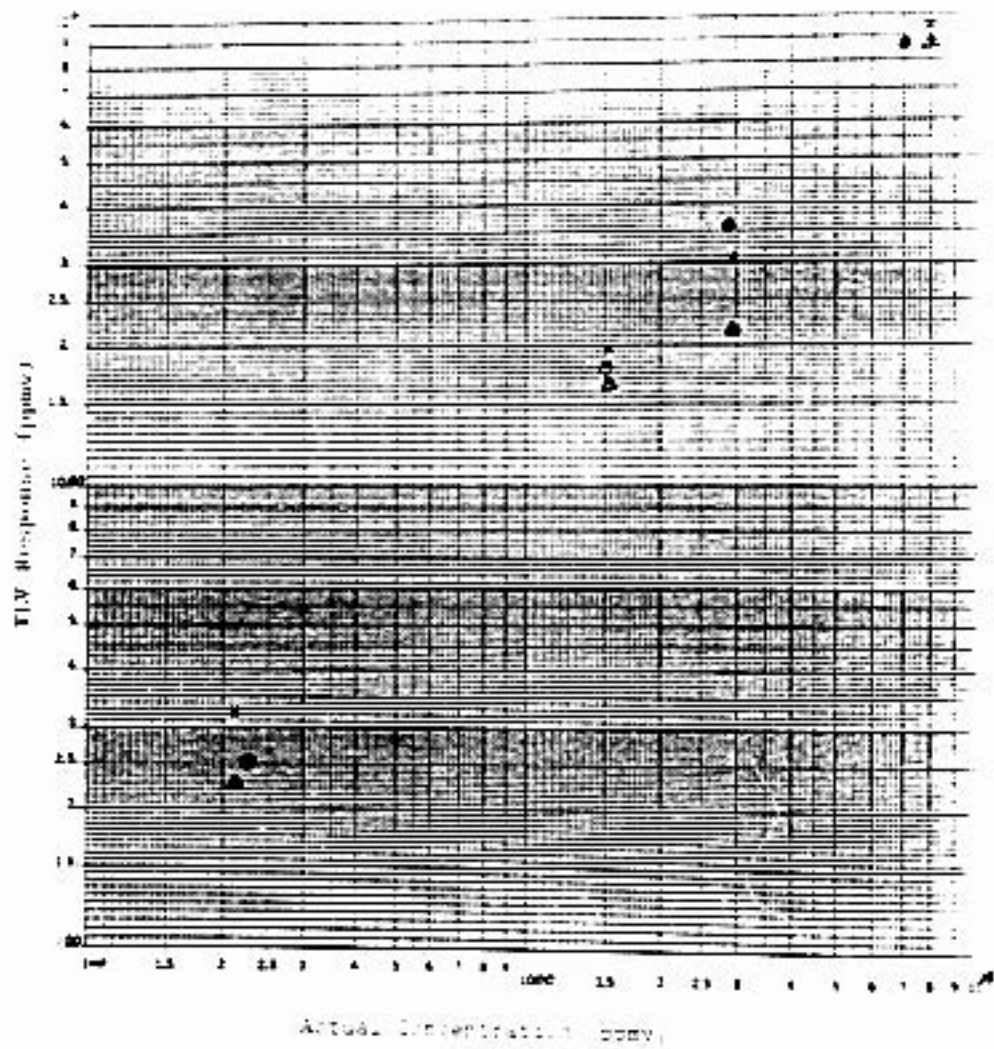


Figure 3-6. TLV recalibration check - chlorobenzene.

### 1.3.1. Preparation of Sample Bags

All the standard gas mixtures used in this study were prepared or collected in chemically-inert gas sampling bags. The early work was done with the aluminized snout bags manufactured by Calibrated Instruments, Inc., but these were later replaced by Tedlar bags manufactured by Engineered Devices, Inc. The bulk of the data was taken using the Tedlar bags, which were preferred for three reasons:

- the Tedlar was believed to be more inert and resistant to adsorption or permeation,
- the clear bags allowed visual inspection of the interior for condensation or contamination, and
- the Tedlar bags were equipped with two valves to facilitate flushing between runs.

The first step in the preparation of each bag was measurement of its volume. This was done by filling the bag completely with air but not at higher than atmospheric pressure, and then emptying the bag into an inverted graduated cylinder filled with water. The volume of water displaced was measured on the graduate, and the standard volume of the bag calculated from that volume by correcting for barometric pressure, ambient temperature, and the partial pressure of water in the trapped air. The calculated volume and an identification number were then imprinted on the bag.

Each bag had to be thoroughly conditioned between runs to prevent cross-contamination. The Tedlar bags were attached to a flushing manifold and continuously purged with ambient air for not less than fifteen minutes. The bags were then evacuated and filled with zero-grade air. The snout bags had only a single valve, which made a continuous purge impractical. They were successively filled and evacuated until no residual hydrocarbons could be detected.



### 3.3.2 Preparation of Standards from Liquids

Standard gas mixtures of chemicals which were liquids at ambient laboratory conditions were prepared by injecting a known weight of the liquid through a septum into a sample bag filled with a known volume of zero-grade air. Three target concentrations were prepared for each chemical, usually 200, 1500, and 8000 ppwv. Occasionally it was not feasible to prepare an 8000 ppwv mixture because of the chemical's volatility or explosivity. For chemicals with relatively low vapor pressures, the upper concentration was limited to 90 percent of the saturated concentration at ambient conditions to prevent condensation in the bag. For obvious safety reasons, no gas mixtures were prepared in excess of 70 percent of the Lower Explosive Limit (LEL).

For each target concentration, the required volume of the liquid chemical was calculated and then measured in a microliter syringe. The syringe was weighed on an electronic balance before and after injection into a clean sample bag filled to capacity with zero-grade air. The bag was then set aside for several minutes to allow the mixture to come to equilibrium before testing. The concentration in the bag can then be calculated by the following relationship:

$$C_A = (62.36 \times 10^6) (W_i - W_f) (T)/(V) (MW_A) (BP)$$

where  $C_A$  is the concentration of chemical "A" in parts per million by volume (ppwv),

$62.36 \times 10^6$  is a combined constant with the units (liters) (mmHg)/(g-mols) ( $^{\circ}$ K). This constant incorporates the ideal gas volume of 22.4 liters per g-mol., standard temperature and pressure, and a factor of  $10^6$  to go from volume fraction to ppwv.

$W_i$  and  $W_f$  are the initial and final weights of the syringe in grams.

T is the laboratory temperature in °K,

V is the sample bag volume in liters,

MW<sub>A</sub> is the molecular weight of chemical "A", and

BP is the barometric pressure in mmHg.

These data were collected on a computer-coded sheet shown as Table J-1.

The two major sources of error in the preparation of standards from liquids were errors in the measurement of bag volumes and errors in the weighing. Only one bag volume was measured twice, but the results were remarkably consistent. The first measurement resulted in a volume of 5.27 liters and the second measurement yielded a volume of 5.29 liters, for a difference of only 0.4% between the two measurements. Six "identical" bags made by one manufacturer were also measured, and the volumes ranged from 5.07 liters to 5.66 liters with a mean value of 5.35 liters. This indicated a range of values within ±5 percent of the mean value. While most of this variation was probably due to real differences in the volumes of the individual sample bags, it did provide a very conservative estimate of the variability in determining sample bag volumes.

The precision of the weighing step was much better than that of bag volume measurement. The Mettler electronic balances (Models H51 and H35 AR) were accurate to ±0.0001 gram. This resulted in an uncertainty of ±0.05 percent when preparing the nominal 8000 ppw bags, and up to 2.0 percent when preparing the 200 ppw bags.

The variance in the calculated concentration of standards prepared from liquids can then be estimated by a standard statistical formula which relates the variance of a ratio to the individual variance of the numerator and

TABLE 3-1. LIQUID RESPONSE FACTOR DATA SHEET

DATE:    TIME:   MIN:

COMPOUND:

SPECIFIC GRAVITY:  g/ml

EXPERIMENTAL CONDITIONS: Temp.  °C, Pressure  mm Hg

NETTLE MARKS: TLP #1  #2  #3  #4  #5  #6  #7  #8  #9  #10  #11  #12

TANKET CONC	STRINGS WEIGHT		SAMPLE MARKING		ALIBERT	
	FULL	EMPTY	TLP #1	#2	TLP #1	#2
1						
2						
3						
4						
5						
6						
7						
8						
9						
10						
11						
12						

Coder: \_\_\_\_\_  
Date: \_\_\_\_\_

Insight:  $C_t, \text{ ppm} = \frac{4.444 \times 10^{-9} \times V_1}{V_2} \times \frac{1}{K} \times \frac{1}{\rho_{\text{Temp.}}} = \frac{V_1}{V_2} \times \frac{1}{K}$

REMARKS: \_\_\_\_\_  
 \_\_\_\_\_  
 \_\_\_\_\_  
 \_\_\_\_\_

denominator.<sup>(6)</sup> In this case, the coefficient of variation in the calculated concentration was estimated to be  $\pm 4.0$  percent for an 8000 ppmv standard and  $\pm 4.4$  percent for a 200 ppmv standard.

### 3.3.3 Preparation of Standards From Gases

A gas mixing apparatus was used to prepare standards of chemicals which were gases at room temperature and of some very volatile liquids. Standard mixtures of these chemicals were purchased in pressurized cylinders at or above the highest required concentration (8000 ppmv). As described in the previous subsection, at least three standards were prepared for each chemical with concentrations ranging from 150 to 8000 ppmv.

The mixing apparatus is shown schematically in Figure 3-7. It consists of two parallel supply and metering systems, one for zero-grade air and the other for the sample gas. Target flow rates were calculated for each stream, and the initial flow rates set using the rotameter. The flow of each stream was then diverted to the bubble meter by a 3-way valve for a precise measurement of the flow rate. Both streams were then redirected through the rotameter, which served both as an indicator of any flow variance and as a mixing chamber. The outlet of the rotameter was collected in a sampling bag. After filling the bag, both streams were diverted to the bubble meters for another flow measurement. The average flow measurements were then used in the following equation:

$$C_m = (F_B) (C_B) / (F_A + F_B)$$

where  $C_m$  is the concentration of the standard mixture to be prepared in ppmv,

$C_B$  is the concentration of the chemical of interest in the sample gas from the purchased cylinder,

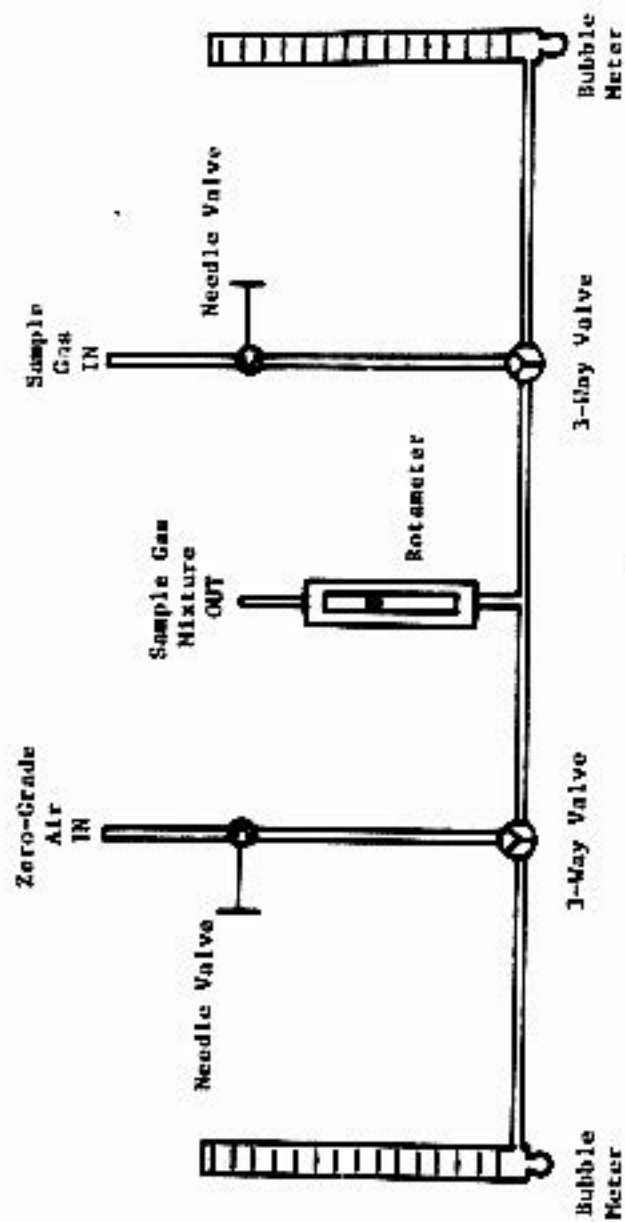


Figure 3-7. Gas-air mixing apparatus.



$F_s$  is the flow rate of the sample gas in milliliters per second,  
and

$F_a$  is the flow rate of air in milliliters per second.

These data were collected on a computer coded sheet shown as Table 3-2.

The primary factors which contributed to uncertainty in the calculated concentration were variances in the measured flow rates and the precision of  $C_p$ , the concentration of the subject chemical in the purchased sample gas. Normally the sample gases were purchased at about 15,000 ppwv in air and were certified to  $\pm 2$  percent of that concentration (or about  $\pm 300$  ppwv). This varied according to the individual gas supplier and type of gas, but the above figures were chosen to represent an "average" situation.

The flow rates were measured on bubble meters with a volume of 100 ml., and the physical measurement was the time for a bubble to travel the column. The stopwatch used was accurate to  $\pm 0.01$  second, but operator reaction time and variations in reading the slightly curved bubble caused the time measurement to be no better than  $\pm 0.2$  seconds. This represents a range of variation of about  $\pm 3.3$  percent for the air measurement which was normally in the 6 second range.

The sample gas times varied from about 5 seconds up to about 30 seconds depending on the desired concentration, which would suggest a range of variation of 0.6 to 4.0 percent. This was true for two repeated readings with little elapsed time in between, but when the readings were repeated a third time after the bag was filled, somewhat larger variations were noted. This was probably due to inadequate flow regulation in the small, low pressure gas cylinders. The range of variation on the lower concentration standards was  $\pm 3$  seconds at the 20 second level, or about  $\pm 15$  percent variation. For the higher concentration standards, the variation was about  $\pm 1$  second at the 5 second level, or about  $\pm 20$  percent variation.



The overall variance can be estimated from the standard formula for estimating the variance of a ratio from the variances of the numerator and denominator.<sup>(6)</sup> In this case, the overall coefficient of variation in the calculated concentration of standards prepared from gases was estimated to be  $\pm 13.7$  percent.

#### 3.4 INSTRUMENT SAMPLING PROCEDURES

The procedures used to obtain response data from the prepared standards were quite simple. A manifold was prepared from a "Y" connector and Teflon tubing to connect a sample bag to two instruments. Normally the two OVA's were read first, followed by the two TLV's. Readings were repeated as often as possible, as limited by the volume of sample remaining after taking the initial four readings. The instrument response data were recorded on the computer coded sheets previously presented as Tables 3-1 and 3-2.

The tubing manifold was flushed with zero-grade air between samples to reduce any cross contamination. At the completion of flushing, the zero-grade air was routed through the manifold to the instruments. The TLV's were electronically zeroed on this gas. The OVA reading was recorded as an "ambient" concentration which was subsequently subtracted from the next sample reading to yield a net response value for the sample gas. While this procedure was a worthwhile safeguard, the flushing alone seemed to be effective enough since no residual concentrations in excess of 10 ppbv were noted.

#### 3.5 QUALITY ASSURANCE

Quality Assurance checks were run throughout the project. A standard gas was read at random intervals by each instrument in use. Generally, this standard was 533 ppbv methane in air but sometimes 7993 ppbv methane in air was also read. These readings were made independently of the routine calibrations. The data from these checks are summarized in Table 3-3.

TABLE 3-3. SUMMARY OF RANDOM CALIBRATION CHECKS  
USED FOR QUALITY ASSURANCE

Date	Time	Standard Concentration (ppmv)	OVA Readings (ppmv)	TLV Readings (ppmv)
3/11	0830*	7993	8000, 8000	-
	0830*	533	650, 700	-
	1535	533	650, 700	519, 498
3/12	0830	7993	7900, 8000	-
	0830	533	610, 720	-
	0905	533	610, 720	547, 533
3/13	0830	7993	7000, 7900	-
	0830	533	710, 690	-
	1010	533	710, 690	547, 533
	1620	533	640, 658	533, 519
3/14	0830	7993	8000, 8000	-
	0830	533	710, 710	-
	1100	533	710, 710	-
	1645	533	710, 690	533, 526
3/17	0830	7993	8000, 8000	-
	0830	533	720, 700	-
	1008	533	720, 700	-
3/18	0830	7993	6500, 8900	-
	0830	533	700, 700	-
3/19	0830	7993	9500, 8700	-
	0830	533	750, 830	-
	0952	533	620, 750	547, 533
	1625	533	830, 650	547, 547
	1625**	7993	8000, 8000	-
	1625**	533	620, 750	-

\*The calibration checks done at 0830 are the daily routine calibrations. They are included in this table for comparison to the random calibration checks used for QA.

\*\*Recalibrated.

TABLE 3-3. SUMMARY OF RANDOM CALIBRATION CHECKS  
USED FOR QUALITY ASSURANCE (continued)

Date	Time	Standard Concentration (ppmv)	OVA Readings (ppmv)	TLV Readings (ppmv)
3/20	0830	7993	9000, 8100	-
	0830	533	700, 750	-
	0900	533	700, 750	519, 505
	1700	533	730, 690	540, 526
3/21	0830	7993	7300, 8000	-
	0830	533	700, 700	-
	0900	533	700, 700	533, 533
3/24	0830	7993	7900, 8000	-
	0830	533	620, 690	-
	0910	533	620, 690	540, 533
	1720	533	710, 700	533, 519
3/25	0830	7993	8000, 8900	-
	0830	533	720, 700	-
	0855	533	720, 700	540, 533
3/26	0830	7993	9000, 8100	-
	0830	533	650, 700	-
	0915	533	650, 700	533, 533
3/27	0830	7993	7000, 8000	-
	0830	533	620, 700	-
	0927	533	620, 700	533, 533
	1645	533	890, 750	533, 526
3/28	0830	7993	6000, 7700	-
	0830	533	700, 710	-
	1117	533	700, 710	540, 533
4/1	0830	7993	7300, 7300	-
	0830	533	730, 720	-
	1153	533	730, 720	526, 519



TABLE 3-3. SUMMARY OF RANDOM CALIBRATION CHECKS  
USED FOR QUALITY ASSURANCE (continued)

Date	Time	Standard Concentration (ppmv)	OVA Readings (ppmv)	TLV Readings (ppmv)
4/2	0830	7993	9000, 7300	-
	0830	533	780, 720	-
	1415	533	780, 720	533, 540
	1700	533	620, 710	533, 526
4/3	0830	7993	8000, 8200	-
	0830	533	680, 780	-
	0900	533	680, 780	519, 505
	1715	533	630, 720	472, 526
4/4	0830	7993	8000, 8000	-
	0830	533	750, 700	-
	0910	533	750, 700	540, 526
4/7	0830	7993	8100, 7800	-
	0830	533	770, 700	-
	0900	533	770, 700	519, 526
	1300	533	670, 770	-
	1300*	7993	7800, 8000	-
4/8	0830	7993	10000, 9200	-
	0830	533	750, 710	-
	0855	533	750, 710	526
4/9	0830	7993	8000, 8000	-
	0830	533	710, 710	-
	1330	533	710, 710	-
4/10	0830	7993	8000, 8000	-
	0830	533	710, 720	-
	1000	533	710, 720	554

\*Recalibrated.

TABLE 3-3. SUMMARY OF RANDOM CALIBRATION CHECKS  
USED FOR QUALITY ASSURANCE (continued)

Date	Time	Standard Concentration (ppmv)	OVA Readings (ppmv)	TLV Readings (ppmv)
4/11	0830	7993	8000, 7900	-
	0830	533	700, 710	-
	0915	533	700, 710	-
4/14	0830	7993	8000, 5200	-
	0830	533	670, 690	-
	1630	533	700, 700	519**
4/15	0830	7993	8500, 9200	-
	0830	533	700, 720	-
	0930	533	700, 720	527, 780
4/16	0830	7993	8900, 8900	-
	0830	533	780, 720	-
	0930	533	780, 720	567, 791
	1705	533	720, 800	-
4/17	0830	7993	7900, 8000	-
	0830	533	610, 750	-
	0925	533	610, 750	516, 780
	1700	533	610, 700	780
4/18	0830	7993	6300, 7500	-
	0830	533	710, 710	-
	1020	533	710, 710	770
4/21	0830	7993	7900, 8200	-
	0830	533	680, 750	-
	0905	533	680, 750	533, 770
4/22	0830	7993	6900, 8200	-
	0830	533	720, 720	-
	1010	533	720, 720	759

\*\*Original TLV's down for repairs, two different TLV's used in subsequent testing.

TABLE 3-3. SUMMARY OF RANDOM CALIBRATION CHECKS  
USED FOR QUALITY ASSURANCE (continued)

Date	Time	Standard Concentration (ppmv)	OVA Readings (ppmv)	TLV Readings (ppmv)
4/23	0830	7993	8000, 8000	-
	0830	533	710, 730	-
	0900	533	710, 730	527, 759
4/24	0830	7993	7200, 8100	-
	0830	533	620, 710	-
	0930	533	620, 710	516, 747
4/25	0830	7993	8000, 8100	-
	0830	533	710, 710	-
	0940	533	710, 710	747
4/28	0830	7993	6900, 8000	-
	0830	533	690, 720	-
	1110	533	690, 720	738
4/29	0830	7993	7100, 8000	-
	0830	533	710, 720	-
	0925	533	710, 720	747
	1540	533	790, 720	717
4/30	0830	7993	7500, 8900	-
	0830	533	750, 750	-
	0945	533	750, 750	759
5/1	0830	7993	7800, 8200	-
	0830	533	750, 790	-
	0845	533	750, 790	749
5/2	0830	7993	8100, 8000	-
	0830	533	750, 600	-
	0915	533	710, 600	539, 738

TABLE 3-3. SUMMARY OF RANDOM CALIBRATION CHECKS  
USED FOR QUALITY ASSURANCE (continued)

Date	Time	Standard Concentration (ppmv)	OVA Readings (ppmv)	TLV Readings (ppmv)
5/5	0830	7993	7800, 8700	-
	0830	533	700, 720	-
	1010	533	700, 720	749
	1430	533	700, 750	759
8/18	0930	7993	8000	8000**
	0930	533	680	540
	1525	7993	8000	8100
	1525	533	700	530
8/19	1015	7993	8000	8200
	1015	533	700	515
8/21	1055	7993	8000	8100
	1055	533	630	530
	1645	7993	6800	7950
	1645	533	580	530
8/22	1300	7993	8000	7900
	1300	533	650	500
	1510	7993	8000	7950
	1510	533	680	480
8/25	1025	7993	8000	8000
	1025	533	700	520
	1530	7993	7900, 8000	7900
	1530	533	700, 600	525
8/26	0915	7993	8000, 8000	8000
	0915	533	700, 530	525
	1745	7993	8000, 8000	-
	1745	533	710, 550	-

\*\*Changed TLV's.

TABLE 3-3. SUMMARY OF RANDOM CALIBRATION CHECKS  
USED FOR QUALITY ASSURANCE (continued)

Date	Time	Standard Concentration (ppmv)	OVA Readings (ppmv)	TLV Readings (ppmv)
8/27	0900	7993	8000, 8000	7950
	0900	533	620, 520	535
	1540	7993	8000, 8000	8050
	1540	533	600, 700	530
8/28	1010	7993	8000, 8000	8000
	1010	533	530, 700	533
8/29	1000	7993	8000, 8000	8000
	1000	533	550, 680	490



Quality Assurance on data transmittal was achieved by adherence to strict procedures. The data recorded on data sheets was keypunched and verified. A computer program added the new data to the permanent data base and printed out the card images, the raw data in tabular form, the routine calculations in tabular form, and a graphic presentation of the data. These computer outputs were returned to the experimenters for verification and anomaly checking. Any errors detected were corrected in the data base.

SECTION 4  
DATA ANALYSIS

For this section, the following definitions apply. The actual concentration is the concentration of vapor in parts per million by volume (ppmv), as described under Test Procedures above. This is the calculated concentration in the bag. The instrument response is the reading (ppmv) obtained from the calibrated instrument as it samples the contents of the bag. The response factor is the number that when multiplied by the instrument response gives the actual concentration. That is:

$$C = (RF) (IR) .$$

so that

$$RF = C/(IR) . \quad (1)$$

where C = actual concentration (ppmv),

IR = instrument response (ppmv), and

RF = response factor.

In Equation (1), RF may be considered a function of C. If, for some chemical, the response factor RF is a constant over some useful range of actual concentrations C, then it would be justified to call this constant value the response factor for the particular chemical. The data collected in this study indicates that there is no single response factor for most chemicals.

Depending on the chemical, the function (1) describes the response factor as an increasing or decreasing function of actual concentration in many cases. Some of the response factor functions appear to peak or trough within the range of concentrations tested. The variability or precision of measured response factors also sometimes varies considerably over the range of concentrations tested.

An average response factor would be justified if the variations in measured response factors from Equation (1) are due only to random errors of measurement:

$$RF = C/(IR) + \text{error} . \quad (2)$$

As discussed above, this does not appear to be the case. It appears that Equation (2) is not a very useful way to represent the data.

The equation

$$IR = B \cdot C + \text{error} , \quad (3)$$

where B is a coefficient, is an alternative model to (2) for the relationship between instrument response and actual concentration. This approach is more realistic since, in the experiments done here, the concentration, C, is measured with much greater precision than the instrument responses. Equation (3) may be fitted by least squares regression. The response factor then is estimated by

$$RF = 1/B .$$

There are several problems with this approach. As discussed above, a single response factor for all concentrations is not justifiable. Estimating the response factor as the reciprocal of a regression coefficient generates a bias that is not easily corrected for. Furthermore, a confidence interval for the estimate is not easy to construct.

Constant variance about the regression line is one assumption necessary for least squares regression estimation. The data collected in this study show greater variation in instrument response associated with higher concentrations. This is not unexpected but is another objection to fitting Equation (3) by least squares.

Transforming the response variable with a logarithmic function is a useful technique for homogenizing variance. Using a logarithmic transformation on both instrument response and actual concentration gives a fairly linear relationship as well as even variability. Thus, the relationship is

$$\ln (IR) = a + b \cdot \ln (C) + \text{error} \quad (4)$$

which is functionally equivalent to

$$IR = e^a \cdot C^b \quad ,$$

if the error is ignored. The regression coefficients  $a$  and  $b$  can be fitted by least squares using Equation (4). This provides a predictive equation for instrument response for a given concentration. The method also allows for estimating the precision of the prediction. This approach generates an empirical functional relationship between the actual concentration and the instrument response. A response factor at any particular actual concentration can be computed from (4) using this empirical relationship.

The following method gives the details of the method used to estimate the response factor at 10,000 ppbv with a 95 percent confidence interval. Let  $C_i$ ,  $i = 1, \dots, n$ , be the actual concentrations tested and  $IR_i$ ,  $i = 1, \dots, n$ , be the observed instrument responses where  $n$  is the number of experimental tests performed. Then the model

$$\ln (IR_i) = a + b \cdot \ln (C_i) + \text{error}_i$$

is fitted by least squares, where error<sub>i</sub> is the unknown measurement error associated with the i<sup>th</sup> test. (7) In addition to the estimates  $\hat{a}$  and  $\hat{b}$  of the parameters a and b, the following quantities are also computed. The mean square error is calculated from

$$S_e^2 = \sum_{i=1}^n [\ln(IR_i) - \hat{a} - \hat{b} \cdot \ln(C_i)]^2 / (n-2) .$$

The mean of the logarithms of the actual concentrations is calculated from

$$\bar{x} = \sum_{i=1}^n \ln(C_i) / n .$$

The sum of squared deviations of the logarithms of the actual concentrations about their mean is calculated from

$$ss_x = \sum_{i=1}^n [\ln(C_i) - \bar{x}]^2 .$$

The logarithm of the instrument response at 10,000 ppwv is estimated by

$$LIR_{10,000} = a + b \cdot \ln(10,000) ,$$

and upper and lower 95 percent confidence limits in the logarithmic scale are estimated by

$$LC_U = LIR_{10,000} + t \cdot S_{IR10000} .$$

$$LC_L = LIR_{10,000} - t \cdot S_{IR10000} .$$



where  $t$  is the tabulated Student's  $t$  with  $n-2$  degrees of freedom for 95 percent confidence, and

$$S_{IR10000} = \sqrt{S_e^2 \cdot [(1/n) + (2n \cdot 10,000 - \bar{x})^2 / SS_x]} .$$

Conversion back to the data scale from the logarithmic scale introduces a bias. The bias correction is approximately  $S_e^2/2$ .<sup>(8)</sup> Thus the estimated instrument response at 10,000 ppw is

$$IR_{10,000} = \exp (LIR_{10,000} + S_e^2/2)$$

and the corresponding 95 percent confidence limits are

$$CL_L = \exp (LCI_L + S_e^2/2)$$

$$CL_U = \exp (LCI_U + S_e^2/2)$$

Therefore, the response factor at 10,000 ppw is estimated by

$$RF_{10,000} = 10,000 / IR_{10,000} ,$$

and the 95 percent confidence interval by

$$(10,000 / CL_U, 10,000 / CL_L) .$$

Note that the limits reverse order by this transformation. No attempt is made to account for bias introduced by this second transformation. The values of  $\hat{a}$ ,  $\hat{b}$ ,  $n$ ,  $S_e$ ,  $SS_x$ , and  $\bar{x}$  necessary for performing these computations at any desired actual concentration are presented in Section 5, Tables 5-169 and 5-170.

In summary, this procedure amounts to estimating the instrument response to a 10,000 ppmv concentration by use of a fitted regression line. The response factor at 10,000 ppmv is then calculated from this estimated response.

If an unknown concentration is near 10,000 ppmv, then application of the 10,000 ppmv response factor to the instrument response will give roughly the correct concentration. Higher or lower concentrations will be estimated inaccurately by this method; however, they will be estimated as being higher or lower than 10,000 ppmv correctly.

For most of the chemicals tested in this survey, 10,000 ppmv is outside the range of tested concentrations. This fact is reflected in the confidence intervals which widen as the range of the data is exceeded.

Besides the statistical effects just noted, there are physical limitations. The instrument response may not continue to follow the projected linear trend (logarithmic scale) beyond the range of the data. It may not even be possible to achieve a concentration of 10,000 ppmv with the chemical in question. Neither the estimates nor confidence intervals reflect these limitations.

SECTION 5  
DETAILED RESULTS

The results of the response factor work for 168 chemicals are summarized in Section 2, with the presentation of a single response factor estimate at 10,000 ppwv. This section will present the actual data on which that estimate is based. There are two sheets for each chemical. The first sheet is a tabular representation of the actual concentrations and the instrument response factors, and includes both weighted mean values and individual instrument response factors. The second sheet presents two graphs of instrument response vs. actual concentration, one for the OVA and one for the TLV. These data are presented as Tables 5-1 through 5-168, and Figures 5-1 through 5-168.

In Section 4, an equation was presented which can be used to calculate the response factors and the 95 percent confidence levels for each chemical at a concentration other than 10,000 ppwv. Table 5-169 gives the values for calculating the OVA response factors and the data for the TLV are presented in Table 5-170.

TABLE 5-1  
RESPONSE FACTOR SUMMARY

ACETIC ACID				RESPONSE FACTORS											
OVA INSTRUMENTS				OVA METERS						TLV METERS					
NOMINAL PPMV	ACTUAL PPMV			OVERALL		1000		2254		2159		1817		SE	
	LOW	HIGH	MEAN	MEAN	SE	SE	N	SE	N	SE	N	SE	N	SE	N
50	49	67	55	12.20	4.55	0	1	7.80	3.01	3	16.75	6.09	3		
200	208	208	208	2.08										2.08	1
500	418	541	498	4.85	0.69	6	1	4.18	0.70	3	5.54	2.24	3		
1500	1564	1564	1564	1.80										1.80	1
5000	5414	5414	5414	1.84	0.03	2	1	1.81		1	1.87		1	1.80	1
8000	8509	8709	8641	3.28	0.80	7	1	3.24	0.67	3	4.00	1.62	3	1.87	1
OVERALL MEANS 5.80 0.09 23				4.73 1.06 10		8.09 2.72 10		1.71 0.19 3							
ESTIMATED AT 10,000 PPMV 1.83 95% CONFIDENCE INTERVAL (1.17, 2.87)															
TLV INSTRUMENTS				RESPONSE FACTORS											
NOMINAL PPMV	ACTUAL PPMV			OVERALL		71		51		70		76		SE	
	LOW	HIGH	MEAN	MEAN	SE	SE	N	SE	N	SE	N	SE	N	SE	N
50	49	62	59	0.90	0.14	9	1	1.07	0.54	2	0.78	0.24	3		
200	208	208	208	2.31							2.31		1		
500	418	541	498	2.41	0.41	6	1	2.81	0.13	2	2.07	0.23	3		
1500	1564	1564	1564	4.93							4.93		1		
5000	5414	5414	5414	8.84	2.87	3	1	8.21		1	4.06		1	4.06	1
8000	8509	8709	8641	5.60	1.23	6	1	7.34	2.48	2	4.72	1.14	4		
OVERALL MEANS 3.81 0.04 20				4.85 1.28 7		2.85 0.56 13									
ESTIMATED AT 10,000 PPMV 5.70 95% CONFIDENCE INTERVAL (4.18, 7.81)															

Figure 5-1  
INSTRUMENT RESPONSE VS CONCENTRATION  
ACETIC ACID


Figure 5-1

INSTRUMENT RESPONSE VS CONCENTRATION

ACETIC ACID

DVA: ORGANIC VAPOR ANALYZER

FLV: HYDROCARBON SHIPPER

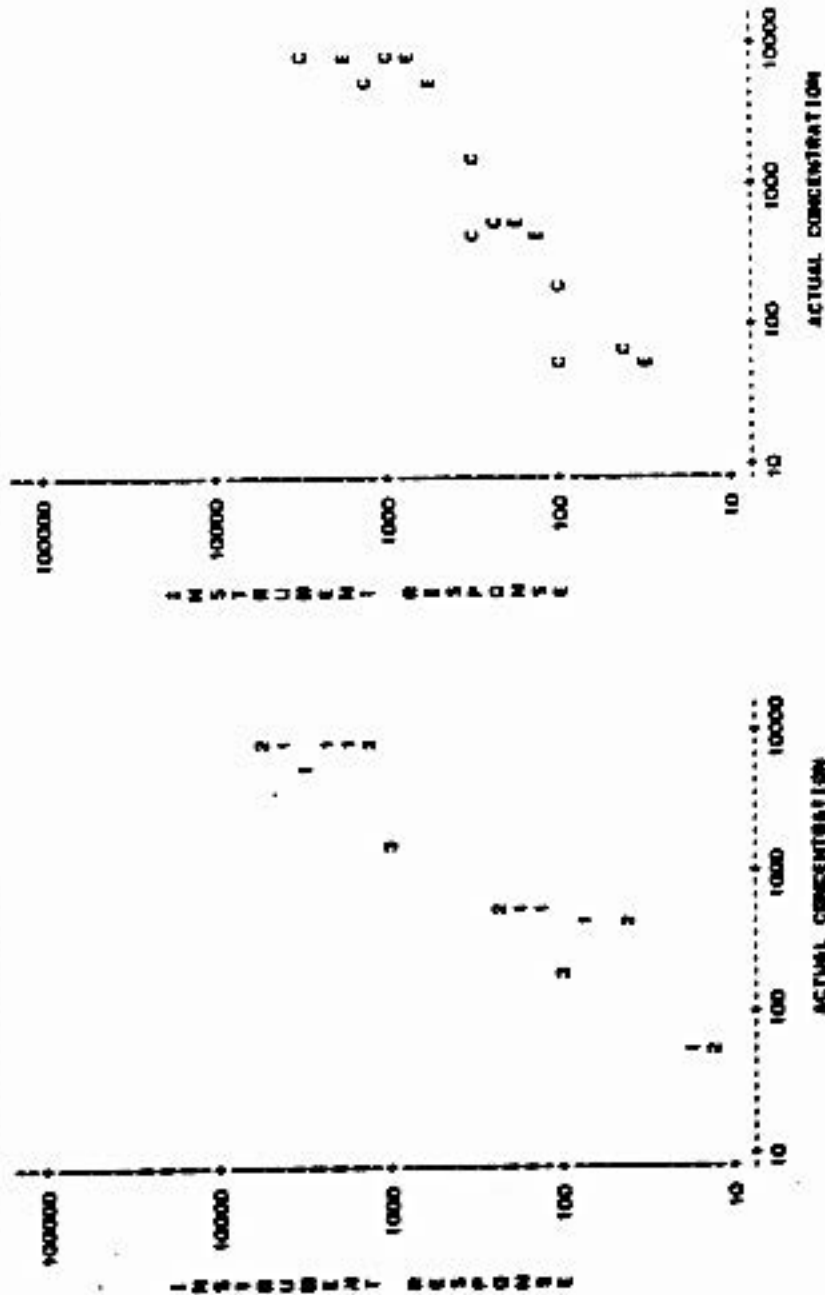

NOTE: \* OBS MISSING OR OUT OF RANGE

NOTE: B OBS HIDDEN



TABLE 5-2

RESPONSE FACTOR SUMMARY

ACETIC ANHYDRIDE

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS												
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2204	SE	N	2159	SE	N	1812	SE	N	
200	212	212	212	1.01	0.03	3	0.98	1	1.08	1	1.08	1	1.08	1	1.08	1	1.08	1	1.08
1800	1807	1807	1807	1.23	0.18	3	1.08	1	1.38	1	1.38	1	1.38	1	1.38	1	1.38	1	1.38
4000	3883	3883	3883	1.24	0.00	3	1.24	1	1.24	1	1.24	1	1.24	1	1.24	1	1.24	1	1.24
OVERALL MEANS				1.16	0.01	8	1.10	0.06	3	1.23	0.10	3							
ESTIMATED AT 10,000 PPMV				1.26															

95 % CONFIDENCE INTERVAL : ( 1.12, 1.63 )

TLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS												
	LOW	HIGH	MEAN	MEAN	SE	N	TE	SE	N	7C	SE	N	7M	SE	N	7O	SE	N	
200	212	212	212	0.88		1											0.99	1	
1800	1807	1807	1807	1.83		1											1.83	1	
4000	3883	3883	3883	1.83		1											1.83	1	
OVERALL MEANS				1.32		3							1.32	0.37	3				

95 % CONFIDENCE INTERVAL : ( 1.82, 5.14 )

Figure 5-2

INSTRUMENT RESPONSE VS CONCENTRATION

ACETIC ANHYDRIDE

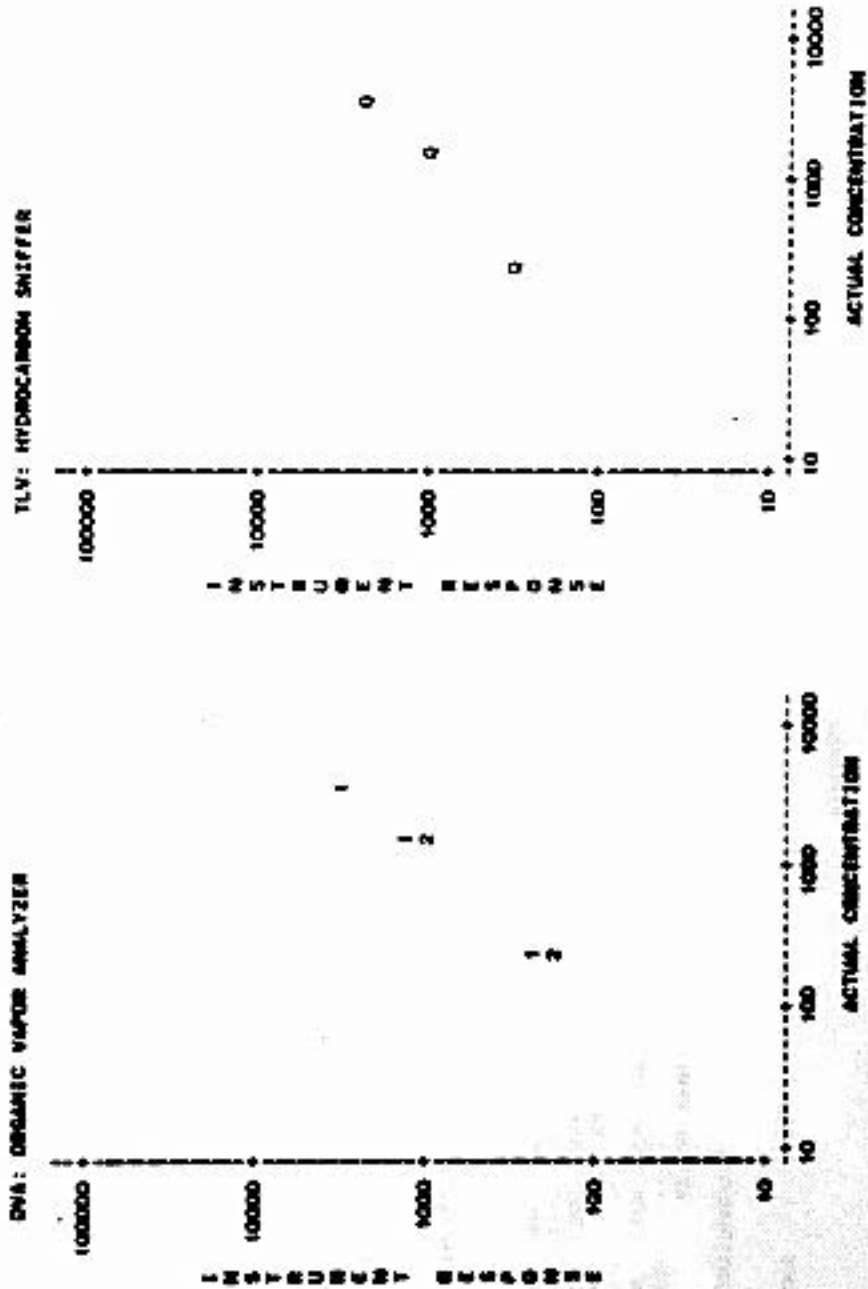


TABLE 5-3

RESPONSE FACTOR SUMMARY

ACETONE

OVA INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OVA METERS								
	LOW	HIGH	MEAN	MEAN	SE	N	1080	SE	N	2384	SE	N	1813	SE	N
50	88	86	87	1.23	0.08	4	1.41	0.44	2	1.26	0.42	2			
500	838	846	848	1.07	0.18	4	1.22	0.60	2	0.82	0.47	2			
4000	4117	4117	4117	1.23	0.08	2	1.27		1	1.28		1			
8000	8848	8848	8803	0.83	0.13	4	0.96	0.03	2	0.88	0.00	2			
OVERALL MEANS				1.11	0.01	14	1.22	0.18	7	1.00	0.17	7			

ESTIMATED AT 10,000 PPMV 0.78

95 % CONFIDENCE INTERVAL : ( 0.83, 1.19 )

TLV INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			TLV METERS								
	LOW	HIGH	MEAN	MEAN	SE	N	78	SE	N	70	SE	N	70	SE	N
50	86	88	87	1.10	0.18	4	1.28	0.12	2	0.82	0.18	2			
500	826	848	846	2.27	1.07	4	1.21	0.20	2	2.34	1.81	2			
4000	4117	4117	4117	1.28	0.12	2	1.27		1	1.19		1			
8000	8848	8848	8803	1.20	0.12	4	1.23	0.03	2	1.07	0.01	2			
OVERALL MEANS				1.48	0.01	14	1.28	0.08	7	1.68	0.98	7			

ESTIMATED AT 10,000 PPMV 1.22

95 % CONFIDENCE INTERVAL : ( 0.81, 1.83 )


Figure 5-3

INSTRUMENT RESPONSE VS CONCENTRATION

ACETONE

GVA: CERAMIC VAPOR ANALYZER

TLV: HYDROCARBON SWIPPER

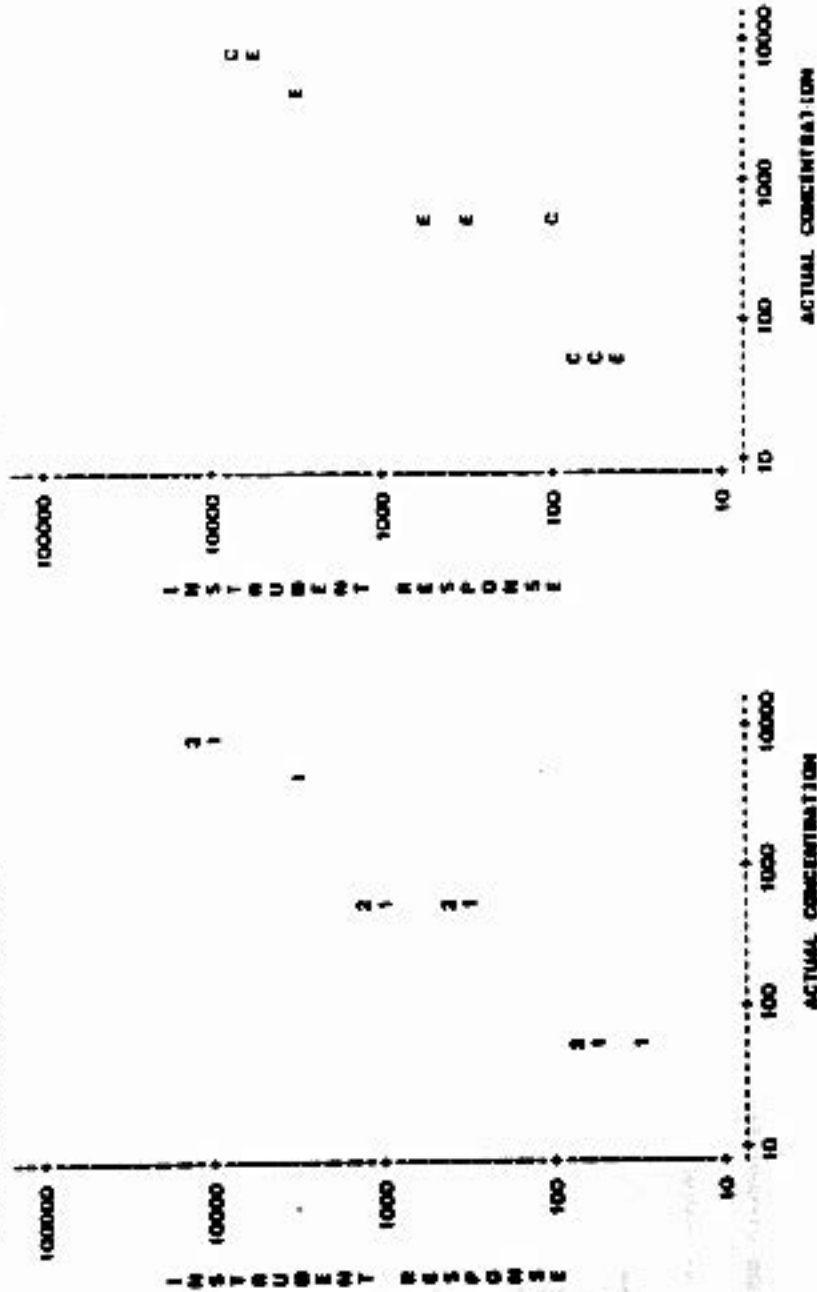

NOTE: 4 OBS HIDDEN

NOTE: 5 OBS HIDDEN

TABLE 5-4

RESPONSE FACTOR SUMMARY

ACETONE CYANHYDRIN

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METERS												
	LOW	HIGH	MEAN	MEAN	SE	N	1080	SE	44	2294	SE	44	2159	SE	44	1813	SE	44	
200	231	231	231	2.18	0.48	2	2.70		1	3.68		1							
400	402	402	402	3.56	0.54	2	3.02		1	4.10		1							
600	650	650	650	3.24	0.71	2	2.68		1	3.81		1							
OVERALL MEANS			3.33	0.09	6	2.80	0.11	3	3.86	0.13	3								

ESTIMATED AT 10,000 PPMV 3.42

95% CONFIDENCE INTERVAL 1.0 20.16 631

TLV INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			TLV METERS												
	LOW	HIGH	MEAN	MEAN	SE	N	71	SE	44	30	SE	44	174	SE	44	151	SE	44	
200	231	231	231	2.22	0.22	2	2.56		1	2.11		1							
400	402	402	402	3.03	0.64	2	3.97		1	2.39		1							
600	650	650	650	3.31	0.86	2	3.06		1	2.65		1							
OVERALL MEANS			2.89	0.08	6	3.40	0.43	3	2.38	0.16	3								

ESTIMATED AT 10,000 PPMV 7.84

95% CONFIDENCE INTERVAL 1.4 40.43 781

Figure 3-4

INSTRUMENT RESPONSE VS CONCENTRATION

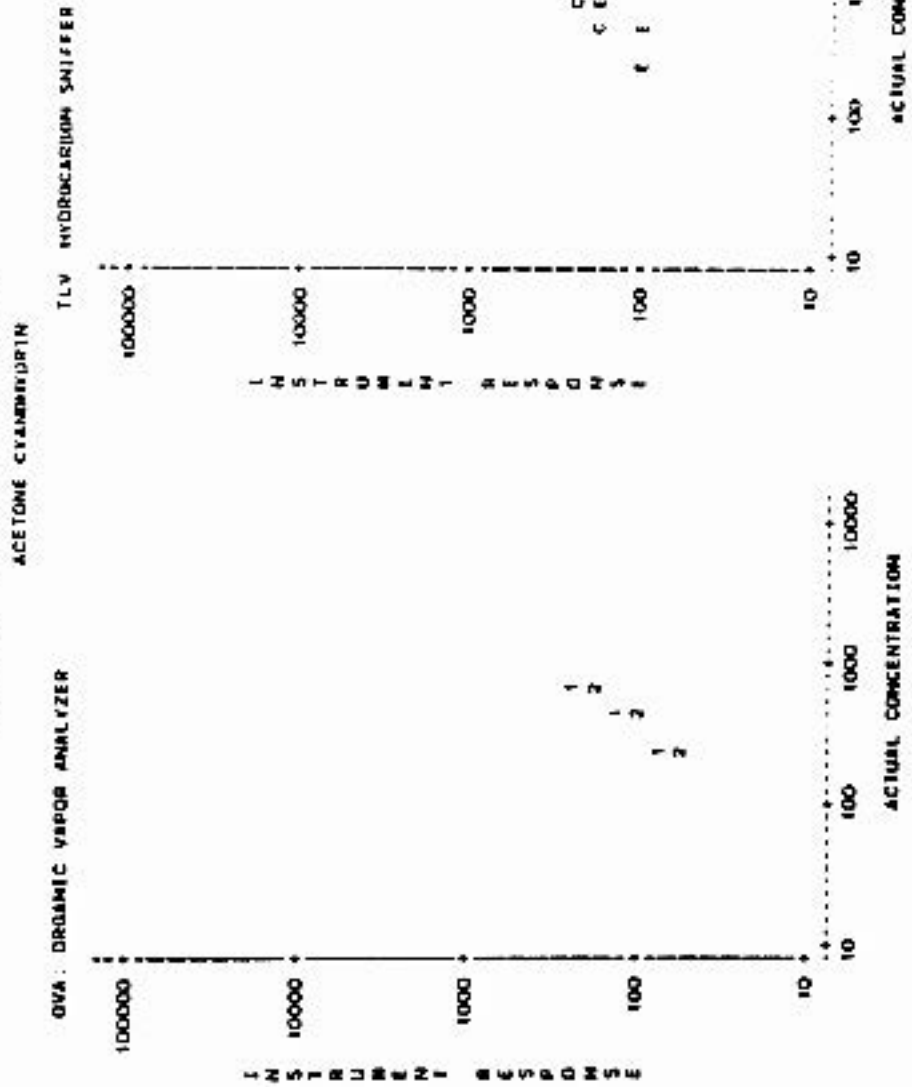




TABLE 5-5

RESPONSE FACTOR SUMMARY

ACETONITRILE

OVA INSTRUMENTS


NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS												
	LOW	HIGH	MEAN	MEAN	SE	N	10SD	SE	M	2254	SE	N	3150	SE	N	4810	SE	N	
200	226	226	226	1.34	0.10	2	1.44					1.24							
1500	1518	1518	1518	1.16	0.03	2	1.12					1.19							
8000	7773	7773	7773	0.95	0.01	2	0.98					0.98							
OVERALL MEANS				1.10	0.00	6	1.17	0.14	3	1.13	0.09	3							
ESTIMATED AT 10,000 PPMV				0.94				95% CONFIDENCE INTERVAL (0.95, 1.05)											

ELV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS												
	LOW	HIGH	MEAN	MEAN	SE	N	7E	SE	N	7C	SE	N	7M	SE	N	7U	SE	N	
200	226	226	226	1.06	0.08	2	1.14					0.98							
1500	1518	1518	1518	1.00	0.03	2	0.96					1.03							
8000	7773	7773	7773	1.22	0.10	2	1.37					1.13							
OVERALL MEANS				1.09	0.01	6	1.14	0.10	3	1.04	0.05	3							
ESTIMATED AT 10,000 PPMV				1.17				95% CONFIDENCE INTERVAL (1.06, 1.42)											

Figure S-5

INSTRUMENT RESPONSE VS CONCENTRATION

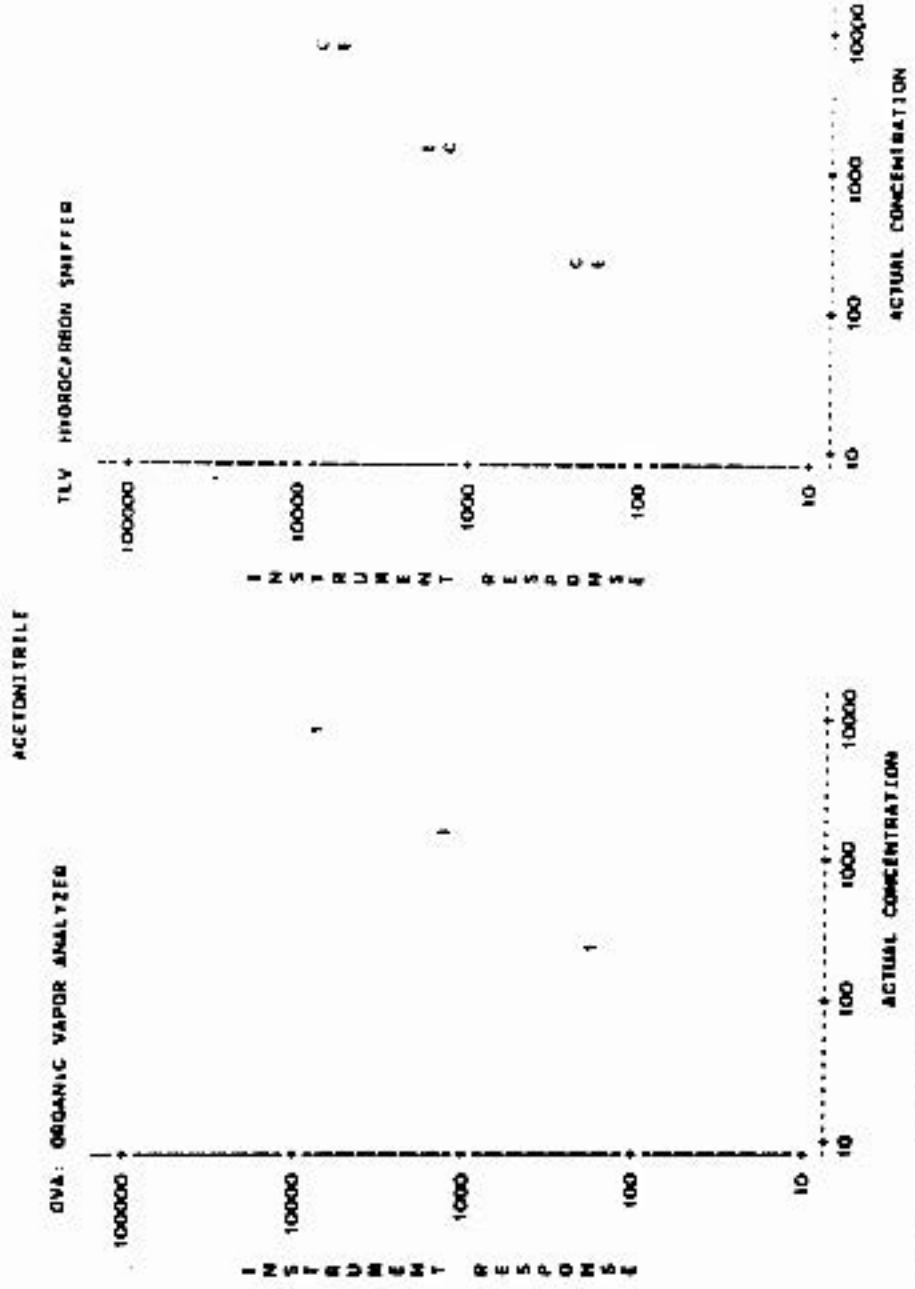

NOTE: 3 OBS HIDDEN

TABLE 5-6

RESPONSE FACTOR SUMMARY

ACETOPHENONE

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTORS													
	LOW	HIGH	MEAN	SE	N	1000	SE	M	2204	SE	M	2109	SE	M	1813	SE	M	
50	47	50	48	19	4	5.71	2.18	2	8.88	3.14	2							
500	517	546	531	6.47	4	9.82	1.18	2	7.11	1.36	2							
5000	5207	5207	5207	15.01	2	12.40		1	18.93		1							
8000	8676	8677	8676	27.83	4	27.58	23.2	2	28.08	22.4	2							

OVERALL MEANS 14.00 0.06 14 13 10 8 40 7 14 80 6 13 7

ESTIMATED AT 10,000 PPMV 10.98

99% CONFIDENCE INTERVAL 1.5 56.21 681

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTORS													
	LOW	HIGH	MEAN	SE	N	76	SE	M	70	SE	M	7M	SE	M	70	SE	M	
50	47	50	48	2.11	4	2.45	0.19	2	1.78	0.22	2							
500	517	546	531	12.53	4	15.85	2.11	2	9.17	2.34	2							
5000	5207	5207	5207	30.30	2	44.81		1	15.78		1							
8000	8676	8677	8676	51.93	4	70.30	3.50	2	53.58	12.3	2							

OVERALL MEANS 28.20 0.20 14 31 72 11 3 7 20 68 9 11 7

ESTIMATED AT 10,000 PPMV 54.88

99% CONFIDENCE INTERVAL 1.20 35.78 481


Figure 5-6

INSTRUMENT RESPONSE VS CONCENTRATION

ACETOPHENONE

QVA ORGANIC VAPOR ANALYZER

FLV HYDROCARBON SNIFFER

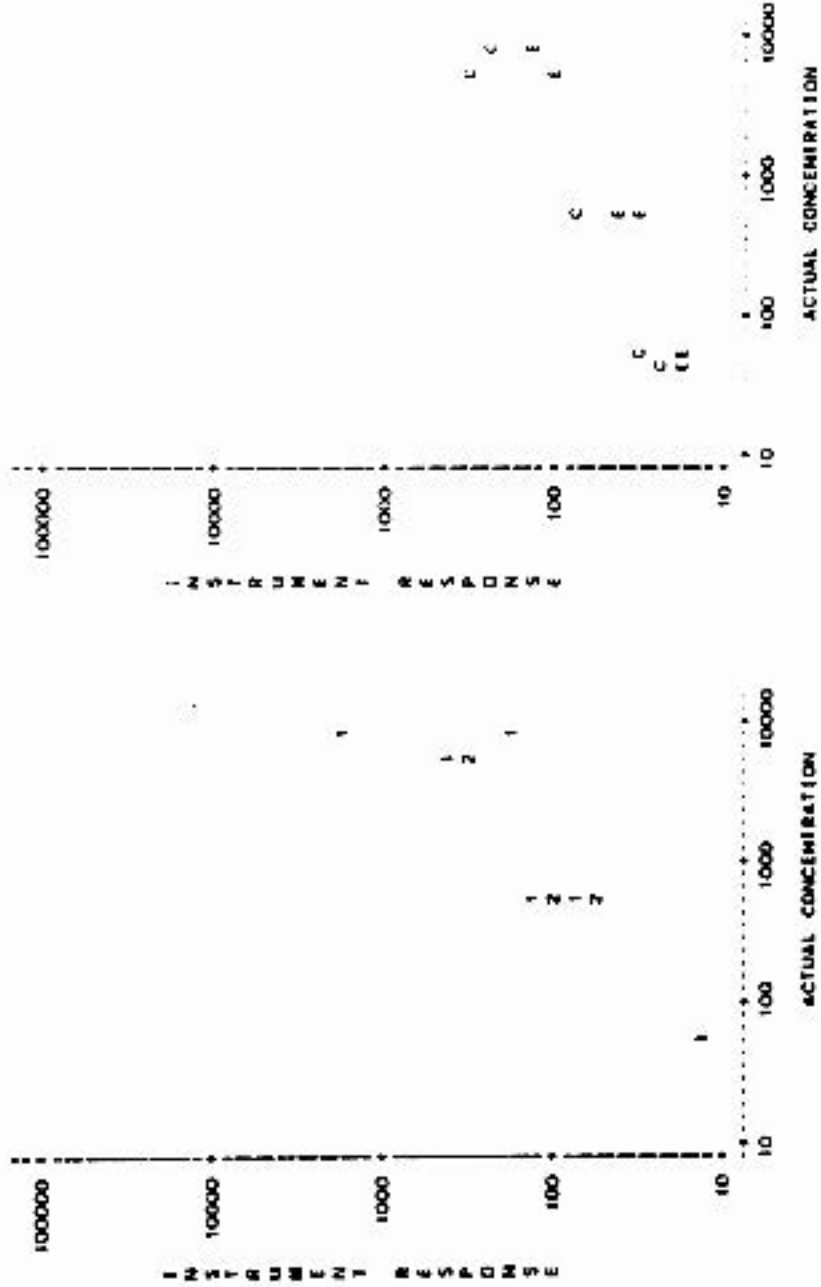

NOTE: 3 OBS MISSING OR OUT OF RANGE

NOTE: 3 OBS HIDDEN

TABIE 5-7

RESPONSE FACTOR SUMMARY

ACETYL CHLORIDE

DVA INSTRUMENTS

M E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV			OVERALL						DVA METERS						
	LOW	HIGH	MEAN	MEAN	SE	N	7E	SE	N	7C	SE	N	7M	SE	N	
200	192	192	192	1.75	0.09	2	1.86		1	1.80		1	1.83		1	
1000	1484	1484	1484	1.86	0.15	2	1.71		1	2.01		1	2.01		1	
8000	8875	8875	8875	2.00	0.11	2	1.89		1	2.12		1	2.12		1	
OVERALL MEANS				1.87	0.07	6	1.75	0.07	3	1.98	0.08	3				

ESTIMATED AT 10,000 PPMV 1.99

95 % CONFIDENCE INTERVAL ( 1.75, 2.261)

TLV INSTRUMENTS

M E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV			OVERALL						TLV METERS						
	LOW	HIGH	MEAN	MEAN	SE	N	7E	SE	N	7C	SE	N	7M	SE	N	
200	192	192	192	2.19	0.47	2	2.48		1	1.71		1	2.17		1	
1000	1484	1484	1484	2.62	0.44	2	3.06		1	2.17		1	2.17		1	
8000	8875	8875	8875	2.57	0.31	2	2.89		1	2.76		1	2.76		1	
OVERALL MEANS				2.46	0.07	6	2.87	0.12	3	2.09	0.17	3				

ESTIMATED AT 10,000 PPMV 2.69

95 % CONFIDENCE INTERVAL ( 1.81, 3.711)

Figure 5-7

INSTRUMENT RESPONSE VS CONCENTRATION

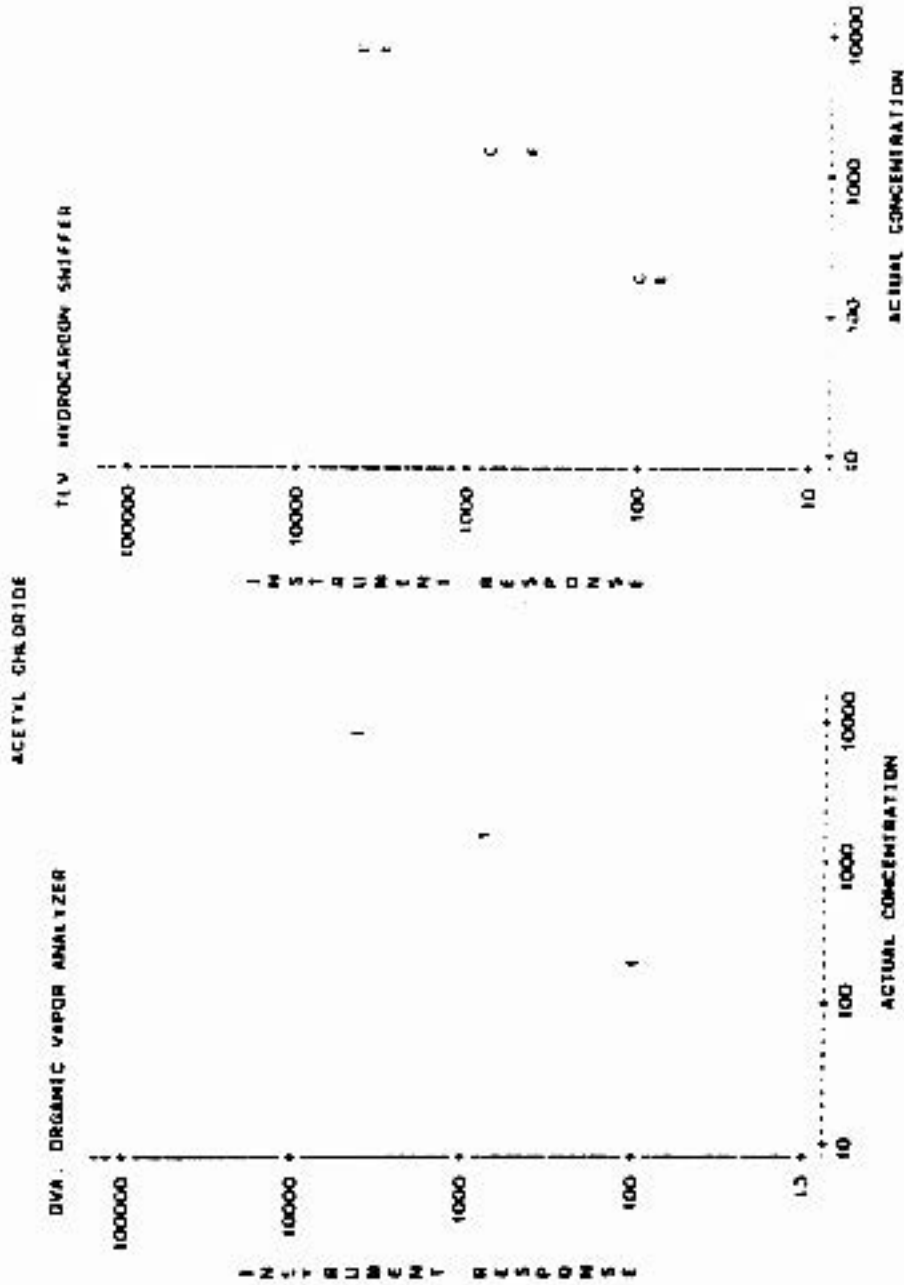




TABLE 5-8

RESPONSE FACTOR SUMMARY

ACETYL I PROPIONDI 3

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METERS							
	LOW	HIGH	MEAN	SE	N	1000	SE	N	2214	SE	N	2150	SE	N
50	52	54	2 17 0 08	4	2 09 0 07	2	2 25 0 06	2						
500	544	559	2 72 0 08	4	2 81 0 02	2	2 83 1 01	2						
5000	5481	5500	14 24 1 14	4	15 31 2 48	2	13 10 2 48	2						
OVERALL MEANS			6 38 0 03	12	6 70 2 81	6	5 99 2 95	6						

ESTIMATED AT 10,000 PPMV 10 BT 95 % CONFIDENCE INTERVAL 1.6 NR 17 95%

TLV IMPRIMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			TLV METERS							
	LOW	HIGH	MEAN	SE	N	18	SE	N	70	SE	N	100	SE	N
50	55	57	1 94 0 41	4	2 38 0 17	2	1 93 0 26	2						
500	544	553	4 90 1 53	4	8 52 2 43	2	4 28 1 29	2						
5000	5481	5500	38 78 20 4	4	59 21 5 49	2	18 34 1 20	2						
OVERALL MEANS			15 21 0 62	12	22 70 8 6	6	1 72 3 49	6						

ESTIMATED AT 10,000 PPMV 25 BT

95 % CONFIDENCE INTERVAL 1.1 TO 48 631

TABLE 5-14

RESPONSE FACTOR SUMMARY

AMYL ALCOHOL, M-

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTORS									
	LOW	HIGH	MEAN	SE	N	1080	SE	N	2254	SE	N	1813	SE	N
200	223	220	219	0.09	2	2.12		1	2.26		1			
1000	1081	1081	1.26	0.14	2	1.11		1	1.29		1			
2000	2188	2188	1.18	0.13	2	1.02		1	1.28		1			
OVERALL MEANS			1.53	0.03	6	1.42	0.35	3	1.64	0.31	3			

ESTIMATED AT 10,000 PPMV 0.88

95% CONFIDENCE INTERVAL 1.07 - 1.401

TLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTORS									
	LOW	HIGH	MEAN	SE	N	TE	SE	N	70	SE	N	TM	SE	N
200	223	223	0.88		1									
1000	1051	1081	1.08		1									
2000	2188	2188	1.17		1									
OVERALL MEANS			0.88		3									


ESTIMATED AT 10,000 PPMV 1.78

95% CONFIDENCE INTERVAL 1.19 - 2.463

Figure 5-14

INSTRUMENT RESPONSE VS CONCENTRATION

OV-17 ORGANIC VAPOR ANALYZER  
 OV-17 HYDROCARBON SNIFFER

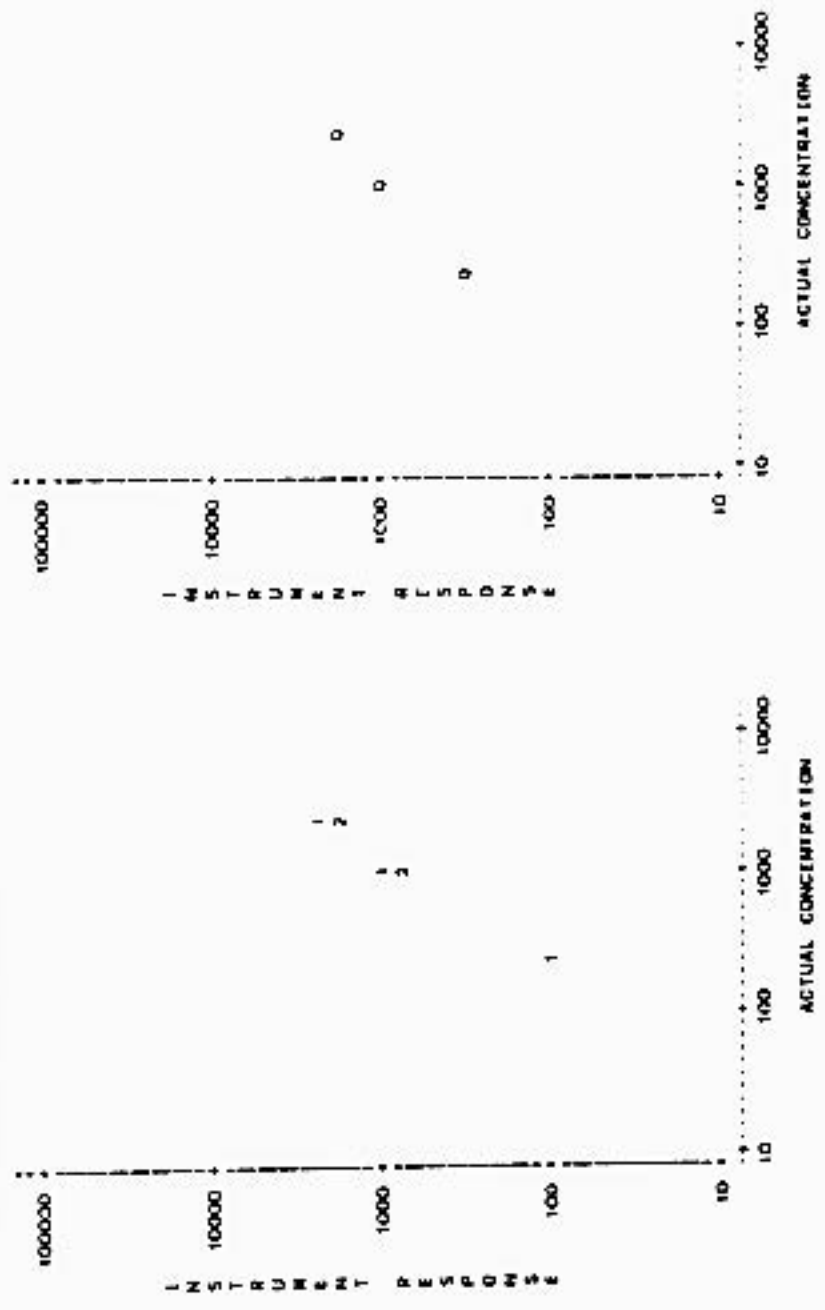

NOTE: 1 OBS HIDDEN

TABLE 5-15  
RESPONSE FACTOR SUMMARY

ARYLENE

R E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV		OVERALL		OVA METERS													
	LOW	HIGH	MEAN	SE	N	1080	SE	N	2254	SE	N	2199	SE	N	1813	SE	N	
300	236	236	236	0.74	2	1.72	1	1.08	1									
1500	1428	1428	1428	0.70	2	0.57	1	0.95	1									
4000	4012	4012	4012	0.45	2	0.40	1	0.51	1									
6000	5848	5848	5848															
8000	7771	7771	7771															
OVERALL MEANS			0.89	0.03	4	0.13	0.20	2	1.05	0.20	2							

ESTIMATED AT 10,000 PPMV 0.31      95% CONFIDENCE INTERVAL 1.019 0.511

FLV INSTRUMENTS

R E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV		OVERALL		FLV METERS															
	LOW	HIGH	MEAN	SE	N	TE	SE	N	3C	SE	N	7M	SE	N	46	SE	N	70	SE	N
300	236	236	236	4.87	2	1.83	1	1.91	1											
1500	1428	1428	1428	2.58	2	4.03	1	1.13	1											
4000	4012	4012	4012	1.30	2	1.73	1	0.87	1											
6000	5848	5848	5848	1.39	1			1.38	1											
8000	7771	7771	7771	2.28	2	3.05	1	1.00	1											
OVERALL MEANS			2.60	0.17	8	4.28	1.38	4	1.26	0.18	5									

ESTIMATED AT 10,000 PPMV 1.03      95% CONFIDENCE INTERVAL 1.046 2.321

Figure 5-15

INSTRUMENT RESPONSE VS CONCENTRATION

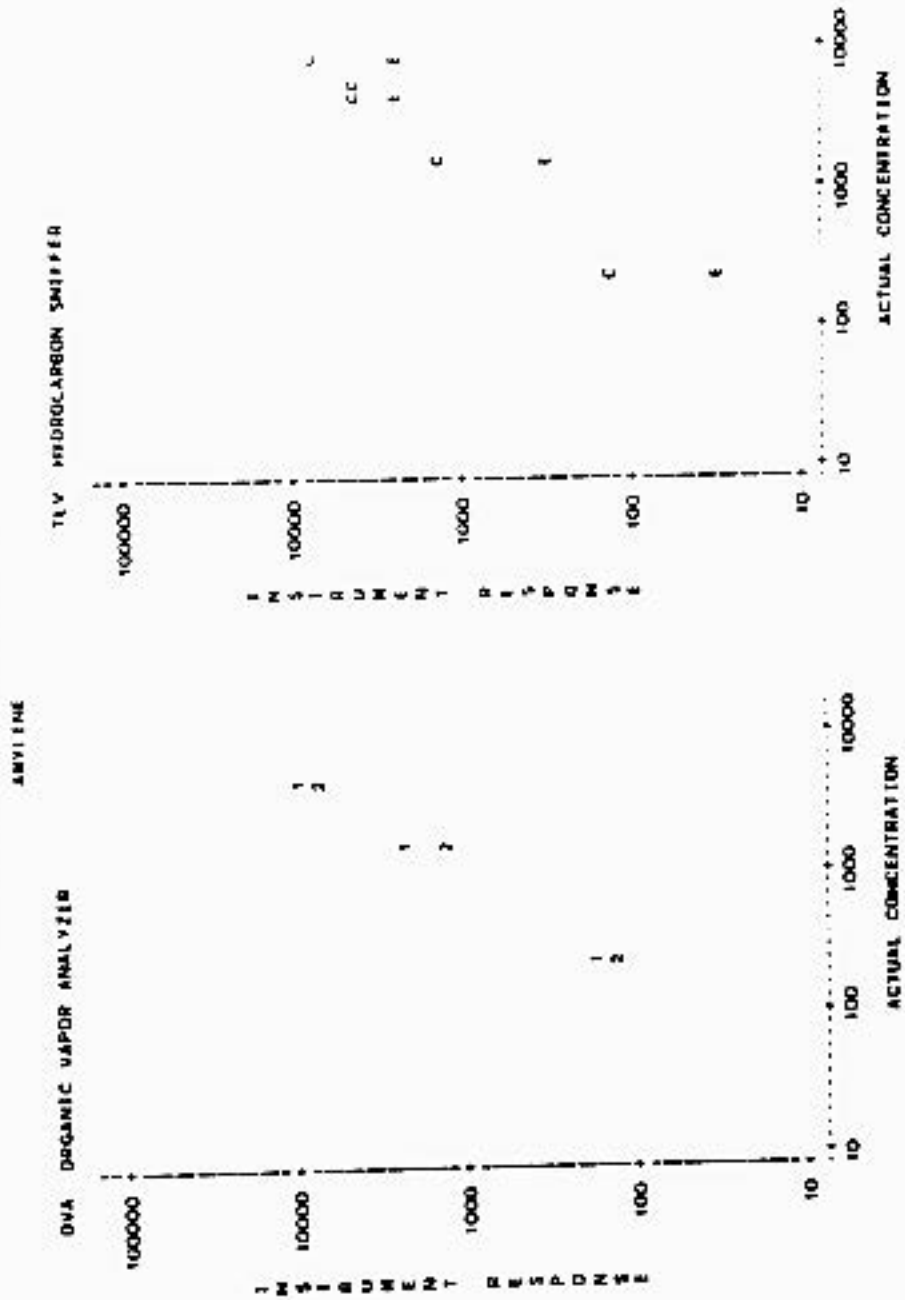


TABLE 5-16

RESPONSE FACTOR SUMMARY

ANISOLE

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS												
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2204	SE	N	2159	SE	N	1813	SE	N	
200	198	198	198	0.97	0.00	2	0.92		1	1.03		1							
1500	1530	1530	1530	0.79	0.06	2	0.72		1	0.85		1							
3200	3443	3443	3443	1.06	0.06	2	0.88		1	1.11		1							
OVERALL MEANS			0.94	0.01	6	0.88	0.08	3	1.00	0.08	3								

ESTIMATED AT 10,000 PPMV 0.92

95% CONFIDENCE INTERVAL (0.64, 1.21)

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS											
	LOW	HIGH	MEAN	MEAN	SE	N	7E	SE	N	7C	SE	N	7M	SE	N	7D	SE	N
200	198	198	198	0.99		1										0.95		1
1500	1530	1530	1530	1.47		1										1.87		1
3200	3443	3443	3443	2.19		1										2.16		1
OVERALL MEANS			1.52		3											1.52	0.15	3

ESTIMATED AT 10,000 PPMV 2.69

95% CONFIDENCE INTERVAL (1.69, 4.21)



Figure 5-16

INSTRUMENT RESPONSE VS CONCENTRATION

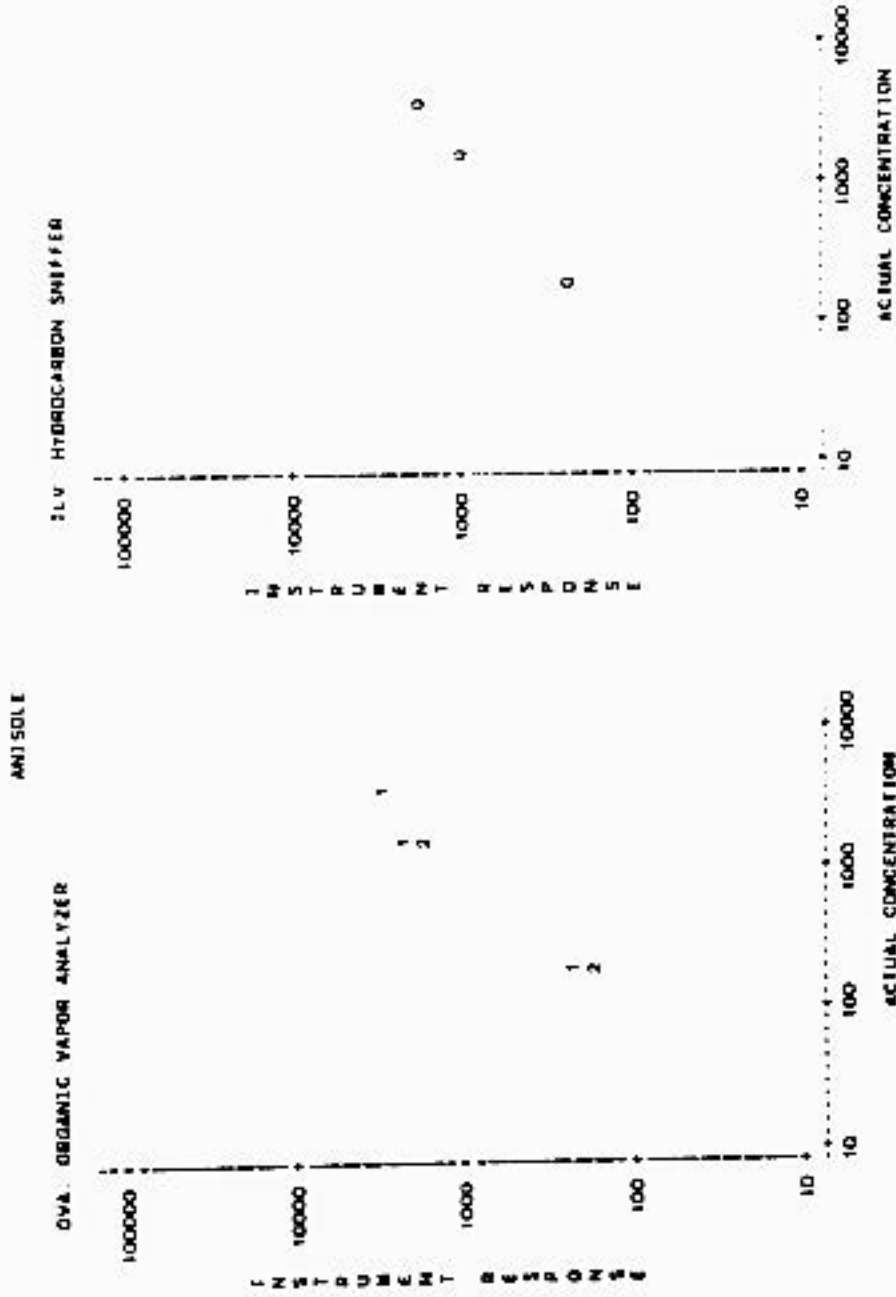


TABLE 5-17

RESPONSE FACTOR SUMMARY

BENZALDEHYDE

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS												
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	M	7304	SE	M	7109	SE	M	1817	SE	M	
200	196	196	196	1.99	0.03	2	1.98		1	2.02		1							
800	798	798	798	2.07	0.06	2	2.13		1	2.02		1							
1200	1179	1179	1179	2.22	0.35	2	1.87		1	2.56		1							
OVERALL MEANS			2.10	0.02	6	1.99	0.07	3	2.20	0.18	3								

ESTIMATED AT 10,000 PPMV 2.38 95% CONFIDENCE INTERVAL 1.19 3.881

FLV INSTRUMENTS


NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS											
	LOW	HIGH	MEAN	MEAN	SE	N	78	SE	N	7C	SE	N	7M	SE	N	7D	SE	N
200	196	196	196	0.89		1										0.89		1
800	798	798	798	1.81		1										1.81		1
1200	1179	1179	1179	2.16		1										2.16		1
OVERALL MEANS			1.62		3							1.82	0.38	1				

ESTIMATED AT 10,000 PPMV 6.30 95% CONFIDENCE INTERVAL 4.57 6.881

Figure 5-17

INSTRUMENT RESPONSE VS CONCENTRATION

BENZALDEHYDE

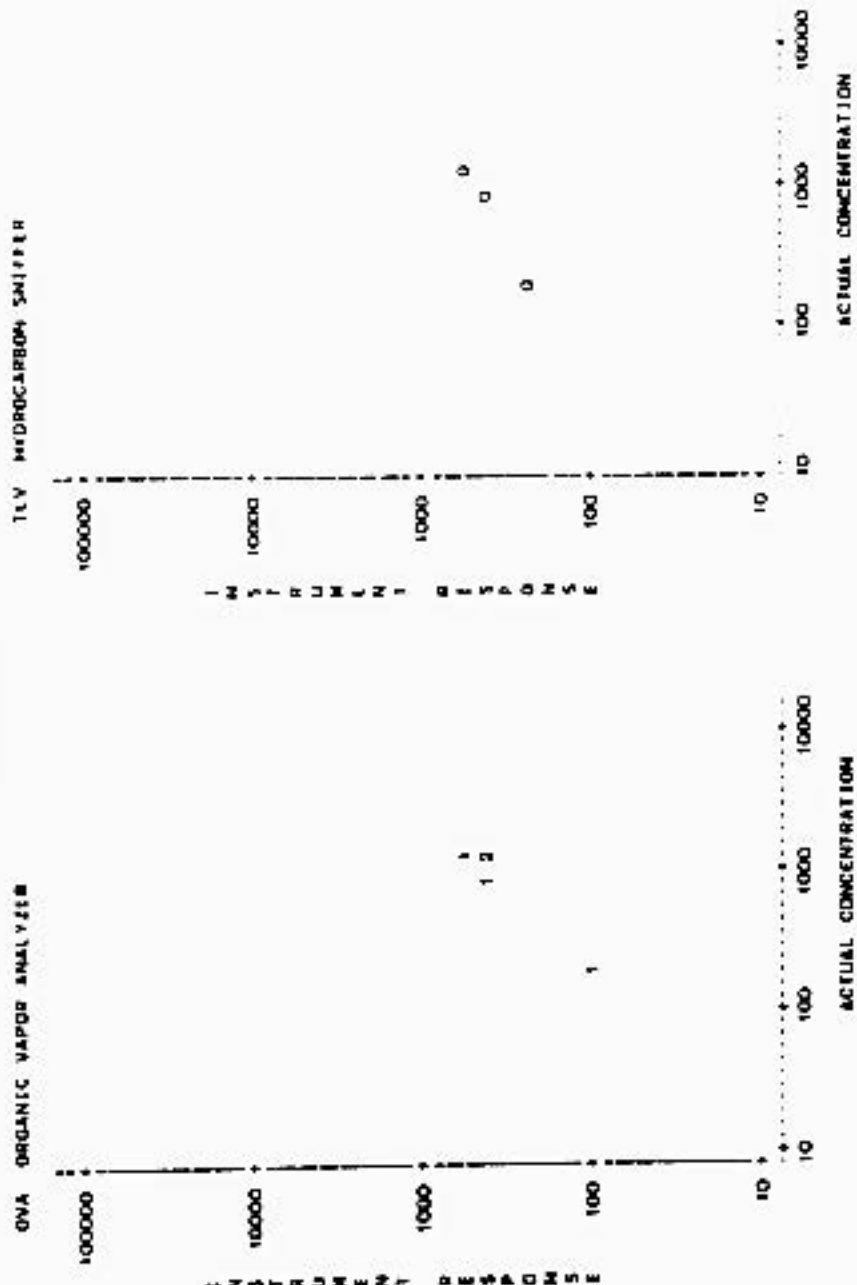

NOTE: 2 OBS HIDDEN

TABLE 5-18

RESPONSE FACTOR SUMMARY

BENZENE

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		OVA METERS												
	LOW	HIGH	MEAN	SE	N	1000	SE	N	2000	SE	N	3150	SE	N	1812	SE	N
50	47	54	0.68	0.06	4	0.95	0.29	2	0.1	0.06	2				0.53		1
150	200	200	0.53		1										0.52		1
700	197	197	0.52		1									0.48		1	
250	262	262	0.48		1									0.45		1	
350	368	368	0.40	0.09	6	0.53	0.01	2	0.98	0.03	2	0.38		0.42		1	
500	516	545	0.40	0.02	2							0.38		0.38		1	
750	760	790	0.38	0.03	2							0.38		0.35		1	
1000	939	939	0.38	0.01	2							0.31		0.31		1	
1250	1372	1372	0.37	0.00	2							0.27		0.27		1	
1500	1572	1572	0.28	0.00	2							0.28		0.28		1	
2000	2122	2122	0.32	0.01	2							0.31		0.31		1	
2400	2434	2434	0.28	0.00	2							0.27		0.27		1	
2800	2756	2756	0.28	0.00	2							0.28		0.28		1	
3000	3176	3176	0.32	0.01	4	0.30	0.02	2	0.33	0.05	2						
3200	3110	3110	0.45	0.00	31	0.59	0.14	6	0.56	0.09	6	0.34	0.01	6	0.40	0.03	11
3600	3922	3922															
4000	3262	3304															

ESTIMATED AT 10,000 PPMV 0.71

95% CONFIDENCE INTERVAL (0.19, 0.24)

TABLE 5-18 (CONTINUED)

RESPONSE FACTOR SUMMARY

BENZENE

NOMINAL PPMV	ACTUAL PPMV			RESPONSE FACTORS										N																															
	LOW	HIGH	MEAN	SE	M	TC	SE	M	TC	SE	M	TC	SE		M	TC																													
50	47	60	54	0.87	0.08	1	0.95	0.07	2	0.79	0.05	2	0.80	0.07	1	0.87	0.07	1	0.85	0.05	3	1.06	1.09	1	0.96	0.06	2	0.98	0.00	2	1.07	1.00	1	1.14	1.08	1	1.24	0.81	0.07	2					
100	100	200	200	0.80	0.08	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1	0.80	0.07	1
200	197	197	197	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1	0.87	0.07	1
250	252	252	252	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1
300	300	300	300	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1	0.85	0.05	1
500	516	545	535	1.07	0.14	5	1.20	0.01	2	0.96	0.02	3	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1
750	750	750	750	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1	1.06	1.06	1
1000	928	928	928	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1	1.09	1.09	1
1250	1372	1372	1372	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1	0.98	0.98	1
1500	1572	1572	1572	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2	0.98	0.98	2
2000	2122	2122	2122	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1
2400	2424	2424	2424	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1	1.00	1.00	1
2800	2756	2756	2756	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1	1.07	1.07	1
3000	3178	3178	3178	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1	1.14	1.14	1
3200	3110	3110	3110	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1	1.08	1.08	1
3600	3922	3922	3922	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1	1.24	1.24	1
4000	3262	3504	3262	0.89	0.09	4	0.98	0.06	2	0.81	0.07	2	0.89	0.09	4	0.89	0.09	4	0.89	0.09	4	0.89	0.09	4	0.89	0.09	4	0.89	0.09	4	0.89	0.09	4	0.89	0.09	4	0.89	0.09	4	0.89	0.09	4	0.89	0.09	4

OVERALL MEANS 0.98 0.00 28  
ESTIMATED AT 10,000 PPMV 1.07

95% CONFIDENCE INTERVAL 1.07 1.19

Figure 5-18

INSTRUMENT RESPONSE VS CONCENTRATION

BENZENE

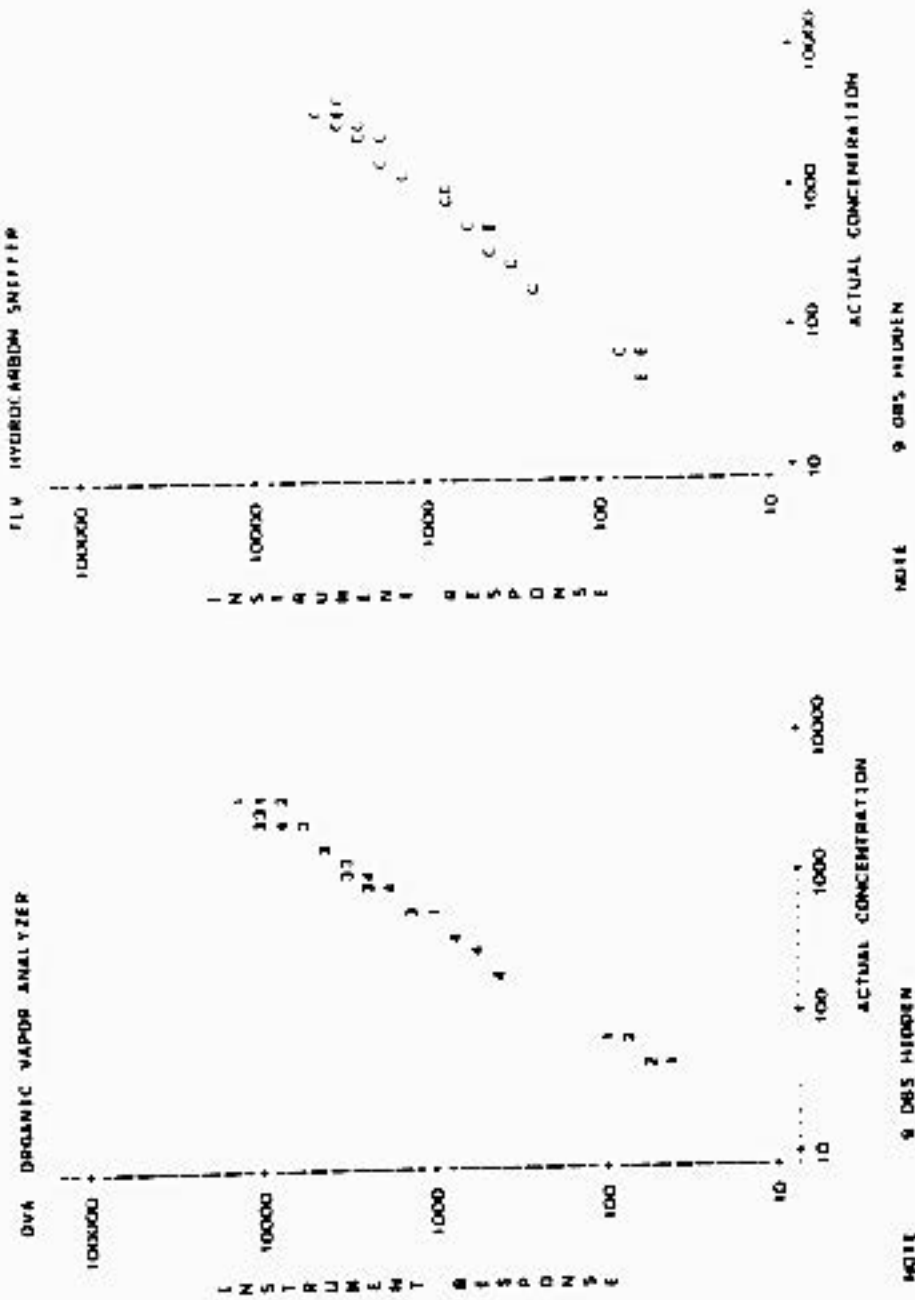




TABLE N-19


RESPONSE FACTOR SUMMARY

BENZONITRILE				RESPONSE FACTOR SUMMARY														
OVA INSTRUMENTS				ACTUAL PPMV				OVERALL				DVA METERS						
NOMINAL PPMV	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2254	SE	N	2859	SE	N	1813	SE	N
700	164	170	167	0.43	0.02	4	0.81	0.02	2	0.85	0.11	2						
850	532	550	541	0.69	0.01	4	0.88	0.00	2	0.90	0.02	2						
1100	871	992	931	1.47	0.03	4	1.41	0.17	2	1.48	0.46	2						
OVERALL MEANS				1.05	0.00	12	1.03	0.15	6	1.07	0.17	6						
ESTIMATED AT 10,000 PPMV				2.24	95% CONFIDENCE INTERVAL 1.18 - 4.241													
FLV INSTRUMENTS				ACTUAL PPMV				OVERALL				TLV METERS						
NOMINAL PPMV	LOW	HIGH	MEAN	MEAN	SE	N	TR	SE	N	TC	SE	N	SM	SE	N	TD	SE	N
200	164	170	167	0.84		2										0.84	0.01	2
850	532	550	541	1.48		2										1.48	0.21	2
1100	871	992	931	2.35		2										2.35	0.82	2
OVERALL MEANS				1.62	95% CONFIDENCE INTERVAL 1.282 - 34.631													
ESTIMATED AT 10,000 PPMV				9.13														

Figure 5-14

INSTRUMENT RESPONSE VS CONCENTRATION

BENZONITRILE

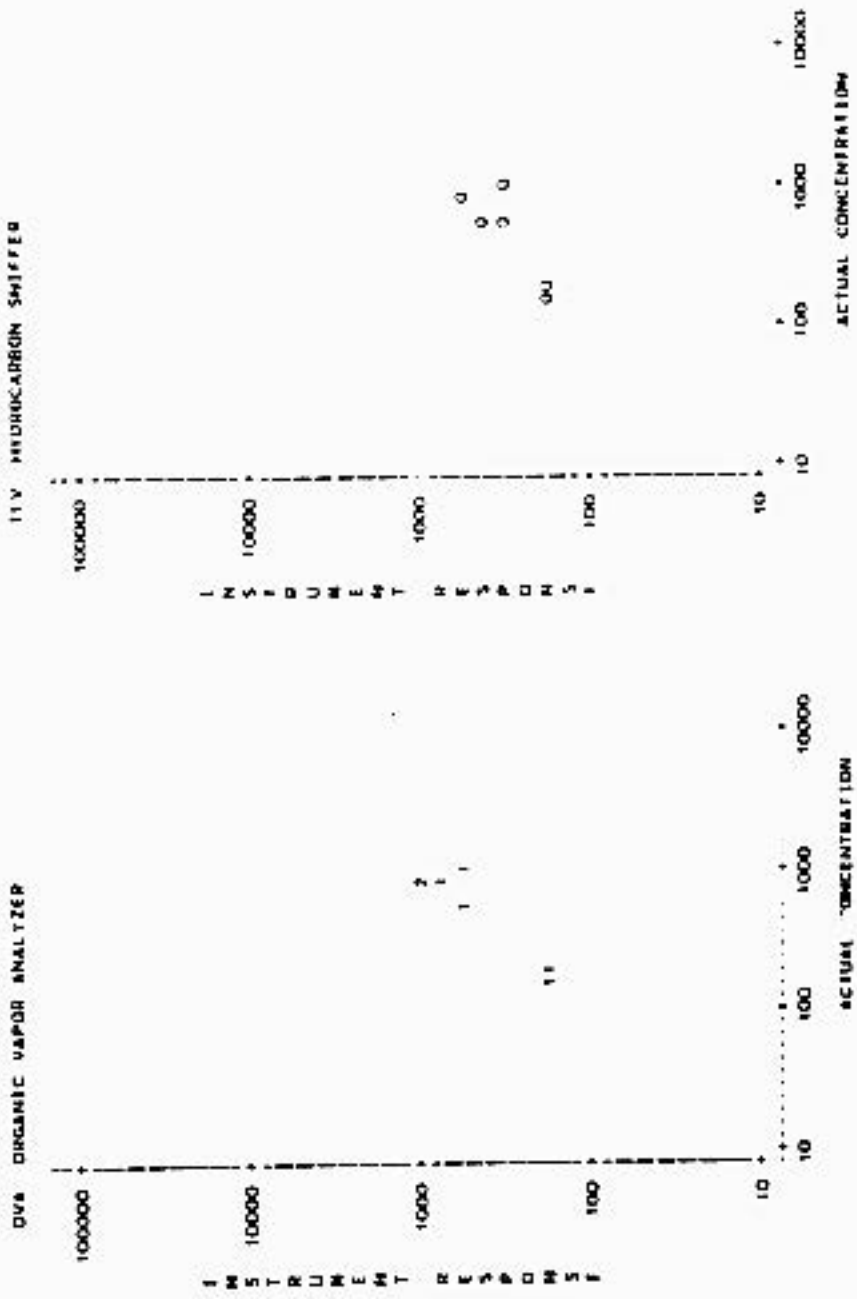

NOTE: 6 OBS HIDDEN

TABLE 5-211


RESPONSE FACTOR SUMMARY

BENZENE CARBON DIOXIDE				RESPONSE FACTOR SUMMARY												
OVA INSTRUMENTS				ACTUAL PPMV						CALCULATED						
NOMINAL PPMV	LOW	HIGH	MEAN	MEAN	SE	N	TC	SE	N	TC	SE	N	TC	SE	N	
200	203	203	203	181	0.08	2	1.75	1.91	1	1.97	1	1812	51	1812	51	N
1500	1482	1482	1482	704	0.13	2	1.91	1.91	1	2.16	1					
8000	7884	7884	7884	811	0.38	2	0.49	1.72	1	1.72	1					
OVERALL MEANS				388	0.01	6	4.05	2.22	3	3.82	1.91	3				
ESTIMATED AT 10,000 PPMV				840												
95% CONFIDENCE INTERVAL																
FLV INSTRUMENTS				RESPONSE FACTOR SUMMARY												
ACTUAL PPMV				ACTUAL PPMV						CALCULATED						
NOMINAL PPMV	LOW	HIGH	MEAN	MEAN	SE	N	TC	SE	N	TC	SE	N	TC	SE	N	
200	203	203	203	0.97		1										
1500	1482	1482	1482	2.11		1										
8000	7884	7884	7884	6.49		1										
OVERALL MEANS				3.19		3										
ESTIMATED AT 10,000 PPMV				640												
95% CONFIDENCE INTERVAL																

FIGURE 5-20

INSTRUMENT RESPONSE VS CONCENTRATION

GENERIC CHEMIST

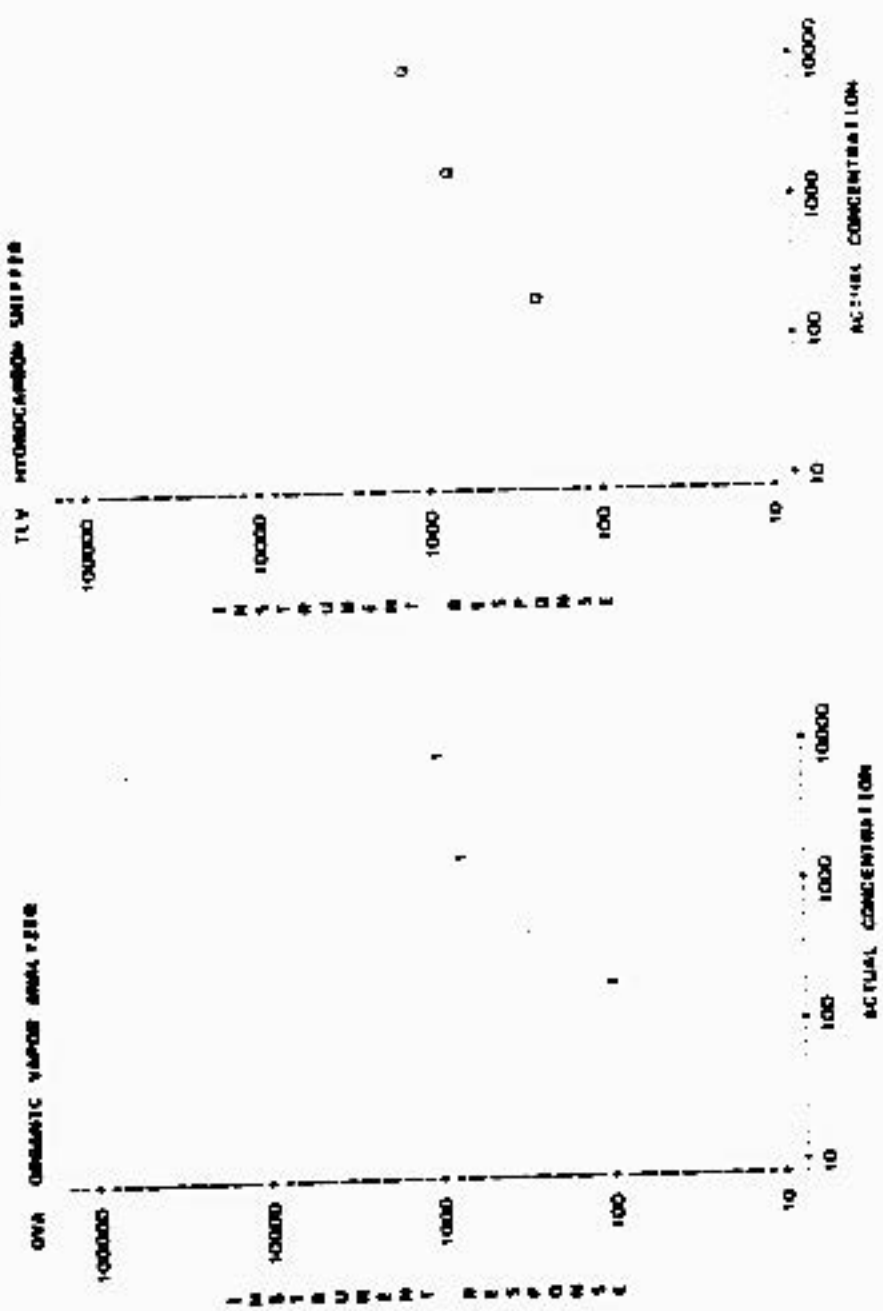

NOTE: 20% H<sub>2</sub>O IN OVA

TABLE 1-21

RESPONSE FACTOR SUMMARY

BENZYNE CHLORIDE

OVA INSTRUMENTS RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV		OVR BIAS		RESPONSE FACTORS								
	LOW	HIGH	MEAN	SE	1000	SE	N	2100	SE	N	4010	SE	N
200	189	199	1.92	0.01	1.02		1	1.04		1			
1500	1823	1823	1.09	0.14	0.91		1	1.18		1			
4000	3648	4246	4.65	0.36	4.28	0.29	2	5.02	0.29	2			
8000	7810	7878	8.16	0.82	4.81	0.70	2	8.87	0.94	2			
OVERALL MEANS			3.81	0.09	3.29	0.06	4	3.83	0.10	4			

ESTIMATED AT 10,000 PPMV 4.23 95% CONFIDENCE INTERVAL ( 3.74 - 4.87)

FLV INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV		OVR BIAS		RESPONSE FACTORS								
	LOW	HIGH	MEAN	SE	100	SE	N	310	SE	N	510	SE	N
200	189	199	0.78										
1500	1823	1823	1.07										
4000	3648	4246	8.14										
8000	7810	7878	8.39										
OVERALL MEANS			3.82										

ESTIMATED AT 10,000 PPMV 4.87 95% CONFIDENCE INTERVAL ( 4.50 - 4.88)

Figure 5-21

INSTRUMENT RESPONSE VS CONCENTRATION

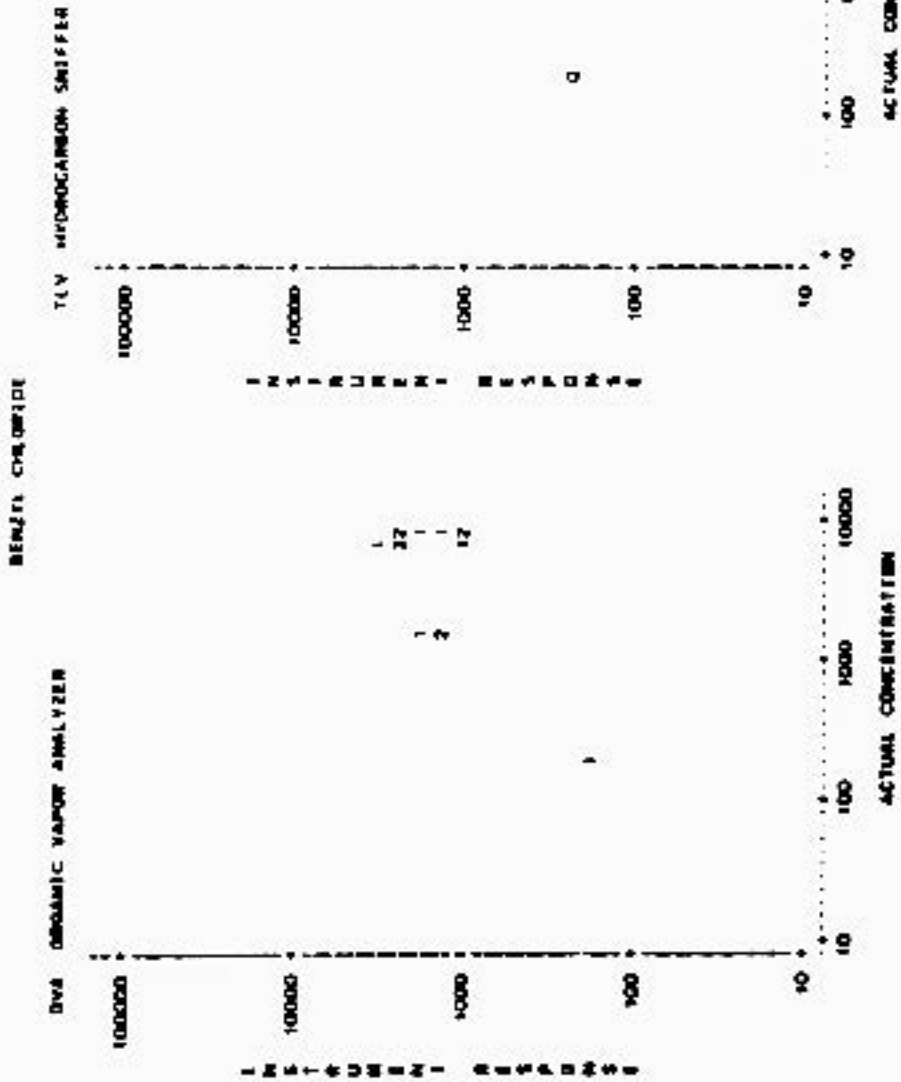


TABLE 5-22

RESPONSE FACTOR SUMMARY

ACTUAL MEASUREMENTS

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR														
	LOW	HIGH	MEAN	SE	7E	5E	N	7C	5A	M	2100	5A	M	1810	5E	N			
200	208	208	208	0.95	0.00	2	0.84	1	0.88	1	0.86	1	0.80	1	0.37	1	0.47	0.08	3
1800	1848	1848	1848	0.81	0.00	2	0.81	1	0.80	1	0.80	1	0.80	1	0.37	1	0.47	0.08	3
2000	2011	2011	2011	0.28	0.00	2	0.28	1	0.28	1	0.28	1	0.28	1	0.37	1	0.47	0.08	3
OVERALL MEANS				0.48	0.00	8	0.48	0.08	0.47	0.08	3								

ESTIMATED AT 10,000 PPMV 0.26

95% CONFIDENCE INTERVAL 1.0 28 0.481

FLV INSTRUMENTS

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR														
	LOW	HIGH	MEAN	SE	7E	5E	N	7C	5A	M	2100	5A	M	1810	5E	N			
200	208	208	208	0.62	1	0.62	1	0.62	1	0.62	1	0.62	1	0.62	1	0.62	1	0.62	1
1800	1848	1848	1848	0.77	1	0.77	1	0.77	1	0.77	1	0.77	1	0.77	1	0.77	1	0.77	1
2000	2011	2011	2011	1.02	1	1.02	1	1.02	1	1.02	1	1.02	1	1.02	1	1.02	1	1.02	1
OVERALL MEANS				0.81	3														

ESTIMATED AT 10,000 PPMV 1.16


95% CONFIDENCE INTERVAL 1.48 1.841



Figure 5-22

INSTRUMENT RESPONSE VS CONCENTRATION

PROBENZENE

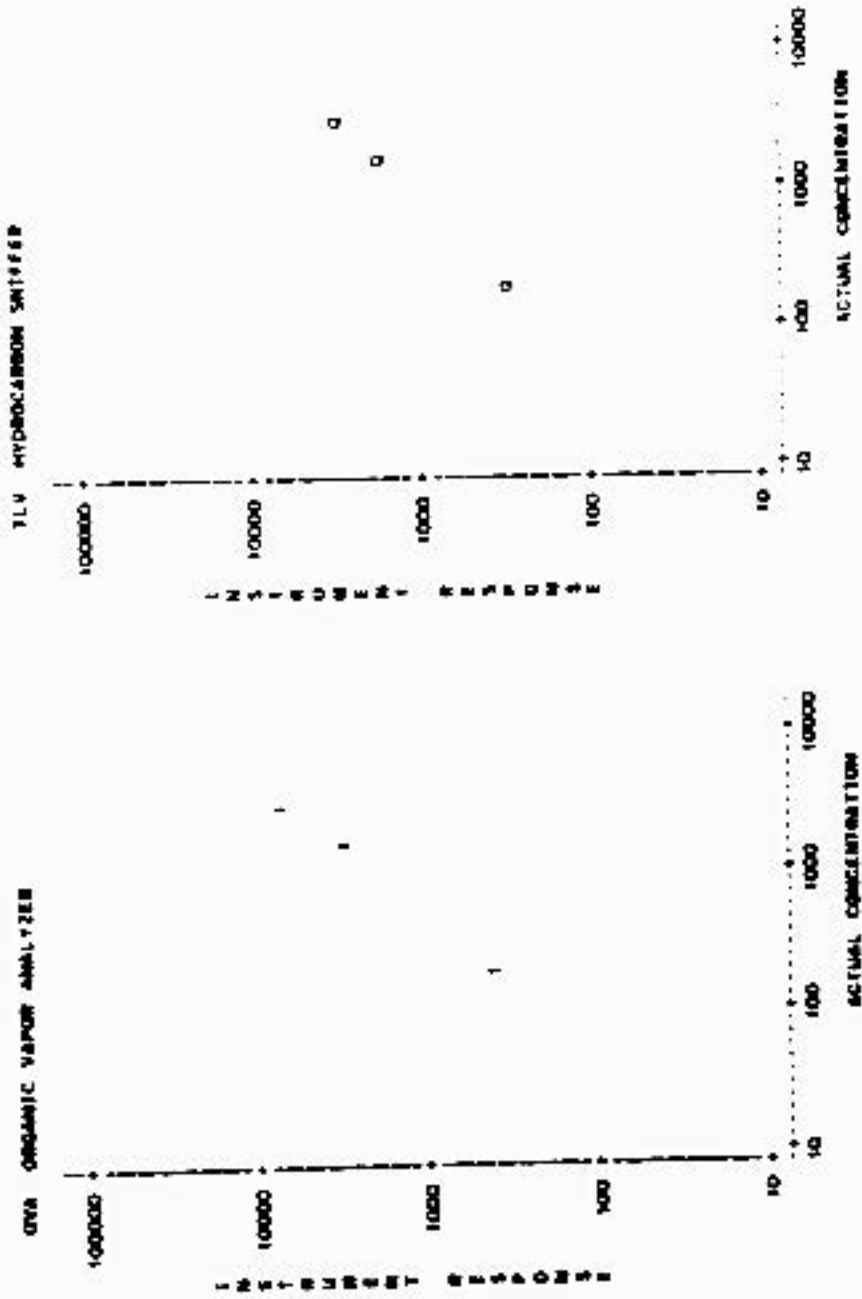

NOTE: 2 60% HUMIDITY

TABLE 5-23

RESPONSE FACTOR SUMMARY

MUTADICENE 1.2

OVA INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL				OVA METERS								
	LOW	HIGH	MEAN	MEAN	SE	N	1000	50	M	2000	SE	N	1000	SE	N	
1000	878	878	878	2.18	0.08	2	2.24		1	2.10		1				
3000	2868	2868	2868	0.94	0.03	2	0.83		1	0.96		1				
5000	4802	4802	4802	0.81	0.03	2	0.80		1	0.83		1				
1883	1883	1883	1883													
OVERALL MEANS				1.28	0.00	4	1.28	0.51	3	1.28	0.45	3				
ESTIMATED AT 10,000 PPMV				0.37												
				99 % CONFIDENCE INTERVAL ( 0.34, 0.42 )												

TLV INSTRUMENTS


RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL				TLV METERS							
	LOW	HIGH	MEAN	MEAN	SE	N	70	50	M	70	SE	N	70	SE	N
1000	878	878	878	3.20		1							3.20		1
3000	2868	2868	2868	4.96		1							4.96		1
5000	4802	4802	4802	5.13		1							5.13		1
1883	1883	1883	1883	5.49		1							5.49		1
OVERALL MEANS				4.88		4							4.88		4
ESTIMATED AT 10,000 PPMV				0.00									0.00		4
				95 % CONFIDENCE INTERVAL ( 0.04, 0.39 )											

Figure 5-23

ENVIRONMENT RESPONSE VS CONCENTRATION

BUTADIENE, 1,3

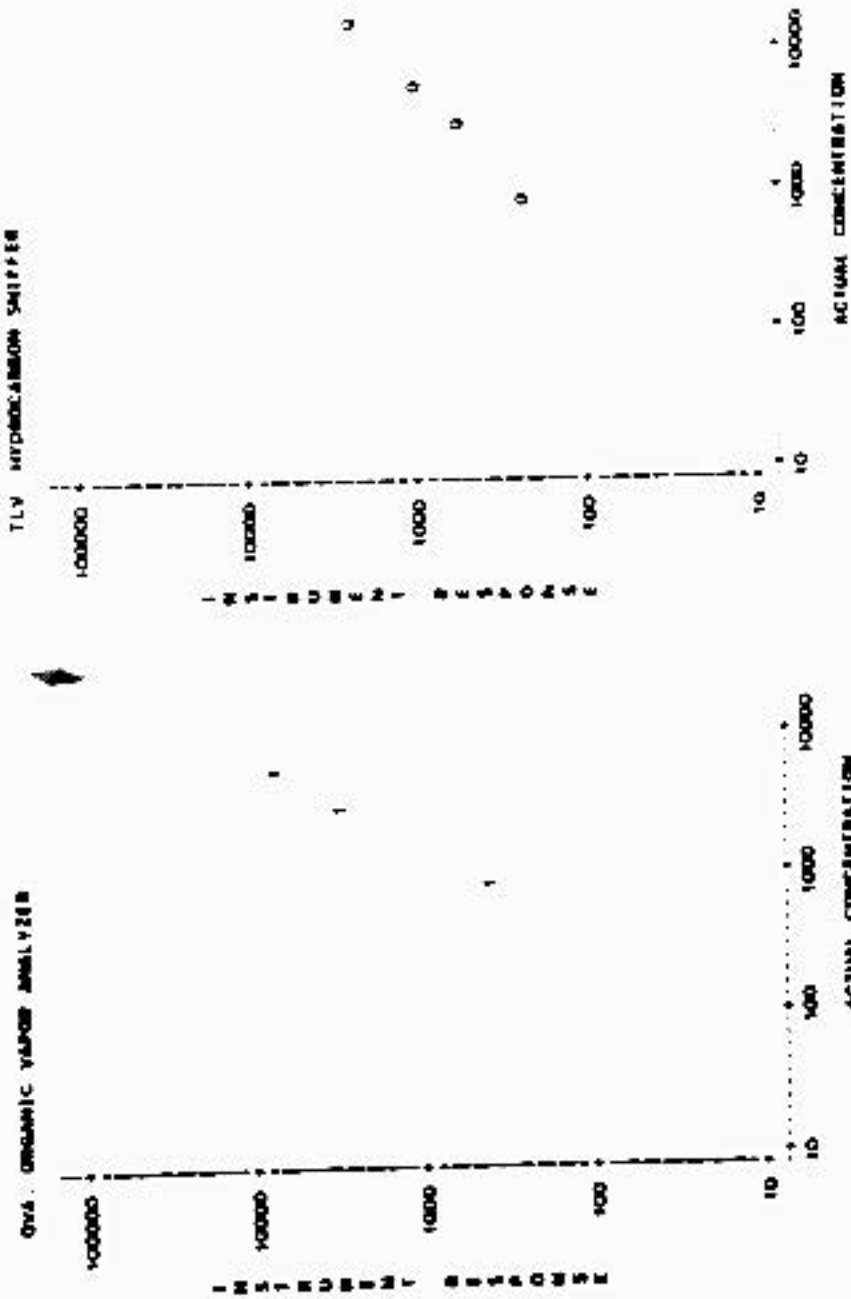

NOTE: 2 ml/min flow

TABLE 5-24

RESPONSE FACTOR SUMMARY

BUTANE, M.

OVA INSTRUMENTS		R E S P O N S E F A C T O R S											
NOMINAL PPM	ACTUAL PPM		OVERALL					OVA METERS					
	LOW	HIGH	MEAN	SE	M	1000 SE	M	2000 SE	M	2100 SE	M	1013 SE	M
1000	964	964	1.02	0.06	2	0.87	1	1.06	1				
4000	4043	4181	4.112	0.81	0.01	4	0.80	0.02	2	0.83	0.02	2	
5000	3988	5026	4480	0.88	0.00	4	0.48	0.02	2	0.48	0.02	2	
8000	8018	8018	8018										
1113	1113	1113	1113										
OVERALL MEANS			0.84	0.00	10	0.82	0.09	5	0.84	0.11	5		
ESTIMATED AT 10,000 PPM			0.38										
95% CONFIDENCE INTERVAL (0.34 0.88)													


112

TIA INSTRUMENTS		R E S P O N S E F A C T O R S											
NOMINAL PPM	ACTUAL PPM		OVERALL					TIA METERS					
	LOW	HIGH	MEAN	SE	M	76 SE	M	76 SE	M	76 SE	M	70 SE	M
1000	964	964	0.47		1							0.47	1
4000	4043	4181	4.112	0.84	2							0.64	0.01
5000	3988	5026	4480	0.88	2							0.88	0.04
8000	8018	8018	8018	0.82	1							0.82	1
1113	1113	1113	1113	0.87	1							0.87	1
OVERALL MEANS			0.80		1							0.80	0.03
ESTIMATED AT 10,000 PPM			0.88									0.81	0.15
95% CONFIDENCE INTERVAL													

Figure 5-24

INSTRUMENT RESPONSE VS CONCENTRATION

BUTANE IN

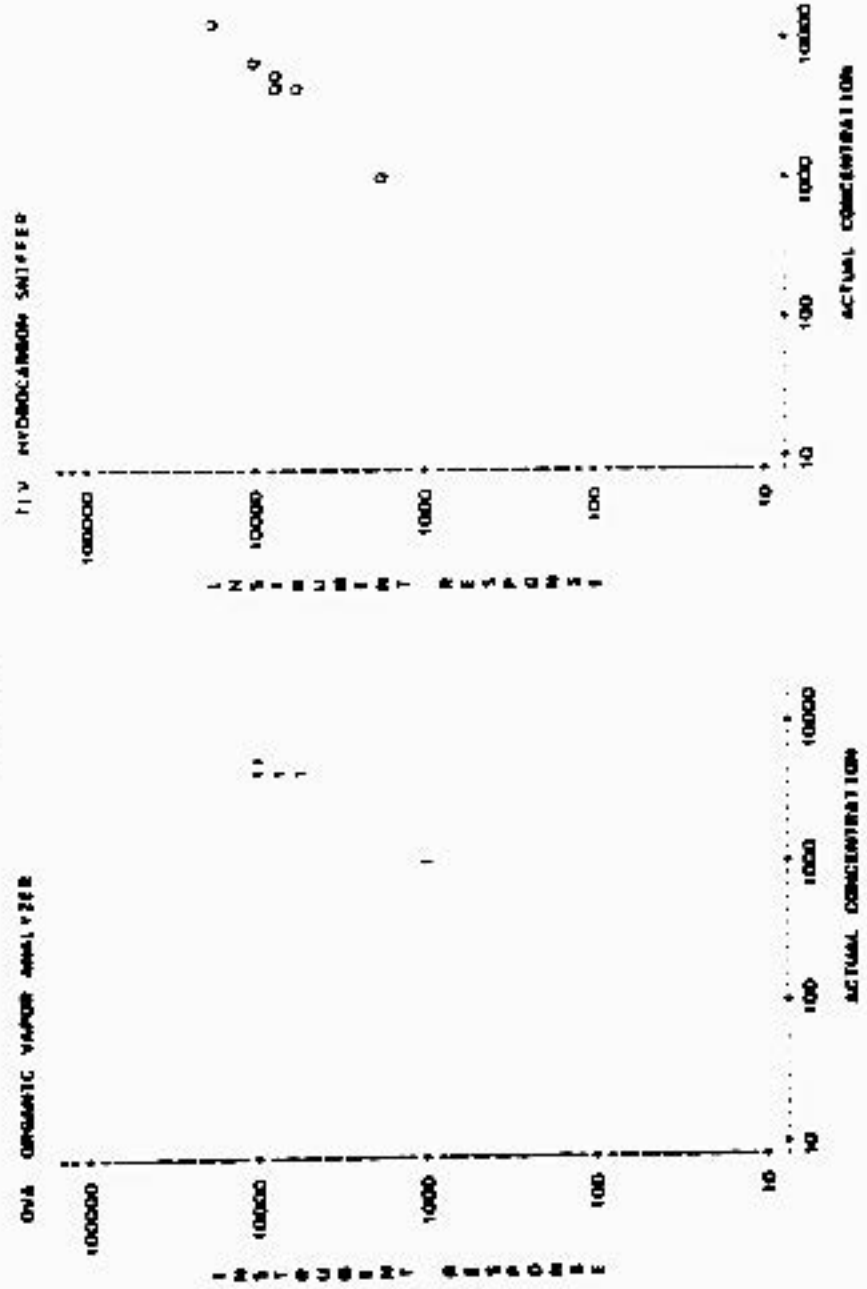

NOTE 8 OBS MEDIUM

NOTE 1 OBS HIDDEN

TABLE 5-25

RESPONSE FACTOR SUMMARY

BUTANED. N

DVB INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			P R E S P O N S E F A C T O R S								
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2254	SE	N	2108	SE	N
200	178	178	178	1.77		1							1.77		1
1500	1822	1822	1822	2.00		1							2.00		1
8000	1864	1864	1864	1.38		1							1.38		1
	OVERALL MEANS			1.71		3							1.71		3

ESTIMATED AT 10,000 PPMV 1.42

95 % CONFIDENCE INTERVAL 1.088 - 3.133

TLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			R E S P O N S E F A C T O R S								
	LOW	HIGH	MEAN	MEAN	SE	N	76	SE	N	76	SE	N	76	SE	N
200	178	178	178	0.84		1							0.84		1
1800	1822	1822	1822	2.03		1							2.03		1
8000	1864	1864	1864	2.23		1							2.23		1
	OVERALL MEANS			1.72		3							1.72		3

ESTIMATED AT 10,000 PPMV 2.80

95 % CONFIDENCE INTERVAL 1.148 - 5.273

Figure 3-25

INSTRUMENT RESPONSE VS CONCENTRATION

BUTANEA . N

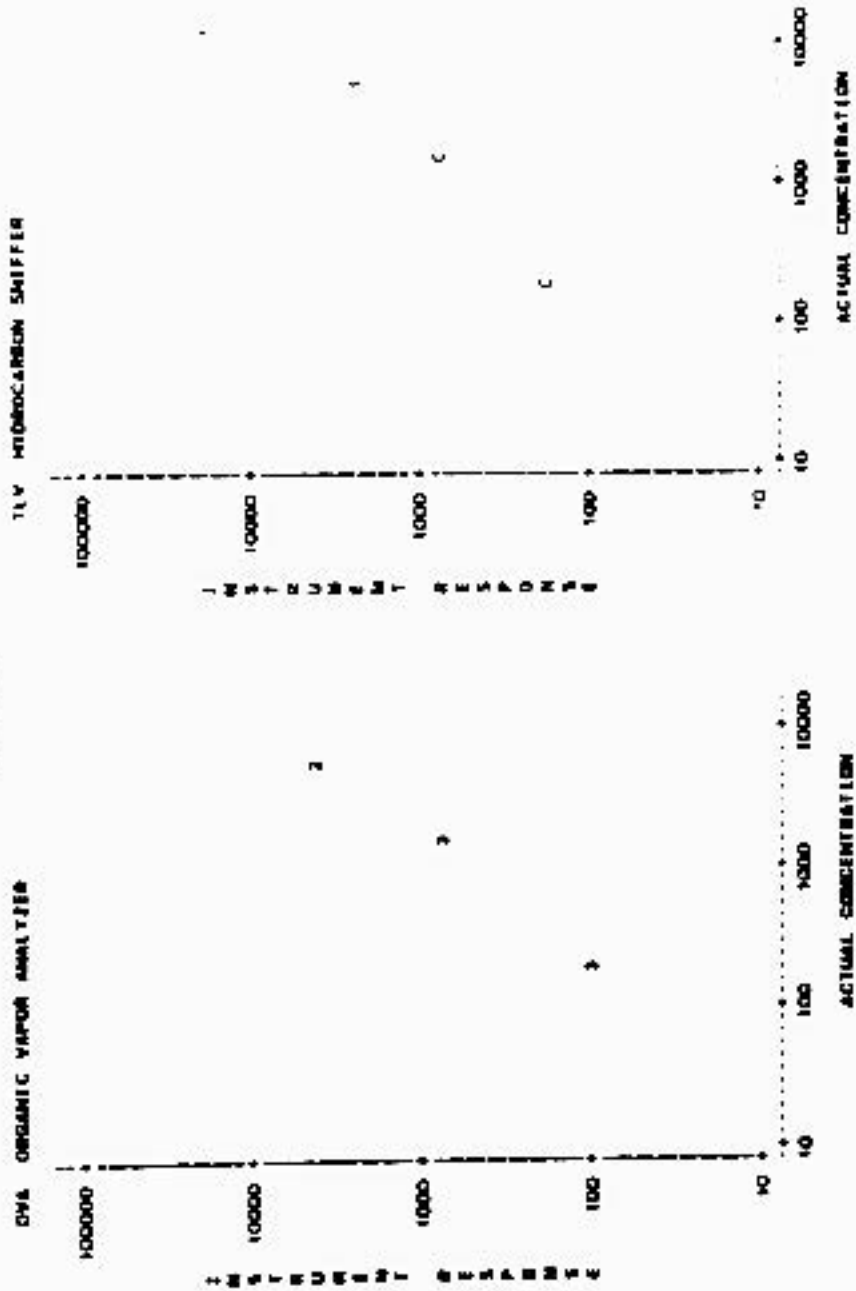




TABLE 3-26

BYPOINT FACILITY SUMMARY

BUTANONE, SEC

OVA INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVAL METERS																
	LOW	HIGH	MEAN	MEAN	SE	M	N	1000	SE	N	2794	SE	N	2059	SE	N	1803	SE	N	
200	230	230	230	2.23	0.08	2	2	2.17	1	2.27	1									
1000	1432	1432	1432	1.34	0.03	2	2	1.31	1	1.37	1									
5000	9968	9968	9968	0.81	0.04	2	2	0.77	1	0.85	1									
8000	7984	7984	7984																	
OVERALL MEANS				1.48	0.04	6	6	1.41	0.41	2	1	1.60	0.42	3						

ESTIMATED AT 10,000 PPMV 0.70

85% COMPLIANCE INTERVAL 1.0 63 0.781

TLV INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			TLV METERS																
	LOW	HIGH	MEAN	MEAN	SE	M	N	71	SE	N	10	SE	N	28	SE	N	70	SE	N	
200	230	230	230	1.21	0.27	2	2	1.03	1	1.08	1									
1000	1432	1432	1432	1.38	0.20	2	2	1.58	1	1.18	1									
5000	9968	9968	9968	1.47	0.20	2	2	1.82	1	1.22	1									
8000	7984	7984	7984	1.16	0.11	2	2	1.27	1	1.08	1									
OVERALL MEANS				1.31	0.02	8	8	1.40	0.08	4	1	1.12	0.04	4						


ESTIMATED AT 10,000 PPMV 1.28

85% COMPLIANCE INTERVAL 1.1 00 1.573

Figure 5-26

INSTRUMENT RESPONSE VS CONCENTRATION

BUTANOL, 5% C

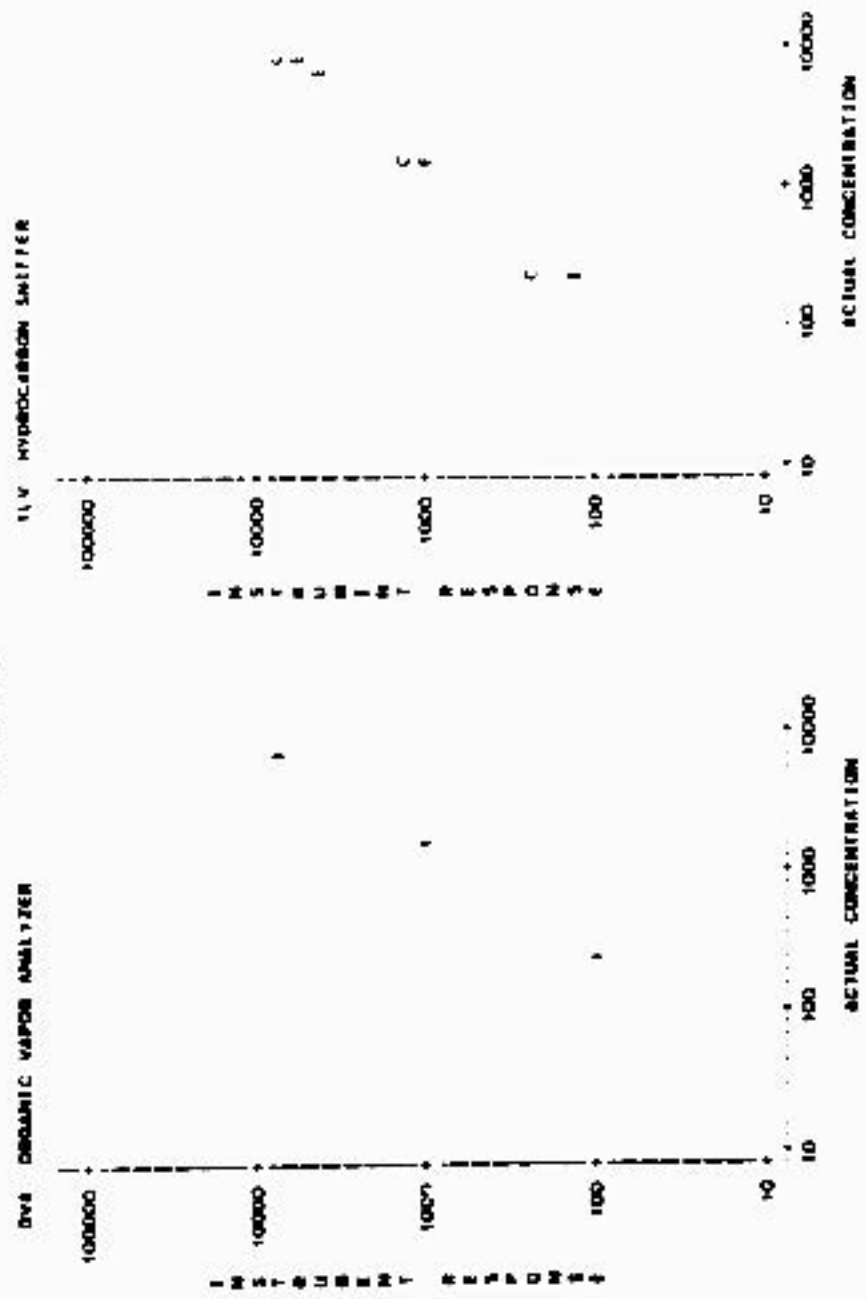

NOTE: 3 OBS HIDDEN

NOTE: 1 OBS HIDDEN

TABLE 5-27  
RESPONSE FACTOR SUMMARY

JANU. 1981

R E S P O N S E F A C T O R S

OVS INSTRUMENTS	ACTUAL PPMV			OVERALL			OVS METERS											
	LOW	HIGH	MEAN	MEAN	SE	N	1080	SE	N	2884	SE	N	1813	SE	N			
NOMINAL PPMV																		
200	229	229	229	1.20	0.11	2							1.30		1			
1800	1871	1871	1871	0.98	0.10	2							1.08		1			
4000	4087	4087	4087	0.80	0.08	2							0.88		1			
8000	8246	8246	8246	0.50	0.05	2							0.54		1			
8000	7718	7718	7718															
OVERALL MEANS	0.88	0.01	8										0.84	0.18	2	0.90	0.28	3

ESTIMATED AT 10,000 PPMV 0.64      99 % CONFIDENCE INTERVAL 1.0 26. 0.141

R E S P O N S E F A C T O R S

OVS INSTRUMENTS	ACTUAL PPMV			OVERALL			OVS METERS									
	LOW	HIGH	MEAN	MEAN	SE	N	78	SE	N	78	SE	N	36	SE	N	
NOMINAL PPMV																
200	229	229	229	2.18		1							2.18		1	
1800	1871	1871	1871	2.88		1							2.88		1	
4000	4087	4087	4087	1.71		1							1.71		1	
8000	8246	8246	8246	2.40		1							2.40		1	
8000	7718	7718	7718	2.27		1							2.27		1	
OVERALL MEANS	2.30		5	2.30	0.18	5							2.30	0.18	5	

ESTIMATED AT 10,000 PPMV 2.19      95 % CONFIDENCE INTERVAL 1.1 94. 2.111

Figure S-27

INSTRUMENT RESPONSE VS CONCENTRATION

AUGUST, 1981

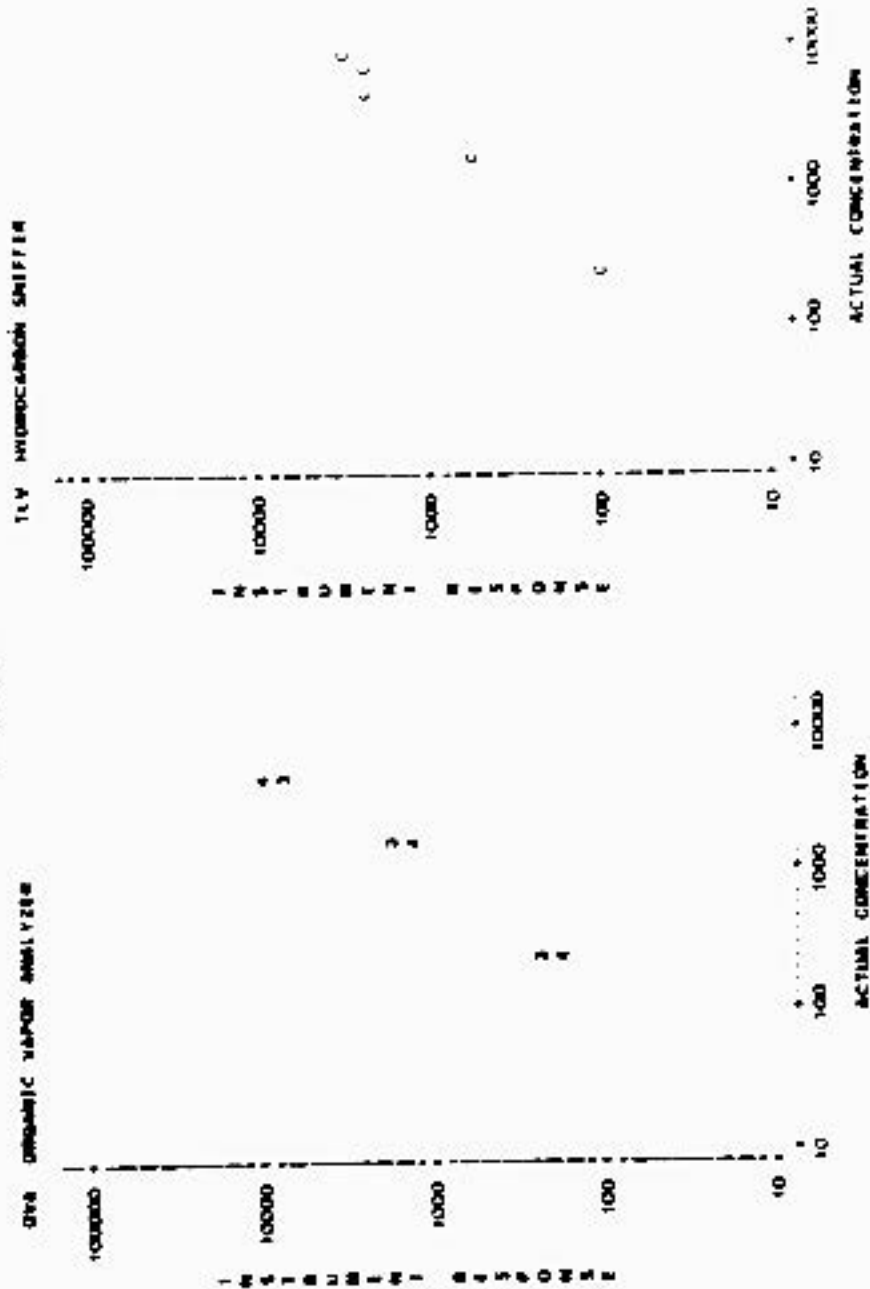


TABLE 1-28

RESPONSE FACTOR SUMMARY

ROUTE 1

OVA INSTRUMENTS

NOMINAL PPM	ACTUAL PPM			OVERALL			RESPONSE FACTORS										
	LOW	HIGH	MEAN	MEAN	SE	N	1000	500	250	125	62.5	31.25	15.625	7.8125	3.90625	1.953125	0.9765625
1000	888	888	888	0.78	0.07	2	0.80										
4000	4001	4001	4001	0.81	0.06	2	0.86										
9000	9084	9084	9084	0.99	0.02	2	0.92										
40000	8881	8881	8881														
12E3	12E3	12E3	12E3														

OVERALL MEANS 0.85 0.00 0.83 0.08 0.86 0.05 0

ESTIMATED AT 10,000 PPM 0.91

95% CONFIDENCE INTERVAL (0.85, 0.88)

FLV INSTRUMENTS

NOMINAL PPM	ACTUAL PPM			OVERALL			RESPONSE FACTORS										
	LOW	HIGH	MEAN	MEAN	SE	N	TE	SE	TC	SE	TM	SE	TH	SE	TL	SE	TR
1000	888	888	888	1.08		1									1.08		
4000	4001	4001	4001	1.84		1									1.84		
9000	9084	9084	9084	2.30		1									2.30		
40000	8881	8881	8881	2.43		1									2.43		
12E3	12E3	12E3	12E3	2.33		1									2.33		

OVERALL MEANS 2.22

ESTIMATED AT 10,000 PPM 2.97

95% CONFIDENCE INTERVAL 1.73, 3.24

Figure 5-28

Instrumental Response vs Concentration

Butene, 1-

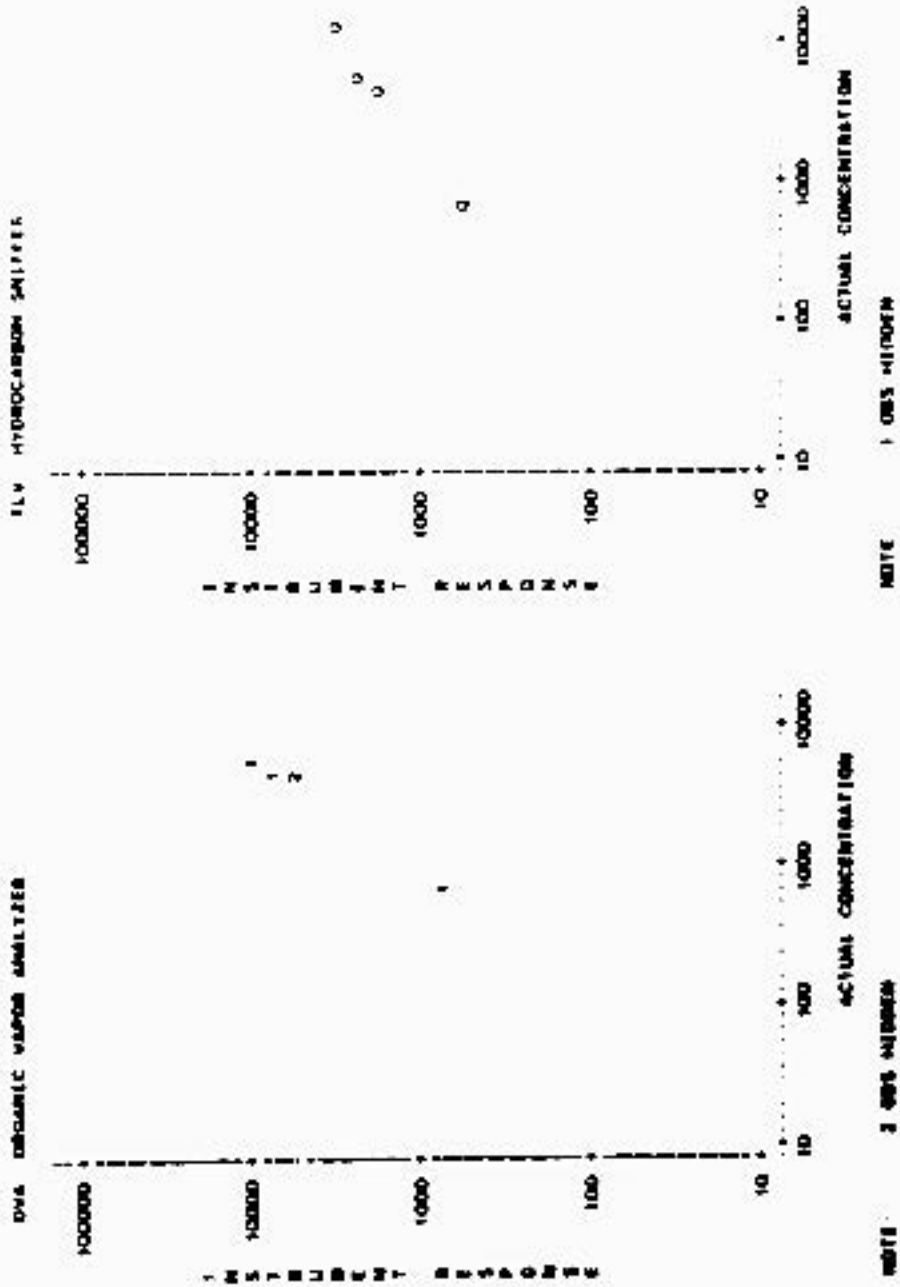


TABLE 5-24

RESPONSE ACTION SUMMARY

ETHYL ACETATE

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE PERFORMANCE												
	LOW	HIGH	MEAN	SE	SE	M	N	2254	SE	M	2150	SE	M	1800	SE	M	
200	217	217	1.36	0.01	2	1	36	1	1	36	1	1	36	1	1	36	1
1000	1002	1002	1.00	0.00	2	1	18	1	1	18	1	1	18	1	1	18	1
5000	5114	5114	0.51	0.00	2	1	63	1	1	63	1	1	63	1	1	63	1
10000	9208	9208															

OVERALL MEANS 1.02 0.00 4 1.11 0.22 2 13.89 0.22 2

ESTIMATED AT 10,000 PPMV 0.80

90% COMPLIANCE ESTIMATED 1.00 0.00 1.781

11V INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE PERFORMANCE												
	LOW	HIGH	MEAN	SE	SE	M	N	76	SE	M	100	SE	M	70	SE	M	
200	217	217	0.85		1												
1000	1002	1002	0.87		1												
5000	5114	5114	1.21		1												
10000	9208	9208	1.26		1												

OVERALL MEANS 1.00 0

ESTIMATED AT 10,000 PPMV 1.20


90% COMPLIANCE ESTIMATED 1.118 1.421



Figure 3-29

INSTRUMENT RESPONSE VS CONCENTRATION

BUTYL ACRYLATE.

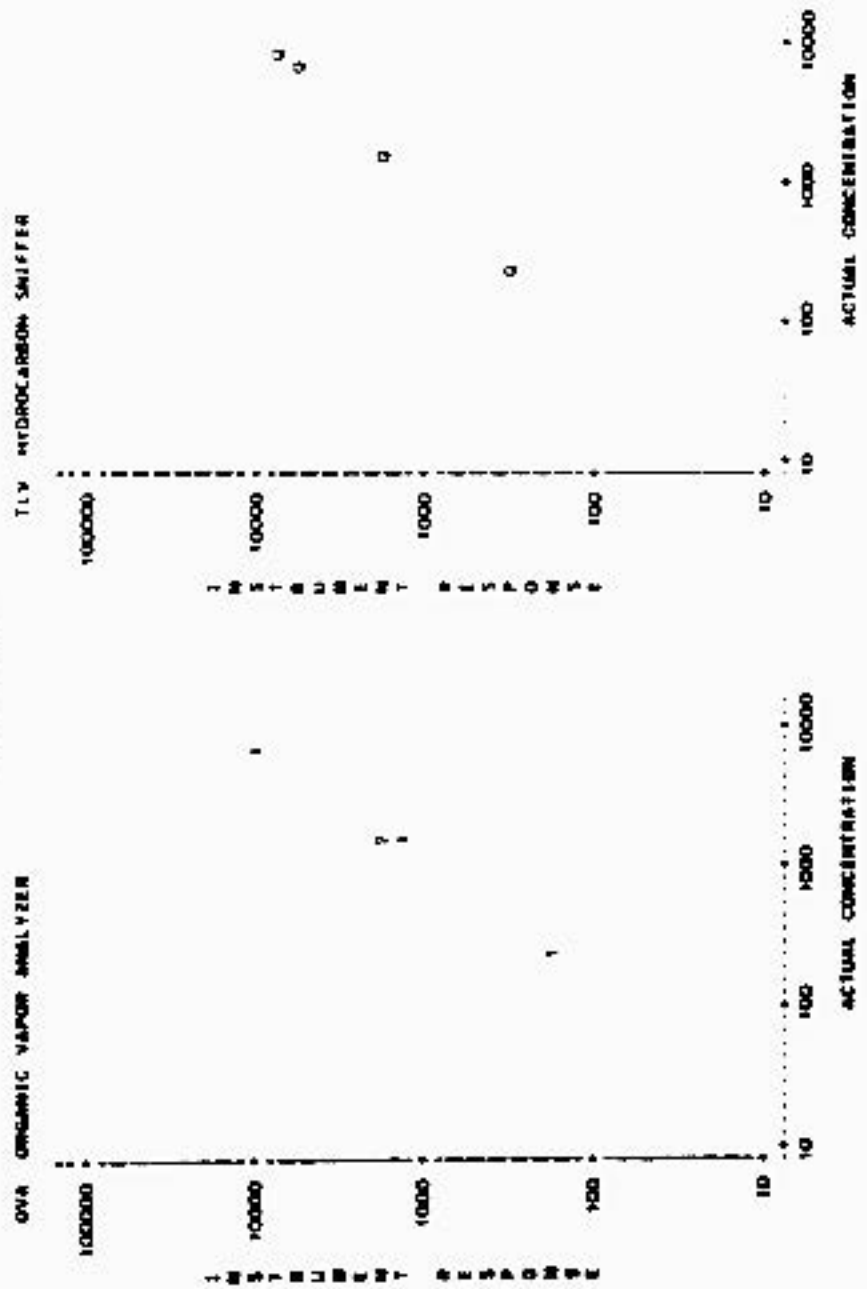

NOTE: 2.0% MICROM

TABLE 5-30

RESPONSE FACTOR SUMMARY

BUTYL ACRYLATE, W

DVA INSTRUMENTS

R E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METERS												
	LOW	HIGH	MEAN	MEAN	SD	SE	1000	50	1	2284	SE	N	2180	SE	N	1011	SE	N	
200	208	208	208	1.84	0.08	2	1.88			1	1.82	1							
1900	1827	1827	1827	1.08	0.04	2	1.02			1	1.06	1							
4700	4888	4888	4888	0.74	0.00	2	0.74			1	0.74	1							
OVERALL MEANS			1.14	0.01	6	1.07	0.21	3	1.18	0.26	3								
ESTIMATED AT 10,000 PPMV			0.88																
			95% CONFIDENCE INTERVAL 1.096 0.941																

FIV INSTRUMENTS

R E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV			OVERALL			FIV METERS												
	LOW	HIGH	MEAN	MEAN	SE	N	71	51	1	71	SE	N	70	SE	N	70	SE	N	
200	208	208	208	0.78		1													
1900	1827	1827	1827	1.04		1													
4700	4888	4888	4888	1.88		1													
OVERALL MEANS			1.23																
ESTIMATED AT 10,000 PPMV			1.08																
			95% CONFIDENCE INTERVAL 1.081 0.871																


Figure 5-30

INSTRUMENT RESPONSE VS CONCENTRATION

BUTYL ACRYLATE, N.

Ova ORGANIC VAPOR ANALYZER

ELV HYDROCARBON SAMPLER

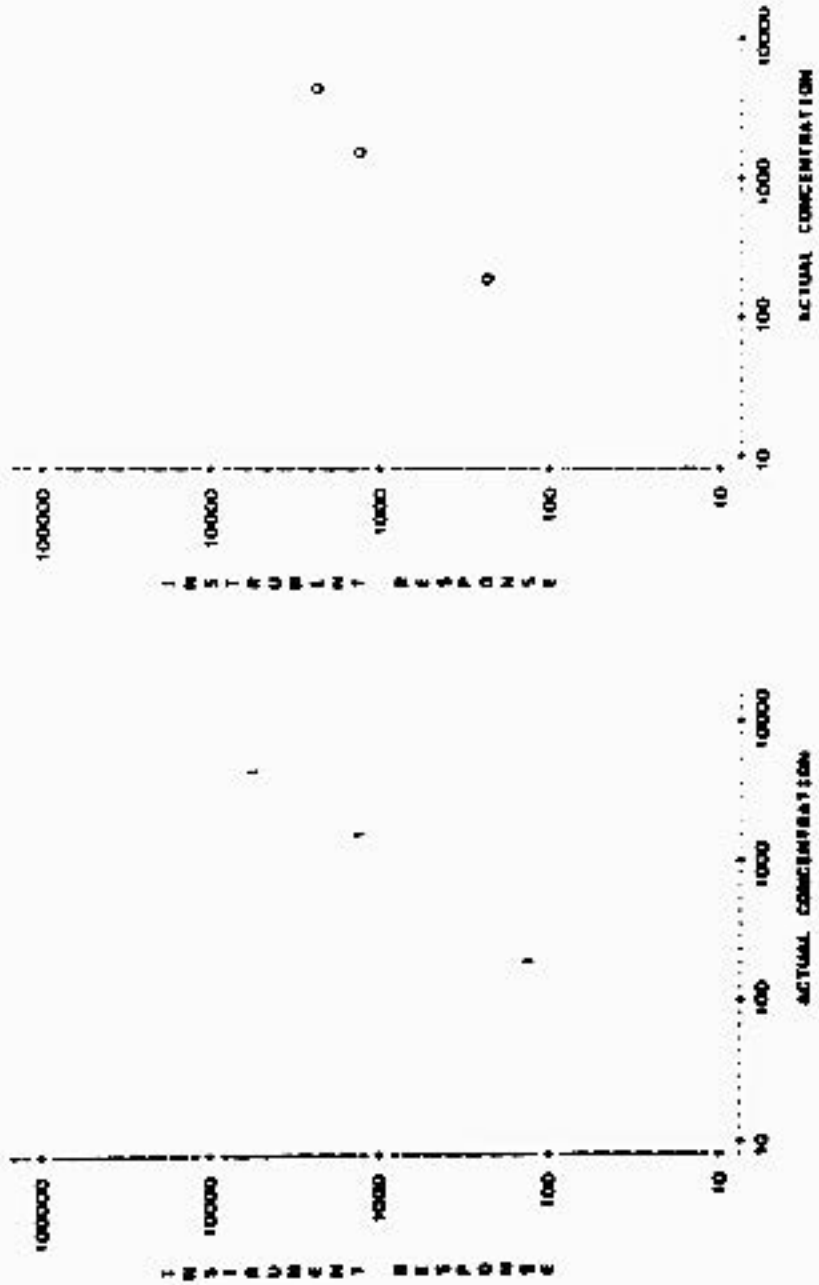

NOTE: 3 CBS HIGHEN

TABLE 5-11

RESPONSE FACTOR SUMMARY

ALIVE RETURN

OVA INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OVA METERS								
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2254	SE	N	1813	SE	N
200	201	201	201	2.87		1					2.97				1
1500	1548	1548	1548	3.17		1					3.13				1
8000	1083	1083	1083	2.85		1					2.99				1
			OVERALL MEANS	2.91		3					2.91				3

ESTIMATED AT 10,000 PPMV 3 TO 99 % CONFIDENCE INTERVAL 1.19, 3.731

TV INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			TV METERS								
	LOW	HIGH	MEAN	MEAN	SE	N	71	SE	N	71	SE	N	71	SE	N
200	201	201	201	1.18		1					1.18				1
1500	1548	1548	1548	2.29		1					2.29				1
8000	1083	1083	1083	2.44		1					2.48				1
			OVERALL MEANS	1.98		3					1.98				3

ESTIMATED AT 10,000 PPMV 2.69 95 % CONFIDENCE INTERVAL 1.42, 4.95

Figure 5-31  
 INSTRUMENT RESPONSE VS CONCENTRATION

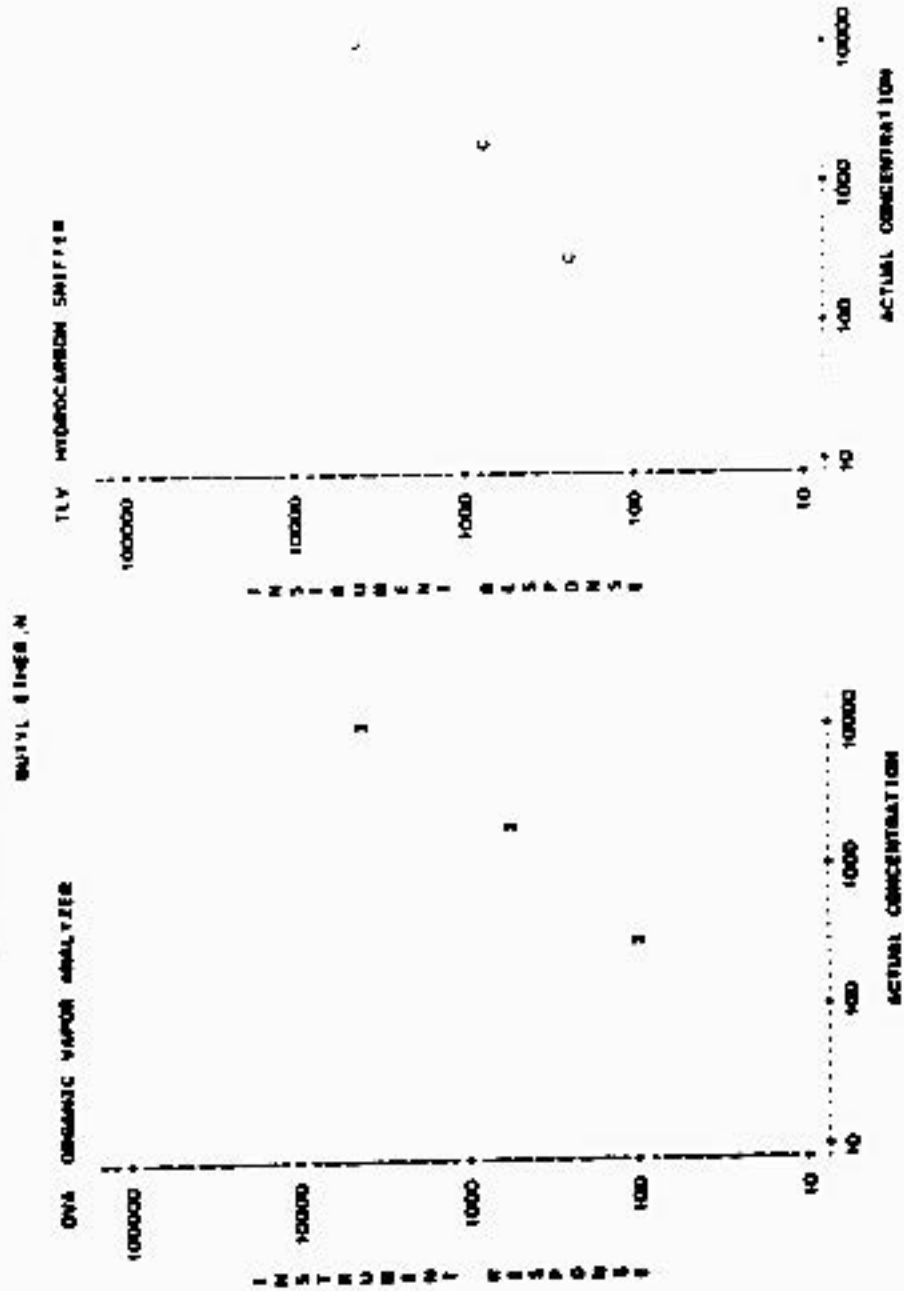


TABLE 5-12

Background Factor Summary

BUTYL ETHER, SFC

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		B E S P D M S E F A C T O R S												
	LOW	HIGH	MEAN	SE	1000	SE	M	2204	SE	N	3109	SE	N	1813	SE	M	
200	208	208	0.73	1													
1800	1801	1801	0.88	1													
3000	3080	3080	0.33	0.01	2												
4000	4208	4208															
8000	8380	8380															
8000	7728	7728															
OVERALL MEANS			0.61	0.02	4	O V A M E T E R S											

ESTIMATED AT 10,000 PPMV 0.28

95% COMPLIANCE INTERVAL 1.01 U 801

ILV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		B E S P D M S E F A C T O R S												
	LOW	HIGH	MEAN	SE	78	SE	M	70	SE	N	78	SE	N	70	SE	M	
200	208	208	0.43	1													
1800	1801	1801	0.84	1													
3000	3080	3080	1.22	1													
4000	4208	4208	1.16	1													
8000	8380	8380	1.35	1													
8000	7728	7728	0.82	1													
OVERALL MEANS			1.03	0.11	6	I L V M E T E R S											

ESTIMATED AT 10,000 PPMV 1.12

95% COMPLIANCE INTERVAL 1.078 1.841

Figure 5-32

INSTRUMENT RESPONSE VS CONCENTRATION

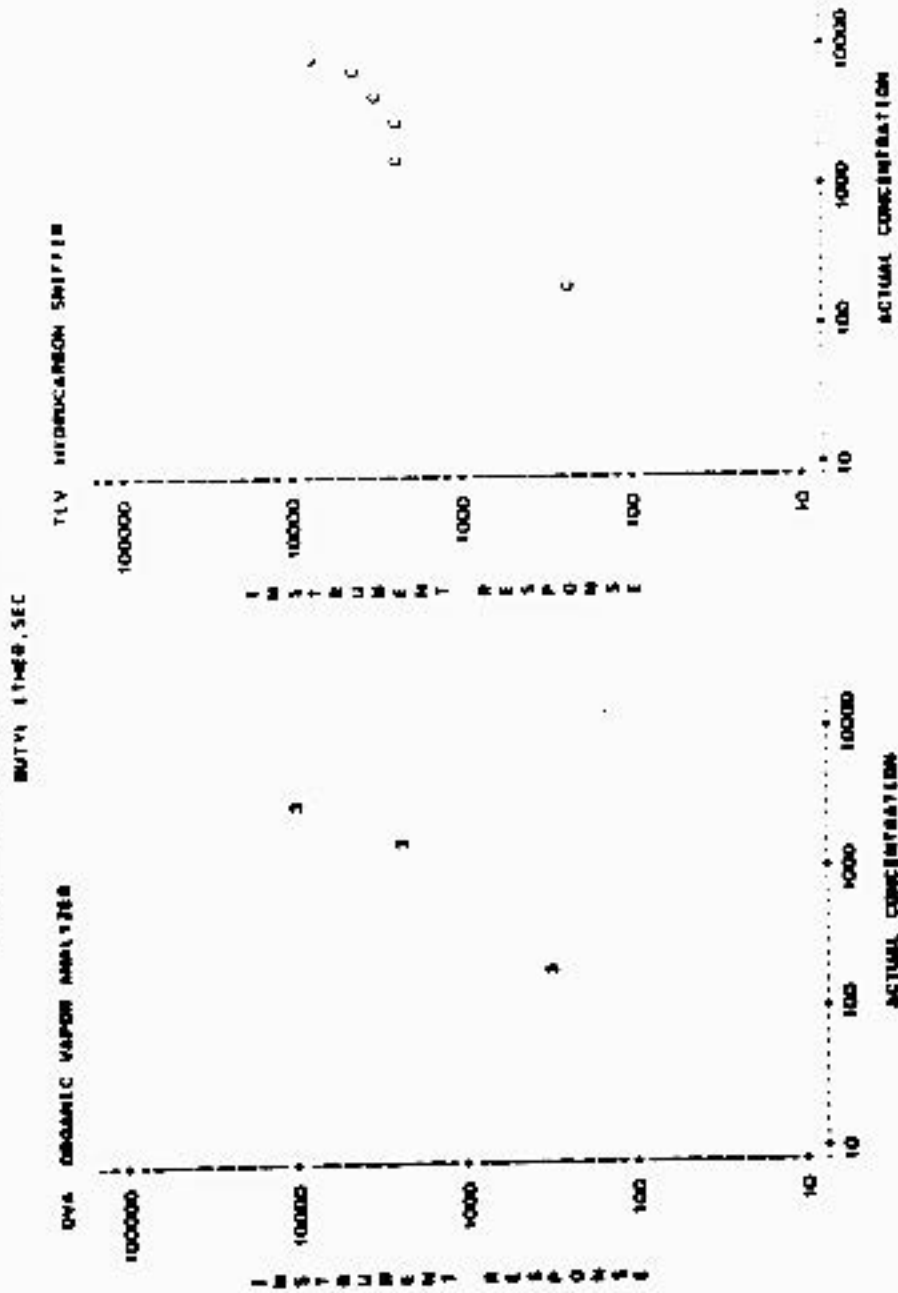




TABLE 5-11

RESPONSE FACTOR SUMMARY

INDIVIDUAL INSTRUMENTS

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS								
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2254	SE	N	3150	SE	N
200	217	217	217	1.98	0.08	2	1.71		1	1.60					
1500	1506	1506	1506	1.37	0.00	2	1.37		1	1.37					
4000	4118	4118	4118	0.84	0.02	2	0.82		1	0.88					
8000	7892	7892	7892												
OVERALL MEANS			1.22	0.00	8	1.74	0.27	3	1.31	0.28	3				

ESTIMATED AT 10,000 PPMV 0.83

95% CONFIDENCE INTERVAL (0.43 0.92)

SLV INSTRUMENTS

SLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS								
	LOW	HIGH	MEAN	MEAN	SE	N	75	SE	N	30	SE	N	70	SE	N
200	217	217	217	1.81		1							1.61		1
1500	1506	1506	1506	1.52		1							1.52		1
4000	4118	4118	4118	1.66		1							1.66		1
8000	7892	7892	7892	2.22		1							2.22		1
OVERALL MEANS			1.73		4								1.73		4


ESTIMATED AT 10,000 PPMV 1.91

95% CONFIDENCE INTERVAL (1.38 2.60)

Figure 5-11

INSTRUMENT RESPONSE VS CONCENTRATION

BUTYLALDEHYDE, N.

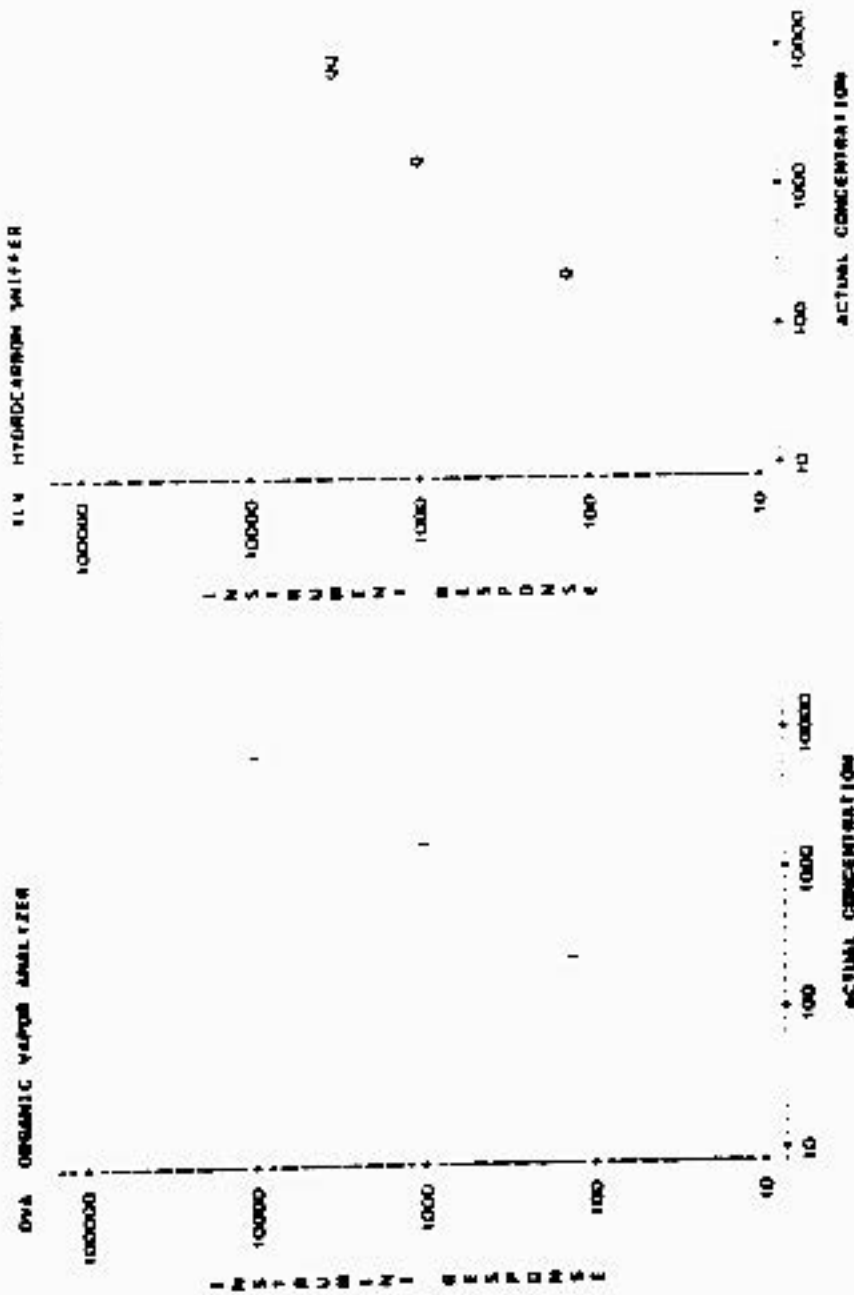

NOTE: 3 MB MICROB

TABLE 5-34

RESPONSE FACTOR SUMMARY

MULTILAMINE .516				RESPONSE FACTORS															
OVA INSTRUMENTS				ACTUAL PPMV					OVERALL					OVA METERS					
NOMINAL PPMV	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	7204	SE	M	2199	SE	N	1813	SE	N	
200	189	198	196	1	10	0.02	2	1	12	1	1	07	1	1	1	1	1	1	
1000	1814	1814	1814	1	01	0.00	2	1	01	1	01	00	1	01	1	00	1	00	
8000	8448	8448	8448	0	85	0.00	2	0	85	1	00	00	1	00	00	00	1	00	
OVERALL MEANS				0.92	0.00	0	0.92	0.14	2	0.91	0.13	2							
ESTIMATED AT 10,000 PPMV				0.87															
95% CONFIDENCE INTERVAL				1.0	0.53	0.84													
TLV INSTRUMENTS				ACTUAL PPMV					OVERALL					TLV METERS					
NOMINAL PPMV	LOW	HIGH	MEAN	MEAN	SE	N	21 <th>SE</th> <th>N</th> <th>70 <th>SE</th> <th>M</th> <th>70 <th>SE</th> <th>N</th> <th>10 <th>SE</th> <th>N</th> </th></th></th>	SE	N	70 <th>SE</th> <th>M</th> <th>70 <th>SE</th> <th>N</th> <th>10 <th>SE</th> <th>N</th> </th></th>	SE	M	70 <th>SE</th> <th>N</th> <th>10 <th>SE</th> <th>N</th> </th>	SE	N	10 <th>SE</th> <th>N</th>	SE	N	
200	196	189	199	1	08	1										1	08	1	
1000	1814	1814	1814	1	25	1										1	25	1	
8000	8448	8448	8448	1	81	1										1	81	1	
OVERALL MEANS				1.27		2											1.21	0.13	2
ESTIMATED AT 10,000 PPMV				1.50													1.26	0.17	2
95% CONFIDENCE INTERVAL				1.1	0.26	1.78													


Figure 5-34

INSTRUMENT RESPONSE VS CONCENTRATION

MULTILAMINE .516

Figure 5-34

INSTRUMENT RESPONSE VS CONCENTRATION

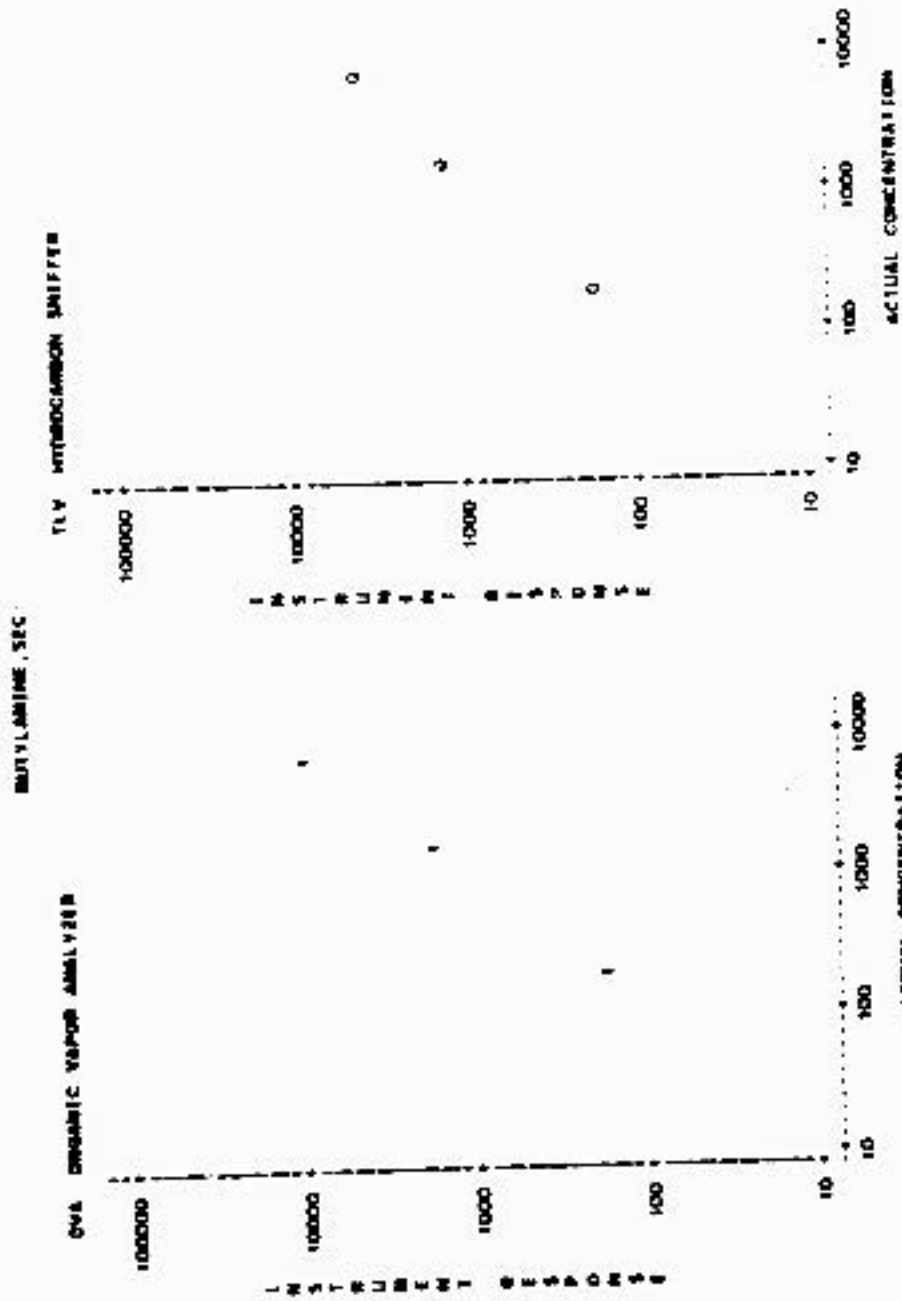

NOTE: 3 OBS MEASUREMENTS

TABLE 5-15

RESPONSE FACTOR SUMMARY

MULTIPLYING FACT

OVER INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS								
	LOW	HIGH	MEAN	MEAN	SE	N	100%	SE	N	25%	SE	N	75%	SE	N
200	224	224	224	1.18	0.03	2	1.21		1	1.16		1			1
1000	1648	1648	1648	0.87	0.08	2	0.82		1	0.82		1			1
5000	8128	8128	8128	0.82	0.03	2	0.82		1	0.82		1			1
8000	8042	8042	8042												

OVERALL MEANS 0.88 0.03 2 0.88 0.17 2 0.80 0.16 2

ESTIMATED AT 10,000 PPMV 0.88 95% CONFIDENCE INTERVAL 1.0 0.7 J 861


FLU INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS								
	LOW	HIGH	MEAN	MEAN	SE	N	75%	SE	N	75%	SE	N	75%	SE	N
200	224	224	224	1.10		1			1	1.10		1			1
1000	1648	1648	1648	1.04		1			1	1.04		1			1
5000	8128	8128	8128	1.72		1			1	1.72		1			1
8000	8042	8042	8042	1.67		1			1	1.67		1			1

OVERALL MEANS 1.52 1.52 4

ESTIMATED AT 10,000 PPMV 1.50 95% CONFIDENCE INTERVAL 1.1 1.9 2 119

Figure S-35  
 INSTRUMENT RESPONSE VS CONCENTRATION  
 BUTYLARINE TEST.

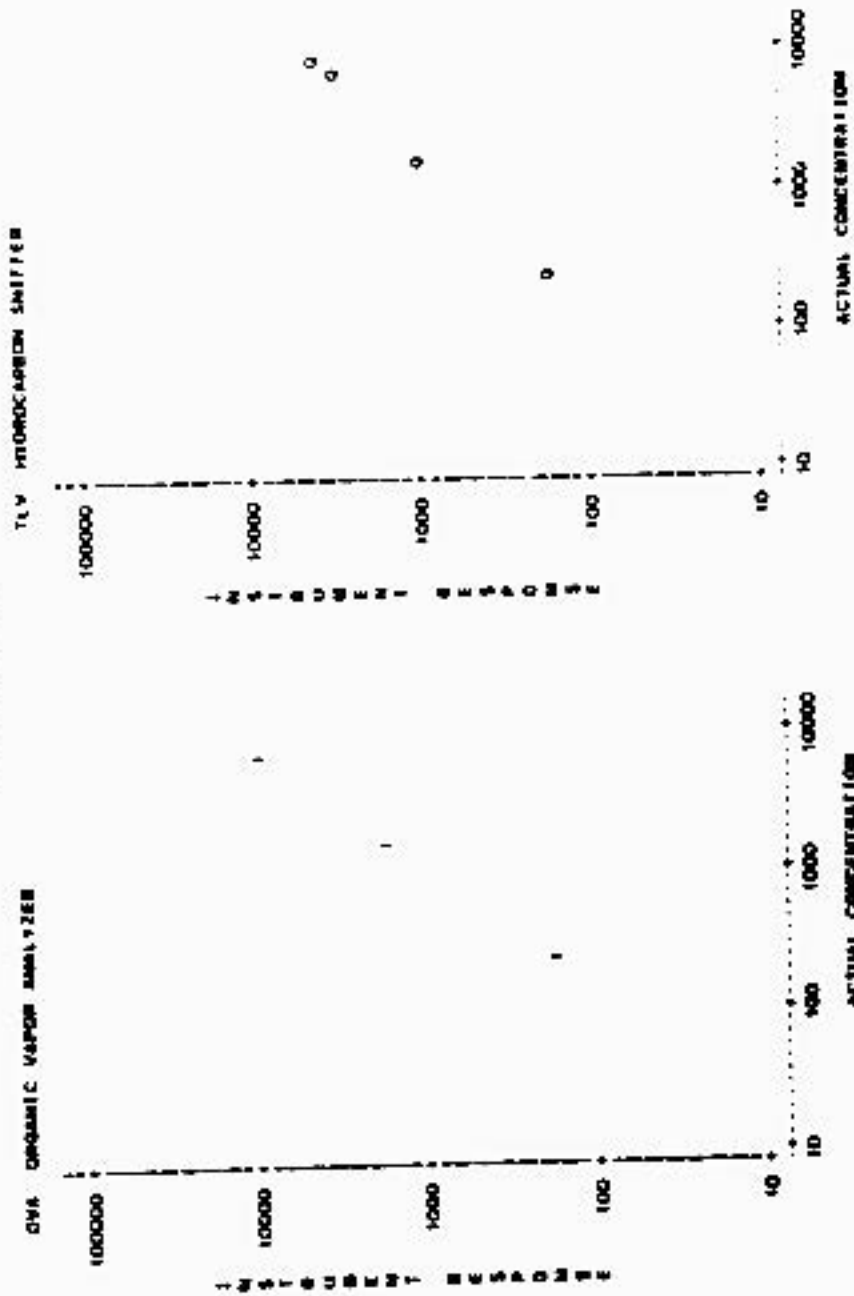

NOTE: 3 GBS NIBBIN

TABLE 5-36

RESPONSE FACTOR SUMMARY

BUYLBRINFORM TEST

OVER INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL					DVA METERS						
	LOW	HIGH	MEAN	MEAN	SE	N	7E	5E	N	7C	SE	N	7D	SE	N
200	196	196	196	0.83	0.11	2	0.72		1	0.84		1			
1800	1800	1800	1800	0.88	0.06	2	0.76		1	0.81		1			
8000	8033	8033	8033	1.39	0.00	2	1.29		1	1.29		1			
OVERALL MEANS			1.02	0.01	6	0.97	0.21	3	1.08	0.19	3				

ESTIMATED AT 10,000 PPMV 1.27 95% CONFIDENCE INTERVAL (0.94, 1.73)

FLV INSTRUMENTS

RESPONSE FACTORS


NOMINAL PPMV	ACTUAL PPMV			OVERALL					FLV METERS						
	LOW	HIGH	MEAN	MEAN	SE	N	7E	5E	N	7C	SE	N	7D	SE	N
200	196	196	196	1.38	0.04	2	1.31		1	0.80		1			
1800	1800	1800	1800	2.45	2.35	2	6.80		1	2.11		1			
8000	8033	8033	8033	6.85	6.48	2	16.32		1	3.37		1			
OVERALL MEANS			5.22	0.87	6	8.35	4.23	3	2.09	0.74	3				

ESTIMATED AT 10,000 PPMV 6.42 95% CONFIDENCE INTERVAL (1.87, 22.87)

Figure 5-36

INSTRUMENT RESPONSE VS CONCENTRATION

STYLBENZENE, (PPM)

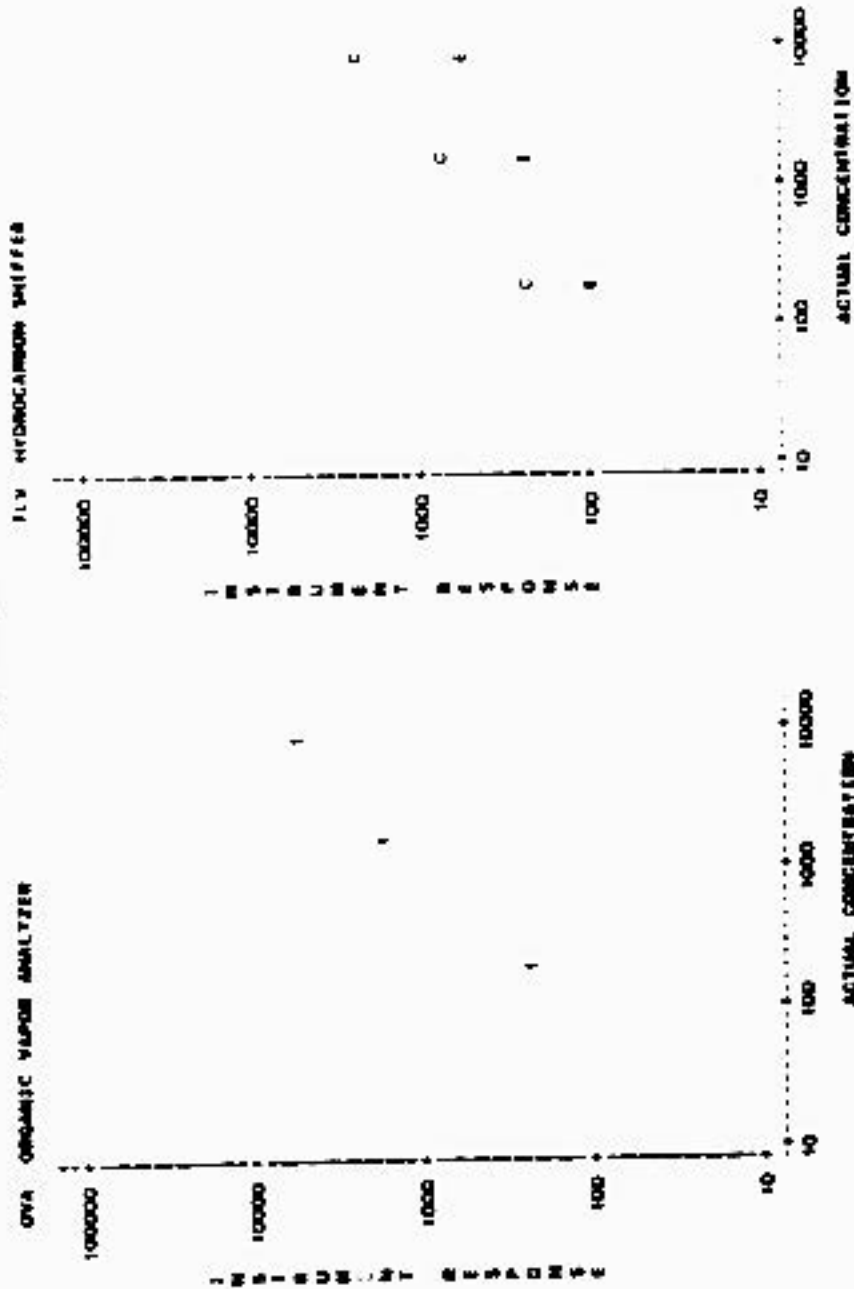

NOTE: 3 CM'S HEADS



TABLE 5-17

RESPONSE FACTOR SUMMARY

BUTYRALDENTONE M-

DVA INSTRUMENTS		R E S P O N S E F A C T O R S											
NOMINAL PPMV	ACTUAL PPMV		OVERALL					DVA ERRORS					
	LOW	HIGH	MEAN	SE	N	1000 SE	M	2004 SE	M	7100 SE	N	1012 SE	N
200	242	242	2.06	0.14	2	2.82		2.80			1		
1800	1808	1808	2.87	0.08	2	2.82		2.72			1		
8000	8118	8118	1.37	0.02	2	1.38		1.29			1		
OVERALL MEANS			2.87	0.01	6	2.80	0.43	2	2.83	0.70	3		
ESTIMATED AT 10,000 PPMV			1.29	95 % CONFIDENCE INTERVAL ( 1.12   1.41 )									


TLV INSTRUMENTS

TLV INSTRUMENTS		R E S P O N S E F A C T O R S											
NOMINAL PPMV	ACTUAL PPMV		OVERALL					TLV ERRORS					
	LOW	HIGH	MEAN	SE	N	70 SE	M	70 SE	M	30 SE	N	70 SE	N
200	242	242	0.77		1							0.77	1
1800	1808	1808	1.28		1							1.28	1
8000	8118	8118	1.74		1							1.74	1
OVERALL MEANS			1.27		3							1.27	0.28
ESTIMATED AT 10,000 PPMV			1.88	95 % CONFIDENCE INTERVAL ( 1.40, 2.23 )									

Figure 5-37

INSTRUMENT RESPONSE VS CONCENTRATION

BUTYRALDEHYDE M.

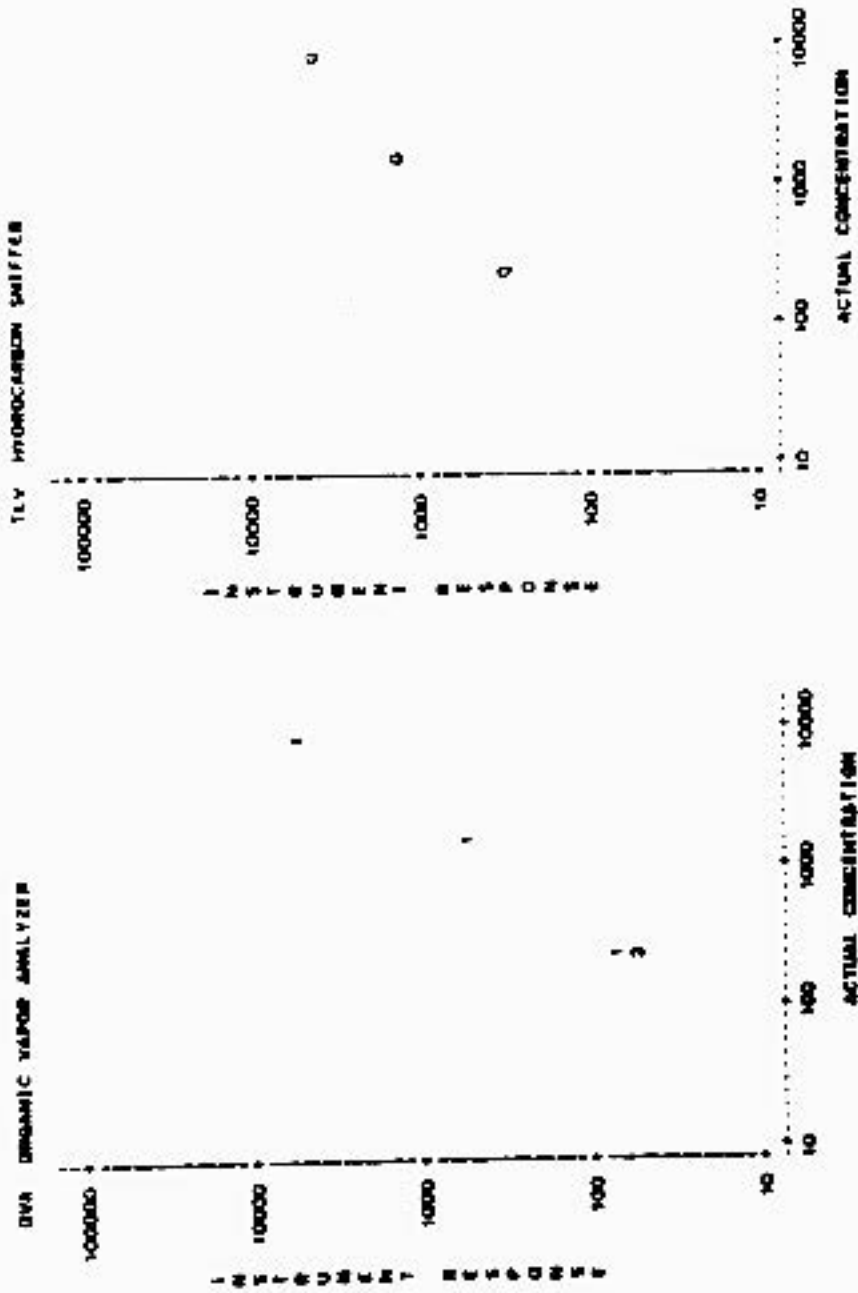

NOTE: 2 OBS NORMED

TABLE 5-18

RESPONSE FACTOR SUMMARY

MALVAC ACID

OVA INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS												
	LOW	HIGH	MEAN	MEAN	SE	N	1000	34	W	2254	5F	N	2158	5E	N	1813	5I	N	
200	208	208	208	2 04	0 17	2	2 82		1	2 20		1							
280	287	287	287	2 33	0 14	2	2 19		1	2 48		1							
800	800	800	800	2 19	0 28	2	1 81		1	2 57		1							
OVERALL MEANS			2 82	0 04	6	2 29	0 31	3	2 26	0 23	3								

ESTIMATED AT 10 000 PPMV 0 74

95 % CONFIDENCE INTERVAL ( 0 22 2 52)

TUV INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS											
	LOW	HIGH	MEAN	MEAN	SE	N	74	5E	N	7C	5E	N	7M	5E	N	7Q	5E	N
200	208	208	208	1 10		1										1 10		1
280	287	287	287	1 38		1										1 38		1
800	800	800	800	1 58		1										1 58		1
OVERALL MEANS			1 32		3											1 32		3

ESTIMATED AT 10 000 PPMV 4 08

95 % CONFIDENCE INTERVAL ( 1 39 6 78)

Figure 5-18

INSTRUMENT RESPONSE VS CONCENTRATION

MUTYRIC ACID

OVA ORGANIC VAPOR ANALYZER

TLV HYDROCARBON SNIFFER

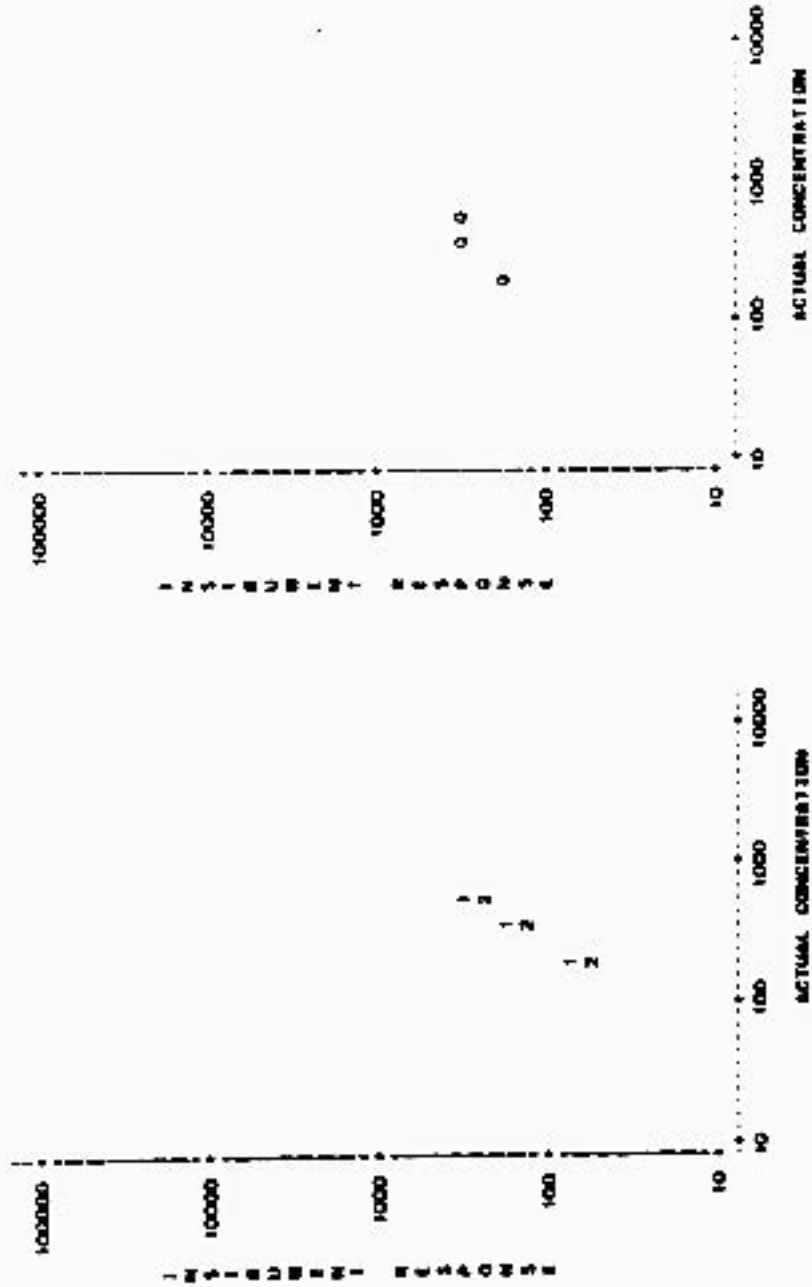


TABLE 5-19

RESPONSE FACTOR SUMMARY

MULTIMETER

DIV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			P P S P O N S E F A C T O R S											
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2254	SE	N	7189	SE	N			
200	228	236	230	0.89	0.17	2					0.22	1	1.07	1				
1000	1481	1491	1481	0.79	0.04	2					0.78	1	0.82	1				
5000	4711	4711	4711	0.49	0.01	2					0.49	1	0.50	1				
8000	7331	7331	7331															
				OVERALL MEANS	0.72	0.01	4						0.48	0.04	3	0.80	0.17	1

ESTIMATED AT 10,000 PPMV 0.88

95 % CONFIDENCE INTERVAL ( 0.31 0.70 )

TIV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			P P S P O N S E F A C T O R S											
	LOW	HIGH	MEAN	MEAN	SE	N	TE	SE	N	7C	SE	N	7M	SE	N	7Q	SE	N
200	238	236	236	0.81		1					0.81	1						
1000	1481	1481	1481	1.80		1					1.80	1						
5000	4711	4711	4711			1					1.18	1						
8000	7331	7331	7331			1												
				OVERALL MEANS	1.23	0.20	3				1.23	0.20	3					

ESTIMATED AT 10,000 PPMV 1.32

95 % CONFIDENCE INTERVAL ( 0.44 3.00 )

Figure 5-39

INSTRUMENT RESPONSE VS CONCENTRATION

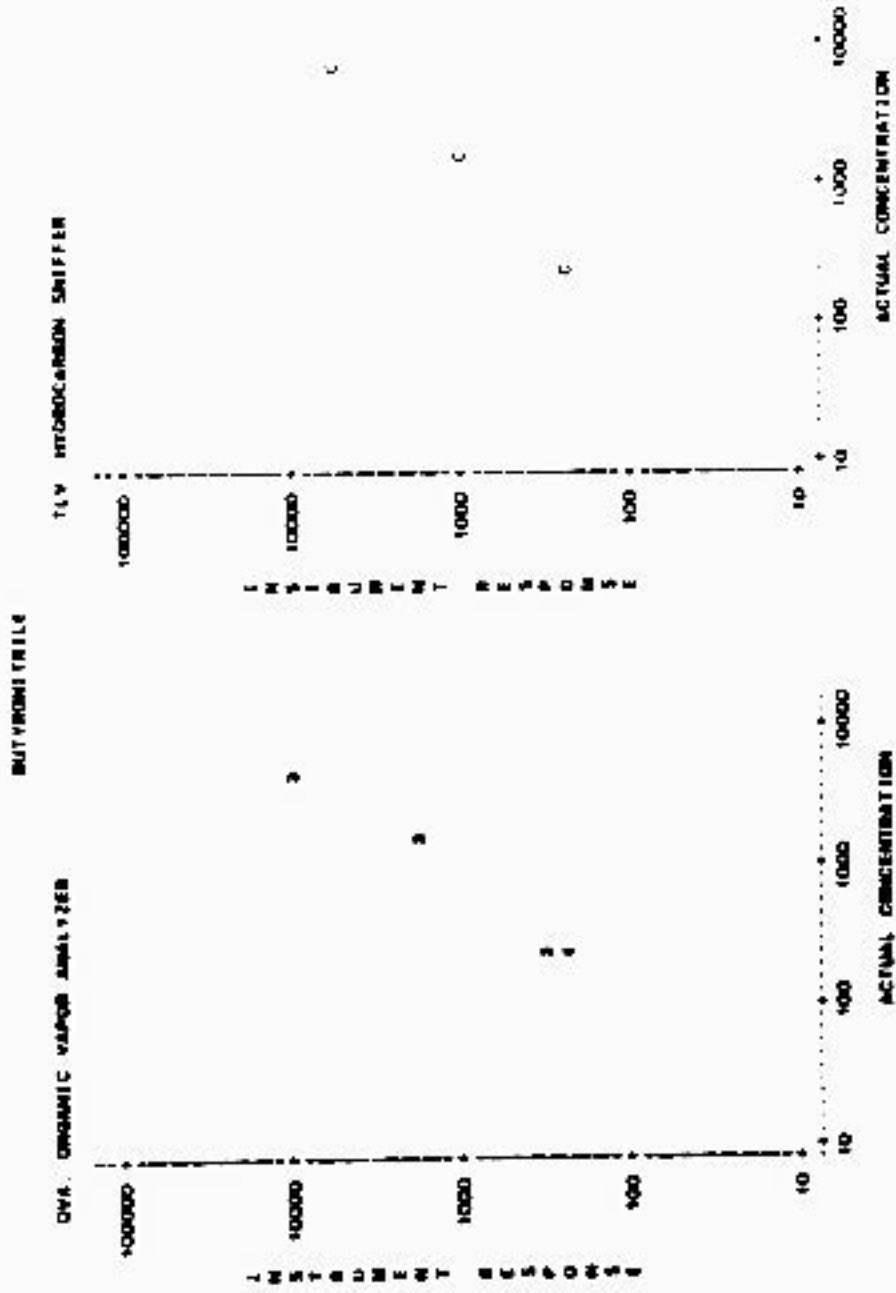


TABLE 5-41

RESPONSE FACTOR SUMMARY

CARBON DISULFIDE

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DESIGN SCHEDULE									
	LOW	HIGH	MEAN	MEAN	SE	N	1080	SE	N	2254	SE	N	3159	SE	N	
300	218	218	218	127.3	18.2	2	108	1	140	2	1					
1500	1510	1510	1510	184.6	47.5	2	137	3	1	277	4	1				
8000	7814	7814	7814	703.5	185.2	2	538	9	1	848	2	1				
OVERALL MEANS 228.6, 12.8, 2							281.8	138.2	410.4	228.2						

ESTIMATED AT 10,000 PPMV 571.9

95% CONFIDENCE INTERVAL 127.6-511.0

FLU INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DESIGN SCHEDULE								
	LOW	HIGH	MEAN	MEAN	SE	N	74	SE	N	11	58	N	78	SE	N
200	218	218	218	1.37		1									
1500	1510	1510	1510	1.94		1									
8000	7814	7814	7814	2.88		1									
OVERALL MEANS 2.08															

ESTIMATED AT 10,000 PPMV 7.96

95% CONFIDENCE INTERVAL 1.2-13.43


Figure 5-40

INSTRUMENT RESPONSE VS CONCENTRATION

CARBON DISULFIDE

OVA ORGANIC VAPOR ANALYZER

TLV MEDDCARBON SNIFFER

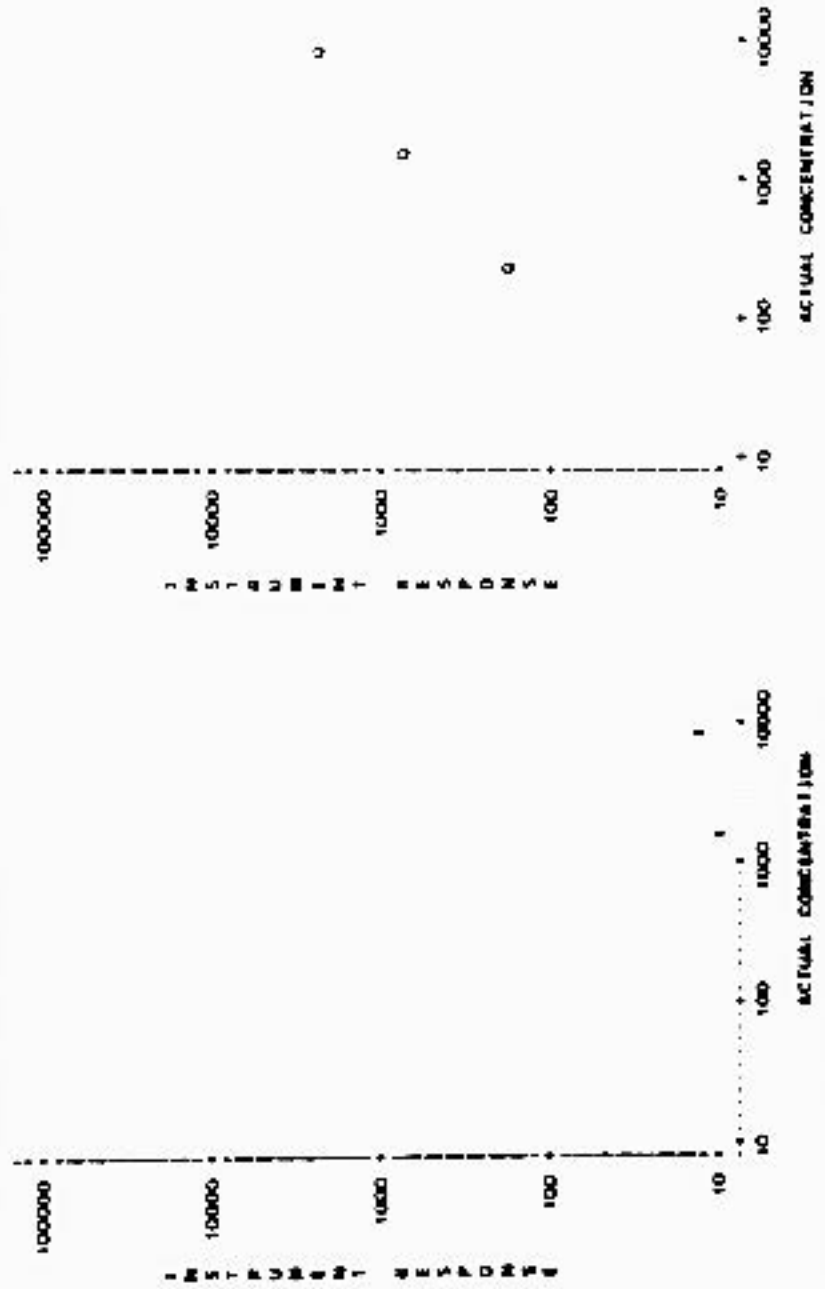

NOTE: 4 OBS HAD MISSING VALUES OR WERE DU



TABLE 5-41  
RESPONSE FACTOR SUMMARY

CARBON TETRACHLORIDE

DVA INSTRUMENTS		R E S P O N S E F A C T O R S																
NOMINAL PPM	ACTUAL PPM		OVERALL			DVA METERS												
	LOW	HIGH	MEAN	SE	N	1000	50	N	2304	51	N	2109	51	N	1013	51	N	
200	197	197	1 99	0 08	2	1 85		1	2 09									
1000	1001	1001	12 99	0 81	2	11 78		1	12 27									
5000	5011	5011	15 77	0 89	2	16 48		1	19 09									
OVERALL MEANS			10 11	0 01	6	10 04		3	10 17		4 08		3					

ESTIMATED AT 10,000 PPM ± 28 99 % COMPLIANCE INTERVAL 110 00 .41 361

FLY INSTRUMENTS

ACTUAL PPM		R E S P O N S E F A C T O R S													
NOMINAL PPM	ACTUAL PPM		OVERALL			TLY METERS									
	LOW	HIGH	MEAN	SE	N	71	50	N	70	50	N	70	50	N	
200	197	197	0 84	0 12	2	0 89		1	0 12						
1000	1001	1001	14 94	1 73	2	24 87		1	9 21						
5000	5011	5011	22 82	5 77	2	28 58		1	13 04						
OVERALL MEANS			13 93	0 76	4	18 07		3	8 99		4 71		2		

ESTIMATED AT 10,000 PPM ± 52 99 % COMPLIANCE INTERVAL 1 8 98 .103 91


Figure 5-41

INSTALLMENT RESPONSE VS CONCENTRATION

CARBON TETRACHLORIDE

11V HYDROCARBON SAMPLER

OVA ORGANIC VAPOR ANALYZER

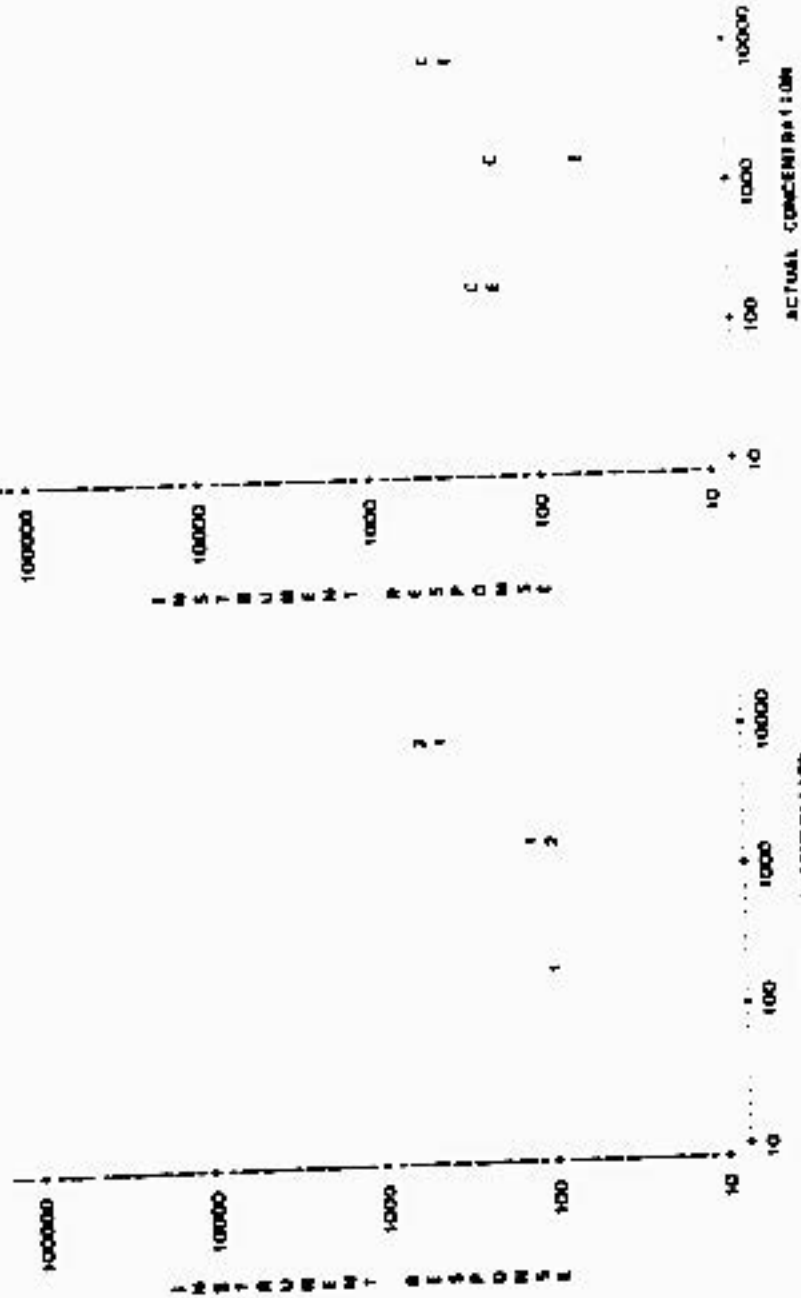

NOTE: 1 OBS HILODEM

TABLE 5-42

RESPONSE FACTOR SUMMARY

CYCLORACETAL DEHYDE

R E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DMA METERS									
	LOW	HIGH	MEAN	SE	N	1000	SE	N	2100	SE	N	1810	SE	N
200	240	240	20	0.85	2	24	0.4	1	34	0.4	1			
1000	1011	1011	21	0.88	2	21	0.6	1	31	0.7	1			
1000	1473	1473	14	0.73	2	14	0.4	1	10	0.3	1			
8000	8185	8185	15	0.78	2	14	0.6	1	10	0.3	1			
OVERALL MEANS		20.36	0.22	8	1.83	2.36	4	23.09	4.32	4				

ESTIMATED AT 10,000 PPMV 13.40

95% CONFIDENCE INTERVAL 1.785 18.247

TV INSTRUMENTS

R E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV		OVERALL		TV METERS									
	LOW	HIGH	MEAN	SE	N	21 <th>SE</th> <th>N</th> <th>70 <th>SE</th> <th>N</th> <th>70 <th>SE</th> <th>N</th> </th></th>	SE	N	70 <th>SE</th> <th>N</th> <th>70 <th>SE</th> <th>N</th> </th>	SE	N	70 <th>SE</th> <th>N</th>	SE	N
200	240	240	5	0.68	2	9	0.6	1	4	0.5	1			
1000	1011	1011	6	0.71	2	7	0.6	1	4	0.5	1			
1000	1473	1473	4	0.81	2	5	0.8	1	4	0.4	1			
8000	8185	8185	5	0.42	2	5	0.7	1	4	0.6	1			
OVERALL MEANS		5.28	0.10	8	6.08	0.50	4	4.48	0.17	4				

ESTIMATED AT 10,000 PPMV 5.07

90% CONFIDENCE INTERVAL 1.285 10.61

Figure 5-42

INSTRUMENT RESPONSE VS CONCENTRATION

ORGANIC VAPOR ANALYZER  
 TLV HYDROCARBON SNIFFER

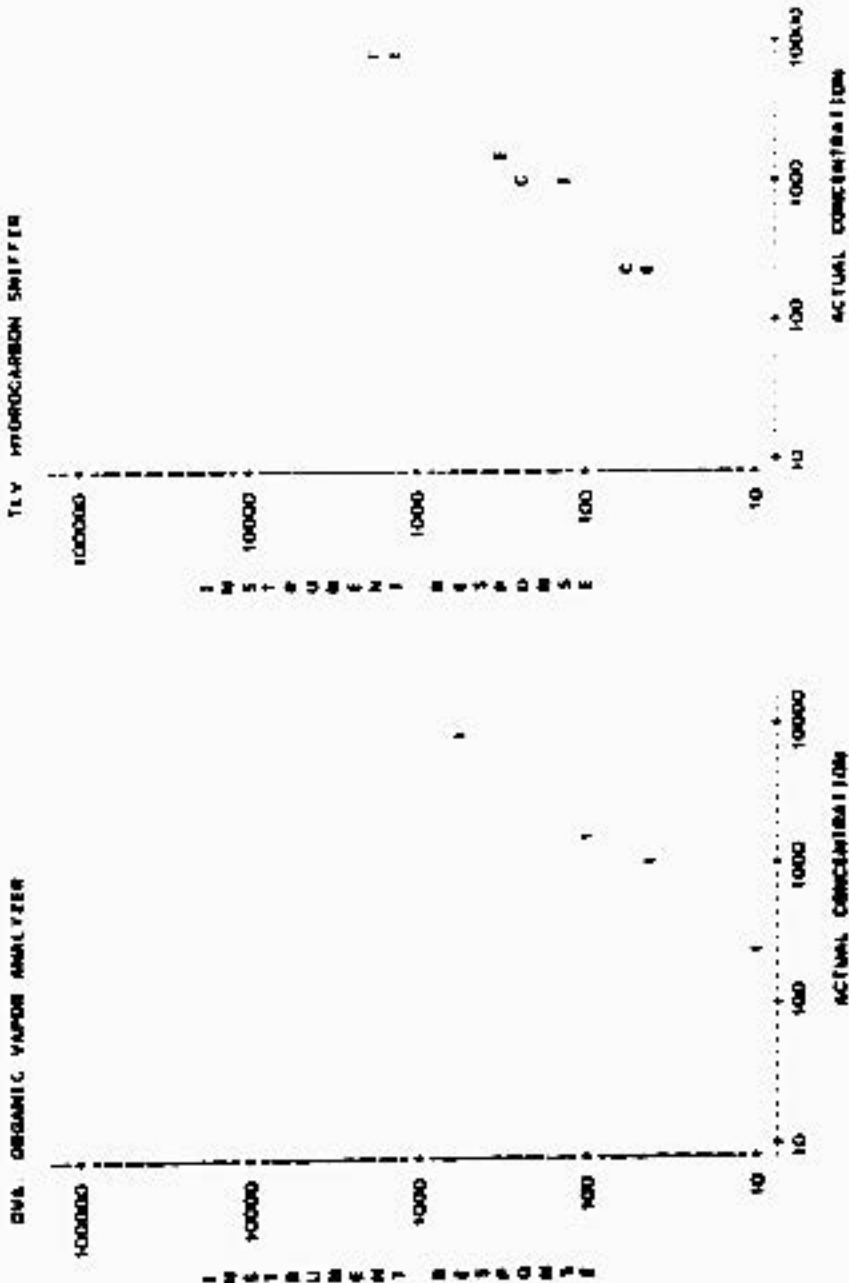


TABLE 4.3

RESPONSE FACTOR SUMMARY

LOW CONCENTRATIONS

ACTUAL PPM

OVERALL MEAN SE

ESTIMATED AT 10,000 PPM 0.76

95% CONFIDENCE INTERVAL 1.026, 0.461

RESPONSE FACTORS

ORIGINAL PPM	LOW	HIGH	MEAN	SE	N	1000	SE	N	2000	SE	N	3000	SE	N	4000	SE	N	
200	211	224	217	0.46	0.03	4	0.47	1	0.46	1	0.36	1	0.32	1	0.31	1	0.25	1
1000	1882	1887	1824	0.34	0.01	4	0.34	1	0.36	1	0.32	1	0.32	1	0.31	1	0.25	1
3000	2800	2857	2828	0.46	0.00	2	0.47	1	0.46	1	0.46	1	0.46	1	0.46	1	0.46	1
1000	7020	7020	7020															
3000	8098	8098	8098															

HIGH CONCENTRATIONS

ACTUAL PPM

OVERALL MEAN SE

ESTIMATED AT 10,000 PPM 0.88

95% CONFIDENCE INTERVAL 1.037, 1.001

RESPONSE FACTORS

ORIGINAL PPM	LOW	HIGH	MEAN	SE	N	70	SE	N	70	SE	N	70	SE	N
200	211	224	217	0.81	0.08	2	0.85	1	0.94	1	0.86	1	0.86	1
1000	1482	1587	1524	0.50	0.00	2	0.43	1	0.94	1	0.78	1	0.78	1
3000	2800	2857	2828	0.84	0.04	2	0.81	1	0.81	1	0.87	1	0.87	1
1000	7020	7020	7020	0.81		1	0.81	1	0.83	1	0.86	1	0.86	1
3000	8098	8098	8098	0.89	0.04	2	0.82	0.01	4	0.94	0.00	2	0.81	0.07

Figure 5-41

INSTRUMENT RESPONSE VS CONCENTRATION

CHLOROBENZENE

DVA ORGANIC VAPOR ANALYZER

TLV HYDROCARBON SNIFFER

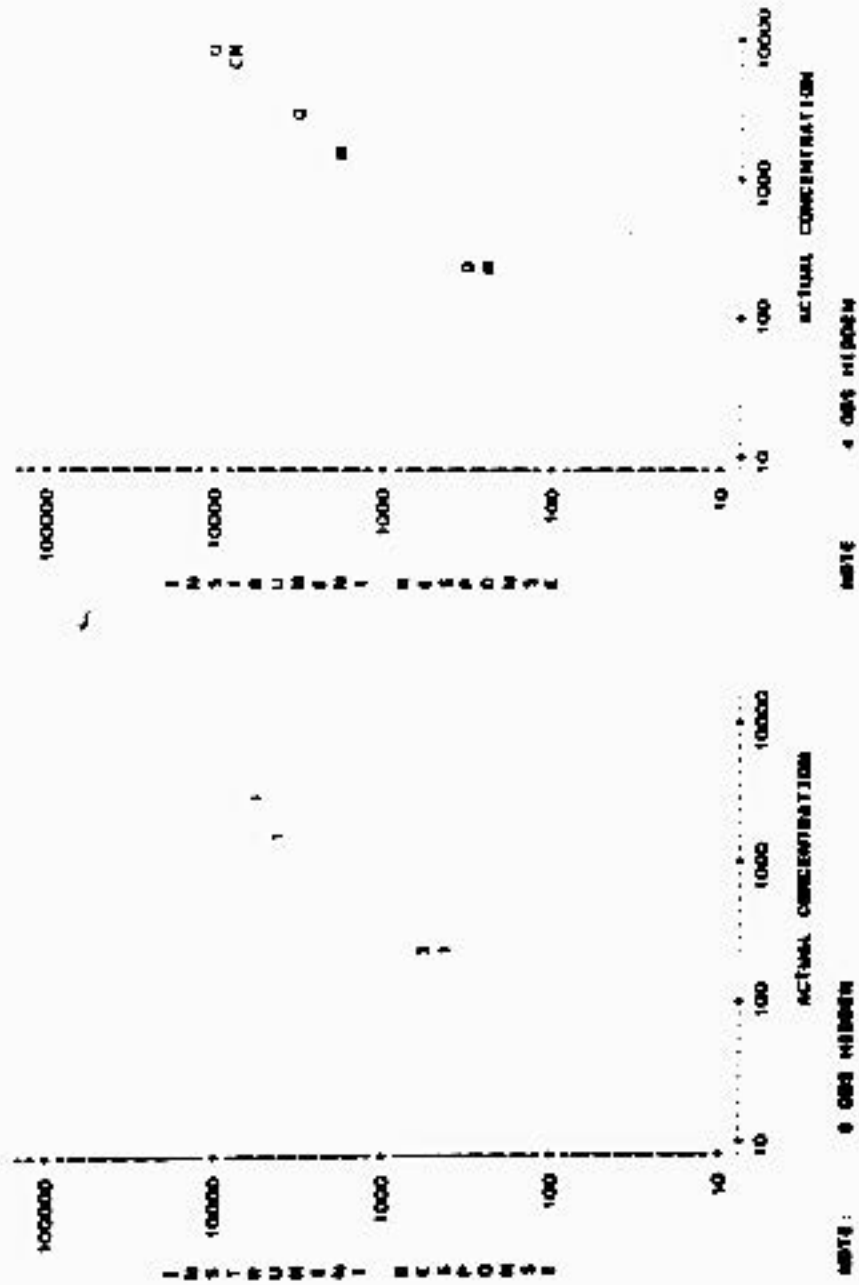


TABLE 5-64

RESPONSE FACTOR SUMMARY

CHLORINE INVADE

RES P O M S E F A C I O M S

OVER INSTRUMENTS

NOMINAL PPM	ACTUAL PPM		OVERALL		OVR METERS														
	LOW	HIGH	MEAN	SE	N	1000	SE	N	2254	SE	N	2159	SE	N	40	1813	SE	N	
200	10	10	0.33	0.04	2	0.78		1	0.20		1								
500	724	724	211	1.20	2	180.9		1	261.2		1								
1500	1540	1540	2.27	0.54	2	2.81		1	1.74		1								
4000	3430	3430	1.61	0.41	2	2.22		1	1.40		1								

OVERALL MEANS 53.87 0.91 8 48.87 44.8 8 81.16 80.4

ESTIMATED AT 10,000 PPM 0.87 95% CONFIDENCE INTERVAL 1 0 02 22 541

FLY INSTRUMENTS

RES P O M S E F A C I O M S

OVER INSTRUMENTS

NOMINAL PPM	ACTUAL PPM		OVERALL		FLY METERS													
	LOW	HIGH	MEAN	SE	N	71	SE	N	71	SE	N	70	SE	N	70	SE	N	
200	10	10	0.18	0.02	2	0.19		1	0.13		1							
500	724	724	13.28	2.41	2	15.80		1	10.97		1							
1500	1540	1540	1.48	0.00	2	1.45		1	1.85		1							
4000	3430	3430	1.22	0.00	2	1.22		1	1.22		1							

OVERALL MEANS 4.08 0.08 8 4.87 3.77 4 3.44 2.53 4

ESTIMATED AT 10,000 PPM 2.16 95% CONFIDENCE INTERVAL 1 0 31.14 853


Figure 5-44

INSTRUMENT RESPONSE VS. CONCENTRATION

CHLOROMETHANE

DVA ORGANIC VAPOR ANALYZER

TLY HYDROCARBON SNIFFER

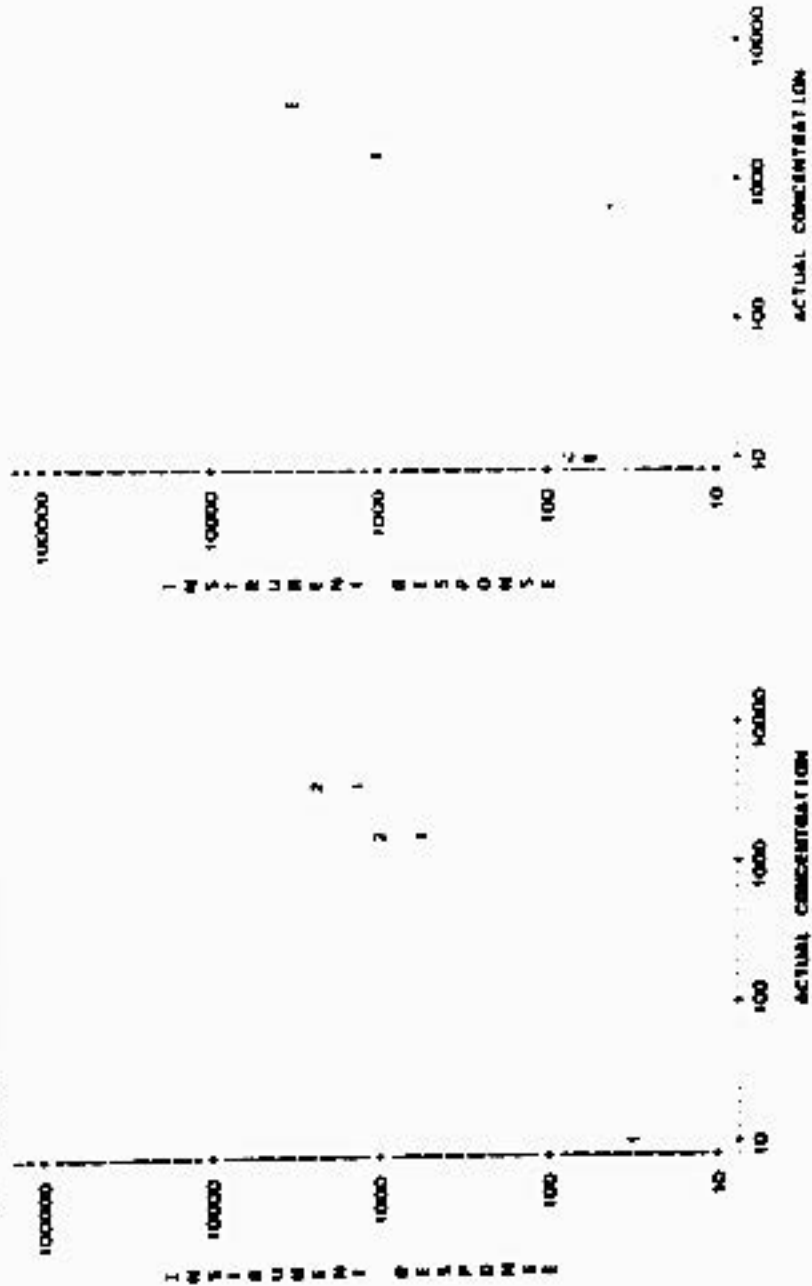

NOTE 2 80% MISSING OR OUT OF RANGE

NOTE 2 80% HIDDEN



TABLE 5-45

RESPONSE FACTOR SUMMARY

CHEMICAL INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OVA METERS									
	LOW	HIGH	MEAN	MEAN	SE	N	1080	SE	N	2204	SE	N	3159	SE	N	
200	222	222	222	2 10	0 08	2	1 20		1	1 44		1				
1500	1528	1528	1528	2 11	0 03	2	2 08		1	2 18		1				
8000	8380	8380	8380	4 64	0 12	2	4 76		1	4 91		1				
OVERALL MEANS			2 71	0 00	6	2 73	1 04	3	2 70	0 93	3					

ESTIMATED AT 10,000 PPMV 4 48

95 % CONFIDENCE INTERVAL 1 280 5 783

TLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			TLV METERS									
	LOW	HIGH	MEAN	MEAN	SE	N	76	SE	N	76	SE	N	76	SE	N	
200	222	222	222	2 03	0 23	2	2 26		1	1 90		1				
1500	1528	1528	1528	6 01	0 90	2	6 87		1	6 18		1				
8000	8380	8380	8380	7 47	0 26	2	7 72		1	7 21		1				
OVERALL MEANS			5 18	0 08	6	5 64	1 71	3	4 73	1 58	3					


ESTIMATED AT 10,000 PPMV 8 77

95 % CONFIDENCE INTERVAL 1 560 12 041

Figure 3-45

INSTRUMENT RESPONSE VS CONCENTRATION

CHLOROPYRIFOS

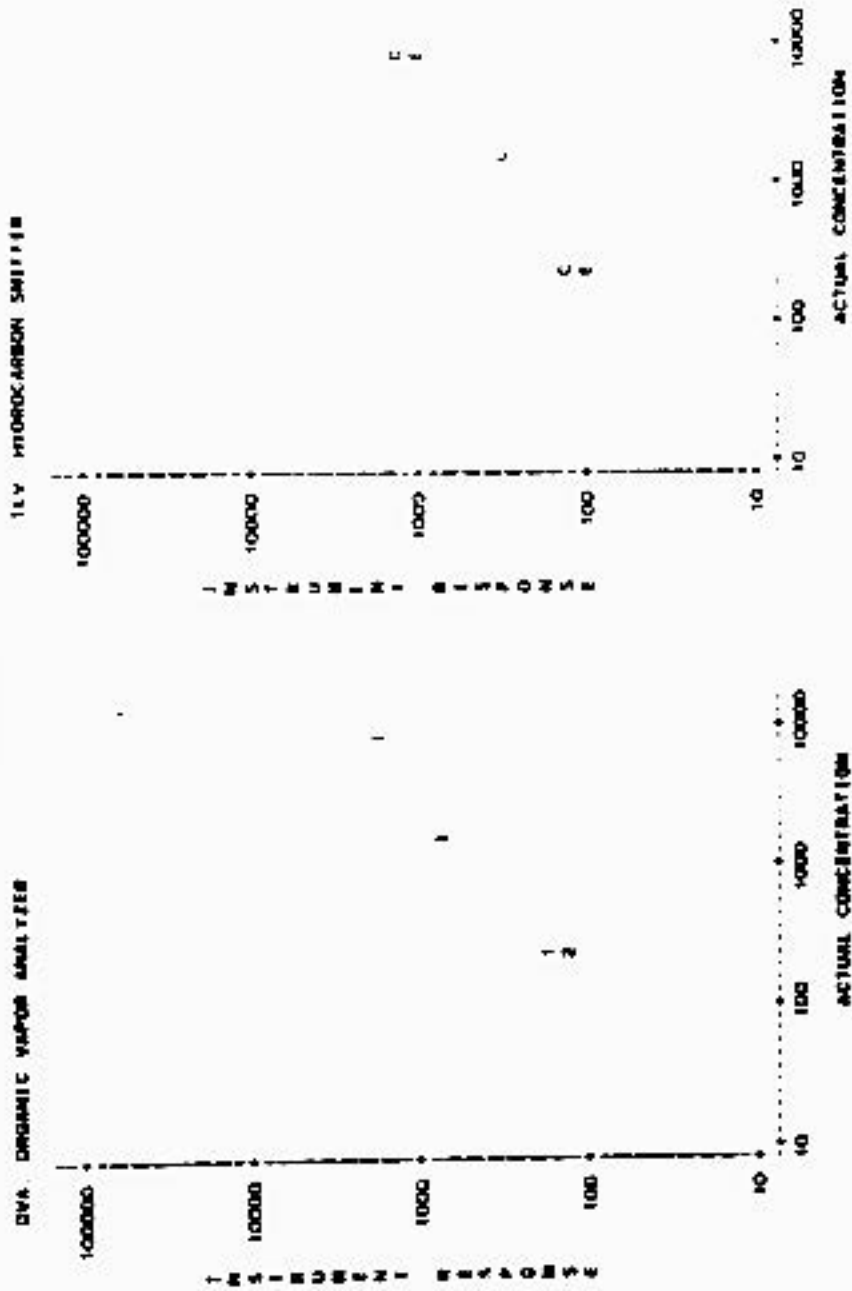

NOTE: 2 MIS HIGHEN

TABLE 5-46

RESPONSE FACTOR SUMMARY

CHLOROPHENOL, D-

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METERS												
	LOW	HIGH	MEAN	MEAN	SE	N	1000	51	W	2284	SE	N	2108	SE	N	1813	SE	N	
200	216	219	216	1.88	0.13	2	1.93			1	1.78								
1000	1033	1033	1033	1.73	0.09	3	1.70			1	1.73								
2000	2147	2147	2147	2.87	0.17	2	3.04			1	3.70								
	OVERALL MEANS			2.09	0.00	6	2.09	0.48	3	2.07	0.31	3							

ESTIMATED AT 10,000 PPMV 3.33

95% CONFIDENCE INTERVAL 1.188, 5.823

TLY IMPURMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			TLY METERS											
	LOW	HIGH	MEAN	MEAN	SE	N	76	SE	M	7C	58	M	7M	5E	N	7D	SE	N
200	216	216	216	1.38		1										1.70		1
1000	1033	1033	1033	2.09		1										2.09		1
2000	2147	2147	2147	3.47		1										3.47		1
	OVERALL MEANS			3.27		3										3.21	0.64	3


ESTIMATED AT 10,000 PPMV 8.87

95% CONFIDENCE INTERVAL 1.240, 14.063

Figure 5-46

INSTRUMENT RESPONSE VS CONCENTRATION

Chloroethene, C<sub>2</sub>H<sub>3</sub>Cl

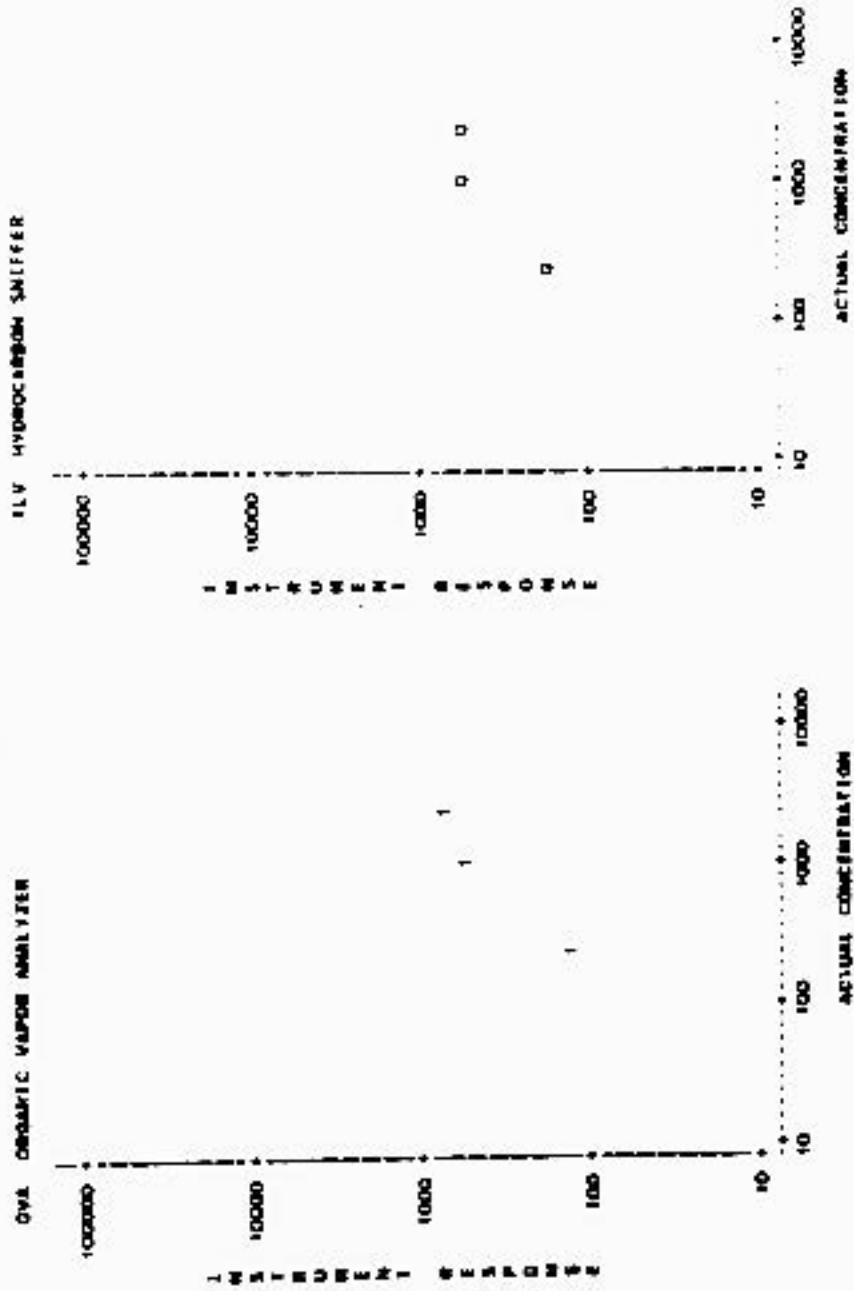

NOTE: 3 ORS HIGHEN

TAB. 5-4

RESPONSE FACTOR SUMMARY

CALCULATIONS

QVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL										QVA METERS									
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	M	2200	SE	N	3150	SE	M	1817	SE	N					
200	223	223	223	1.82	0.09	2	1.73		1	1.92		1											
1500	1289	1288	1288	1.14	0.04	3	1.08		1	1.20		1											
5000	4687	4687	4687	0.74	0.03	3	0.86		1	0.76		1											
7000	6482	6482	6482																				
8000	7742	7742	7742	0.82		1				0.82		1											
OVERALL MEANS				1.15	0.00	2	1.17	0.20	3	1.12	0.28	4											

ESTIMATED AT 10,000 PPMV 0.99

95% CONFIDENCE INTERVAL 1.053 - 0.887


TUV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL										TUV METERS									
	LOW	HIGH	MEAN	MEAN	SE	N	76	SE	M	76	SE	N	100	SE	M	100	SE	N					
200	223	223	223	1.06	0.04	2	1.01		1	1.56		1											
1500	1289	1288	1288	1.27	0.06	2	1.32		1	1.23		1											
5000	4687	4687	4687	0.89	0.01	2	0.70		1	0.88		1											
7000	6482	6482	6482																				
8000	7742	7742	7742	1.20	0.03	2	1.23		1	1.16		1											
OVERALL MEANS				1.19	0.00	6	1.20	0.18	4	1.18	0.18	4											

ESTIMATED AT 10,000 PPMV 0.88

95% CONFIDENCE INTERVAL 1.004 - 1.157

Figure 5-47  
 INSTRUMENT RESPONSE VS. CONCENTRATION

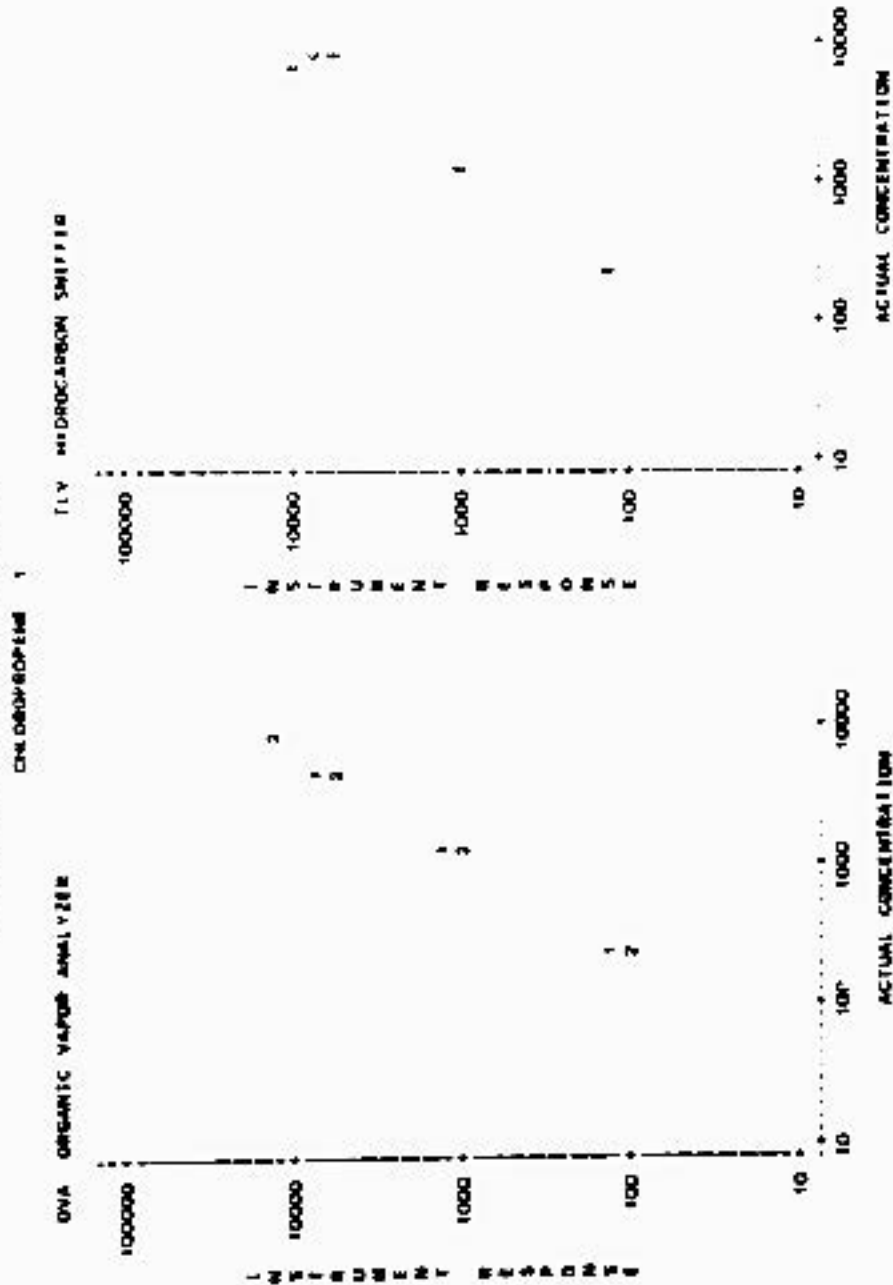

NOTE 3 CBS HIDDEN

TABLR 5-4B

RESPONDE FACTOR SUMMARY

CHLOROPHENE, 3.

NOMINAL PPMV	ACTUAL PPMV				M E S P D M S E F A C T O R S													
	LOW	HIGH	MEAN	SE	OVA METERS													
			MEAN	SE	M	TC	SE	N	2204	SE	M	2100	SE	N	2013	SE	M	
50	54	54	54	2.11	0.27	4	2.84	0.01	2	3.37	0.02	2						
500	534	548	540	2.02	0.02	4	2.06	0.00	2	1.86	0.02	2						
5000	5792	5978	5936	0.74	0.04	4	0.78	0.02	2	0.70	0.00	2						
OVERALL MEANS				1.80	0.01	12	1.80	0.36	6	2.02	0.80	6						
ESTIMATED AT 10,000 PPMV				0.76	95 % CONFIDENCE INTERVAL ( 0.60, 0.87 )													

ILV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV				M E S P D M S E F A C T O R S													
	LOW	HIGH	MEAN	SE	ILV METERS													
			MEAN	SE	M	TC	SE	N	20	SE	M	20	SE	N	20	SE	M	
50	54	54	54	1.29	0.16	4	1.45	0.14	2	1.14	0.07	2						
500	524	548	540	1.32	0.13	4	1.40	0.08	2	1.18	0.04	2						
5000	5792	5978	5936	1.23	0.08	4	1.31	0.06	2	1.16	0.00	2						
OVERALL MEANS				1.28	0.01	12	1.40	0.08	6	1.14	0.02	6						
ESTIMATED AT 10,000 PPMV				1.34	95 % CONFIDENCE INTERVAL ( 1.10, 1.41 )													

Figure 5-48

INSTRUMENT RESPONSE VS CONCENTRATION

CH<sub>4</sub> CARTRIDGE (ME) 3

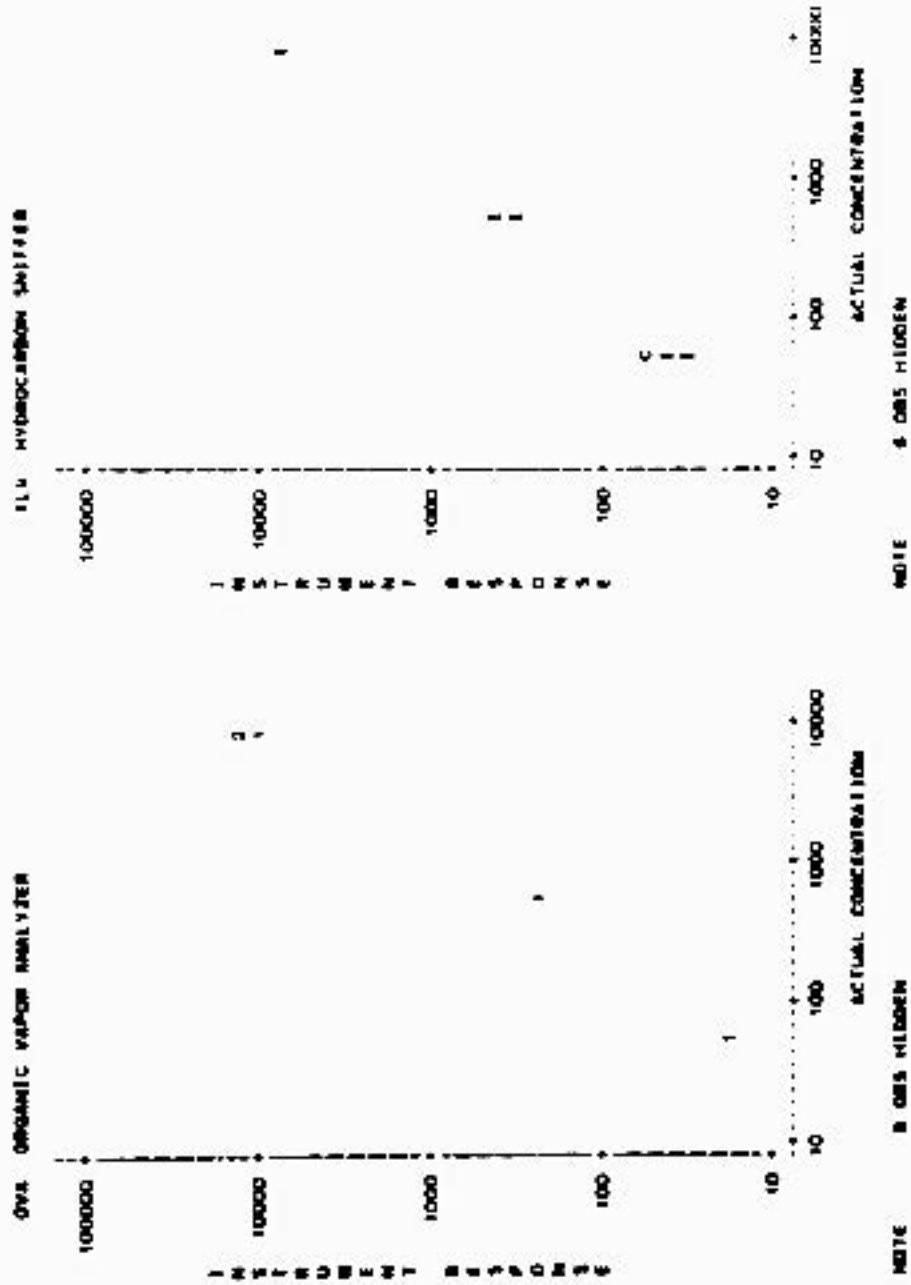




TABLE 3-64

RESPONSE FACTOR SUMMARY

CHA ORDOLUINE . M

RESPONSE FACTORS

OVA METERS

NOMINAL Ppmv	ACTUAL PPMV			OVERALL			1000	SE	N	2784	SE	N	2180	SE	N	1017	SE	N	
	LOW	HIGH	MEAN	MEAN	SE	SE													SE
200	217	217	217	0.78	0.03	2	0.72	1	1	0.77	1	1							
1500	1528	1528	1528	0.88	0.02	2	0.83	1	1	0.87	1	1							
3200	3208	3208	3208	0.91	0.00	2	0.81	1	1	0.82	1	1							
OVERALL MEANS				0.80	0.00	6	0.89	0.07	3	0.82	0.08	3							

ESTIMATED AT 10,000 PPMV 0.82  
90% CONFIDENCE INTERVAL 1.0 TO 0.471

ELY INSTRUMENTS

RESPONSE FACTORS

ELY METERS

NOMINAL Ppmv	ACTUAL PPMV			OVERALL			75	SE	N	71	SE	N	73M	SE	N	10	SE	N	
	LOW	HIGH	MEAN	MEAN	SE	SE													SE
200	217	217	217	0.88	0.00	1													
1500	1528	1528	1528	0.73	0.00	1													
3200	3208	3208	3208	0.88	0.00	1													
OVERALL MEANS				0.78	0.00	3													

ESTIMATED AT 10,000 PPMV 0.87  
90% CONFIDENCE INTERVAL 1.0 TO 1.219

FIGURE 5-44  
 INSTRUMENT RESPONSE VS. CONCENTRATION  
 CHLOROTOLUENE - B

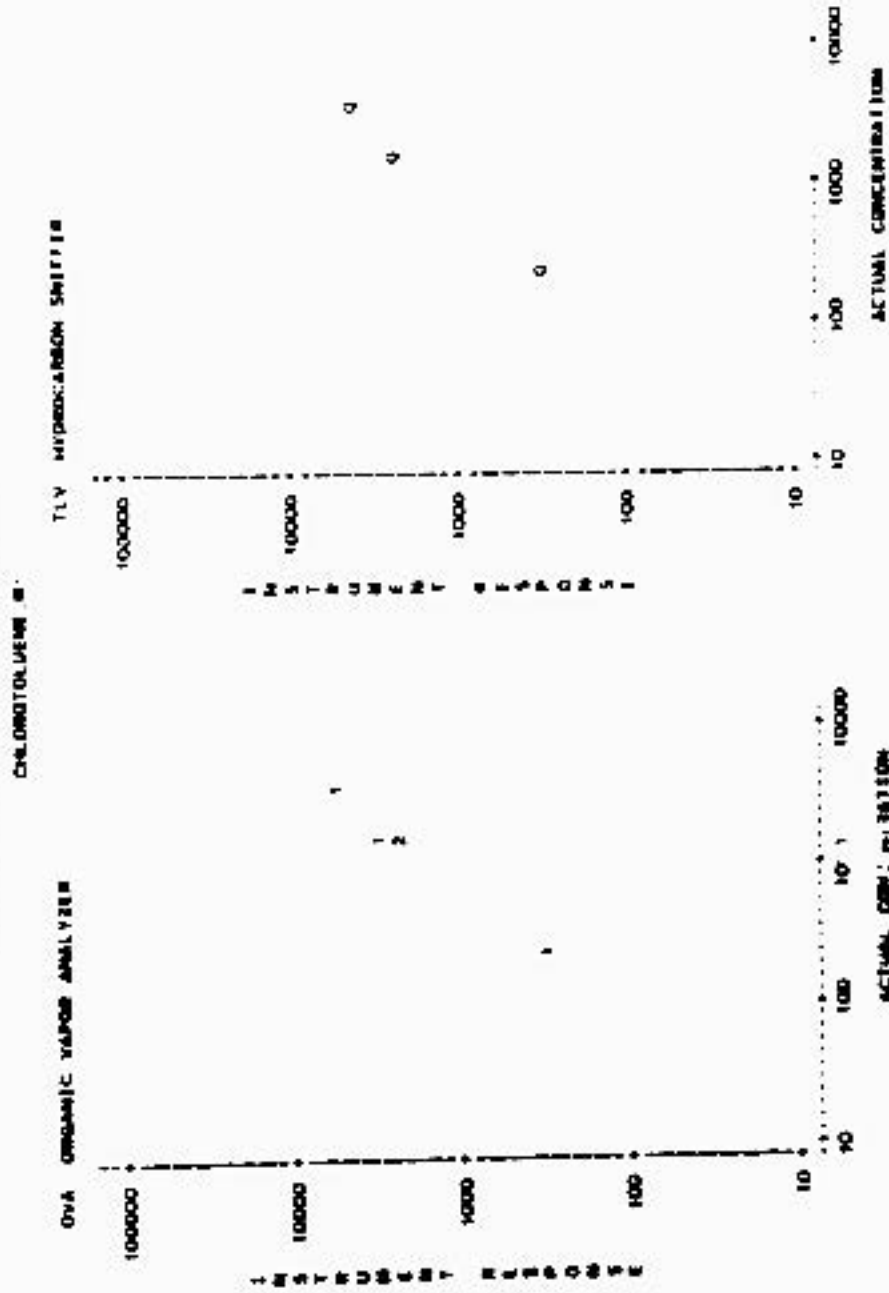


TABLE 3-50

RESONANT FREQUENCY SUMMARY

CRECINDOTOLINE, D.

OVA INSTRUMENTS

RESONANCE FACTORS

NOMINAL PMM	ACTUAL PMM		OVERALL		OVA MEASUREMENTS							
	LOW	HIGH	MEAN	SE	1000	SE	2000	SE	3000	SE	4000	SE
200	207	207	0.91	0.08	0.98	1	0.97	1				
1800	1804	1804	0.93	0.03	0.90	1	0.96	1				
3100	3028	3028	0.90	0.01	0.98	1	0.90	1				
OVERALL MEANS			0.93	0.00	0.92	0.02	0.98	0.00				

ESTIMATED AT 10,000 PMM 0.95

95% CONFIDENCE INTERVAL 0.88 - 0.99

FLV INSTRUMENTS


RESONANCE FACTORS

NOMINAL PMM	ACTUAL PMM		OVERALL		FLV MEASUREMENTS							
	LOW	HIGH	MEAN	SE	70	SE	100	SE	150	SE	200	SE
200	207	207	0.95									
1800	1804	1804	0.77									
3100	3028	3028	0.96									
OVERALL MEANS			0.90									

ESTIMATED AT 10,000 PMM 0.96

95% CONFIDENCE INTERVAL 0.70 - 0.99

Figure 5-50  
 INSTRUMENT RESPONSE VS CONCENTRATION  
 CHLOROFLUORENE D

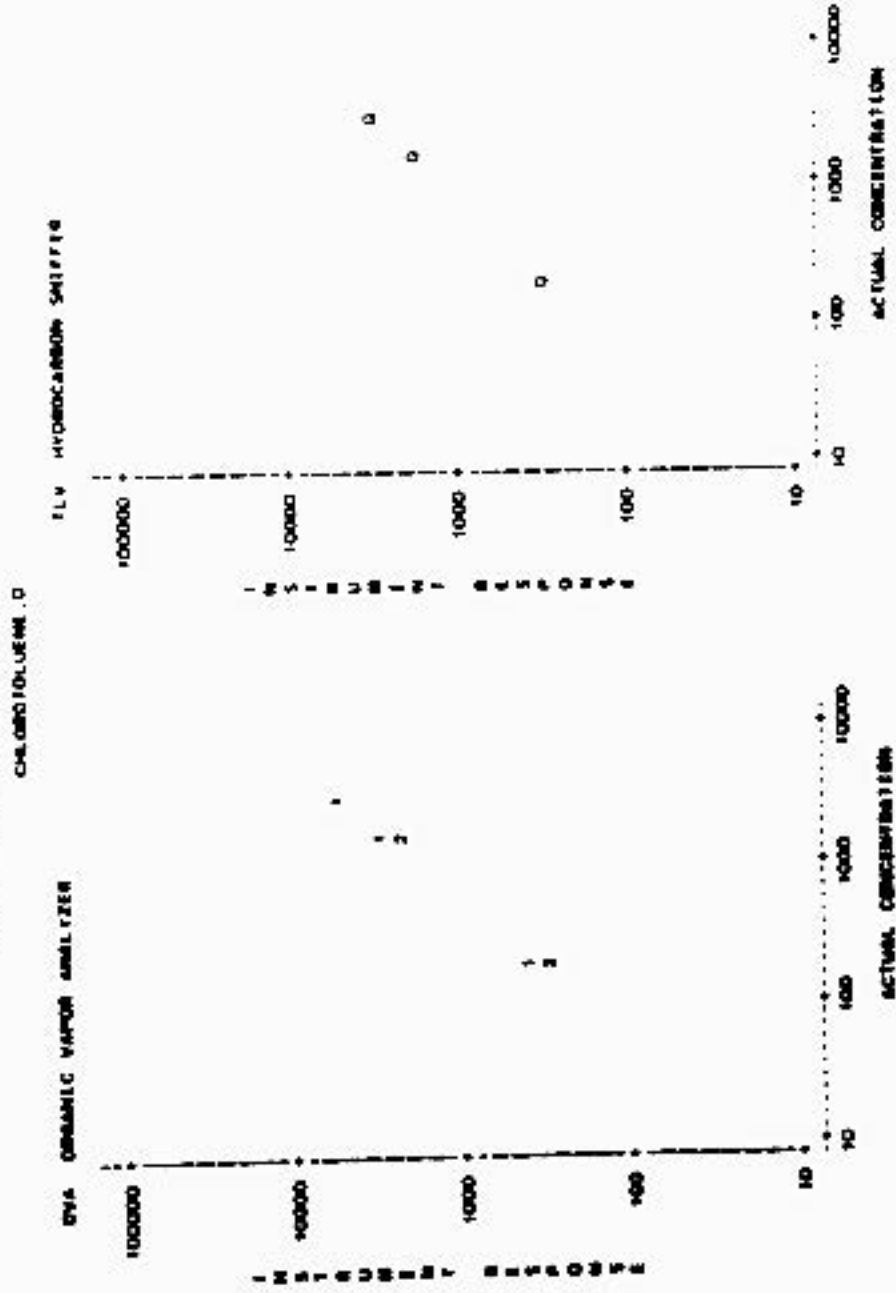

NOTE: 100% HUMIDITY

TABLE 5-5)

RESPONSE FACTOR SUMMARY

CHLOROPOLYMER P.

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DATA METERS													
	LOW	HIGH	MEAN	SE	1000	SE	1	2004	SE	1	2100	SE	1	1810	SE	1	N	
200	217	217	0.88	0.02	0.87		1	0.82										
1800	1800	1800	0.83	0.01	0.84		1	0.81										
3100	3126	3126	0.83	0.01	0.83		1	0.82										
OVERALL MEANS			0.70	0.00	0.71	0.08	3	0.68	0.07	3								
ESTIMATED AT 10,000 PPMV			0.83	98% CONFIDENCE INTERVAL (0.47 - 0.98)														


ELY INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DATA METERS													
	LOW	HIGH	MEAN	SE	78	SE	1	70	SE	1	78	SE	1	70	SE	1	N	
200	217	217	0.88	0.02										0.84			1	
1800	1800	1800	0.88	0.02										0.84			1	
3100	3126	3126	1.19											1.15			4	
OVERALL MEANS			0.94	98% CONFIDENCE INTERVAL (0.82 - 1.21)														
ESTIMATED AT 10,000 PPMV			1.15															

Figure 5-51

INSTRUMENT RESPONSE VS CONCENTRATION

CHLOROTOLUENE, P.

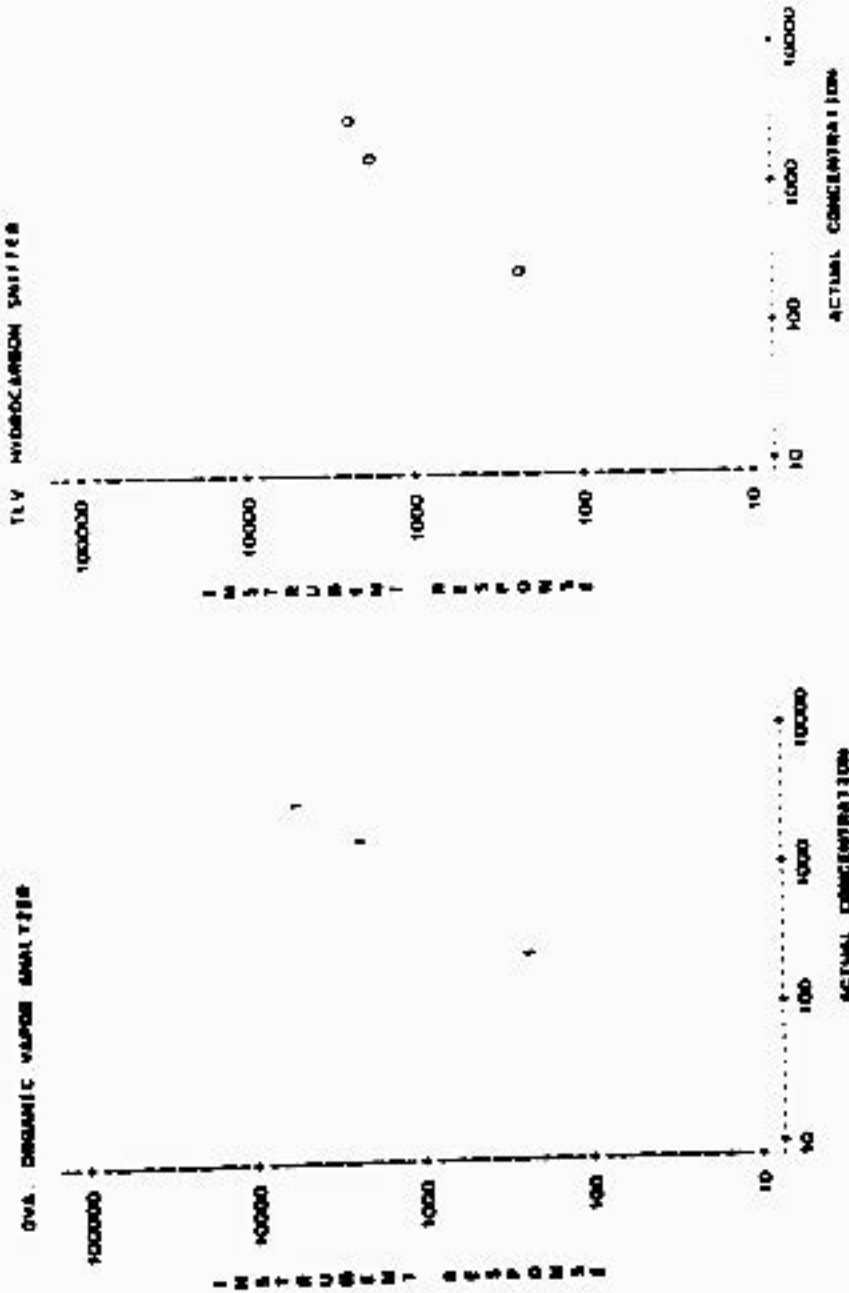

NOTE: 3 OPS MINIMUM

TABLE 5-52

RESPONSE FACTOR SUMMARY

CBS 50x .0

OVA INCUBATIONS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL																	
	LOW	HIGH	MEAN	MEAN	SE	M	HCMD	SE	N	25%	SE	M	75%	SE	M	10%	SE	M			
200	210	210	210	3.86	0.49	2	5.28		1	6.36											
800	708	708	708	3.78	0.11	2	3.84		1	3.86											
1100	1117	1117	1117	3.82	0.00	2	3.91		1	2.82											
OVERALL MEANS				4.06	0.03	6	3.89	0.84	2	4.26	1.12	2									
ESTIMATED AT 10,000 PPMV				0.96	95% CONFIDENCE INTERVAL															1.00	1.521

TLV INCUBATIONS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL																		
	LOW	HIGH	MEAN	MEAN	SE	M	TE	SE	M	7C	SE	M	7M	SE	M	7D	SE	M				
200	210	210	210	0.82		1										0.82						
800	708	708	708	1.86		1										1.86						
1100	1117	1117	1117	1.43		1										1.43						
OVERALL MEANS				1.41	95% CONFIDENCE INTERVAL															1.00	2.272	0.81
ESTIMATED AT 10,000 PPMV				3.98																		


Figure 5-52

INSTRUMENT RESPONSE VS CONCENTRATION

CAS# 94-01-1

DVA: ORGANIC VAPOR ANALYZER

TLV: HYDROCARBON SNIFTER

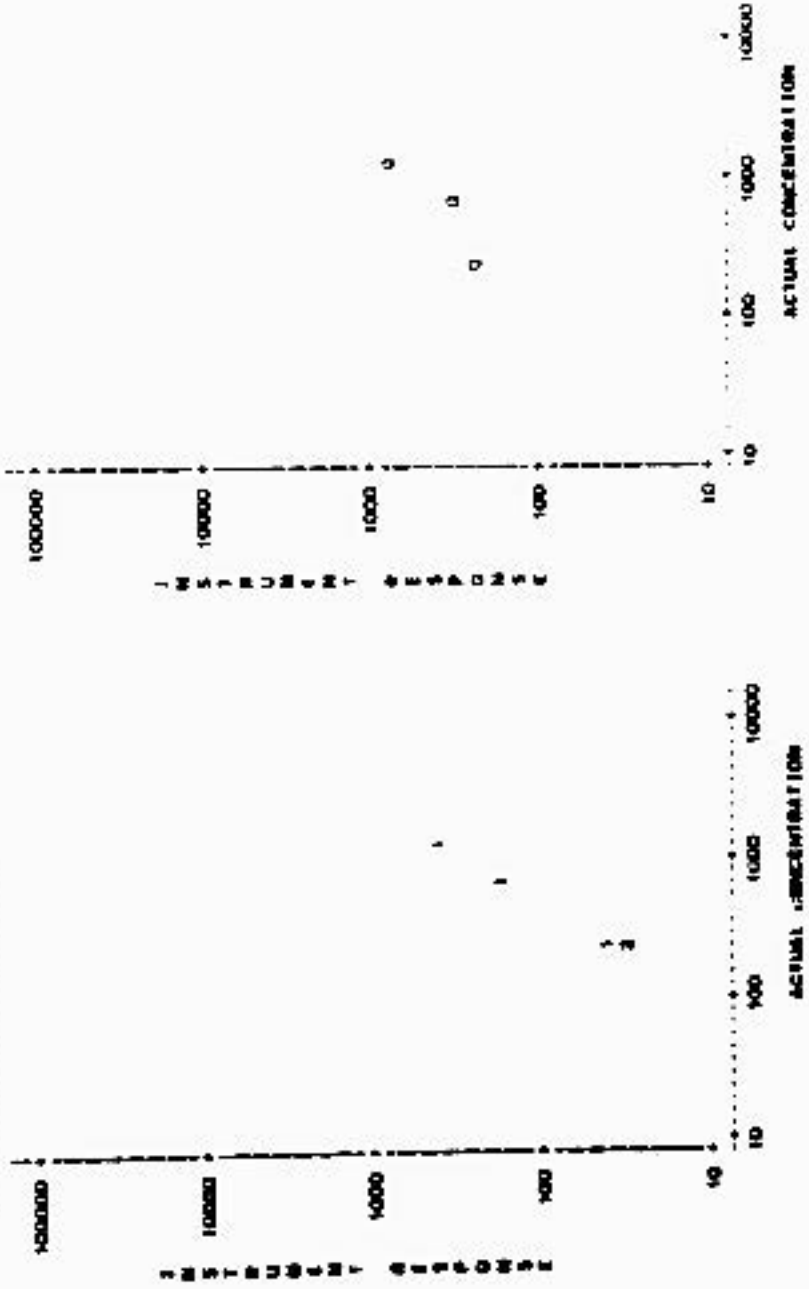

NOTE: 2 89% HUMIDITY



TABLE 5-51

RESPONSE FACTOR SUMMARY

CYD10MALDENHYDE

RESPONSE FACTOR SUMMARY

NOMINAL PPMV	ACTUAL PPMV		OVERALL		OVA METERS													
	LOW	HIGH	MEAN	SE	N	1000	50	N	2354	51	M	2189	57	N	1813	51	N	
200	245	245	2.81	0.16	2	3.43		1	2.78		1							
1000	1083	1083	2.78	0.10	2	2.80		1	2.89		1							
1800	1898	1898	2.28	0.07	2	2.23		1	2.26		1							
8000	8723	8723	1.08	0.01	2	1.08		1	1.08		1							
OVERALL MEANS					2.85	0.00	8	2.81	0.47	4	2.48	0.49	4					

ESTIMATED AT 10,000 PPMV 1.32 99% CONFIDENCE INTERVAL 1.07 18 2.33

TLV INSTRUMENTS

RESPONSE FACTOR SUMMARY


NOMINAL PPMV	ACTUAL PPMV		OVERALL		TLV METERS													
	LOW	HIGH	MEAN	SE	N	71	50	N	70	50	N	70	50	N	70	50	N	
200	245	245	2.01	0.33	2	2.24		1	1.78		1							
1000	1083	1083	2.89	1.88	2	5.55		1	2.23		1							
1800	1898	1898	4.82	3.28	2	8.94		1	3.18		1							
8000	8723	8723	23.88	18.7	2	42.84		1	3.18		1							
OVERALL MEANS					8.83	0.78	8	18.07	8.28	4	7.60	0.35	4					

ESTIMATED AT 10,000 PPMV 8.84 95% CONFIDENCE INTERVAL 1.2 33.31 26.1

FIGURE 5-53

INSTRUMENT RESPONSE VS CONCENTRATION

CIRCUMALOHENTOL

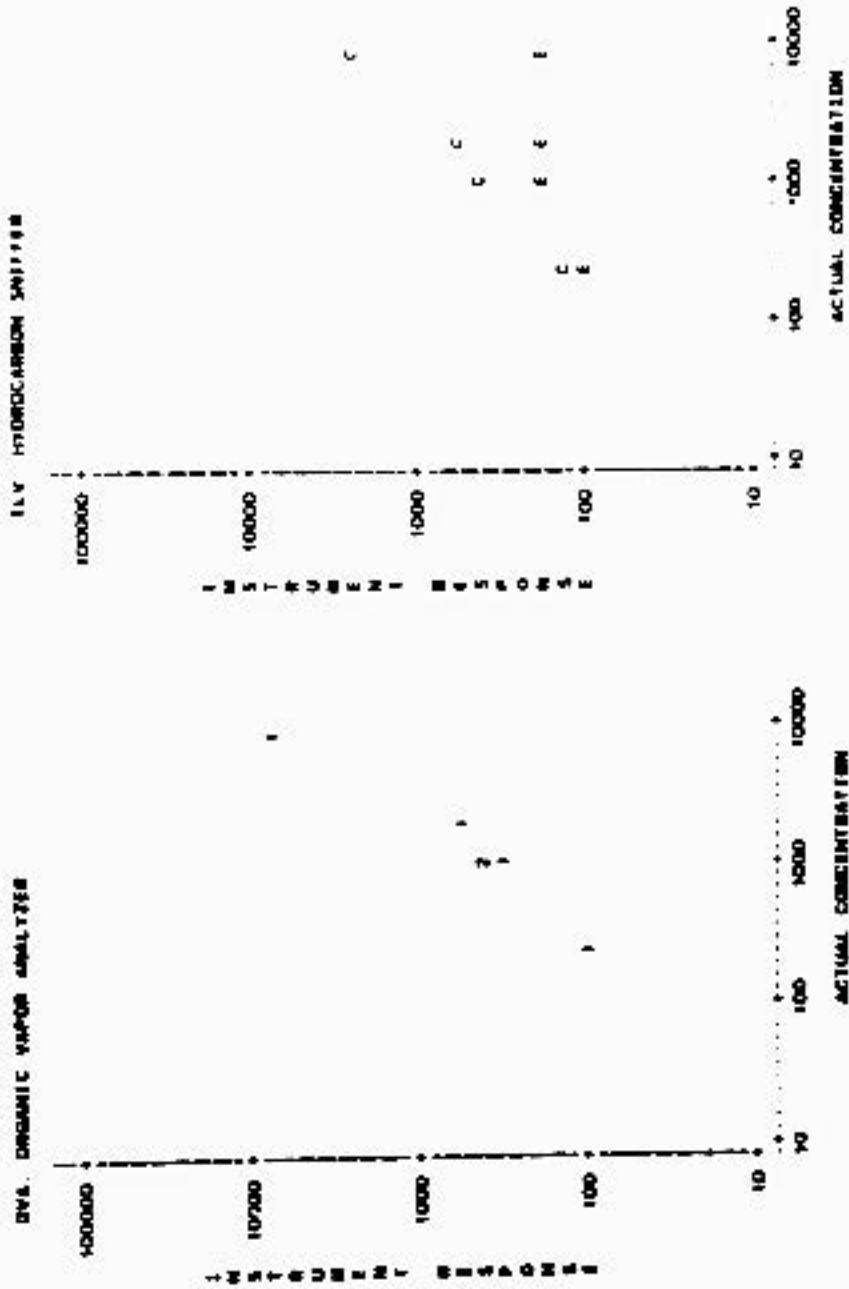

NOTE: 3 OBS MISSED

TABLE 5-54

RESPONSE FACTOR SUMMARY

CURB ME

OVA INSTRUMENTS

R E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV		OVERALL		OVA METERS										
	LOW	HIGH	MEAN	SE	N	1000	SE	N	2500	SE	N	1000	SE	N	
50	54	57	56	2.17	0.86	4	2.81	1.37	2	2.83	1.11	2	2.80	0.63	2
500	545	548	547	2.73	0.07	4	2.68	0.91	2	2.80	0.63	2	2.47	0.74	2
5000	5025	5745	5405	2.85	0.03	4	2.48	1.38	2	2.47	0.74	2			
OVERALL MEANS		2.76		0.02	12	2.55		0.55	6	2.01		0.48	6		

ESTIMATED AT 10,000 PPMV 1.82

95% CONFIDENCE INTERVAL 1.13 - 2.83

11V INSTRUMENTS

R E S P O N S E F A C T O R S


NOMINAL PPMV	ACTUAL PPMV		OVERALL		11V METERS										
	LOW	HIGH	MEAN	SE	N	31	SE	N	76	SE	N	10	SE	N	
50	54	57	56	2.34	0.48	4	2.82	0.17	2	1.86	1.17	2			
500	545	548	547	10.07	1.02	4	15.09	0.24	2	5.05	0.34	2			
5000	5025	5745	5405	20.06	14.0	4	24.98	3.04	2	5.49	1.30	2			
OVERALL MEANS		10.82		0.58	12	17.50		0.70	6	4.11		0.31	6		

ESTIMATED AT 10,000 PPMV 12.49

95% CONFIDENCE INTERVAL 5.62 - 27.14

Figure 5-54

INSTRUMENT RESPONSE VS CONCENTRATION

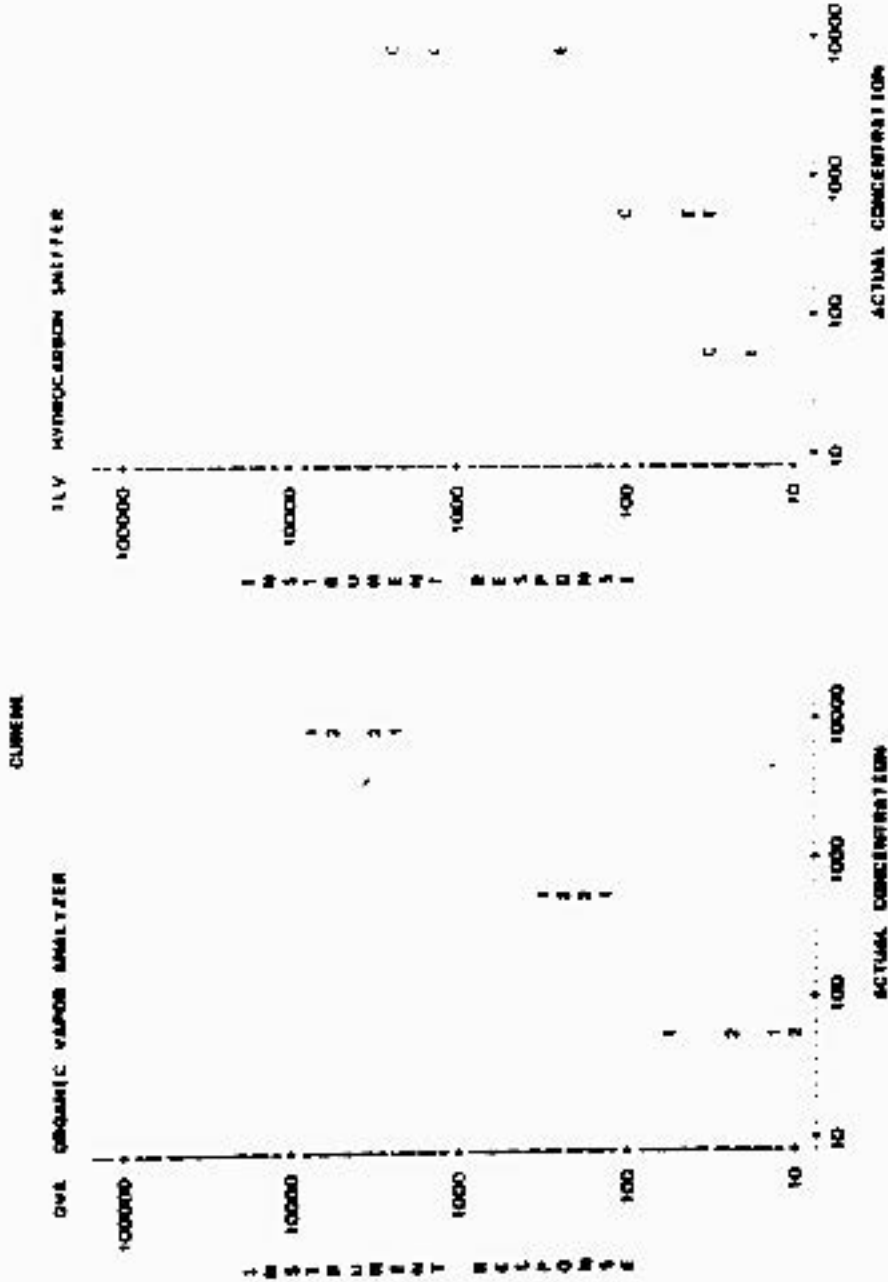

NOTE: 4 OBS. HIDDEN

TABLE 5-15

RESPONSE FACTOR SUMMARY

CYCLE NAME

OVER INSTRUMENTS

M E S P O M S E F A I T O R S

INSTRUMENT	ACTUAL PPMV		OVERALL		DVA METERS													
	LOW	HIGH	MEAN	SE	N	1000	50	N	2204	SE	N	2100	SE	N	1013	SE	N	
200	220	220	220	0.00	2	1.27		1	1.22		1							
1000	1001	1001	1001	0.75	0.04	2	0.74		0.81		1							
3000	3163	3163	3163	0.88	0.03	2	0.88		0.91		1							
5000	5114	5114	5114															
8000	7000	7000	7000															

OVERALL MEANS 0.84 0.10 0.6 0.83 0.74 0.86 0.77 0.8

ESTIMATED AT 10 000 PPMV 0.76

95% CONFIDENCE INTERVAL 1 0.20 0.200

FLV INSTRUMENTS

M E S P O M S E F A I T O R S

INSTRUMENT	ACTUAL PPMV		OVERALL		11.4 METERS													
	LOW	HIGH	MEAN	SE	N	FE	SE	M	TE	SE	N	70	SE	N	70	SE	N	
200	220	220	220	0.90	0.04	2	0.81		1	0.82		1						
1000	1001	1001	1001	0.90	0.08	2	0.82		1	0.88		1						
3000	3163	3163	3163	0.70	0.01	2	0.72		1	0.67		1						
5000	5114	5114	5114	0.85	0.01	2	0.83		1	0.84		1						
8000	7000	7000	7000	0.78	0.02	2	0.78		1	0.74		1						

OVERALL MEANS 0.88 0.05 1.0 0.88 0.07 0.86 0.07 0.8

ESTIMATED AT 10 000 PPMV 0.72

95% CONFIDENCE INTERVAL 1 0.63 0.623


Figure 5-55

INSTANTANEOUS RESPONSE VS CONCENTRATION

CYCLORANINE

ENV. ANALYTICAL VAPOR ANALYZER

TLV IMMEDIATELY HAZARDOUS

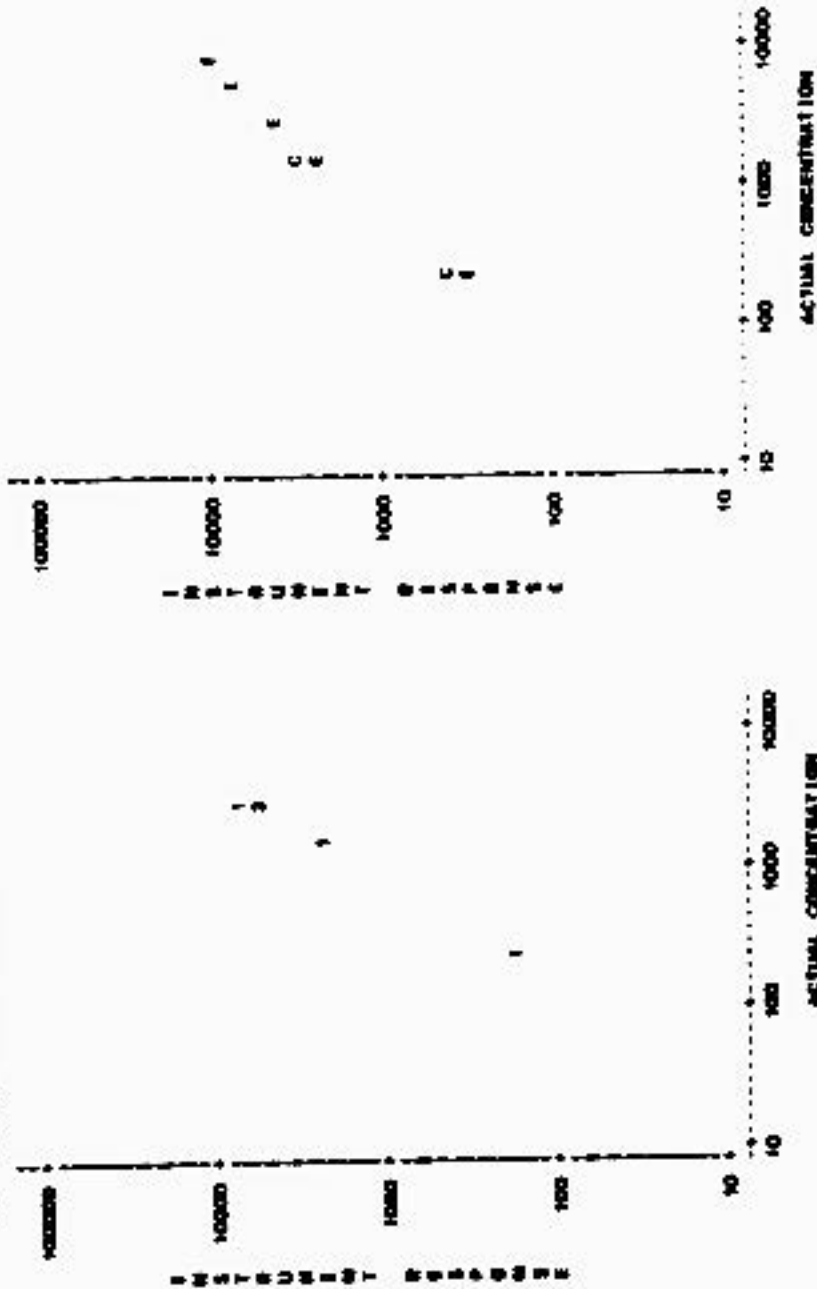

NOTE: 2 MMS HILBOM

NOTE: 3 OES HILBOM

TABLE 3-54

RESPONSE FACTOR SUMMARY

CYCLOMETER		RESPONSE FACTORS																			
DVA INSTRUMENTS		ACTUAL PPMV					OVERALL														
NOMINAL PPMV	LOW	HIGH	MEAN	SE	N	MEAN	SE	N	1000	SE	4	2000	SE	N	1000	SE	N				
200	190	190	180	1.88	2	1.88	1.88	2	1.88	1.88	1	2.21	1.88	1	1.88	1.88	1	1.88			
700	876	876	876	1.67	2	1.67	1.67	2	1.67	1.67	1	1.41	1.67	1	1.67	1.67	1	1.67			
1200	1208	1208	1208	1.21	2	1.21	1.21	2	1.21	1.21	1	1.41	1.21	1	1.21	1.21	1	1.21			
OVERALL MEANS		1.70		0.01	6	1.62		0.22	3	1.76		0.22	3	1.76		0.22	3	1.76		0.22	3
ESTIMATED AT 10,000 PPMV		0.82																			

90% CONFIDENCE INTERVAL 4.000 1.171

ELV INSTRUMENTS		RESPONSE FACTORS																			
DVA INSTRUMENTS		ACTUAL PPMV					OVERALL														
NOMINAL PPMV	LOW	HIGH	MEAN	SE	N	MEAN	SE	N	76	SE	4	2000	SE	N	76	SE	N				
200	190	190	190	0.20	2	0.96	0.96	2	0.96	0.96	1	0.96	0.96	1	0.96	0.96	1	0.96			
700	876	876	876	1.55	2	1.55	1.55	2	1.55	1.55	1	1.37	1.55	1	1.55	1.55	1	1.55			
1200	1208	1208	1208	2.32	2	2.32	2.32	2	2.32	2.32	1	1.37	2.32	1	2.32	2.32	1	2.32			
OVERALL MEANS		1.70		0.07	6	1.14		0.62	3	0.96		0.27	3	0.96		0.27	3	0.96		0.27	3
ESTIMATED AT 10,000 PPMV		4.02																			

90% CONFIDENCE INTERVAL 4.110 20.481


Figure 5-5b

INSTRUMENT RESPONSE VS CONCENTRATION

CYCLORHEXANE

DVS ORGANIC VAPOR ANALYZER

TLV HYDROCARBON SNIFFER

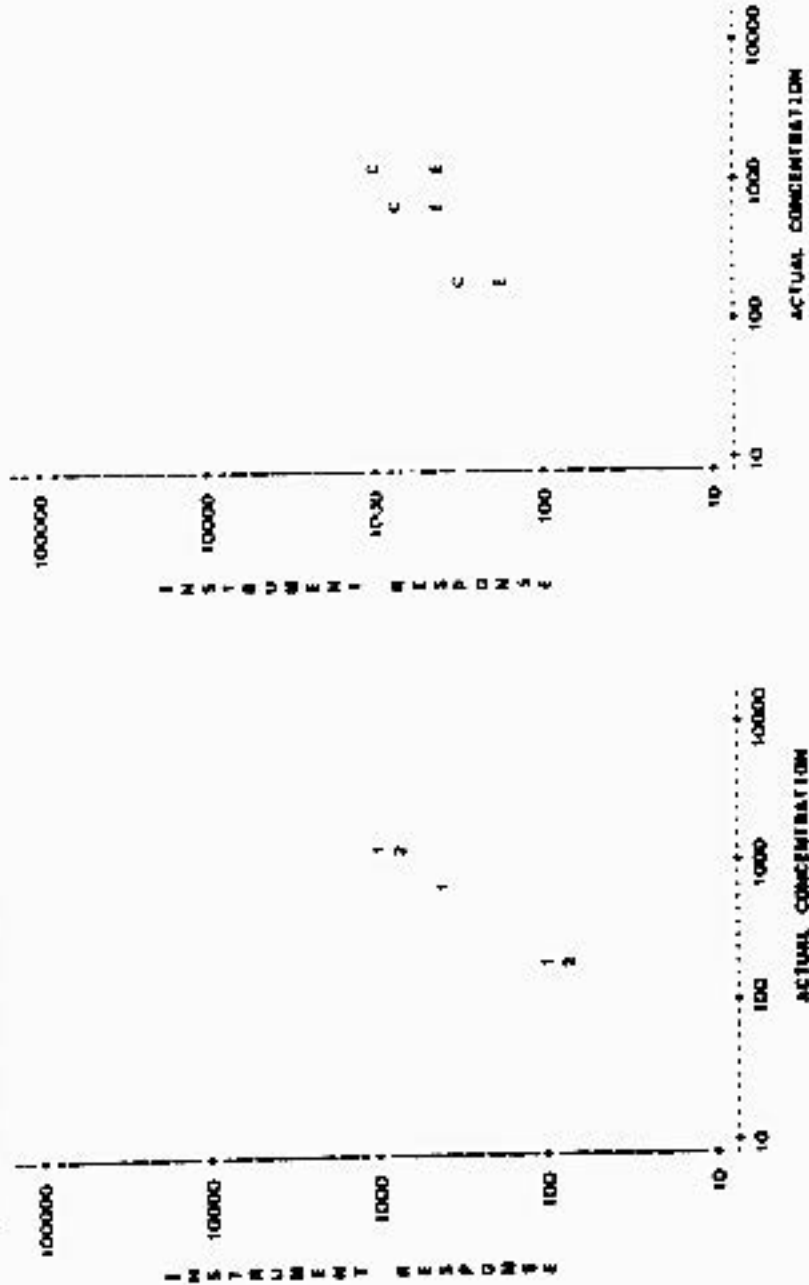

NOTE: 1 OBS MEMBER



TABLE 5-57

RESPONSE FACTOR SUMMARY

CYCLONERACHINE

DVA INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DVA METERS									
	LOW	HIGH	MEAN	SE	1000	SE	N	2254	SE	N	1413	SE	N	
200	189	189	1.43	0.28	2	1.22	1	1.22	1	1.22	1	1.22	1	
2000	2078	2078	1.82	0.08	2	1.74	1	1.90	1	1.90	1	1.90	1	
4000	4039	4039	1.33	0.02	2	1.31	1	1.32	1	1.32	1	1.32	1	
OVERALL MEANS			1.54	0.02	6	1.42	0.16	3	1.65	0.18	3	1.65	0.18	3

ESTIMATED AT 10,000 PPMV 1.50

95% CONFIDENCE INTERVAL (1.01, 2.22)

FIV INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		FIV METERS									
	LOW	HIGH	MEAN	SE	TE	SE	N	TC	SE	N	FN	SE	N	
200	189	189	1.90	0.60	2	2.09	1	0.90	1	0.90	1	0.90	1	
2000	2078	2078	2.91	0.76	2	3.88	1	2.18	1	2.18	1	2.18	1	
4000	4039	4039	3.47	1.07	2	4.88	1	2.40	1	2.40	1	2.40	1	
OVERALL MEANS			2.62	0.13	6	3.43	0.72	3	1.83	0.47	3	1.83	0.47	3

ESTIMATED AT 10,000 PPMV 3.99

95% CONFIDENCE INTERVAL (1.79, 6.91)


Figure 5-57

INSTRUMENT RESPONSE VS. CONCENTRATION

CYCLOHEXANONE

OVA ORGANIC VAPOR ANALYZER

11-V HYDROCARBON SNIFFER

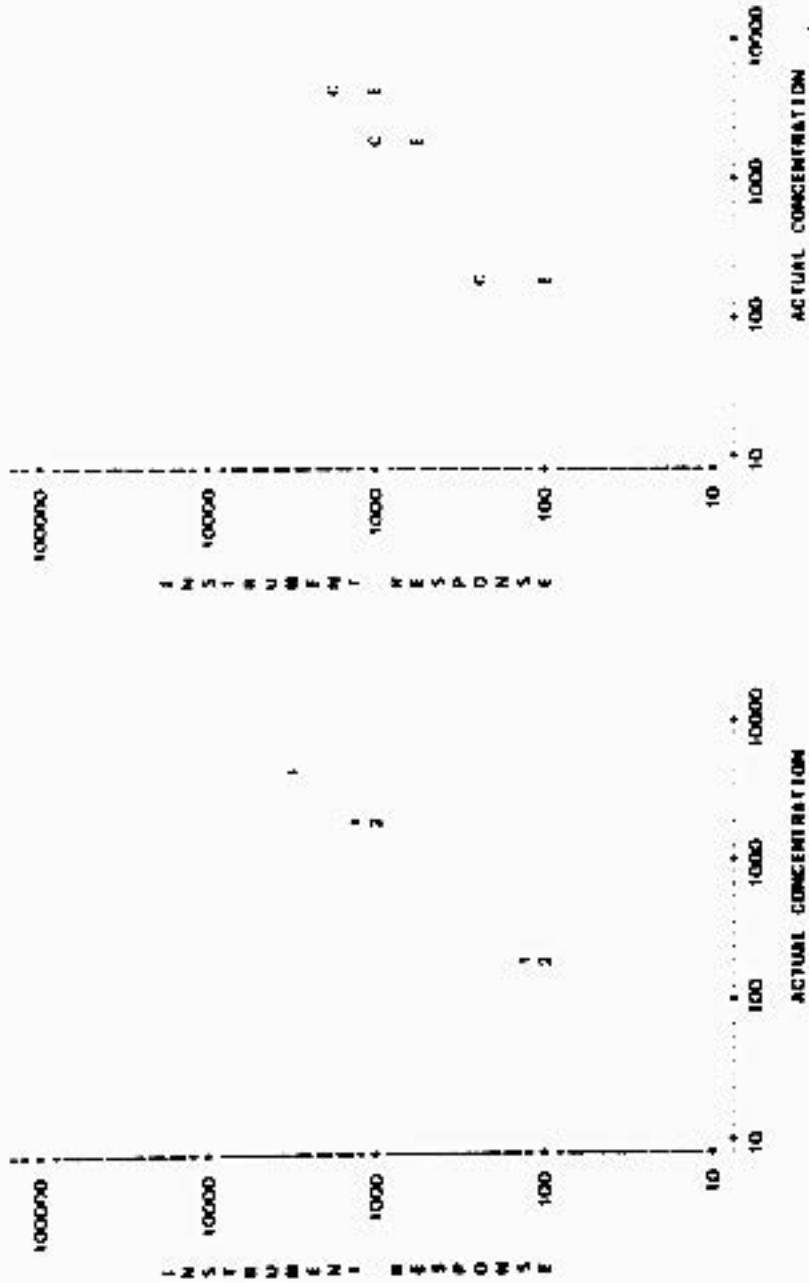

NOTE 1 CBS HIDDEN

TABLE 5.5A

RESPONSE FACTOR SUMMARY

CYCLOHEXANE		DESIGN FACTOR												
DVA INSTRUMENTS		OVERALL					DVA METERS							
NOMINAL PPMV	LDW	HIGH	MEAN	SE	N	10MED	SE	N	25%V	SE	N	50%V	SE	N
200	204	204	204	1.07	0.09	2	1.16	1	0.97	1	0.97	1	0.97	1
1500	1888	1888	1539	0.76	0.04	2	0.76	1	0.72	1	0.72	1	0.72	1
3000	3320	3320	3320	0.53	0.03	2	0.49	1	0.54	1	0.54	1	0.54	1
4000	4238	4238	4238	0.48		1			0.48				0.48	
6000	6008	6008	6008											
8000	8074	8074	8074											
OVERALL MEANS		0.33	0.04	3	0.67	0.11	4							
ESTIMATED AT 10,000 PPMV		0.40												
DESIGN FACTOR		DESIGN FACTOR												
11V INSTRUMENTS		OVERALL					11V METERS							
NOMINAL PPMV	LDW	HIGH	MEAN	SE	N	75%	SE	N	70%	SE	N	50%	SE	N
200	204	204	204	0.84	1				0.84	1			0.84	1
1500	1888	1888	1569	1.13	1				1.13	1			1.13	1
3000	3320	3320	3320	1.44	1				1.44	1			1.44	1
4000	4238	4238	4238	1.44	1				1.44	1			1.44	1
6000	6008	6008	6008	1.77	1				1.77	1			1.77	1
8000	8074	8074	8074	1.88	1				1.88	1			1.88	1
OVERALL MEANS		1.42	0.16	6					1.42	0.16	6			
ESTIMATED AT 10,000 PPMV		1.84							1.84					

FIGURE 5-5B

INSTRUMENT RESPONSE VS. CONCENTRATION

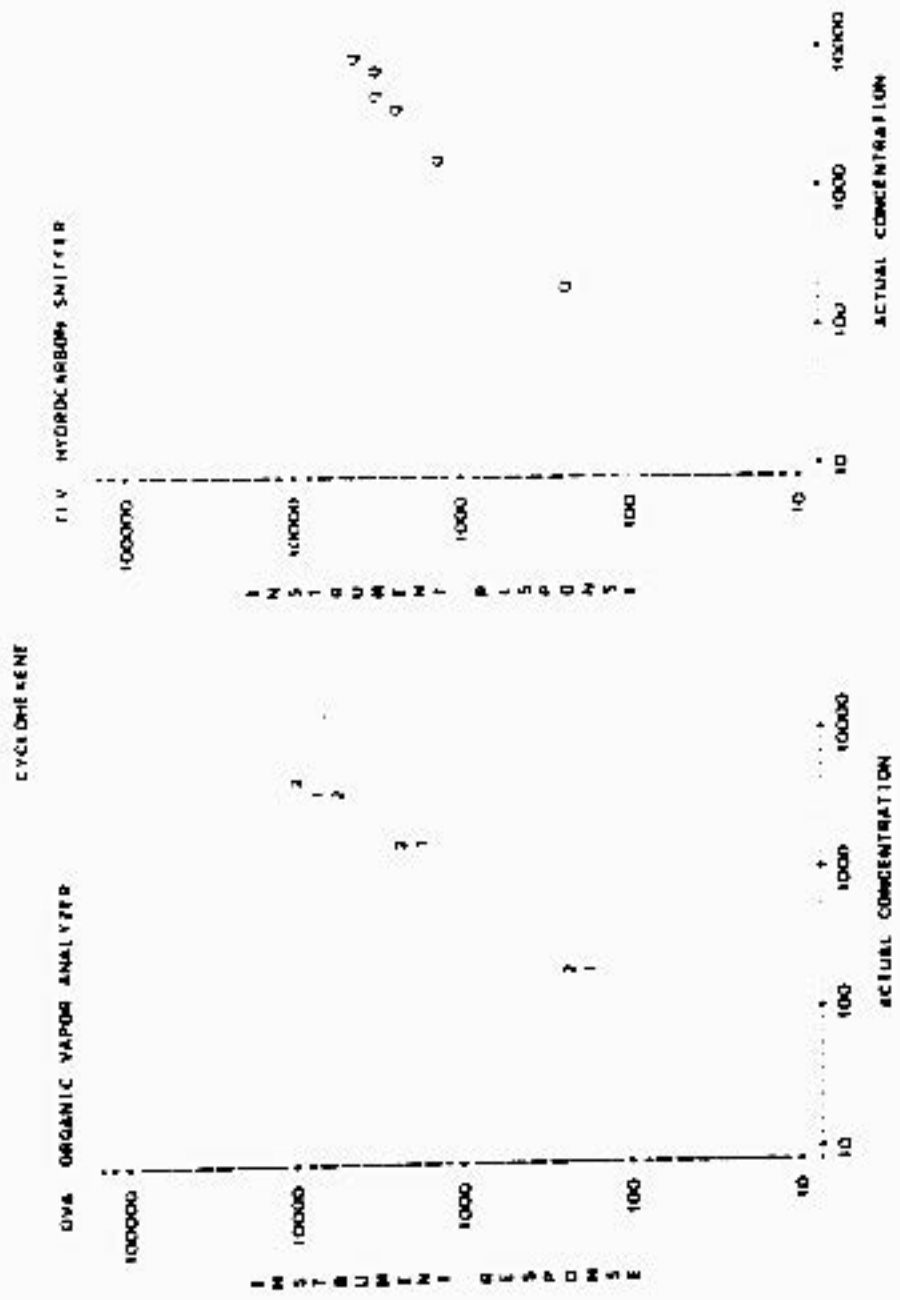


TABLE 5.5)

RESPONSE FACTOR SUMMARY

CYCLONE RELATIME

DVA INSERTMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTORS									
	LOW	HIGH	MEAN	SE	N	10SD	SE	N	2254	SE	N	1013	SE	N
200	212	212	1.73	0.26	2	1.99	1	1.42	1	1.42	1	1.44	1	1.44
1500	1725	1725	1.15	0.19	2	1.34	1	0.87	1	0.87	1	1.28	1	1.28
4000	4488	4488	0.58	0.03	2	0.52	1	0.56	1	0.56	1	1.44	1	1.44
8000	8478	8478												

OVERALL MEANS 1.14 D.02 6 1.28 0.42 2 1.00 0.78 2

ESTIMATED AT 10,000 PPMV 0.47

95% CONFIDENCE INTERVAL 1.0 28 1.0 791

FIV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTORS									
	LOW	HIGH	MEAN	SE	N	7E	SE	N	7C	SE	N	7M	SE	N
200	212	212	1.44		1									
1500	1725	1725	1.38		1									
4000	4488	4488	1.28		1									
8000	8478	8478	1.25		1									

OVERALL MEANS 1.40


ESTIMATED AT 10,000 PPMV 1.38

95% CONFIDENCE INTERVAL 1.1 31 1.451

Figure 5-59

INSTRUMENT RESPONSE VS CONCENTRATION

CYCLOHEXANAMINE

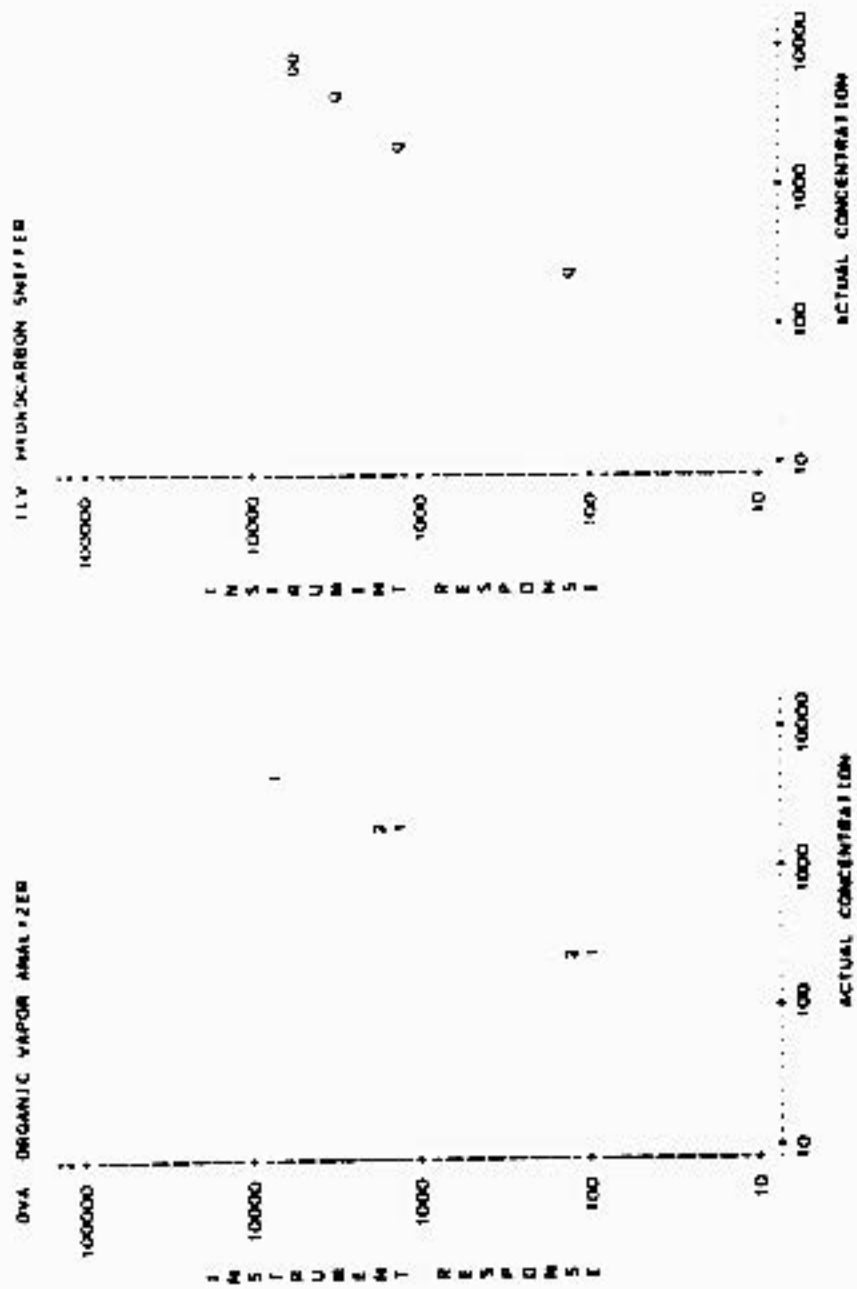

NOTE: 1 OBS. HIGHEN

TABLE 5-40

RESPONSE FACTOR SUMMARY

DECANE

OVA INSTRUMENTS

8 5 P 0 4 5 1 1 0 0 5

ACTUAL PPMV

OVERALL

OVA METERS

2 204 5 1 2 10 5 1 1 0 0 5

NOMINAL PPMV	LOW	HIGH	MEAN	SE	M	1000	SE	M	2204	SE	N	2100	SE	M	1000	SE	M
200	188	188	188	1.80	2	0.88	1	12.57	1								
300	300	300	300	0.87	2	0.87	1	0.98	1								
400	438	438	438	1.30	2	1.30	1	2.12	1								
OVERALL MEANS		440	440	1.40	6	3.88	3	5.27	3	5.27	3	5.27	3	5.27	3	5.27	3

ESTIMATED AT 10,000 PPMV 0.00

95 % CONFIDENCE INTERVAL 1 0 00 7.313

11V INSTRUMENTS

8 5 P 0 4 5 1 1 0 0 5

ACTUAL PPMV

OVERALL

11V METERS

2 204 5 1 2 10 5 1 1 0 0 5

NOMINAL PPMV	LOW	HIGH	MEAN	SE	M	1000	SE	M	2204	SE	N	2100	SE	M	1000	SE	M
200	188	480	334	2.92	2	2.92	1	2.17	1								
300	300	300	300	1.25	2	1.25	1	0.76	1								
400	438	438	438	2.12	2	2.12	1	1.32	1								
OVERALL MEANS		308	308	2.10	6	2.10	3	1.42	3	1.42	3	1.42	3	1.42	3	1.42	3

ESTIMATED AT 10,000 PPMV 0.70

95 % CONFIDENCE INTERVAL 1 0 00 11.017

Figure 5-640

INSTRUMENT RESPONSE VS CONCENTRATION

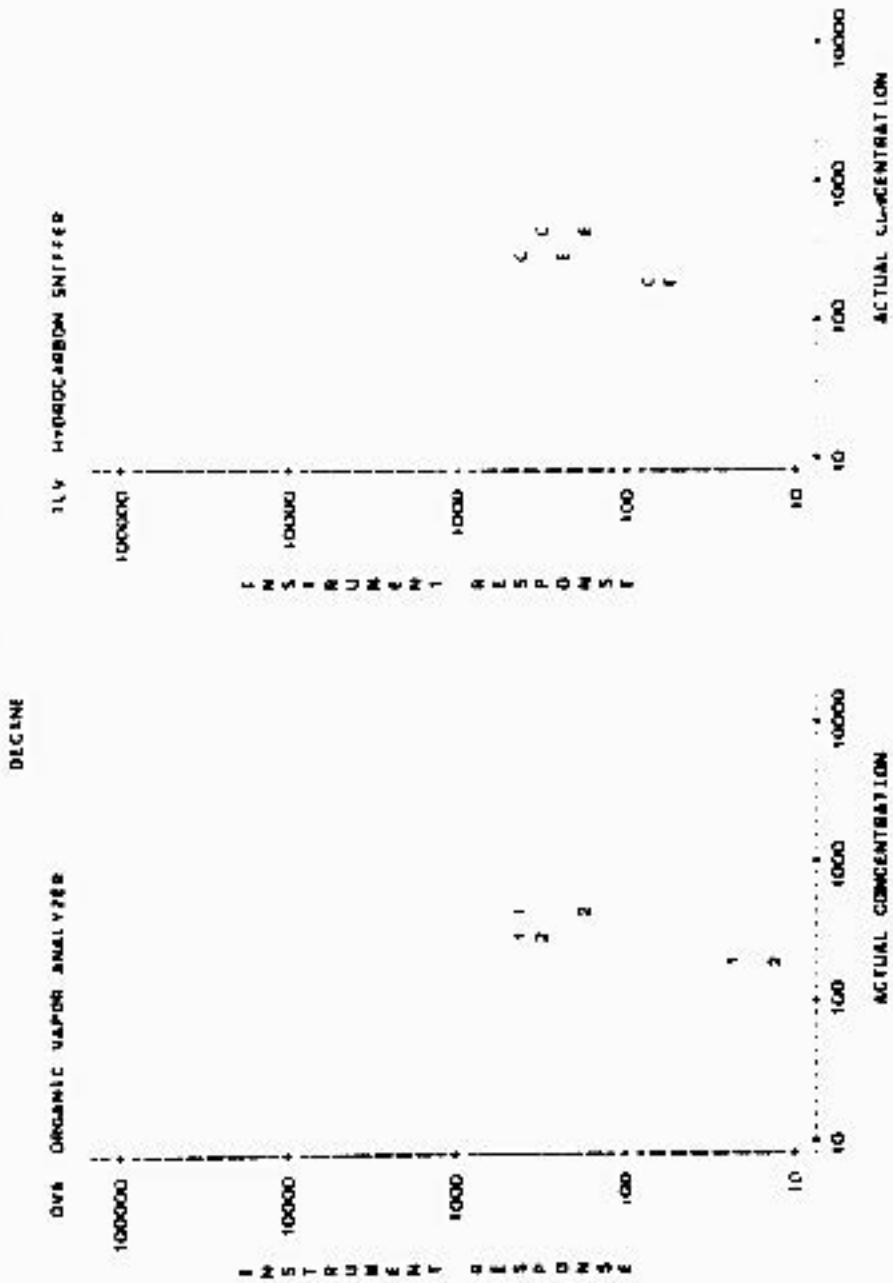




TABLE 5-61

RESPONSE FACTOR SUMMARY

GLACIATION ALCOHOL

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			RESPONSE FACTORS														
	LOW	HIGH	MEAN	SE	M	1000	SE	N	2004	SE	N	2100	SE	N	1817	SE	N	
200	227	227	227	2.80	0.18	2	2.41	1	2.80	1	2.80	1	2.80	1				
1500	793	793	793	2.44	0.18	2	2.28	1	2.60	1	2.60	1	2.60	1				
8000	1387	1387	1387	1.83	0.07	2	1.88	1	2.00	1	2.00	1	2.00	1				
OVERALL MEANS				2.22	0.02	6	2.18	0.13	3	2.48	0.24	3						

ESTIMATED AT 10,000 PPMV 1.03

95% CONFIDENCE INTERVAL 1.01 - 2.01

11V INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			RESPONSE FACTORS														
	LOW	HIGH	MEAN	SE	M	TE	SE	M	TC	SE	M	TM	SE	M	TD	SE	M	
200	427	227	223	2.64	0.82	2	2.25	1	2.02	1	2.02	1	2.02	1				
1500	793	793	793	2.36	0.71	2	2.97	1	1.55	1	1.55	1	1.55	1				
8000	1387	1387	1387	1.60	0.28	2	1.88	1	1.27	1	1.27	1	1.27	1				
OVERALL MEANS				2.10	0.09	6	2.10	0.42	3	1.82	0.21	3						

ESTIMATED AT 10,000 PPMV 0.98

95% CONFIDENCE INTERVAL 0.79 - 1.05



TABLE 5-62

RESPONSE FACTOR SUMMARY

DIACETYL

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS									
	LOW	HIGH	MEAN	MEAN	SE	N	100%	5%	N	2.5%	SE	N	10%	5%	N	
500	68	70	69	3.19	0.13	4	3.07	0.22	2	3.36	0.15	2				
5000	68	68	68	2.03	0.05	4	2.08	0.46	2	1.00	0.13	4				
8000	6560	6730	6645	1.79	0.23	4	2.01	0.29	2	1.51	0.34	2				
OVERALL MEANS			2.24	0.00	12	2.37	0.23	6	2.30	0.25	6					
ESTIMATED AT 10,000 PPMV ± 0.1																
95% CONFIDENCE INTERVAL																

1,1-DICHLOROETHANE

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS									
	LOW	HIGH	MEAN	MEAN	SE	N	100%	5%	N	2.5%	SE	N	10%	5%	N	
500	68	70	69	1.40	0.16	4	1.64	0.27	2	1.28	0.19	2				
5000	68	68	68	2.28	0.42	4	2.11	0.21	2	1.85	0.14	2				
8000	6560	6730	6645	2.87	0.61	4	2.54	0.57	2	2.19	0.24	2				
OVERALL MEANS			2.20	0.04	12	2.62	0.20	6	1.68	0.19	6					
ESTIMATED AT 10,000 PPMV ± 0.1																
95% CONFIDENCE INTERVAL																

FIGURE 5-62  
 INSTRUMENT RESPONSE VS CONCENTRATION

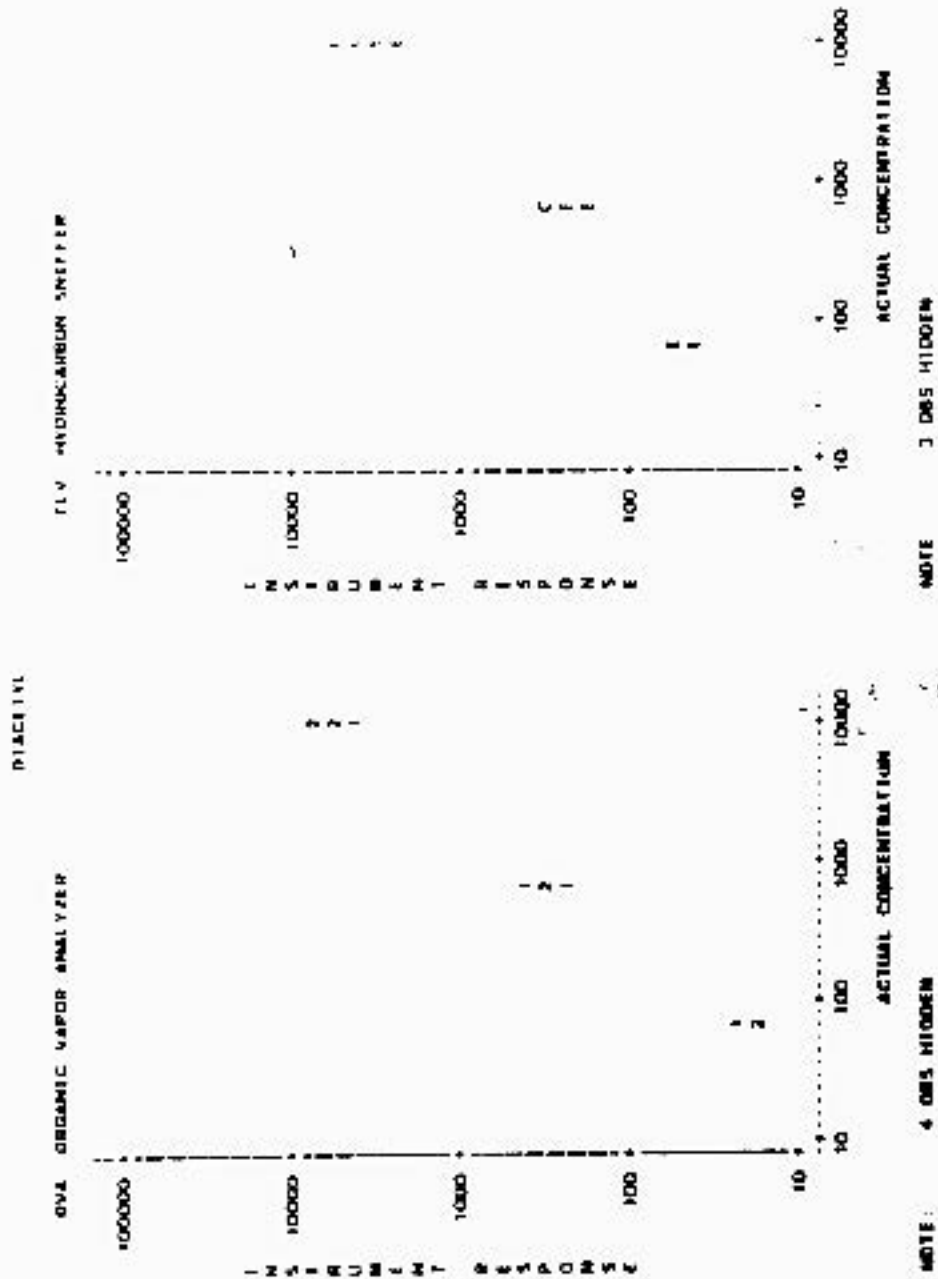


TABLE 5-13

RESPONSE FACTOR SUMMARY

DIVISIONS FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DIVISIONS								
	LOW	HIGH	MEAN	SE	N	1000	SE	N	2204	SE	N	1819	N	N	
200	812	212	212	03	10	17	7	25	40	1	70	40	1	70	
1500	1488	1488	1488	38	30	8	19	7	21	03	1	41	27	1	
8000	8470	8470	8470	81	48	1	37	7	83	04	1	39	81	1	
OVERALL MEANS			96	52	1	18	6	49	82	10	3	84	03	11	3

ESTIMATED AT 10,000 PPMV 61 51

95% CONFIDENCE INTERVAL (30 13 129 51)

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DIVISIONS									
	LOW	HIGH	MEAN	SE	N	14	SE	N	14	SE	N	10	SE	N		
200	212	212	212	3	52	0	36	2	2	88	1	2	16	1		
1500	1488	1488	1488	10	46	3	33	2	12	82	1	8	17	1		
8000	8470	8470	8470	50	83	4	58	2	35	41	1	26	20	1		
OVERALL MEANS			14	61	0	40	6	17	03	9	82	3	12	19	1	24


ESTIMATED AT 10,000 PPMV 34 34

90% CONFIDENCE INTERVAL (27 80 49 53)

Figure 5-63

INSTRUMENT RESPONSE VS CONCENTRATION

MICHLORD I PROGRAM 2.3

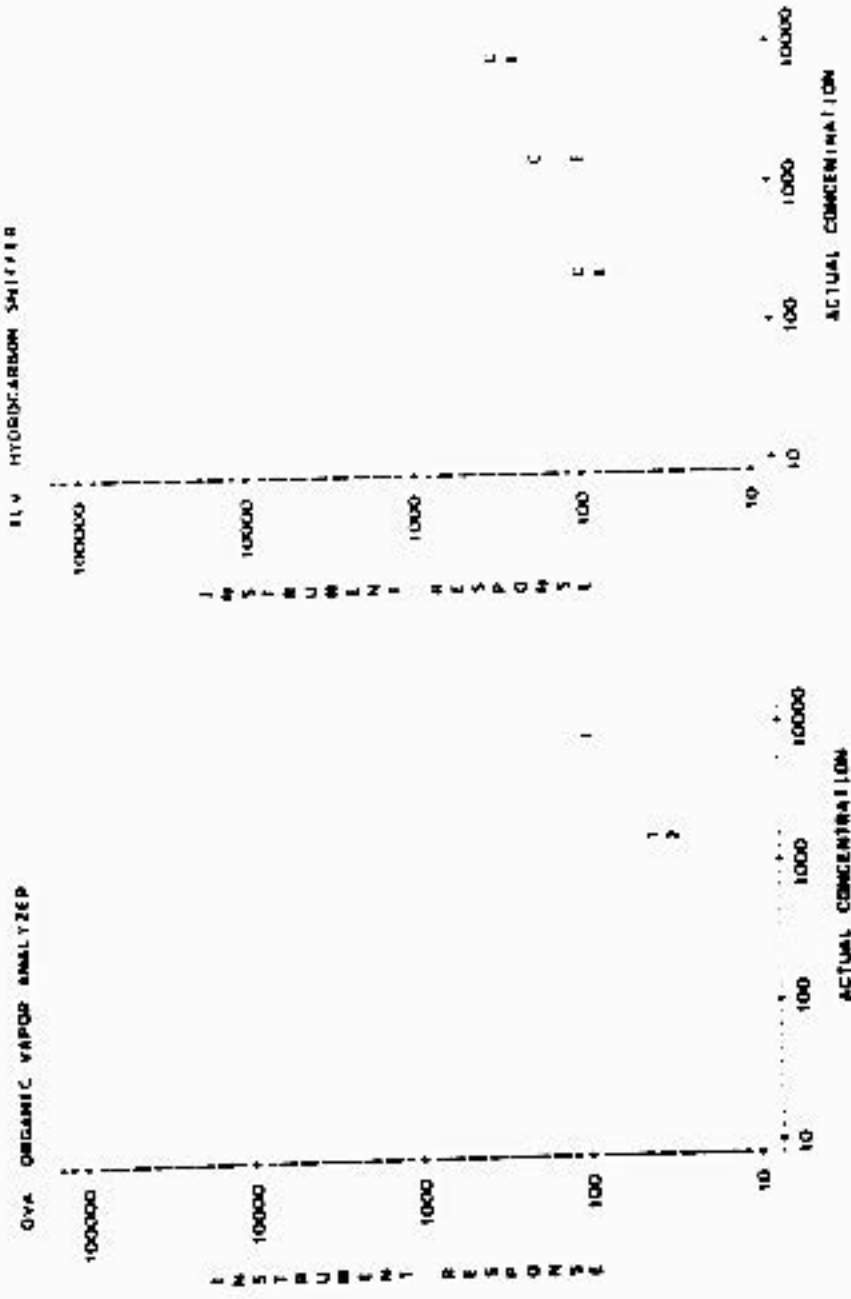

NOTE: 1 OBS MISSING OR OUT OF RANGE

TABLE 5-14

RESPONSE FACTOR SUMMARY

DELETERIOUS PARTICULATE

GVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY							
	LOW	HIGH	MEAN	SE	N	100%	5%	4%	220%	SE	N	215%	SE	N
200	206	206	206	1.70	0.07	2	1.82	1	1.77	1	1	1.77	1	1
1500	1518	1518	1518	1.40	0.07	2	1.26	1	1.02	1	1	1.02	1	1
5000	5177	5177	5177	0.74	0.04	2	0.67	1	0.76	1	1	0.76	1	1
8000	8093	8093	8093											

OVERALL MEANS: 1.30 0.14 6 1.23 0.20 3 1.30 0.11 1

ESTIMATED AT 10 000 PPMV: 0.70

95% CONFIDENCE INTERVAL: 1.04 1.05

FLY INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY							
	LOW	HIGH	MEAN	SE	N	100%	5%	4%	220%	SE	N	215%	SE	N
200	206	206	206	0.88	1	0.88	1	0.88	1	1	0.88	1	1	1
1500	1518	1518	1518	1.59	1	1.59	1	1.59	1	1	1.59	1	1	1
5000	5177	5177	5177	0.58	0.06	2	0.58	1	0.47	1	1	0.47	1	1
8000	8093	8093	8093	1.39	1	1.39	1	1.39	1	1	1.39	1	1	1

OVERALL MEANS: 1.38 0.07 5 1.59 1.16 1 1.16 1.16 1

ESTIMATED AT 10 000 PPMV: 1.62

95% CONFIDENCE INTERVAL: 1.22 1.41


Figure 5-44

INSTRUMENT RESPONSE VS CONCENTRATION

DICHLORO & PROPENE 7 J

DVA ORGANIC VAPOR ANALYZER

ELV HYDROCARBON SNIFFLER

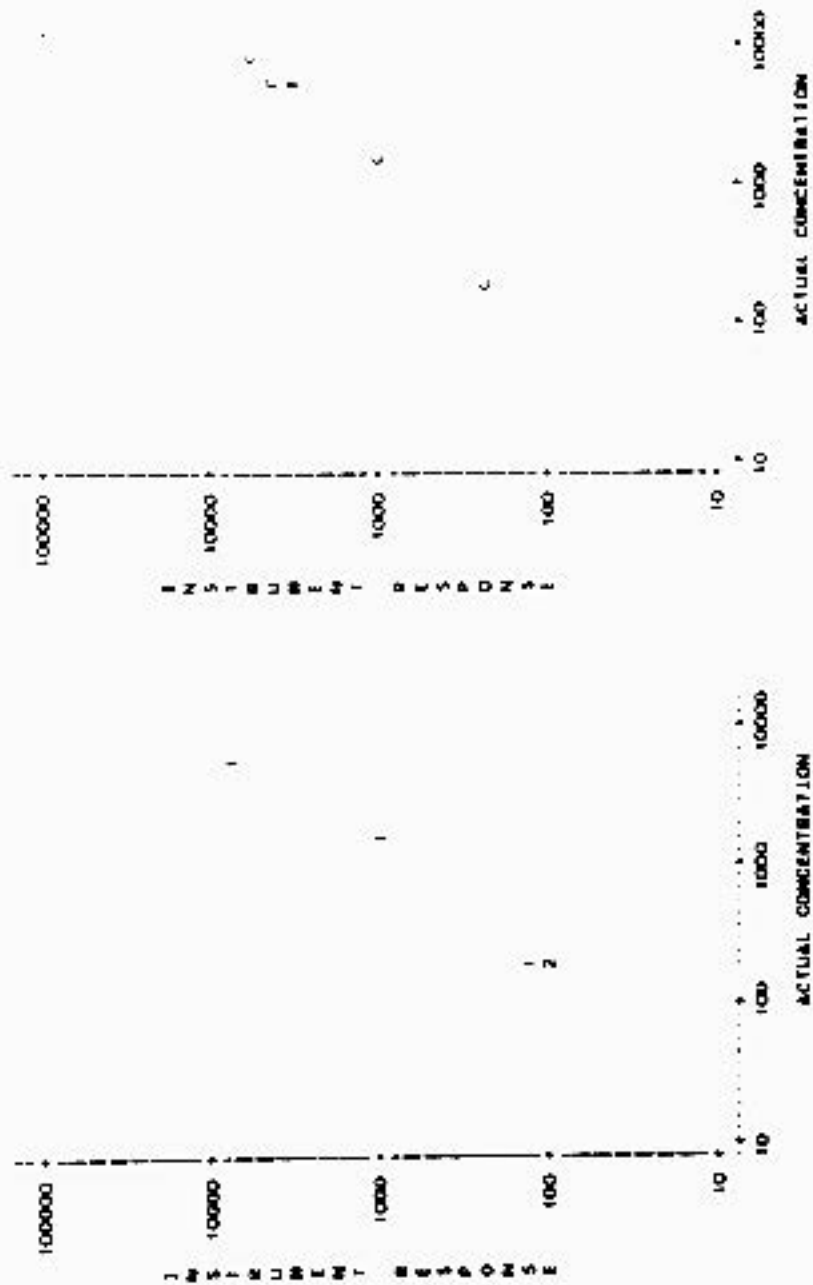

NOTE 3 DBS HIDDEN



TABLE 5.65

RESPONSE FACTOR SUMMARY

DELETED 2 PREPARATION 1 1

DATA INSTANCES

SCHEMATA PPMV	ACTUAL PPMV			OVERALL			95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	SE	N	SCHEMATA	SE	N	25%	50%	75%	95%
2000	224	224	224	13.22	2	10	43	1	10	10	1	10
4000	1427	1427	1427	11.30	2	14	14	1	14	14	1	14
6000	5225	5225	5225	20.98	2	18	18	1	18	18	1	18
8000	1960	1960	1960	20.07	2	24	42	1	24	24	1	24
OVERALL MEANS			22.64	4.76	8	20.53	8.01	4	24.75	5.87	8	

ESTIMATED AT 95% CONFIDENCE INTERVAL

DATA INSTANCES

SCHEMATA PPMV	ACTUAL PPMV			OVERALL			95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	SE	N	SCHEMATA	SE	N	25%	50%	75%	95%
2000	224	224	224	6.92	2	2	13	1	4	10	1	10
4000	1427	1427	1427	6.75	2	6	46	1	1	52	1	52
6000	5225	5225	5225	17.24	2	18	64	1	15	85	1	85
8000	1960	1960	1960	19.09	2	24	11	1	16	31	1	31
OVERALL MEANS			17.38	11.15	8	13.23	10.04	4	11.52	8.21	8	

ESTIMATED AT 95% CONFIDENCE INTERVAL


Figure 5-85

INSTANTANEOUS RESPONSE VS CONCENTRATION

DICHLOROPROPANE 1,1

QVA ORGANIC VAPOR ANALYZER

FLV \*\*\*DRY CARBON SNIFFER

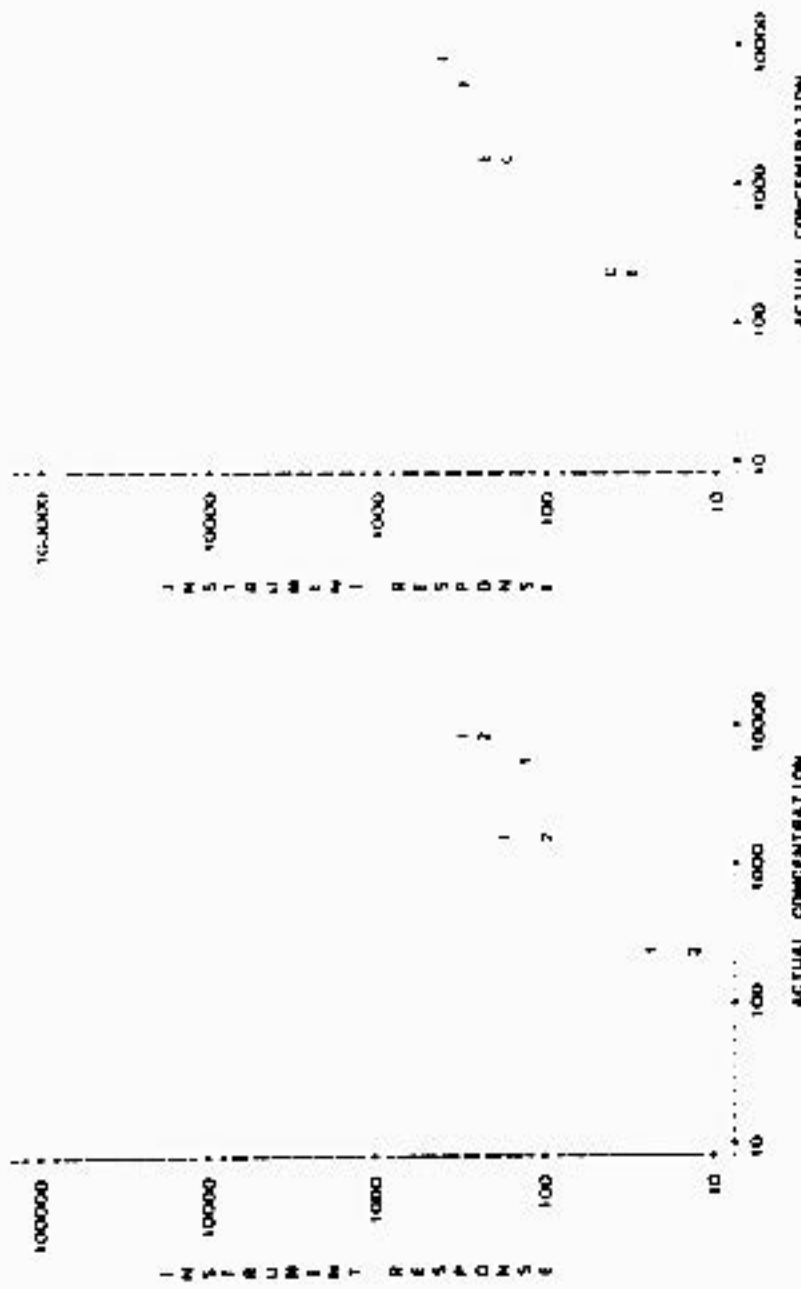

NOTE 1 USE MIDDLEM

NOTE 2 USE MIDDLEM

TABLE 5.166

MEASURE FACTOR SUMMARY

DECAHORIENZERE III

DVA INSTRUMENTS		H I S P O R N S E F A C T O R S														
NOMINAL PUMP	LOW HIGH	ACTUAL PUMP					DVA METERS									
		MEAN	ST	SE	95% U	95% L	M	2284 SE	N	2159 SE	N	2011 SE	N			
2000	201	201	0.01	0.00	2	0.01	1	0.01	1							
10000	10000	10000	0.09	0.00	2	0.08	1	0.09	1							
20000	1985	1985	0.08	0.04	2	0.07	1	0.08	1							
OVERALL MEANS		0.56	0.00	0.00	6	0.58	0.03	0.58	0.02	1						
ESTIMATED AT 10000 PUMP		0.06									95% CONFIDENCE INTERVAL 1.056 0.781					


SLV INSTRUMENTS

SLV INSTRUMENTS		H I S P O R N S E F A C T O R S														
NOMINAL PUMP	LOW HIGH	ACTUAL PUMP					SLV METERS									
		MEAN	ST	SE	95% U	95% L	M	20 SE	N	20 SE	N	20 SE	N			
2000	201	201	0.10	0.10	1											
10000	10000	10000	0.99	0.99	1											
20000	1985	1985	1.28	1.28	1											
OVERALL MEANS		0.99			3											
ESTIMATED AT 10000 PUMP		1.00									95% CONFIDENCE INTERVAL 1.117 0.811					

Figure 5-6b

INSTRUMENT RESPONSE VS CONCENTRATION

DICHA DIBROMBENZENE M 1% HYDROCLARBDM SAITFER

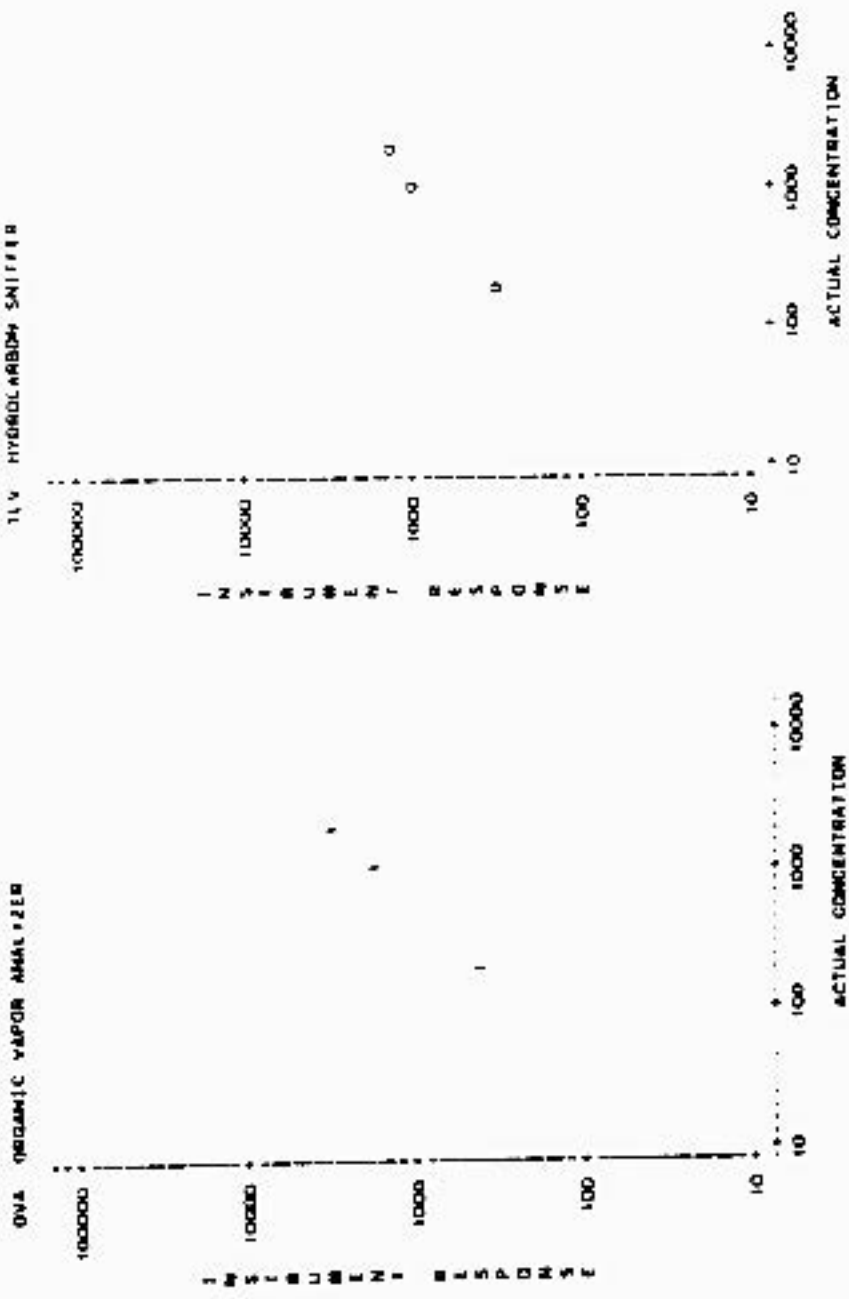

NOTE 2 OBS HIDDEN

TABLE 1-6

RESPONSE FACTOR SUMMARY

DECA COMBINEMENTS

DATA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DATA INSTRUMENTS											
	LOW	HIGH	MEAN	SE	N	10001	51	N	2254	51	N	2154	51	N	1814	51
200	212	212	212	0.00	0.02	2	U	48	1	0.02	1					
700	707	707	707	0.01	0.03	2	0	58	1	0.05	1					
1200	1219	1219	1219	0.00	0.03	2	0	53	1	0.05	1					
OVERALL MEANS			0.96	U	0.02	4	0	53	0.02	1	0.04	1				

ESTIMATED AT 10,000 PPMV 0.10

95% CONFIDENCE INTERVAL 1.000 1.011

11V INSTRUMENTS


NOMINAL PPMV	ACTUAL PPMV		OVERALL		DATA INSTRUMENTS											
	LOW	HIGH	MEAN	SE	N	71	51	N	74	51	N	76	51	N	70	51
200	212	212	212	0.72	1											
700	707	707	707	0.90	1											
1200	1219	1219	1219	0.88	1											
OVERALL MEANS			0.84	1												

ESTIMATED AT 10,000 PPMV 1.22

95% CONFIDENCE INTERVAL 1.080 1.061

Figure 5-67

INSTRUMENT RESPONSE VS. CONCENTRATION  
DICHLOROBENZENE D

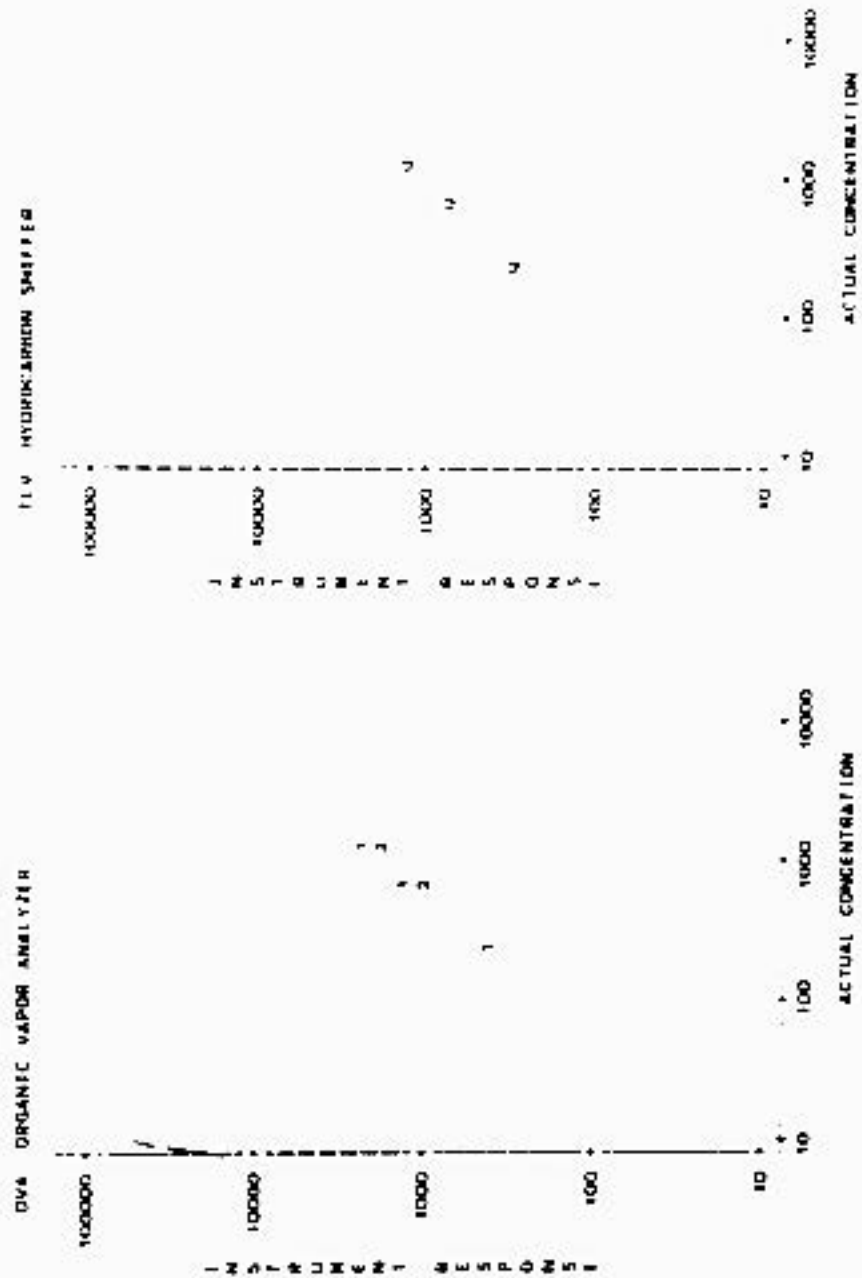

NOTE: 1 DBS HIDDEN

TABLE 5.6B

RESPONSE FACTOR SUMMARY

DECAURGE RANGE 1.1

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY												
	LOW	HIGH	MEAN	MEAN	SE	N	10SD	5B	N	2254	SE	N	215M	SE	N	18+3	SP	N	
200	221	221	221	0.00	0.14	2	0.75		1	1.00		1							
1000	1498	1498	1498	0.01	0.08	2	0.73		1	0.88		1							
5000	9870	9870	9870	0.80	0.00	2	0.80		1	0.80		1							
8000	7838	7838	7838																
OVERALL MEANS			0.82	0.01	8	0.16	0.02	1	0.80	0.07	1								
ESTIMATED AT 10,000 PPMV			0.77																

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY												
	LOW	HIGH	MEAN	MEAN	SE	N	7E	5E	N	1L	SE	N	1M	5L	N	7U	5M	N	
200	221	221	221	1.82	0.27	2	1.79		1	1.28		1							
1000	1498	1498	1498	1.87	0.04	2	1.71		1	1.61		1							
5000	9870	9870	9870	1.81	0.00	2	1.81		1	1.80		1							
8000	7838	7838	7838	1.74	0.00	2	1.74		1	1.75		1							
OVERALL MEANS			1.80	0.01	8	1.16	0.02	4	1.61	0.12	4								
ESTIMATED AT 10,000 PPMV			1.80																

Figure 5.6B

INSTRUMENT RESPONSE VS. CONCENTRATION



Figure 3.4A

INCUBATION PERIODS OF 1000 PARTICLES

PERCENTAGE INACTIVE

PERCENTAGE INACTIVE

PERCENTAGE INACTIVE

10000

10000

10000  
10000  
10000  
10000  
10000  
10000  
10000  
10000  
10000  
10000

10000  
10000  
10000  
10000  
10000  
10000  
10000  
10000  
10000  
10000

10

10

10000

10000

10000

10000

10000

10000

10000

4.11e-004

4.11e-004

4.11e-004

4.11e-004

10000

10000

10000

10000

10000



TABLE 3-47

RESPONSE FACTOR SUMMARY

DICOM DURETANE 1-2

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR SUMMARY													
	LOW	HIGH	MEAN	SE	N	MEAN	SE	N	2.5% CL	50% CL	97.5% CL	N	2.5% CL	50% CL	97.5% CL	N		
200	208	206	207	0.03	2	1.01	1	1.01	1	1.01	1	1.01	1	1.01	1	1.01	1	
1500	1579	1579	1579	0.02	2	1.22	1	1.17	1	1.17	1	1.17	1	1.17	1	1.17	1	
6000	6013	6013	6013	0.00	2	0.89	1	0.89	1	0.89	1	0.89	1	0.89	1	0.89	1	
OVERALL MEANS					1.04	0.00	6	1.04	0.00	3	1.04	0.00	3	1.04	0.00	3	1.04	0.00

ESTIMATED AT 10,000 PPMV 0.95

95% CONFIDENCE INTERVAL 1.00 TO 1.08

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR SUMMARY													
	LOW	HIGH	MEAN	SE	N	MEAN	SE	N	2.5% CL	50% CL	97.5% CL	N	2.5% CL	50% CL	97.5% CL	N		
200	206	208	207	0.24	2	1.48	1	1.50	1	1.50	1	1.50	1	1.50	1	1.50	1	
1500	1579	1579	1579	0.06	2	2.14	1	2.03	1	2.03	1	2.03	1	2.03	1	2.03	1	
6000	6013	6013	6013	0.01	2	2.01	1	2.02	1	2.02	1	2.02	1	2.02	1	2.02	1	
OVERALL MEANS					1.94	0.02	6	1.94	0.02	3	1.94	0.02	3	1.94	0.02	3	1.94	0.02

ESTIMATED AT 10,000 PPMV 2.08

95% CONFIDENCE INTERVAL 1.91 TO 2.01


FIGURE 5-69

INSTRUMENT RESPONSE VS CONCENTRATION

(ELECTRONIC FILTER 1, 2)

DVA ORGANIC VAPOR ANALYZER

1, 2 HYDROCARBON ANALYZER

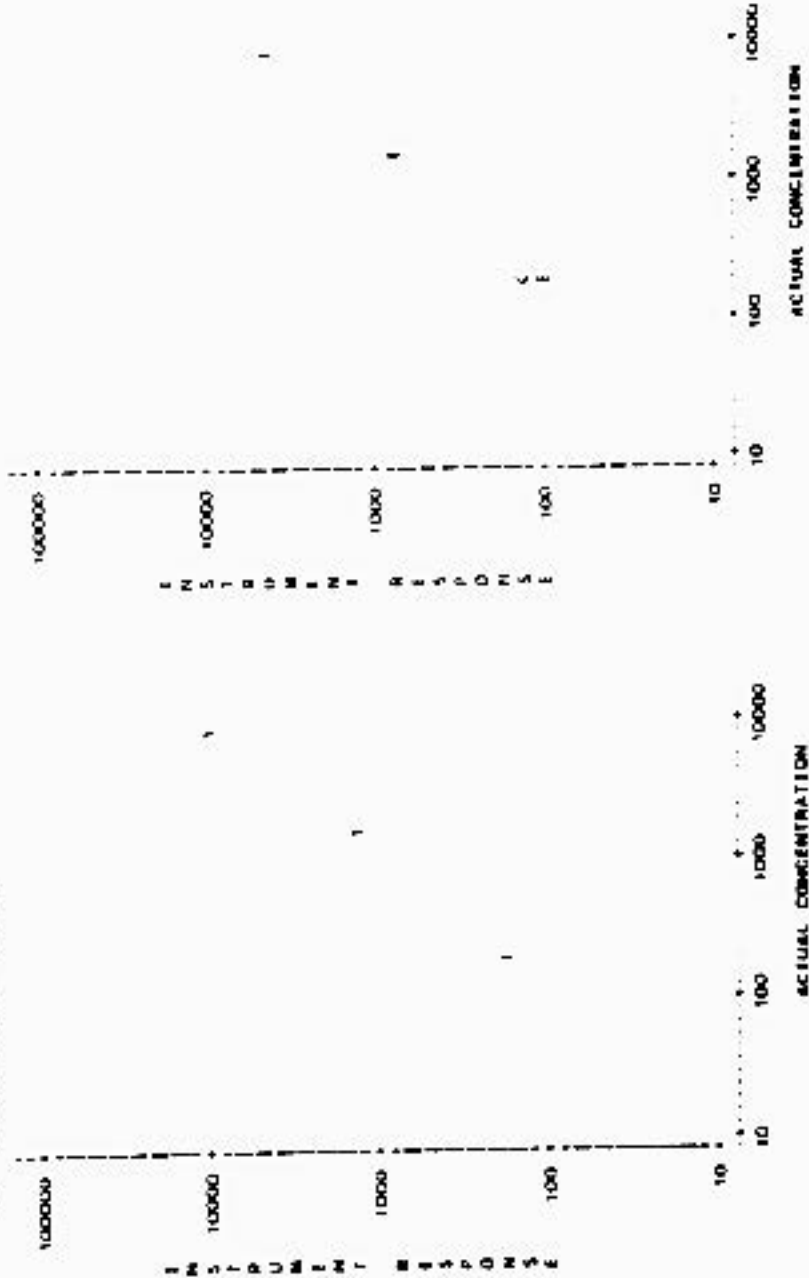

NOTE 3 OBS HIDDEN

NOTE 3 OBS HIDDEN

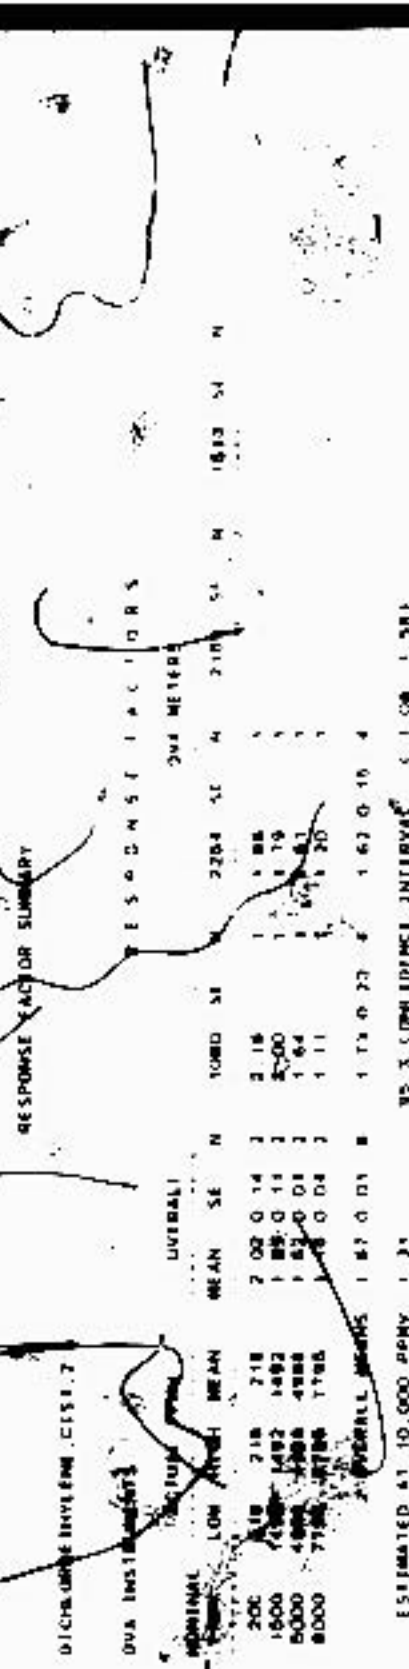


TABLE 5-70  
RESPONSE FACTOR SUMMARY

NOMINAL PPMV	LOW		MEAN		SE		N		1000		SE		N		1800		SE		N		
	LOW	HIGH	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	
200	218	218	7.02	0.14	2	2	2.18	1	1.88	1	2284	2284	210	1833	54	1833	54	1833	54	1833	54
1500	1492	1492	1.88	0.11	3	3	5.00	1	1.19	1											
5000	4988	4988	1.82	0.08	3	3	1.64	1	1.81	1											
8000	7786	7786	1.18	0.04	3	3	1.11	1	1.20	1											
OVERALL MEANS		1.87	0.03	8	8	1.73	0.23	4	1.62	0.16	4										

ESTIMATED AT 10,000 PPMV 1.31 MS X CONFIDENCE INTERVAL 6.108 1.581

TABLE 5-71  
RESPONSE FACTORS


NOMINAL PPMV	LOW		MEAN		SE		N		1000		SE		N		1800		SE		N	
	LOW	HIGH	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE
200	218	218	10.70	0.00	2	2	4.20	1	11.29	1										
1500	1492	1492	4.11	1.48	3	3	2.63	1	5.60	1										
5000	4988	4988	2.76	0.07	3	3	2.43	1	2.29	1										
8000	7786	7786	2.92	0.55	3	3	3.38	1	3.47	1										
OVERALL MEANS		5.04	0.27	8	8	7.01	0.43	4	7.10	0.45	4									

ESTIMATED AT 10,000 PPMV 1.93 MS X CONFIDENCE INTERVAL 5.102 1.661

Figure 5-711

INSTRUMENT RESPONSE VS. CONCENTRATION

DICHLOROPHENYLENE C1513

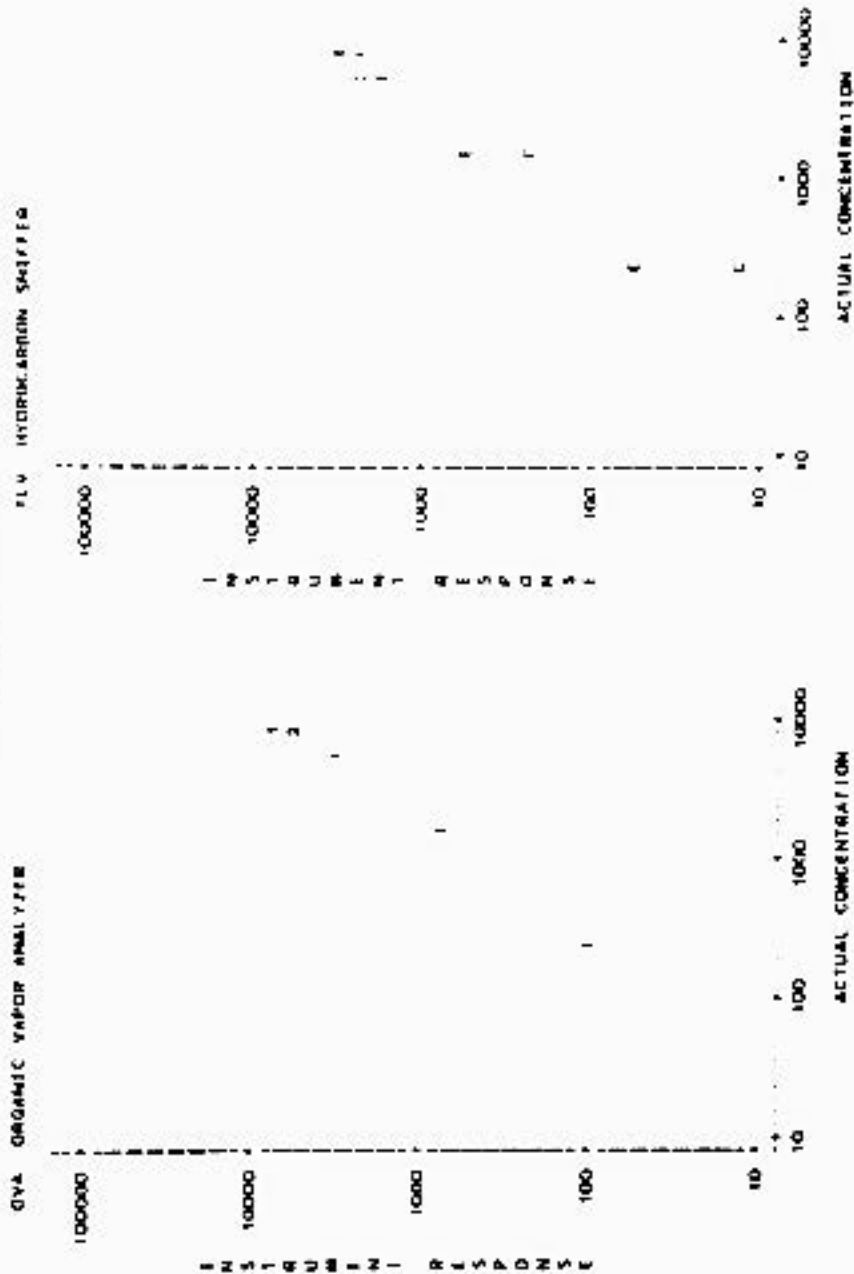

NOTE: 3 LABS HIDDEN

TABLE 5-71

RESPONSE FACTOR SUMMARY

DELTA DIBENZOPHLENE IONS 7

GVA INSTRUMENTS		UNIT SPONSOR LABORATORY												
NOMINAL PPMV	LOW HIGH	ACTUAL PPMV		OVERALL					GVA METERS					
		MEAN	SE	MEAN	SE	SD	N	27%	51%	78%	95%	INTERVAL		
250	225	235	235	2.20	0.04	2	2.31				1	2.12		
500	417	617	617	2.16	0.08	2	2.08				1	2.14		
1500	1404	1404	1404	1.81	0.07	2	1.88				1	1.14		
6000	7893	7893	7893	1.14	0.04	2	1.18				1	1.10		
OVERALL MEANS		1.85	0.02	1.88	0.24	4	1.83	0.27	4					

ESTIMATED AT 10 000 PPMV 1.13

95% COMPLIANCE INTERVAL 1.00N 1.80D

TIV INSTRUMENTS

TIV INSTRUMENTS		UNIT SPONSOR LABORATORY												
NOMINAL PPMV	LOW HIGH	ACTUAL PPMV		OVERALL					TIV METERS					
		MEAN	SE	MEAN	SE	SD	N	27%	51%	78%	95%	INTERVAL		
250	225	235	235	12.28	0.70	2	2.59				1	20.98		
500	417	617	617	2.54	0.28	2	2.82				1	2.25		
1500	1404	1404	1404	4.80	2.38	2	2.45				1	2.15		
6000	7893	7893	7893	3.06	0.72	2	2.14				1	1.18		
OVERALL MEANS		5.87	0.36	2.80	0.28	4	8.54	4.21	4					


ESTIMATED AT 10 000 PPMV 1.85

95% COMPLIANCE INTERVAL 1.05N 6.28D

Figure 5-31

INSTRUMENT RESPONSE VS CONCENTRATION

DICHLOROMETHYLENE TRANS 2

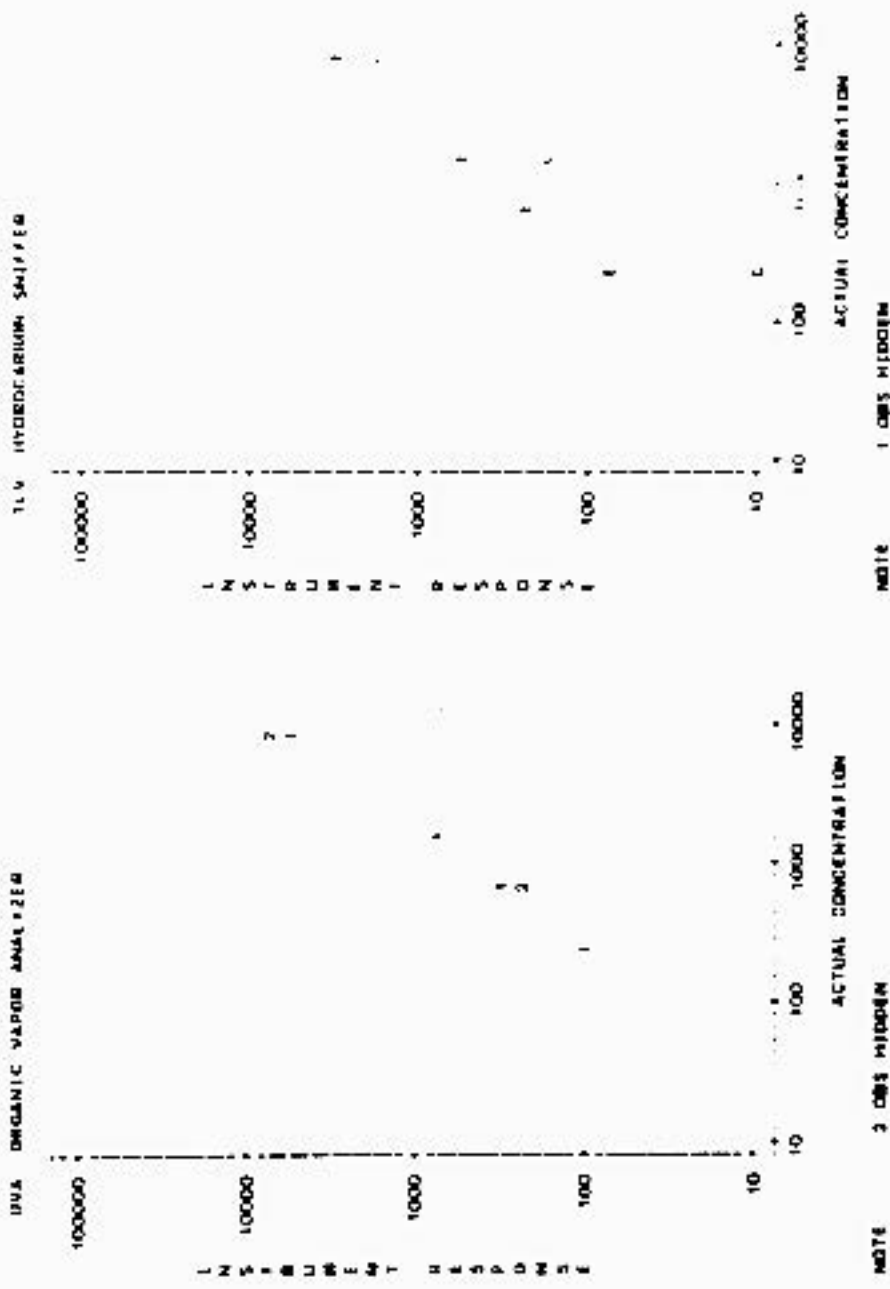

NOTE 2 OBS HIDDEN

NOTE 1 OBS HIDDEN

TABLE 5-77

RESPONSE FACTOR SUMMARY

TECHNICAL SUPPORT

OVERALL INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			US % COMPLIANCE INTERVAL							
	LOW	HIGH	MEAN	MEAN	SI	R	SI	N	SI	N	SI	N	SI	N
2000	214	214	214	1.01	0.03	2	1.00	1	1.00	1	1.00	1	1.00	1
1500	1573	1573	1573	1.40	0.03	2	1.37	1	1.34	1	1.34	1	1.34	1
1000	7935	7935	7935	2.29	0.08	2	2.21	1	2.11	1	2.11	1	2.11	1
OVERALL MEANS			1.59	0.01	6	1.54	0.04	4	1.54	0.04	4	1.54	0.04	4
ESTIMATED AT 10,000 PPMV			2.26	US % COMPLIANCE INTERVAL										
				1.94 2.64										


TECHNICAL SUPPORT

OVERALL INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			US % COMPLIANCE INTERVAL							
	LOW	HIGH	MEAN	MEAN	SI	R	SI	N	SI	N	SI	N	SI	N
2000	214	214	214	1.14	0.72	2	1.06	1	1.02	1	1.02	1	1.02	1
1500	1573	1573	1573	2.50	0.21	2	1.11	1	1.10	1	1.10	1	1.10	1
1000	7935	7935	7935	1.58	0.05	2	1.61	1	1.54	1	1.54	1	1.54	1
OVERALL MEANS			1.41	0.05	6	1.11	0.07	4	1.08	0.34	4	1.08	0.34	4
ESTIMATED AT 10,000 PPMV			3.61	US % COMPLIANCE INTERVAL										
				1.23 4.94										

Figure 5-72

INSTRUMENT RESPONSE VS CONCENTRATION

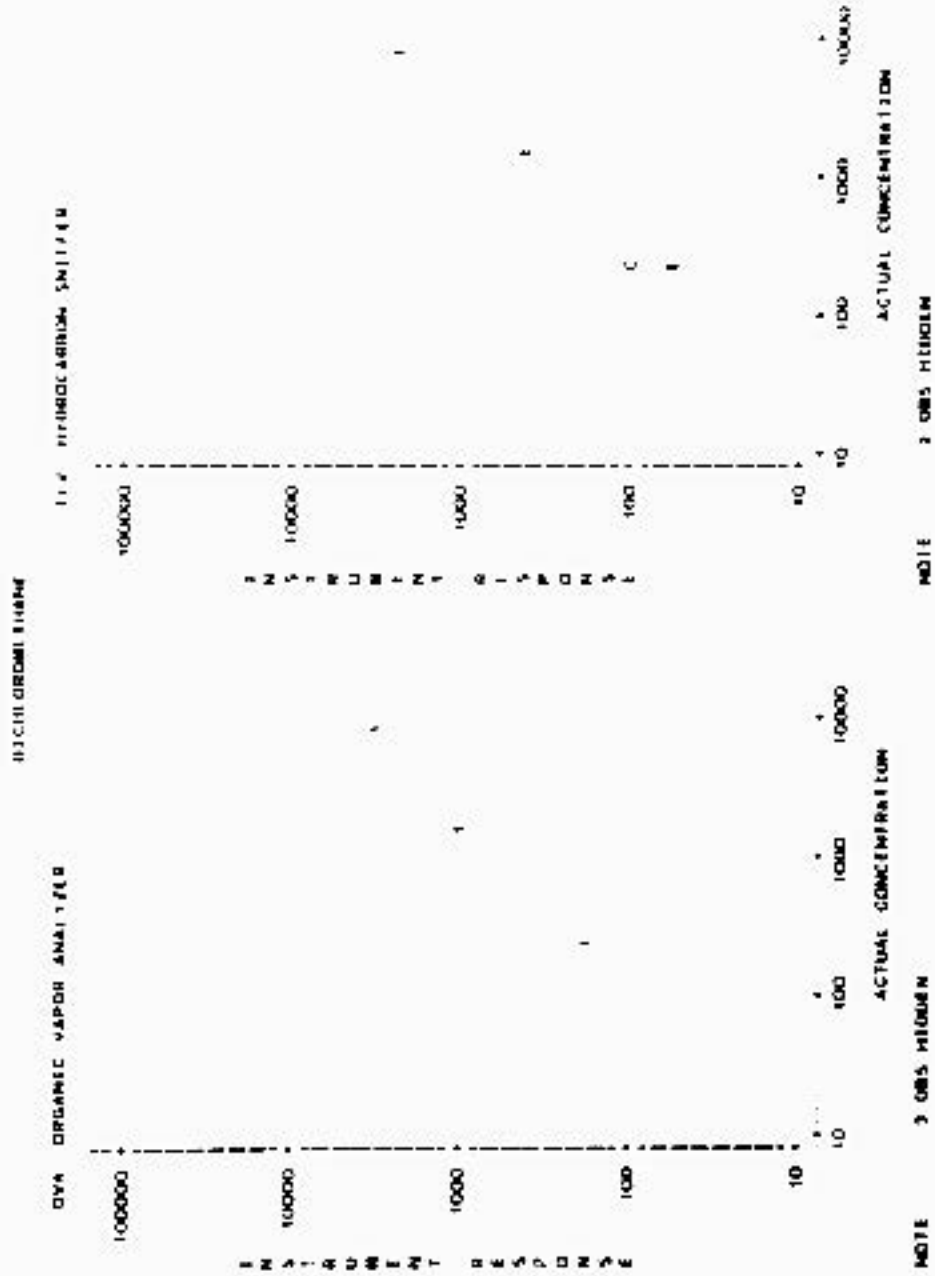

NOTE 3 OBS HEADEN

NOTE 3 OBS HEADEN



TABLE 5.75

RESPONSE FACTOR SUMMARY

1,1-DICHLOROETHANE 1.2

UVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR DATA														
	LOW	HIGH	MEAN	SE	ME	SE	1	2	3	4	5	6	7	8	9	10	11	12	
300	223	223	223	1.46	0.19	2	1.27	1	1.04	1	1.04	1	1.04	1	1.04	1	1.04	1	1.04
1500	1448	1448	1448	1.20	0.09	2	1.21	1	1.08	1	1.08	1	1.08	1	1.08	1	1.08	1	1.08
3000	989	989	989	1.06	0.08	2	1.15	1	1.04	1	1.04	1	1.04	1	1.04	1	1.04	1	1.04
6000	722	722	722																

OVERALL MEANS 1.22 0.07 6 1.21 0.08 2 1.14 0.09 3

ESTIMATED AT 10 000 PPMV 1.03

95% CONFIDENCE INTERVAL 1.02 1.04

UVB INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR DATA														
	LOW	HIGH	MEAN	SE	ME	SE	1	2	3	4	5	6	7	8	9	10	11	12	
300	223	223	223	3.88	1.71	2	2.27	1	5.89	1	5.89	1	5.89	1	5.89	1	5.89	1	5.89
1500	1448	1448	1448	3.19	1.20	2	3.09	1	4.49	1	4.49	1	4.49	1	4.49	1	4.49	1	4.49
3000	989	989	989	2.17	0.23	2	1.90	1	3.76	1	3.76	1	3.76	1	3.76	1	3.76	1	3.76
6000	722	722	722	1.88	0.24	2	1.75	1	3.20	1	3.20	1	3.20	1	3.20	1	3.20	1	3.20

OVERALL MEANS 2.81 0.11 6 1.94 0.12 4 1.89 0.15 4


ESTIMATED AT 10 000 PPMV 1.80

95% CONFIDENCE INTERVAL 1.72 1.87

Figure 5-73

INSTRUMENT RESPONSE VS CONCENTRATION

DICHLOROPROPANE 1,2

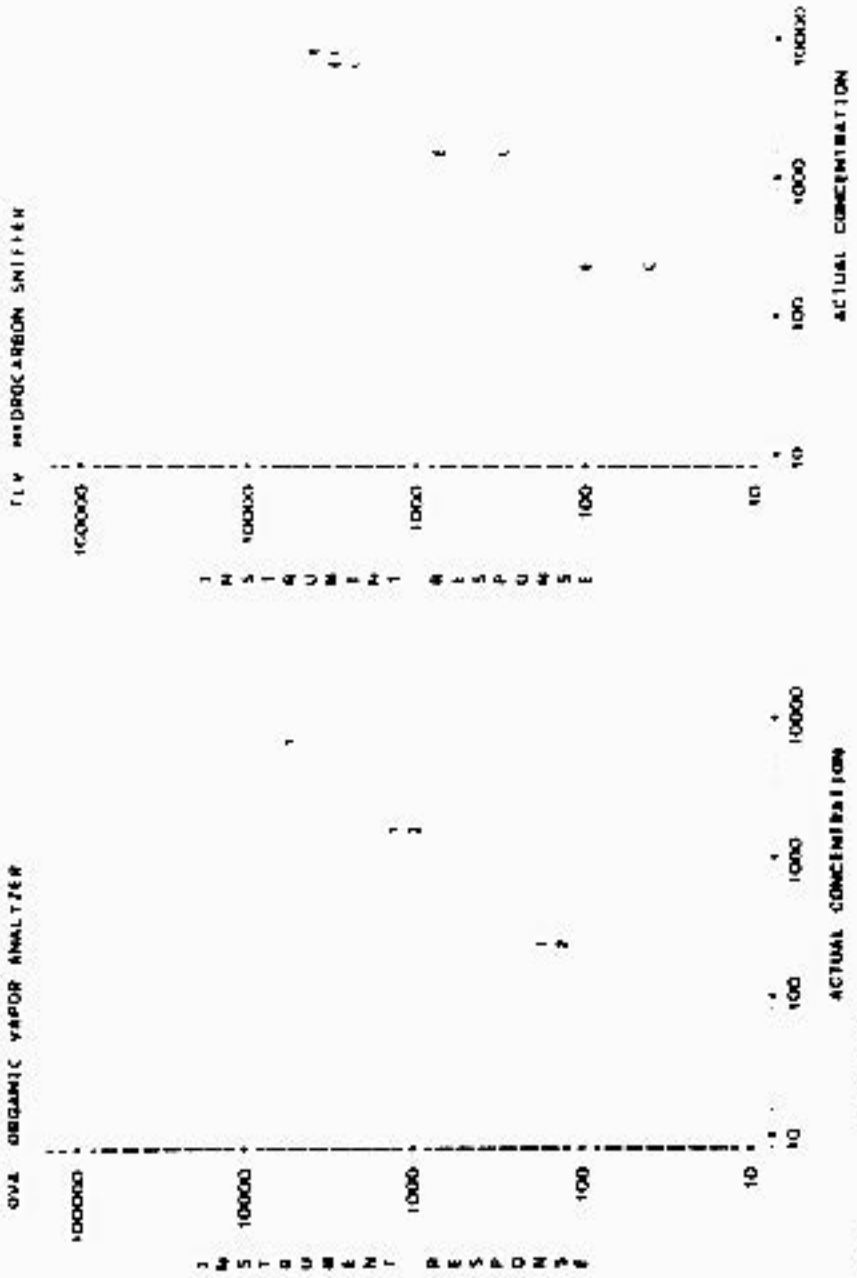

NOTE 1 DEG MIN/MIN

TABLE 5-74

RESPONSE FACTOR SUMMARY

DISCONTINUOUS

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METERS							
	LOW	HIGH	MEAN	MEAN	SE	SI	M	1000	50	25	10	5	2	1
200	222	222	222	0.86	0.04	2	0.90	1	1.02	1	1	1	1	1
1000	1558	1558	1558	0.86	0.02	2	0.58	1	0.80	1	1	1	1	1
2000	3186	3186	3186	0.23	0.02	2	0.32	1	0.35	1	1	1	1	1
4000	3815	3815	3815											
8000	6613	6613	6613											

OVERALL MEANS 0.82 0.01 0 0.59 0.17 0 0.86 0.40 0

ESTIMATED AT 10000 PPMV 0.24

VS 3 (DVA) INTERMEDIATE INTERVAL 1 0 0 0 0 0 0 0 0

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METERS							
	LOW	HIGH	MEAN	MEAN	SE	SI	M	1000	50	25	10	5	2	1
200	222	222	222	1.50	0.13	2	1.16	1	1.81	1	1	1	1	1
1000	1558	1558	1558	1.25	0.26	2	1.92	1	2.49	1	1	1	1	1
2000	3186	3186	3186	1.49	0.23	2	1.72	1	2.25	1	1	1	1	1
4000	3815	3815	3815	1.26	0.19	2	1.86	1	2.55	1	1	1	1	1
8000	6613	6613	6613	1.59	0.04	2	1.82	1	2.55	1	1	1	1	1

OVERALL MEANS 1.45 0.03 10

ESTIMATED AT 10000 PPMV 1.30

VS 3 (DVA) INTERMEDIATE INTERVAL 1 0 0 0 0 0 0 0 0

FIGURE 5-74

INSTRUMENT RESPONSE VS CONCENTRATION

DISCRIMINATION

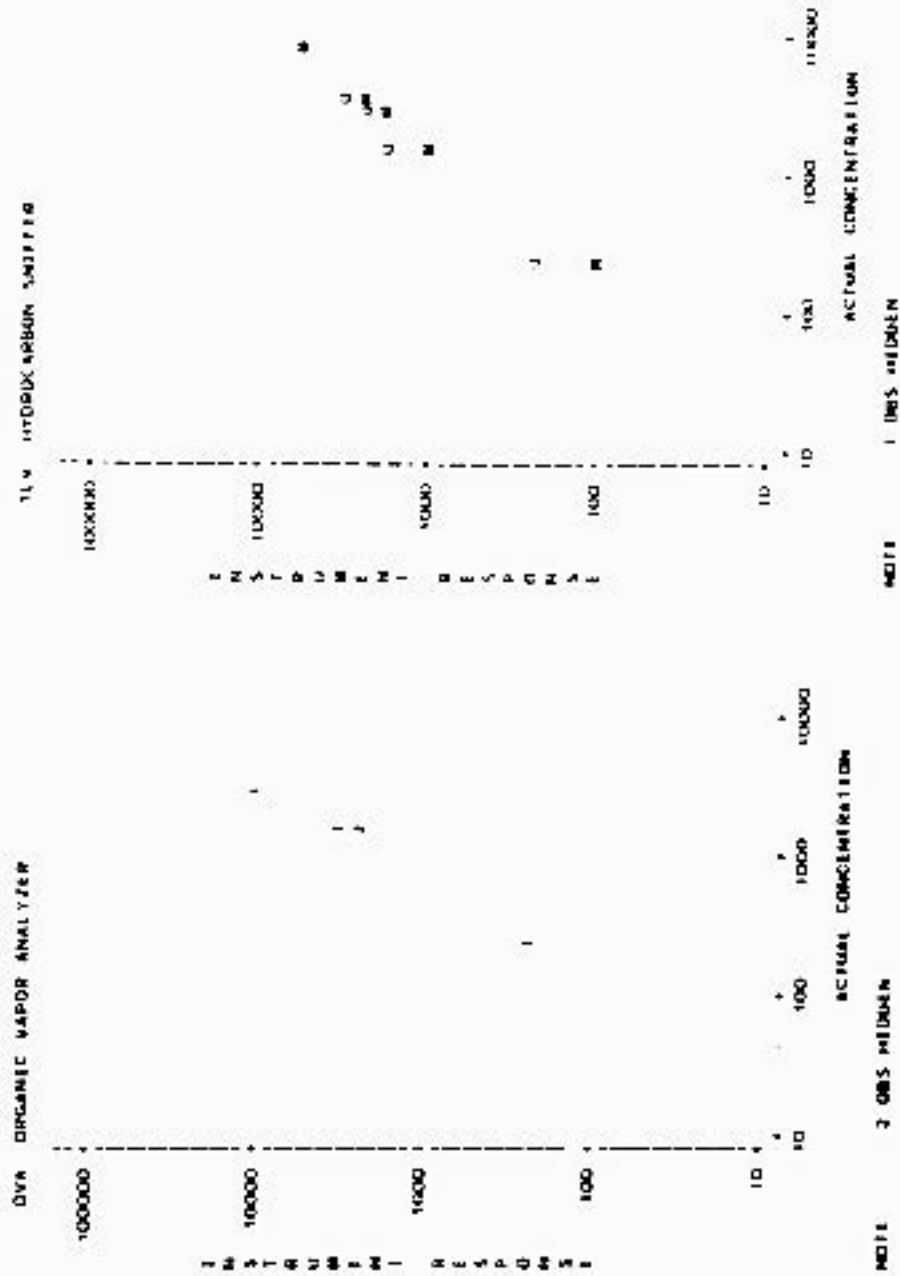


TABLE 5-25

RESPONSE FACTOR SUMMARY

DISSOLVED BENZENE 1-3

OVA INSTRUMENTS		R I S P D N S 4 1 A C I O R S																	
NOMINAL PPMV	ICM	ACTUAL PPMV		OVERALL		N	TUBED	SE	N	2254	SE	M	2159	SE	M	1933	SE	M	
		MEAN	SE	MEAN	SE														OVA MEANS
50	38	38	38	1.24	0.09	2	1.15	1	1.33	1	1.45	1	1.45	1	1.45	1	1.45	1	1.45
500	502	502	502	1.50	0.08	2	1.56	1	1.45	1	1.45	1	1.45	1	1.45	1	1.45	1	1.45
8000	7819	7819	7819	13.60	1.17	2	14.77	1	13.82	1	13.82	1	13.82	1	13.82	1	13.82	1	13.82
OVERALL MEANS		5.45	0.08	6	5.83	4.48	1	5.07	1.45	1	5.07	1.45	1	5.07	1.45	1	5.07	1.45	1
ESTERATED AT 10 0000 PPMV		V 4.2		95 % CONFIDENCE INTERVAL 1 MAR 24 1961															

ELY INSTRUMENTS

ACTUAL PPMV		R I S P D N S 4 1 A C I O R S																	
NOMINAL PPMV	ICM	HEIGHT	MEAN	SE	M	7E	SE	M	11	SE	M	16	SE	M	20	SE	M		
																		ELY MEANS	
50	38	38	38	1.95	0.48	2	2.13	1	1.57	1	1.57	1	1.57	1	1.57	1	1.57	1	
500	502	502	502	3.85	1.56	2	8.10	1	1.90	1	1.90	1	1.90	1	1.90	1	1.90	1	
8000	7819	7819	7819	53.87	35.2	2	84.12	1	18.84	1	18.84	1	18.84	1	18.84	1	18.84	1	
OVERALL MEANS		19.72	2.07	6	32.52	28.5	3	7.31	2.75	1	7.31	2.75	1	7.31	2.75	1	7.31	2.75	
ESTERATED AT 10 0000 PPMV		24.96		95 % CONFIDENCE INTERVAL 1 MAR 24 1961															

FIGURE 5-25

INSTRUMENT RESPONSE VS. CONCENTRATION


Figure 5/5

INSTRUMENT RESPONSE VS CONCENTRATION

DISISOPROPYL BENZENE 1.1

QVA ORGANIC VAPOR ANALYZER

115 PERIOD ARBON SMIPER

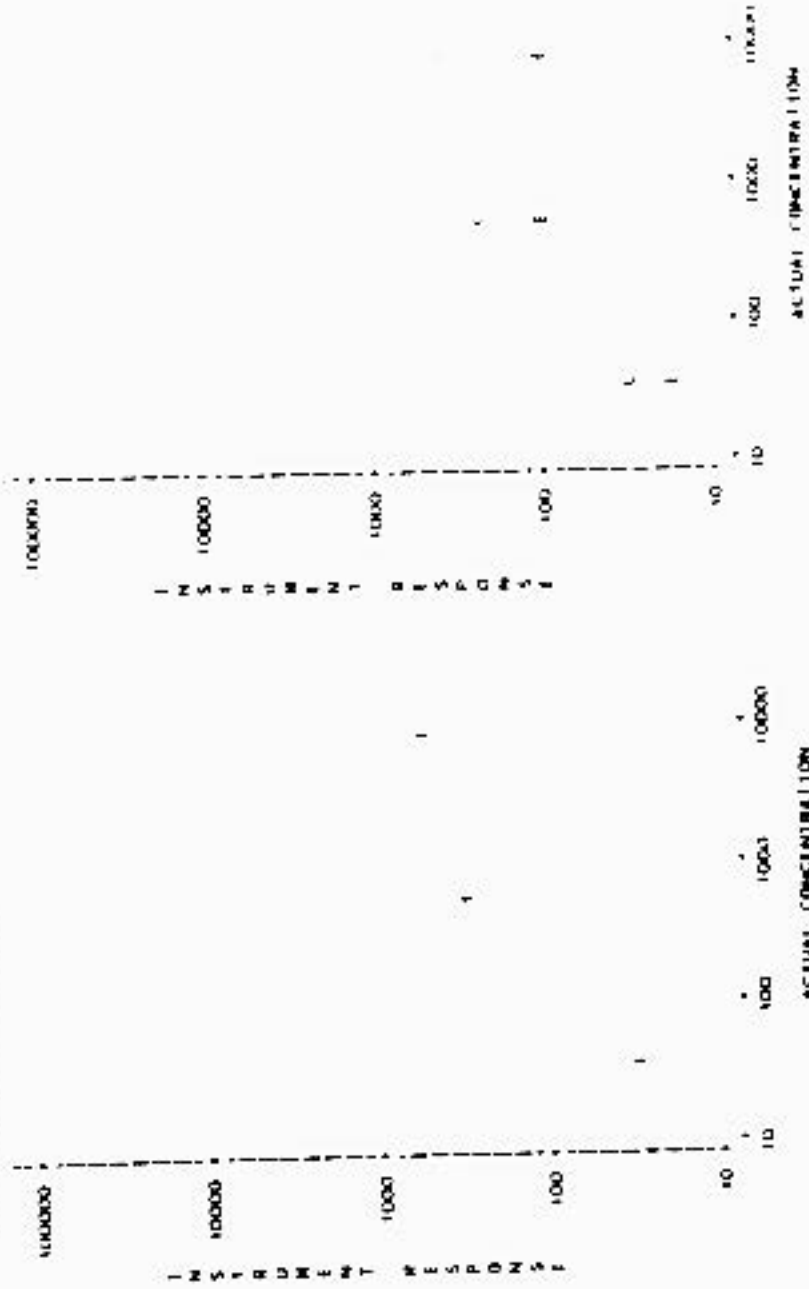

NOTE 3 PPS HIGH

TABLE 4.14

RESPONSE FACTOR SUMMARY

DIETHYLZINC ETHANE 1.2

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METHODS												
	LOW	HIGH	MEAN	MEAN	SE	N	100%	SE	N	22%	SE	N	15%	SE	N	10%	SE	N	
200	202	202	202	2.25	1.23	2						2.02			1	4.48			1
1500	1531	1533	1537	3.47	0.82	2						2.85			1	2.09			1
8000	7578	7676	7578	1.22	0.12	2						1.50			1	1.14			1
OVERALL MEANS			2.65	0.11	6							1.85			1	1.65			1

ESTIMATED AT 10 (00) PPMV 1.28

95% CONFIDENCE INTERVALS 1.04-2.30

DV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METHODS												
	LOW	HIGH	MEAN	MEAN	SE	N	100%	SE	N	22%	SE	N	15%	SE	N	10%	SE	N	
200	202	202	202	0.78		1				0.14		1			1				1
1500	1537	1537	1537	1.14		1				1.14		1			1				1
8000	7578	7578	7578	1.72		1				1.33		1			1				1
OVERALL MEANS			1.06		3					1.06		3			3				3

ESTIMATED AT 10 (00) PPMV 1.47

95% CONFIDENCE INTERVALS 0.76-2.18

Figure 5-7b

INSTRUMENT RESPONSE VS. CONCENTRATION

DIMETHYL ETHANE 1.2

OVA ORGANIC VAPOR ANALYZER

TLV HYDROCARBONS SAMPLES

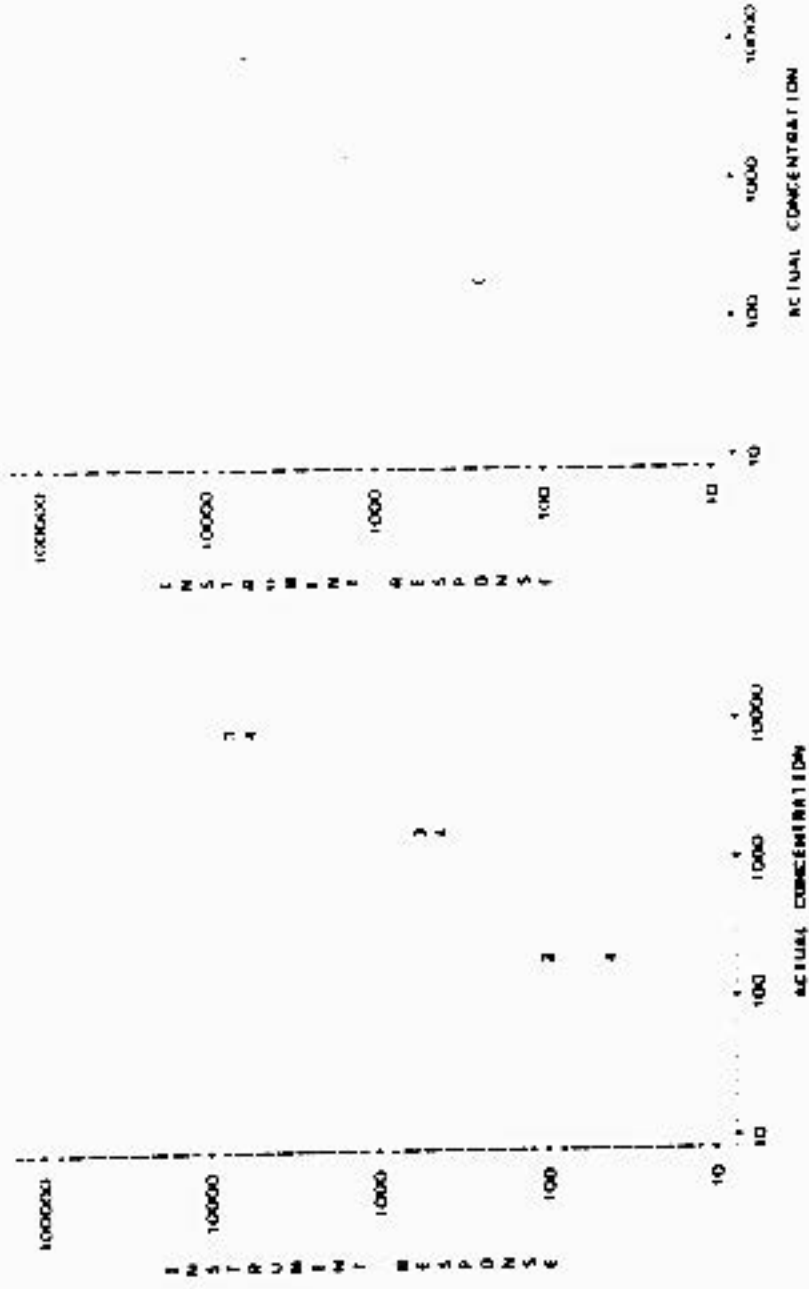




TABLE 5-72

RESPONSE FACTOR SUMMARY

DIMETHYLFORMAMIDE, N,N

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	MEAN	SE	N
200	218	218	218	3.30	0.03	2
1500	1524	1524	1524	2.14	0.13	2
4400	4325	4325	4325	8.04	0.08	2
OVERALL MEANS				2.51	0.28	3

ESTIMATED AT 10,000 PPMV 3.89

DVA METERS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	MEAN	SE	N
200	218	218	218	3.30	0.03	2
1500	1524	1524	1524	2.14	0.13	2
4400	4325	4325	4325	8.04	0.08	2
OVERALL MEANS				2.51	0.28	3

ESTIMATED AT 10,000 PPMV 4.88

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	MEAN	SE	N
200	218	218	218	0.77		1
1500	1524	1524	1524	1.51		1
4400	4325	4325	4325	2.30		1
OVERALL MEANS				1.49		3

ESTIMATED AT 10,000 PPMV 2.95

DVA METERS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	MEAN	SE	N
200	218	218	218	0.77		1
1500	1524	1524	1524	1.51		1
4400	4325	4325	4325	2.30		1
OVERALL MEANS				1.49		3

ESTIMATED AT 10,000 PPMV 1.88


Figure 5-17

INSTRUMENT RESPONSE VS CONCENTRATION

DIMETHYLBENZAMIDE M.M.

115 HINDOLABSDM SNIFFER

DVA ORGANIC VAPOR ANALYZER

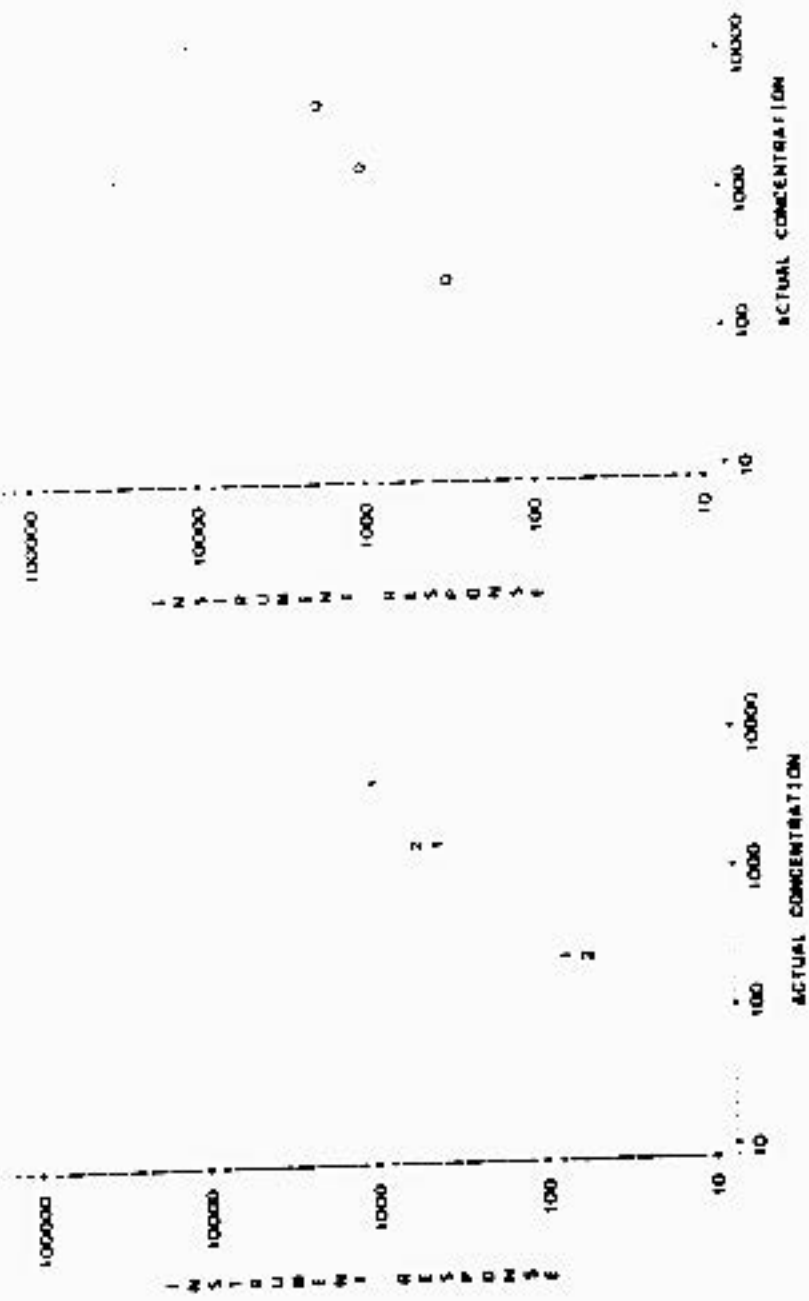

NOTE 1 OBS HIDDEN

TABLE 5.7M

RESPONSE FACTOR SUMMARY

DIPHENYLDIAZINE 1.1

OVA INSTALMENTS RESPONSE FACTOR SUMMARY

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR SUMMARY									
	LOW	HIGH	MEAN	SE	N	YOMD	SE	N	2150	SE	N	1810	SE	N
700	226	226	226	0.31	2	5.02	1	5.64	1	3.64	1	3.64	1	1
1500	1512	1512	1512	0.30	2	1.85	1	2.21	1	2.21	1	2.21	1	1
8000	8527	8527	8527	0.14	2	1.12	1	1.40	1	1.40	1	1.40	1	1
OVERALL MEANS			2.83	0.09	6	2.86	1.23	3	3.50	1.29	3	3.50	1.29	3

ESTIMATED AT 10 000 PPMV 1.04

95% CONFIDENCE INTERVAL 1.61 - 1.521

1.1V INSTALMENTS

RESPONSE FACTOR SUMMARY

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR SUMMARY									
	LOW	HIGH	MEAN	SE	N	1E	SE	N	51	SE	N	70	SE	N
700	226	226	226	0.18	1	1.76	1	1.76	1	1.76	1	1.76	1	1
1500	1512	1512	1512	0.48	1	2.48	1	2.48	1	2.48	1	2.48	1	1
8000	8527	8527	8527	0.01	1	3.01	1	3.01	1	3.01	1	3.01	1	1
OVERALL MEANS			2.88	0.22	3	2.88	0.22	3	2.88	0.22	3	2.88	0.22	3

ESTIMATED AT 10 000 PPMV 2.74

95% CONFIDENCE INTERVAL 1.561 - 4.611


Figure 3-7B

INSTRUMENT RESPONSE VS CONCENTRATION

DIMETHYLHYDRAZINE (1)

QVA ORGANIC VAPOR ANALYZER

FIV HYDROCARBON SMITTER

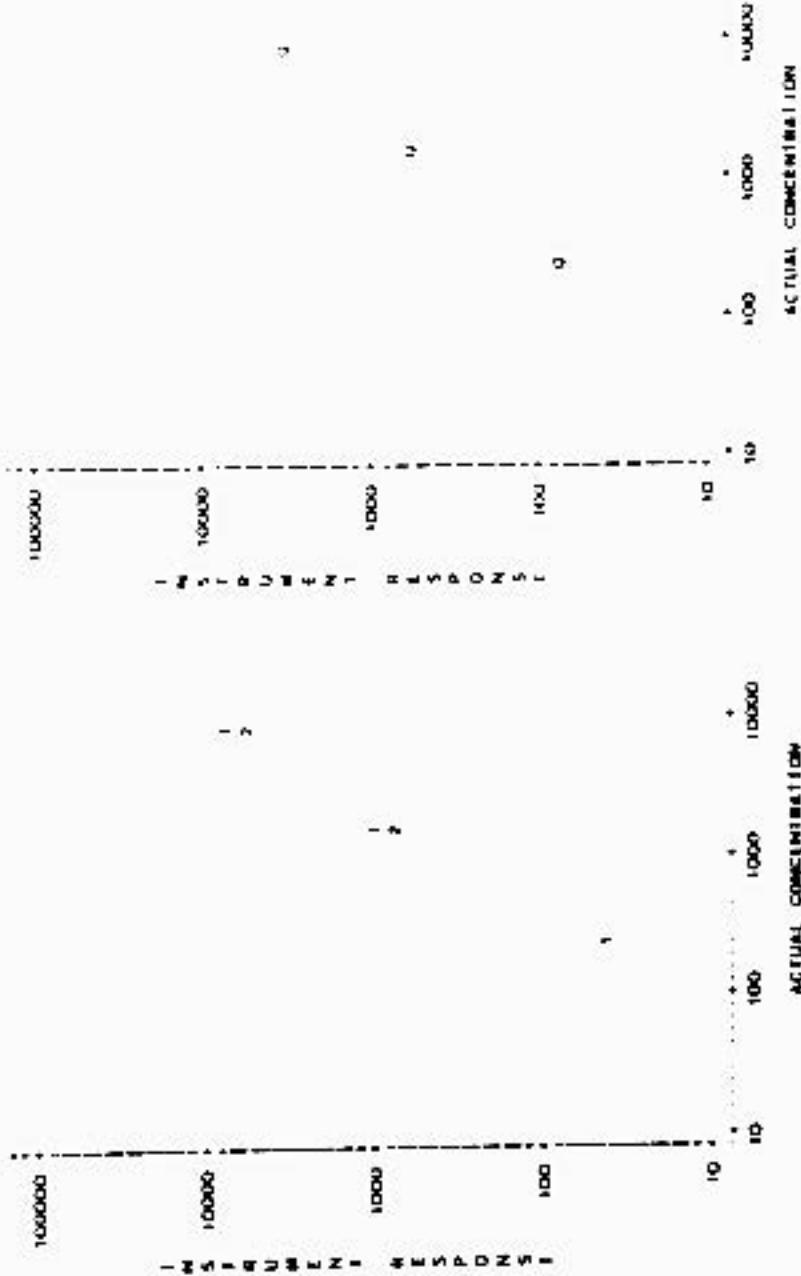

NOTE: 1 OBS HIDDEN

TABLE 1. 79

RESPONSE FACTORS SUMMARY

TIME INSTRUMENTS 2 4

DVA INSTRUMENTS

D E S I G N S P E R I M E N T S

MEASUREMENT	ACTUAL PPMV			OVERALL			DVA METERS									
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2004	SE	N	2150	SE	N	
2000	216	216	216	16.40	3.28	2	13.12			1	19.68					
1500	1625	1625	1625	24.78	4.22	2	20.52			1	29.02					
8704	8704	8704	8704	31.97	6.44	2	34.54			1	44.41					
OVERALL MEANS			26.39	0.71	6	23.14	5.95	1	11.03	1.21	1					

ESTIMATED AT 100 INDEX PPMV 37.099

95% 3-DIGIT INTERVAL 1.25 IN 50.920

DVA INSTRUMENTS

M E T E R S P E R I M E N T S

MEASUREMENT	ACTUAL PPMV			OVERALL			DVA METERS									
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2004	SE	N	2150	SE	N	
2000	216	216	216	5.71	1.03	3	6.74			1	4.67					
1500	1625	1625	1625	22.06	6.43	2	40.94			1	24.11					
8704	8704	8704	8704	75.22	30.59	2	106.1			1	44.14					
OVERALL MEANS			82.27	7.4	6	51.26	29.1	1	24.17	11.4	1					

ESTIMATED AT 100 INDEX PPMV 18.086

95% 3-DIGIT INTERVAL 1.18 IN 50.920

Figure 5-29

INSTRUMENT RESPONSE VS. CONCENTRATION

DIMETHYLSTIRENE 2-4


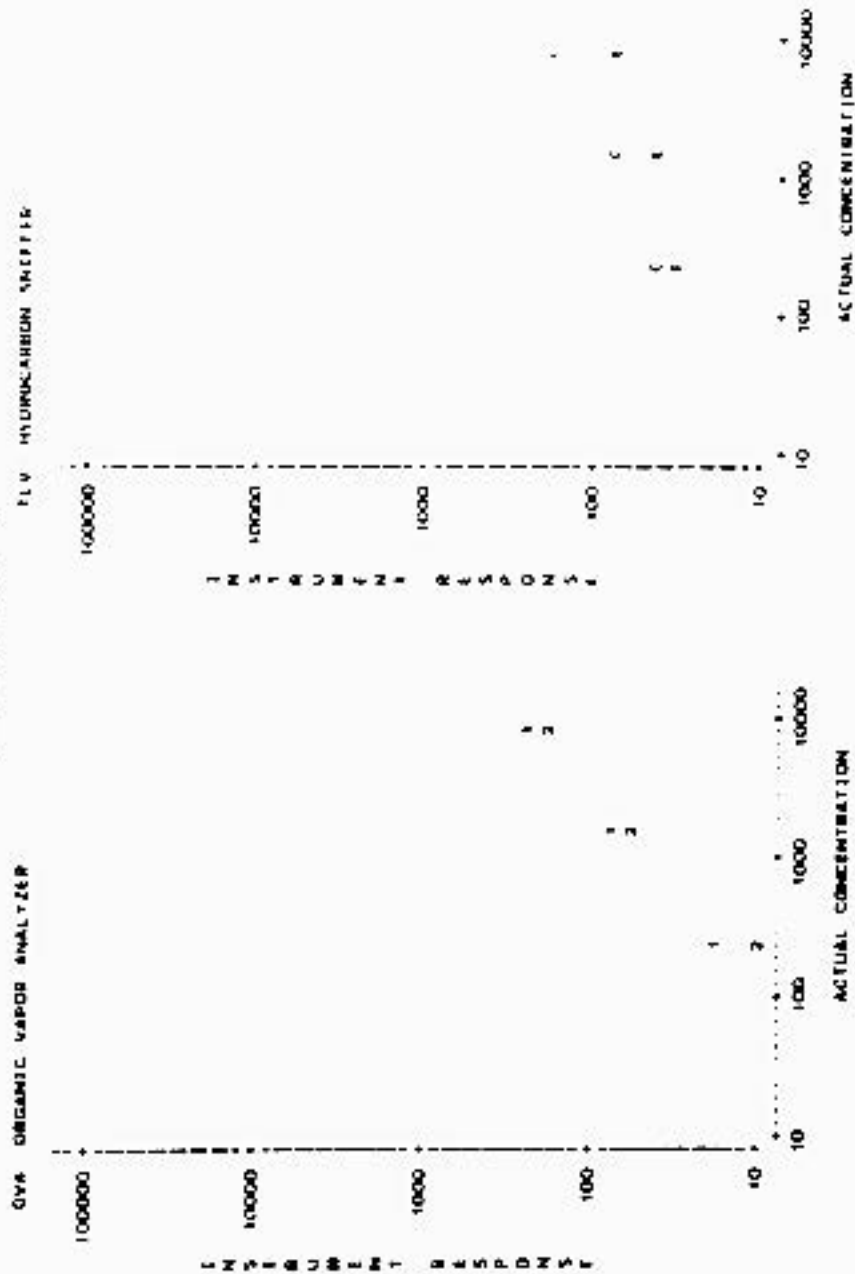




Figure 5-10

INSTRUMENT RESPONSE VS CONCENTRATION

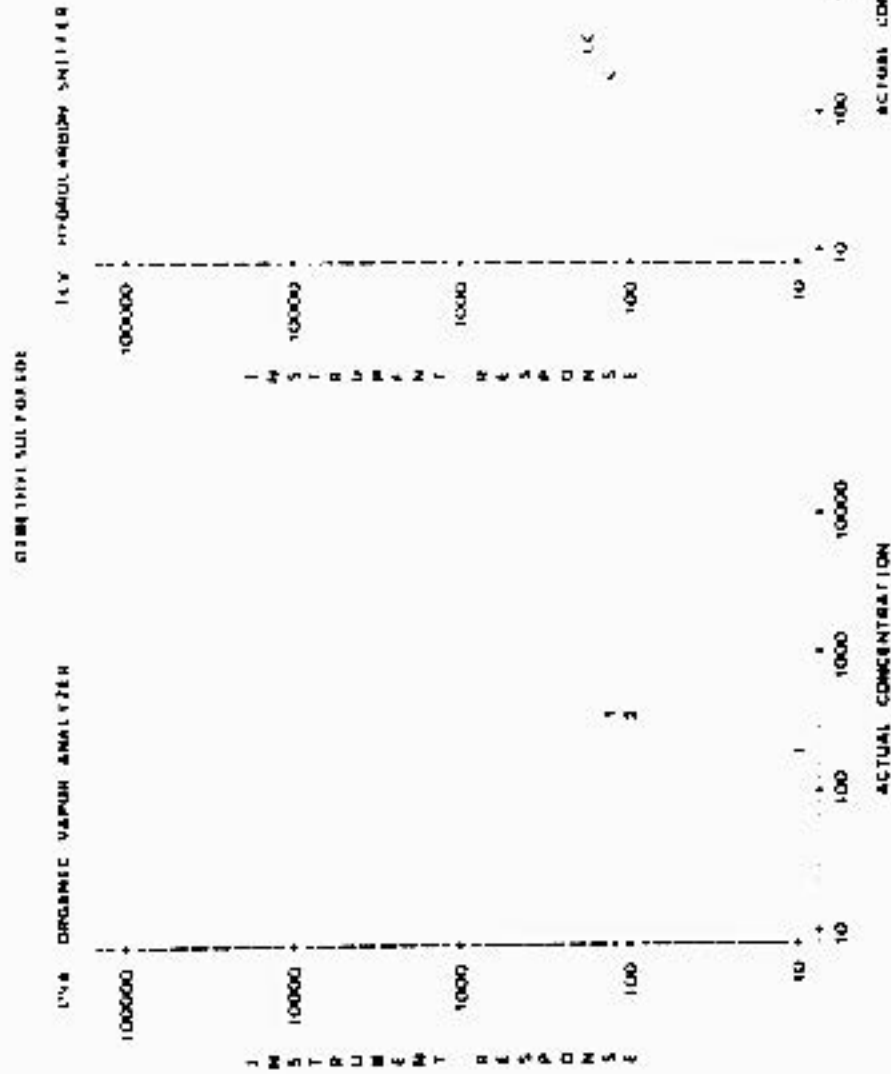

NOTE: 3 OBS HAD MISSING VALUES OR WERE DU



TABLE 5.41

RESPONSE FACTOR SUMMARY

01000000

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		SE	N	1000	SE	N	2250	SE	N	2150	SE	N	1011	SE	
	LOW	HIGH	MEAN	SE														
200	209	209	200	0.01	2	2	2	0.01	1	2	0.01	1	2	0.01	1	2	0.01	1
1500	1508	1508	1500	0.08	2	2	2	0.08	1	2	0.08	1	2	0.08	1	2	0.08	1
8000	7681	7687	7682	0.00	2	2	2	0.00	1	2	0.00	1	2	0.00	1	2	0.00	1
OVERALL	MEANS	200	0.01	6	2	16	0.01	3	2	41	0.01	1						

ESTIMATED AT 10 OXCI PPMV 1.58

95% CONFIDENCE INTERVALS 1.10 2.26

1.5 INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		SE	N	10	SE	N	20	SE	N	20	SE	N	10	SE
	LOW	HIGH	MEAN	SE													
200	209	209	200	0.50	1	1	2	0.50	1	2	0.50	1	2	0.50	1	2	0.50
1500	1508	1508	1500	0.83	1	1	2	0.83	1	2	0.83	1	2	0.83	1	2	0.83
8000	7681	7687	7682	1.14	1	1	2	1.14	1	2	1.14	1	2	1.14	1	2	1.14
OVERALL	MEANS	200	0.82	1													

ESTIMATED AT 10 OXCI PPMV 1.23

95% CONFIDENCE INTERVALS 0.40 1.43


PLATE 381

INSTRUMENT RESPONSE VS CONCENTRATION

DIBAZINE

QVA ORGANIC VAPOR ANALYZER

TUV HYDROCARBON SWITZER

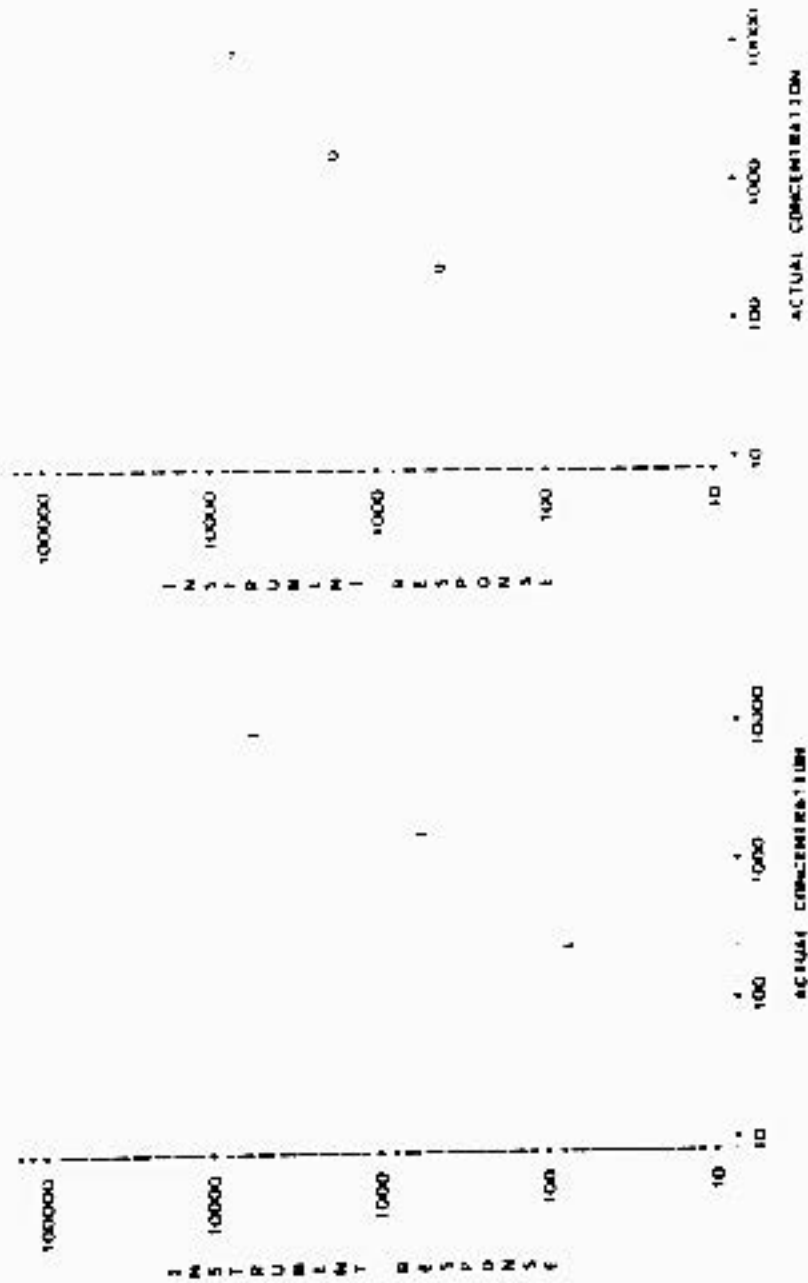

NOTE 3 DIBS HIDDEN

TABLE 5. B2

RESPONSE FACTOR SUMMARY

EPICHA OREPHEPDRIN

OVA INSTRUMENTS				95% CONFIDENCE INTERVAL			
NOMINAL PPMV	ACTUAL PPMV		OVERALL		DVA METERS		INSTRUMENT
	LOW	HIGH	MEAN	SE	N	SE	
200	210	210	1.98	0.05	2	1.91	1
1500	1511	1511	1.84	0.06	2	1.90	2
8070	8070	8070	1.70	0.02	2	1.98	3
OVERALL MEANS			1.86	0.02	6	1.93	1
ESTIMATED AT 10,000 PPMV 1.72							

11V INSTRUMENTS

ACTUAL PPMV				95% CONFIDENCE INTERVAL			
NOMINAL PPMV	ACTUAL PPMV		OVERALL		DVA METERS		INSTRUMENT
	LOW	HIGH	MEAN	SE	N	SE	
200	210	210	1.93	0.11	2	1.82	1
1500	1511	1511	2.08	0.06	2	2.03	1
8070	8070	8070	1.98	0.01	2	1.98	1
OVERALL MEANS			2.03	0.05	6	1.95	1
ESTIMATED AT 10,000 PPMV 2.02							



Figure 5. B2

Figure 1 B/2

EXPERIMENTAL RESPONSE AS A FUNCTION OF CONCENTRATION  
 EPICHLOROHYDRIN

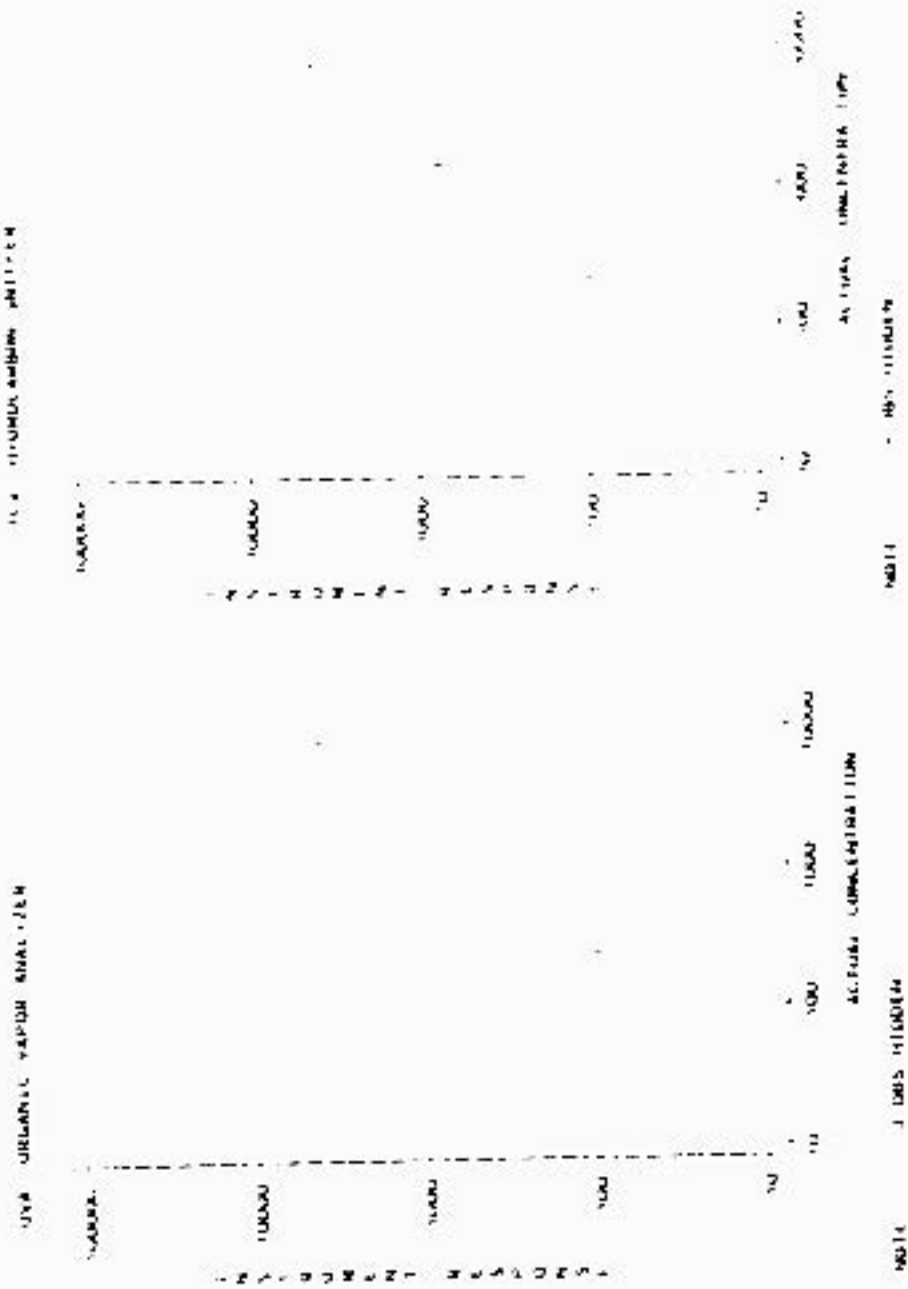


TABLE 1.11

OVERALL FACTOR SUMMARY

11/10/64

DVA INSTRUMENTS

U T S P H N S E T A C T I O N S

APPROXIMATE PPMV	ACTUAL PPMV			OVERALL			DVA METERS										
	LOW	HIGH	MEAN	MEAN	SE	N	1000	50	N	250	SE	N	500	SE	N		
1000	1083	1083	1083	1.04	0.05	7					0.94	1	1.10	1	1.10	1	
3000	3289	3289	3289	1.16	0.05	1					1.11	1	1.21	1	1.21	1	
4000	4588	4588	4588	0.57	0.04	1					0.58	1	0.57	1	0.57	1	
8000	7857	7857	7857														
OVERALL MEANS							0.92	0.04	8								

ESTIMATED AT 10 000 PPMV 0.57

95 % CONFIDENCE INTERVAL 1.10 26 1.261

FV INSTRUMENTS

R P S P O M V T P E T I O N S

APPROXIMATE PPMV	ACTUAL PPMV			OVERALL			FV METERS								
	LOW	HIGH	MEAN	MEAN	SE	N	75	SE	N	75	SE	N	75	SE	N
1000	1083	1083	1083	0.52		1					0.52	1			1
3000	3289	3289	3289	0.80		1					0.80	1			1
4000	4588	4588	4588	0.56		1					0.56	1			1
8000	7857	7857	7857												
OVERALL MEANS							0.63		1			0.63	0.69	1	

ESTIMATED AT 10 000 PPMV 0.11

95 % CONFIDENCE INTERVAL 1.11 25 1.521


Figure 5-81

INSTRUMENT RESPONSE VS CONCENTRATION

ETHANE

OVM ORGANIC VAPOR ANALYZER

TUV HYDROCARBON SWIPE

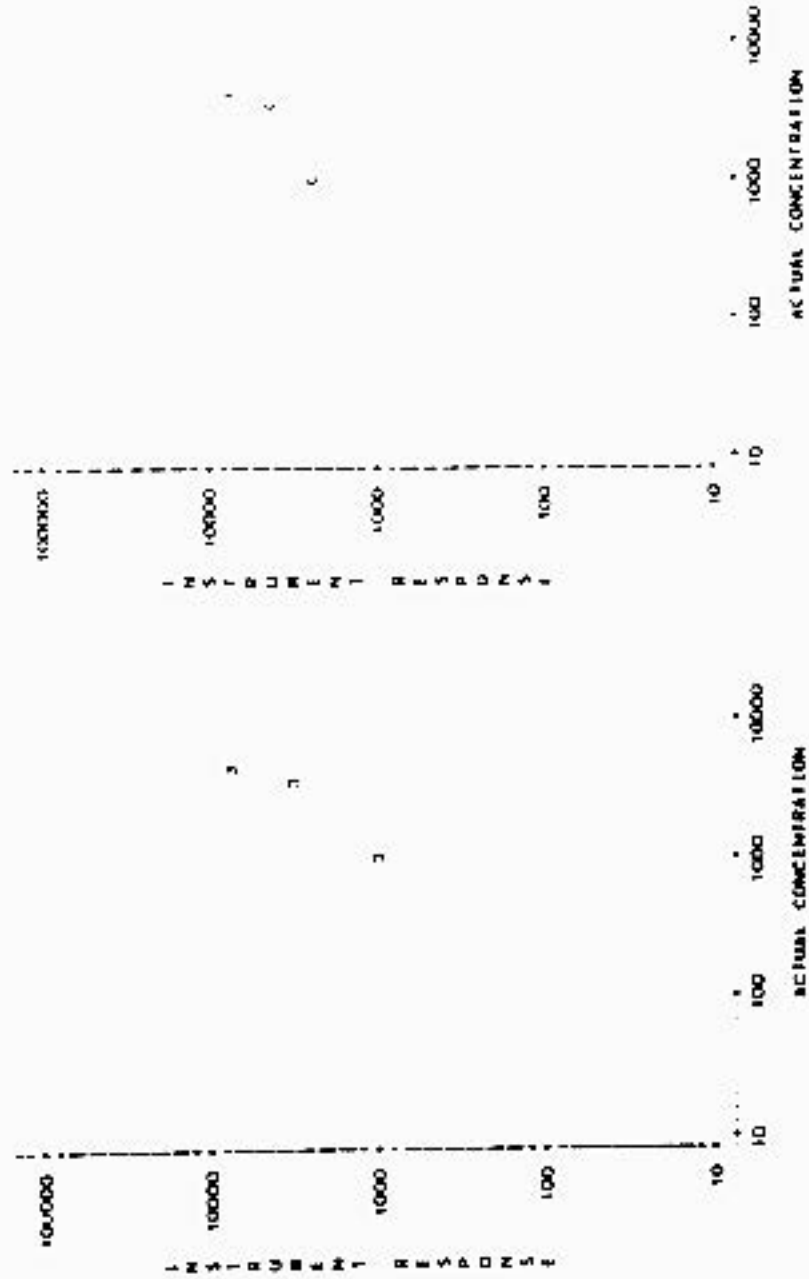

NOTE 3 USES MIDEEM

TABLE 1. M4

RESPONSE FACTOR SUMMARY

4THRU00L

QVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		MEAN	SD	COV	SE	N
	LOW	HIGH					
200	178	178	178	5.45	0.031	3	3
1500	1478	1478	1478	3.6	0.0024	3	3
8000	9019	9019	9019	2.3	0.00026	3	3

OVERALL MEANS 3.98 O.D.

ESTIMATED AT 10,000 PPMV 2.04

M E S P O M S E F A I T O D U S

NOMINAL PPMV	ACTUAL PPMV		MEAN	SD	COV	SE	N
	LOW	HIGH					
200	178	178	178	5.45	0.031	3	3
1500	1478	1478	1478	3.6	0.0024	3	3
8000	9019	9019	9019	2.3	0.00026	3	3

OVERALL MEANS 3.98 O.D.

ESTIMATED AT 10,000 PPMV 1.93

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		MEAN	SE	N
	LOW	HIGH			
200	178	178	178	5.45	3
1500	1478	1478	1478	3.6	3
8000	9019	9019	9019	2.3	3

OVERALL MEANS

ESTIMATED AT 10,000 PPMV

M E S P O M S E F A I T O D U S

NOMINAL PPMV	ACTUAL PPMV		MEAN	SE	N
	LOW	HIGH			
200	178	178	178	5.45	3
1500	1478	1478	1478	3.6	3
8000	9019	9019	9019	2.3	3

OVERALL MEANS

ESTIMATED AT 10,000 PPMV

Figure 5-B4

INSTRUMENT RESPONSE VS. CONCENTRATION

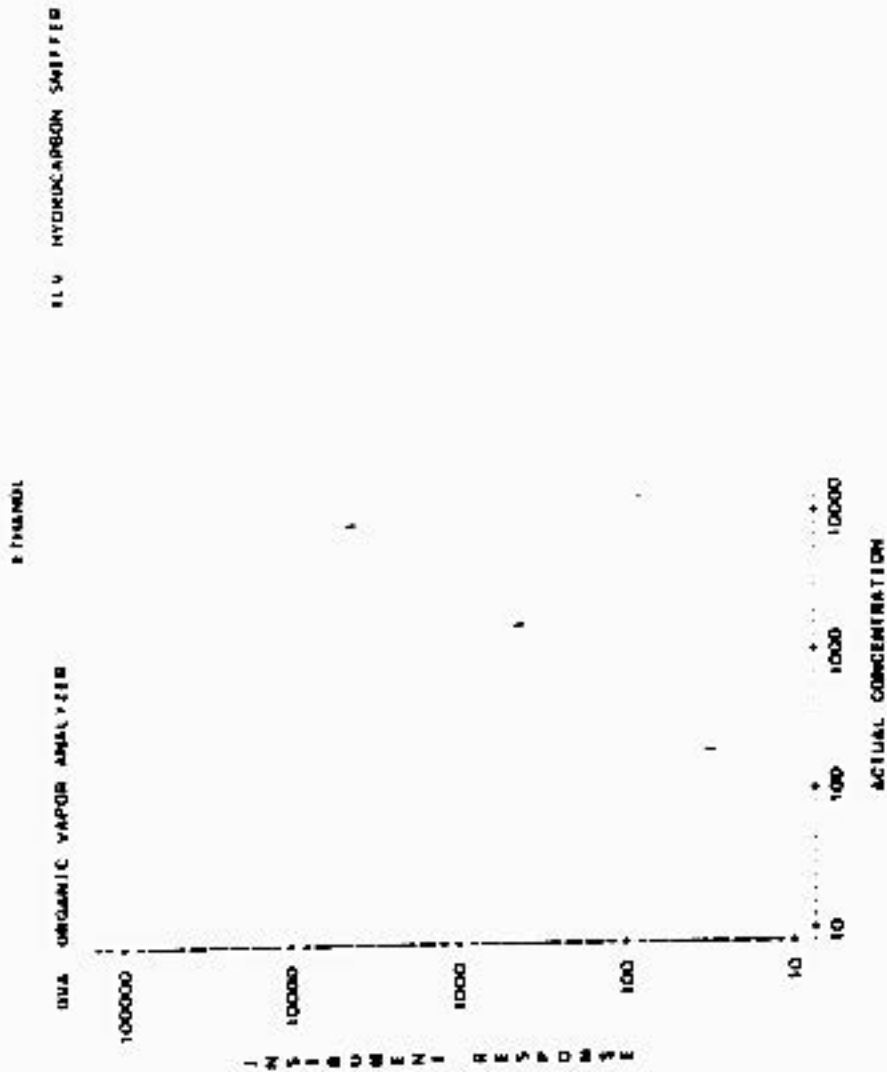




TABLE 10

RESPONSE FACTOR SUMMARY

ESTIMATED AT 10,000 PPMV

DATA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	SE	2000	SE	4000	SE	6000	SE
200	203	203	2 82	0 03	1	2 55	1	2 55	1	2 55
1500	1505	1505	2 70	0 04	1	2 49	1	2 49	1	2 49
4000	4388	4388	1 87	0 04	1	1 83	1	1 83	1	1 83
OVERALL MEANS		2 10	0 03	0	2 77	0 06	1	2 62	0 06	1

ESTIMATED AT 10,000 PPMV

DATA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	SE	200	SE	400	SE	600	SE
200	203	203	0 74	1	1	0 74	1	0 74	1	0 74
1500	1505	1505	1 07	1	1	1 07	1	1 07	1	1 07
4000	4388	4388	1 30	1	1	1 30	1	1 30	1	1 30
OVERALL MEANS		1 07	1	1	1 42	1 04	1	1 42	1 04	1

ESTIMATED AT 10,000 PPMV


DATA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	SE	200	SE	400	SE	600	SE
200	203	203	0 74	1	1	0 74	1	0 74	1	0 74
1500	1505	1505	1 07	1	1	1 07	1	1 07	1	1 07
4000	4388	4388	1 30	1	1	1 30	1	1 30	1	1 30
OVERALL MEANS		1 07	1	1	1 42	1 04	1	1 42	1 04	1

Figure 3-B5

INSTRUMENT RESPONSE VS CONCENTRATION

ETHYL ETHANEDIOL

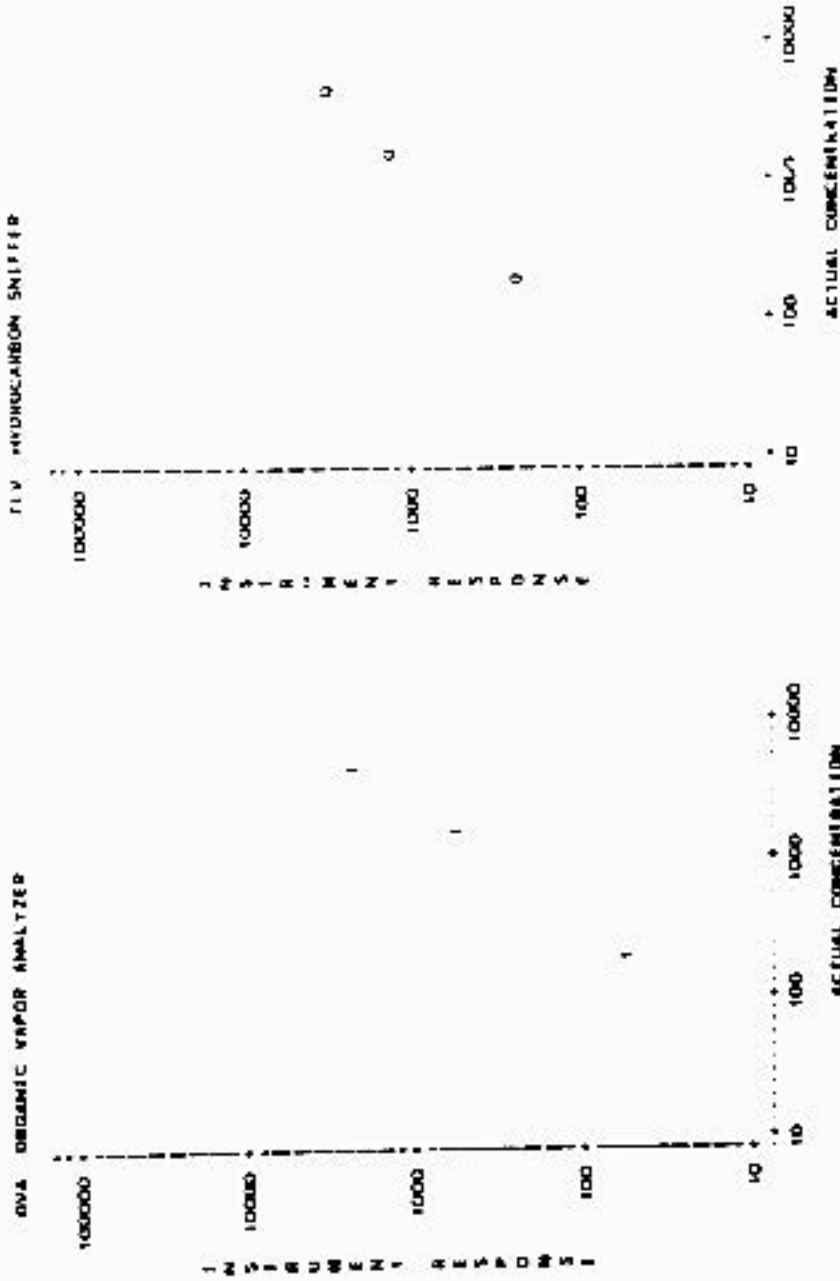

NOTE: 3 CBS MIXTURE

TABLE 5. 185

RESPONSE FACTOR SUMMARY

ESTIMATE

OVER INSTRUMENTS

ACTUAL PPMV

OVERALL

NOMINAL PPMV	LOW		HIGH		MEAN		SE		SD		SE		SD		SE		SD		
	LOW	HIGH	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	
50	82	80	80	0.21	4	1.25	0.18	2	1.92	0.31	2								
200	222	222	222	0.08	2	3.58		3	3.14		3								
500	538	542	540	0.02	4	3.48	0.22	2	3.48	0.05	2								
1500	1407	1407	1407	0.14	2	3.12		1	1.91		1								
4000	1923	1923	1923	0.03	6	0.88	0.12	3	0.82	0.04	3								
OVERALL MEANS																			
1.80																			
ESTIMATED AT 50 INNO PPMV																			
1.18																			
45% COMBINED INSTRUMENT																			
1.14																			
1.940																			

ESTIMATE

OVER INSTRUMENTS

ACTUAL PPMV

OVERALL

NOMINAL PPMV	LOW		HIGH		MEAN		SE		SD		SE		SD		SE		SD		
	LOW	HIGH	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	MEAN	SE	
50	82	80	80	0.04	4	0.85	0.40	2	0.78	0.42	2								
200	222	222	222	0.04	2	3.14		1	0.96		1								
500	538	542	540	0.01	4	3.26	0.06	2	1.12	0.31	2								
1500	1407	1407	1407	0.02	2	1.28		1	1.21		1								
4000	1923	1923	1923	0.02	6	1.25	0.02	1	1.24	0.05	1								
OVERALL MEANS																			
1.54																			
ESTIMATED AT 50 INNO PPMV																			
1.17																			
45% COMBINED INSTRUMENT																			
1.14																			
1.940																			


PLATE 5 Bb

INSTRUMENT RESPONSE VS CONCENTRATION

ELUENT ACETATE

DIVISION ORGANIC VAPOR ANALYZER

1LV HYDROCARBON SAMPLE

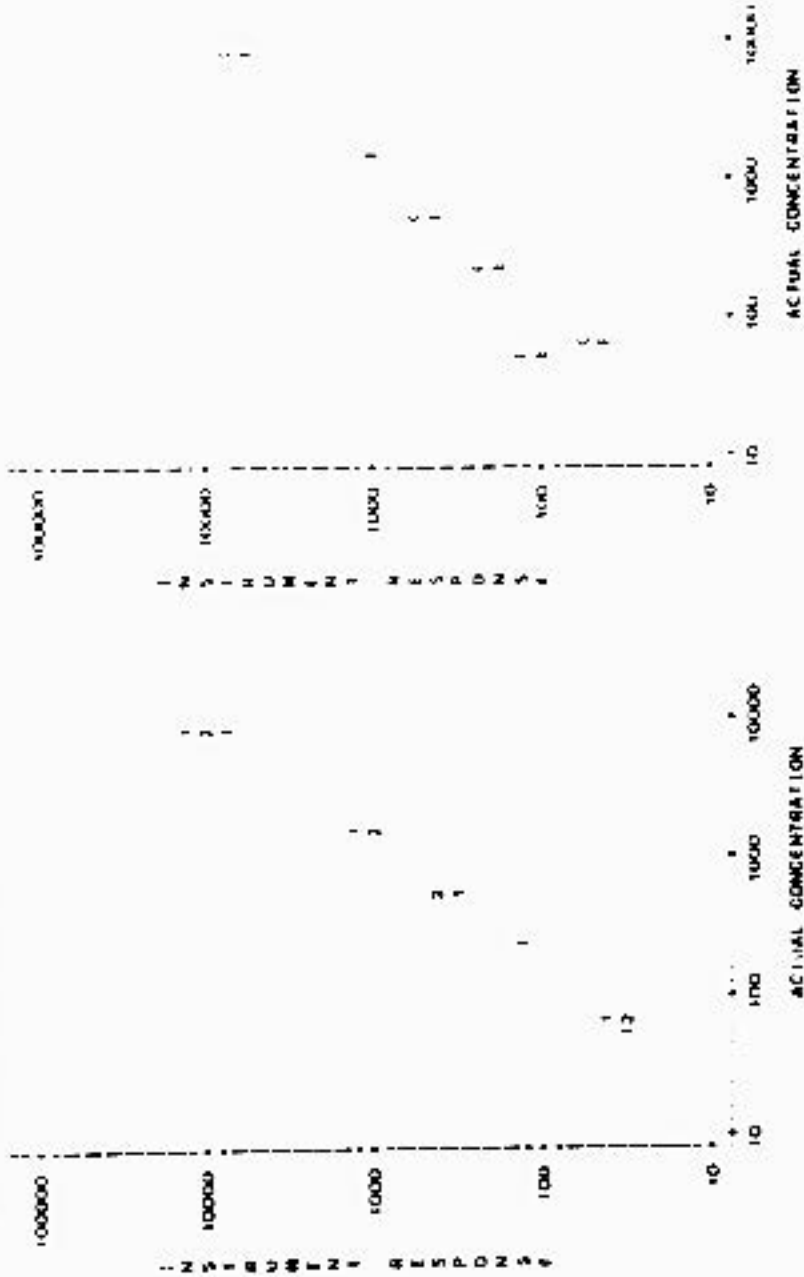

NOTE 7 OBS HIDDEN

NOTE 7 OBS HIDDEN

TABLE 5.87

DISPERSE FACIOM SUMMARY

TYPE		M E S P O N S E F A C I O M S										
INSTRUMENTS		ACTUAL PPMV					OVERALL					
NOMINAL PPMV	LOW	HIGH	MEAN	SE	N	COEFF SE	N	2254 SE	N	2159 SE	N	1871 SE
2000	189	189	189	0.16	2	1.40	1	1.14	1			
7000	111	113	112	0.11	3	1.08	1	1.90	1			
12000	1166	1186	1186	0.106	3	2.14	1	2.26	1			
OVERALL MEANS		180		0.03	6	1.74	0.23	3	1.06	0.16	3	
ESTIMATED AT 10 INKX PPMV		3.02										
		95 % CONFIDENCE INTERVAL										
		1.48					3.92					
TYPE		M E S P O N S E F A C I O M S										
INSTRUMENTS		ACTUAL PPMV					OVERALL					
NOMINAL PPMV	LOW	HIGH	MEAN	SE	N	COEFF SE	N	21 SE	N	19 SE	N	15 SE
2000	189	189	189	0.02	1	0.82	1	0.82	1			
7000	112	113	113	0.11	1	1.11	1	1.11	1			
12000	1166	1186	1186	0.106	1	1.04	1	1.04	1			
OVERALL MEANS		124										
ESTIMATED AT 10 INKX PPMV		3.11										
		95 % CONFIDENCE INTERVAL										
		1.21					4.91					


Figure 5-87

INSTRUMENT RESPONSE VS CONCENTRATION

ETHYL ACETOACRYLATE

JVA ORGANIC VAPOR ANALYZER

TUV HYDROCARBON UNIT/EN

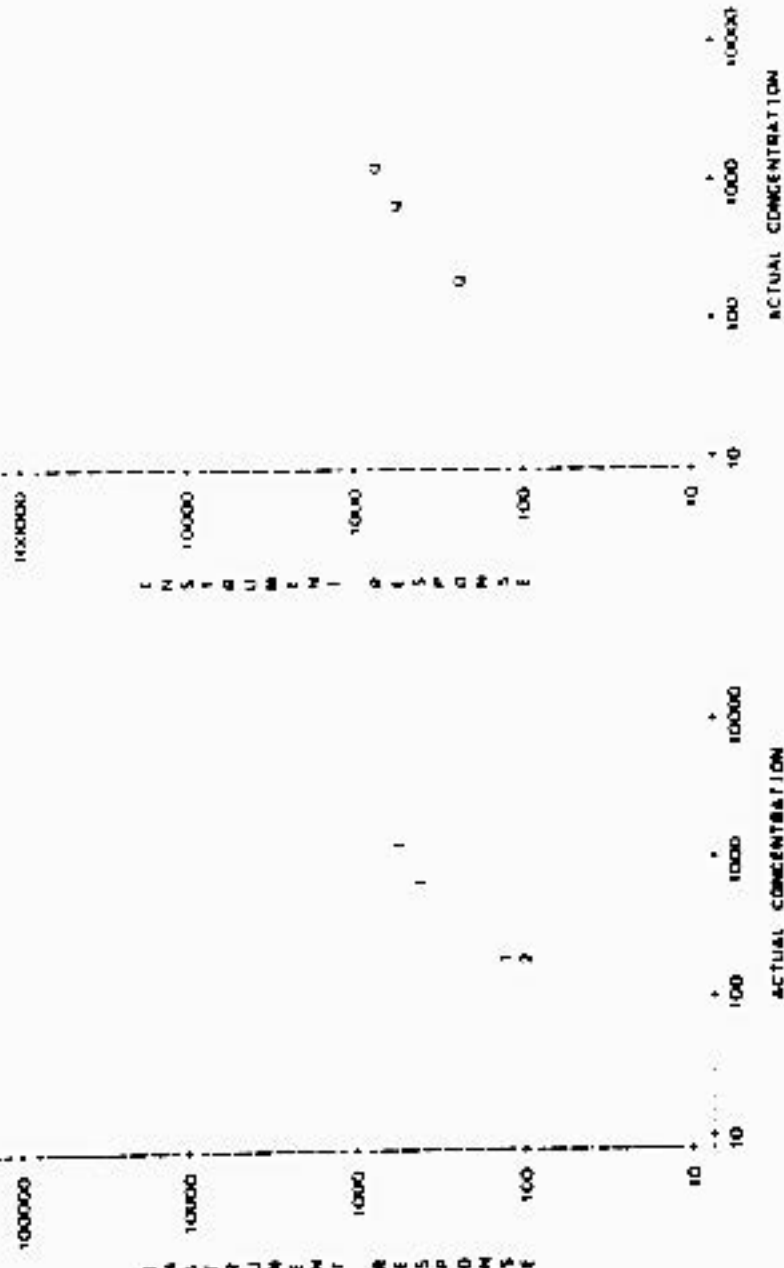

NOTE 2 OBS MIDDEN

TABLE 5. MR.

RESPIRATOR FIELD SUMMARS

TYPE SUBJECT

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPIRATOR FIELD SUMMARS									
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2254	SE	N	3010	SE	N	
2000	212	212	212	1.00	0.000	2	1.00		1	1.00		1				
15000	1495	1495	1495	1.41	0.10	2	1.54		1	1.18		1				
60000	6204	6204	6204	0.75	0.000	2	0.15		1	0.15		1				
80000	7927	7927	7927													

OVERALL MEANS 1.36 (1.04) 0.13 1.11 (1.03) 0.14

ESTIMATED AT 10 000 PPMV 0.12

95 % CONFIDENCE INTERVAL 1.05 0.99 0.94 1.17

FLY INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPIRATOR FIELD SUMMARS									
	LOW	HIGH	MEAN	MEAN	SE	N	10	SE	N	77	SE	N	70	SE	N	
200	212	212	212													
1500	1495	1495	1495													
6000	6204	6204	6204													
8000	7927	7927	7927													

OVERALL MEANS

ESTIMATED AT 10 000 PPMV

95 % CONFIDENCE INTERVAL


Figure 3-BB

INSTRUMENT RESPONSE VS. CONCENTRATION

ETHYL ACETATE

FLY HYDROCARBON SNIFFER

UVA ORGANIC VAPOR ANALYZER

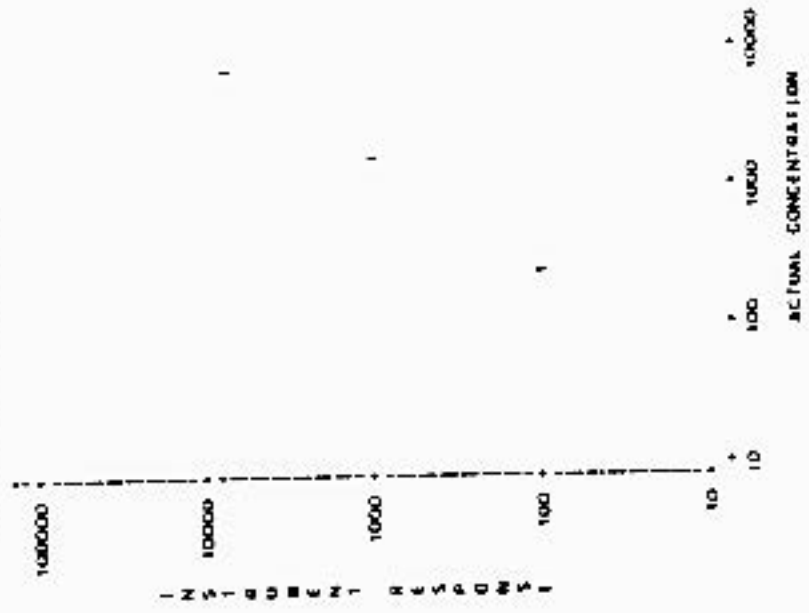

NOTE: 3 OBS HIDDEN



PARTY 5 HV

RESPONSE FAILURE SUMMARY

FIFTY CHLORACETATE

OVA INSTRUMENTS

DISCONTINUED TESTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OVA METERS									
	LOW	HIGH	MEAN	MEAN	SE	NO. OF	NO.	SE	N	NO.	SE	N	NO.	SE	N	
200	210	215	215	1.98	0.18	2	1.80		1	1.08						
1500	1520	1525	1525	1.90	0.13	2	1.89		1	1.92						
4200	3981	3981	3981	1.90	0.100	2	1.89		1	1.92						
OVERALL MEANS							1.94	0.14	6	1.89	1.08	3	2.00	1.05	1	

ESTIMATED AT 10,000 PPMV 1.97 95% CONFIDENCE INTERVAL 1.516 - 2.211

FIVE INSTRUMENTS

DISCONTINUED TESTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OVA METERS									
	LOW	HIGH	MEAN	MEAN	SE	NO. OF	NO.	SE	N	NO.	SE	N	NO.	SE	N	
200	215	215	215	0.82		1										
1500	1525	1525	1525	1.00		1										
4200	3981	3981	3981	1.35		1										
OVERALL MEANS							1.06		3							

ESTIMATED AT 10,000 PPMV 1.47 95% CONFIDENCE INTERVAL 1.0197 - 1.731



Figure 5 (H)

COMPARISON OF SPINNE VS. THERM DEGRADATION  
 ETHYL CHLORIDE FALL

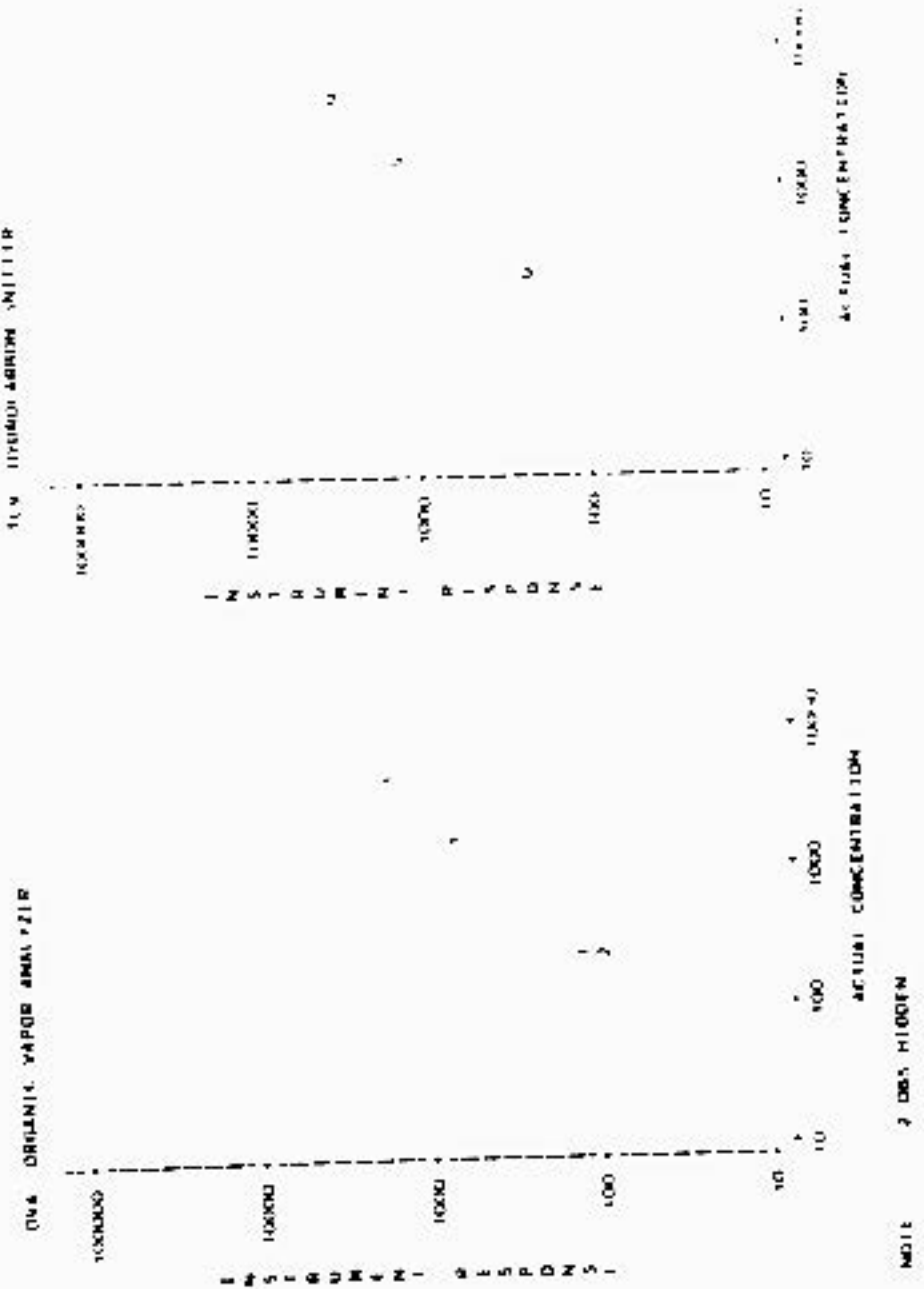


TABLE 1-10

RESPIRE FACIOP SUMMERY

DATA TABLE

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR ITEMS												
	LOW	HIGH	MEAN	SE	N	1020	54	N	2254	54	N	3150	54	N	1014	54	N
2000	2006	2006	2006	2006	2	1.98		1	1.04								
15000	1487	1487	1487	1487	2	1.76		1	1.88								
60000	6148	6148	6148	6148	2	1.01		1	0.95								
80000	8390	8390	8390	8390	2			1									

OVERALL MEANS 1.51 0.00 6 1.59 0.30 1 1.56 0.12 1

ESTIMATED AT 10,000 PPMV 0.97

95% CONFIDENCE INTERVAL 1.01 1.281

FLY INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTOR ITEMS												
	LOW	HIGH	MEAN	SE	N	71	58	N	71	58	N	101	58	N	70	58	N
2000	2006	2006	2006	0.35	1										1.95		
15000	1487	1487	1487	0.75	1										2.75		
60000	6148	6148	6148	1.08	1										1.46		
80000	8390	8390	8390	1.01	1										1.01		


OVERALL MEANS 0.86

ESTIMATED AT 10,000 PPMV 1.11

95% CONFIDENCE INTERVAL 1.11 1.211

Figure 5-90

INSTRUMENT RESPONSE VS CONCENTRATION

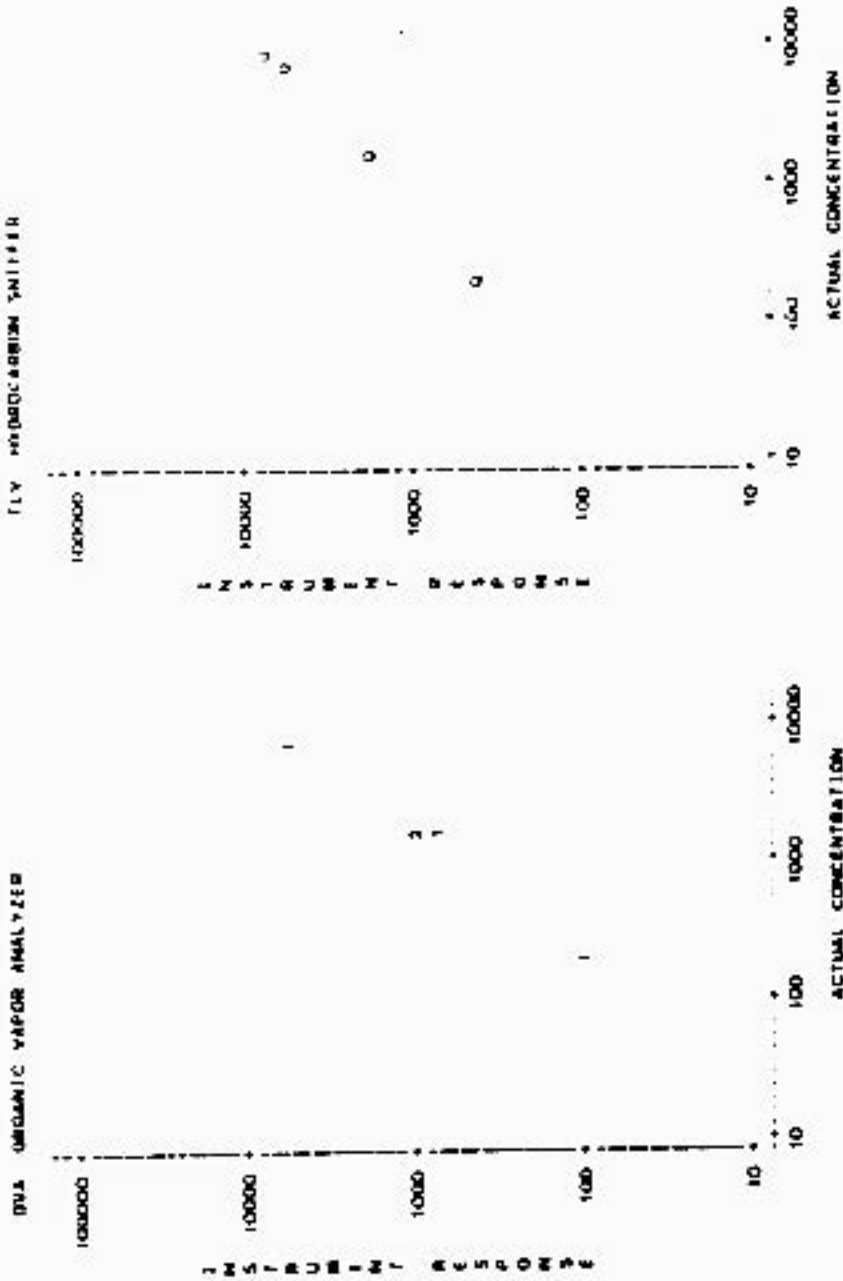

NOTE: 2 ORS HIGH

TABLE 5-91

RESPONSE FACTOR SUMMARY

11V INSTRUMENTS

11V INSTRUMENTS

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METERS								
	LOW	HIGH	MEAN	MEAN	SE	N	1080	SE	M	2704	SE	M	2	31	M
50	50	60	55	2.01	0.20	4	1.82	0.18	2	2.31	0.02	2			
200	201	201	201	0.01	0.01	2	0.66		1	0.88		1			
500	506	562	559	2.08	0.02	4	2.07	0.08	2	2.11	0.02	2			
1500	1482	1482	1482	0.52	0.00	2	0.52		1	0.52		1			
3000	3254	3254	3254	0.35	0.01	2	0.34		1	0.36		1			
4000	4024	4906	4485	1.28	0.02	2	1.28		1	1.28		1			
8000	7439	8848	8329	1.23	0.04	4	1.28	0.13	2	1.17	0.21	2			
OVERALL MEANS				1.35	0.00	20	1.11	0.21	10	1.38	0.24	10			

ESTIMATED AT 10,000 PPMV 0 TO

95% CONFIDENCE INTERVAL 1.045 1.001

11V INSTRUMENTS

11V INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METERS								
	LOW	HIGH	MEAN	MEAN	SE	N	1080	SE	M	2704	SE	M	2	31	M
50	50	60	55	1.80	0.38	4	1.93	0.01	2	1.18	0.01	2			
200	201	201	201	0.80		1			1			1			
500	506	562	559	8.56	1.94	4	10.50	0.12	2	2.62	0.12	2			
1500	1482	1482	1482	0.82		1			1			1			
3000	3254	3254	3254	1.41		1			1			1			
4000	4024	4906	4485	12.89	10.7	2	32.62		1	4.1		1			
8000	7439	8848	8329	12.28	8.56	5	27.09	1.20	2	3.05	0.31	2			
OVERALL MEANS				7.11	0.18	19	15.95	4.84	7	2.54	0.41	7			

ESTIMATED AT 10,000 PPMV 3.14

95% CONFIDENCE INTERVAL 1.42 0.921

FIGURE 5-91

INSTRUMENT RESPONSE VS CONCENTRATION

ETHYLBENZENE

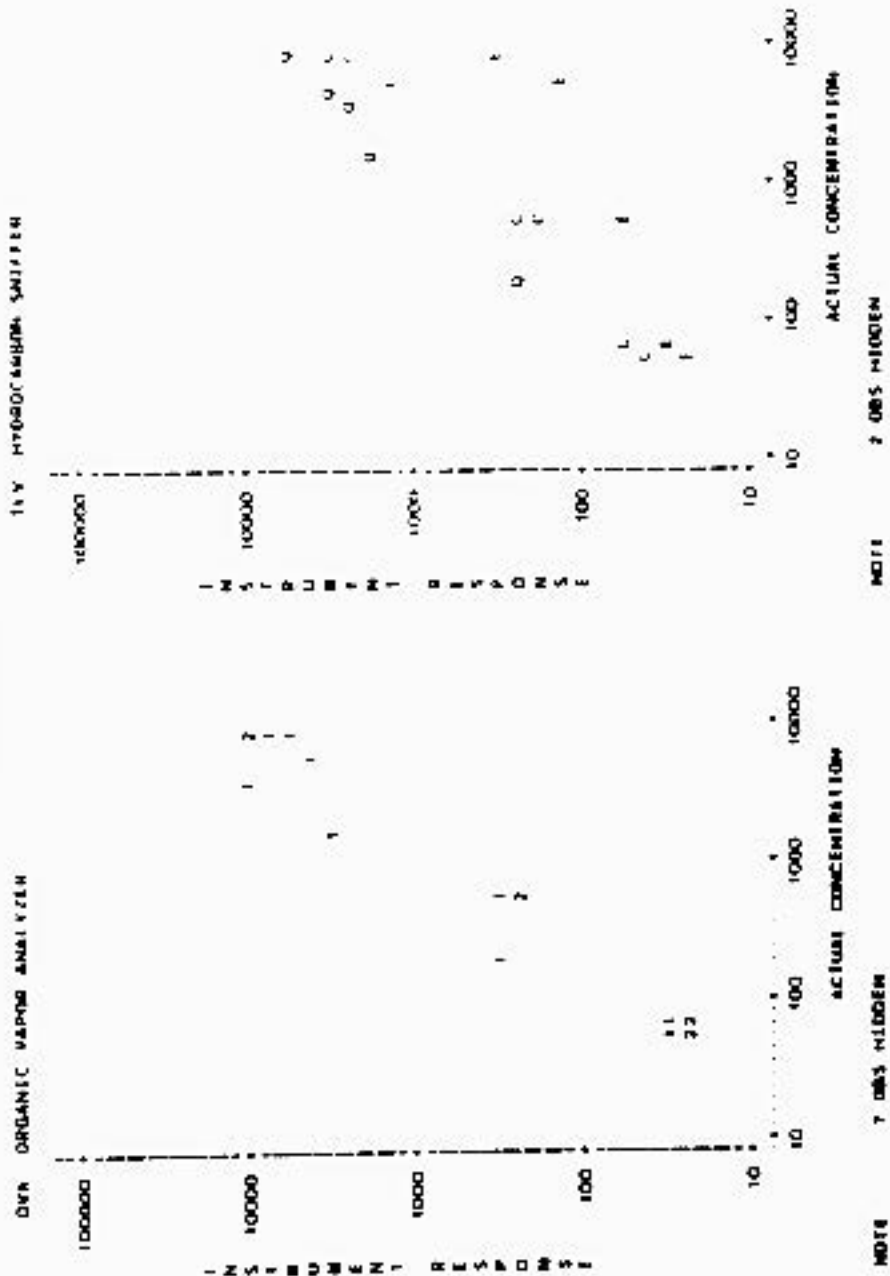


TABLE 1.97

RESPONSE FACTOR SUMMARY

PLUTONIUM

OVA INSTRUMENTS R I S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV		OVERHAUL		OVA METERS											
	LOW	HIGH	MEAN	SE	MEAN	SE	M	SE	M	SE	M	SE	M	SE	M	SE
1000	989	989	989	4.79	0.23	2	5.02	1	4.56	1						
4000	4482	4482	4482	0.94	0.03	2	0.95	1	0.93	1						
6000	6220	6220	6220	0.94	0.02	2	0.96	1	0.92	1						
8000	8411	8411	8411													
20E3	20E3	20E3	20E3													

OVERALL MEANS 2.23 0.01 6 2.31 0.02 2.14 1.21 1

ESTIMATED AT 10 000 PPMV 0.53 95% CONFIDENCE INTERVAL 1.00 0.99 0.987

TLV INSTRUMENTS

R E S P O N S E F A C T O R S

NOMINAL PPMV	ACTUAL PPMV		OVERHAUL		TLV METERS											
	LOW	HIGH	MEAN	SE	MEAN	SE	M	SE	M	SE	M	SE	M	SE	M	SE
1000	989	989	989	1.35		1										1.15
4000	4482	4482	4482	1.95		1										1.15
6000	6220	6220	6220	1.35		1										1.85
8000	8411	8411	8411	1.34		1										1.84
20E3	20E3	20E3	20E3	1.79	0.02	2										1.74

OVERALL MEANS 1.48 0.02 6

ESTIMATED AT 10 000 PPMV 1.49 95% CONFIDENCE INTERVAL 1.52 1.481

Figure 5-92

INSTRUMENT RESPONSE VS CONCENTRATION

ELEMENTS

ORGANIC VAPOR ANALYZER

FLUORINE ANALYZER

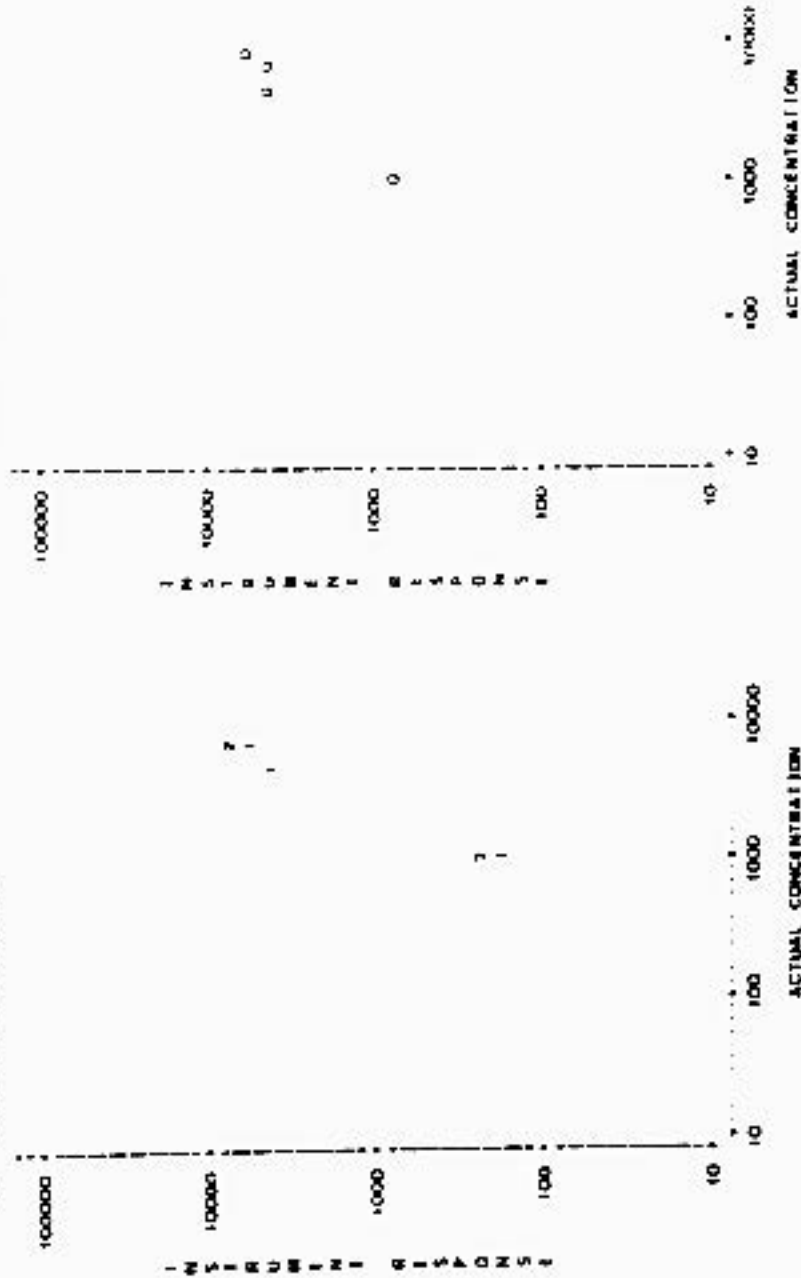




TABLE 5-11

RESPONSE FACTOR SUMMARY

ETHYLENE OXIDE

UVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		UVA INSTRUMENTS											
	LOW	HIGH	MEAN	SE	%	NO. 1	NO. 2	NO. 3	NO. 4	NO. 5	NO. 6	NO. 7	NO. 8	NO. 9	NO. 10	
1000	998	999	998	0.33	2											
4500	4444	4444	4444	0.075	2											
8000	8430	8430	8430	0.02	2											
OVERALL MEANS					1.0000											

ESTIMATED AT 10,000 PPMV 2.12

95% CONFIDENCE INTERVAL 1.741 - 2.501

UVB INSTRUMENTS


NOMINAL PPMV	ACTUAL PPMV		OVERALL		UVB INSTRUMENTS											
	LOW	HIGH	MEAN	SE	%	NO. 1	NO. 2	NO. 3	NO. 4	NO. 5	NO. 6	NO. 7	NO. 8	NO. 9	NO. 10	
1000	998	999	998	0.33	2											
4500	4444	4444	4444	0.075	2											
8000	8430	8430	8430	0.02	2											
OVERALL MEANS					1.0000											

ESTIMATED AT 10,000 PPMV 2.41

95% CONFIDENCE INTERVAL 1.92 - 2.901

FIGURE 5-91

INSITU AND IN VAPOR ANALYSIS VS. CONCENTRATION

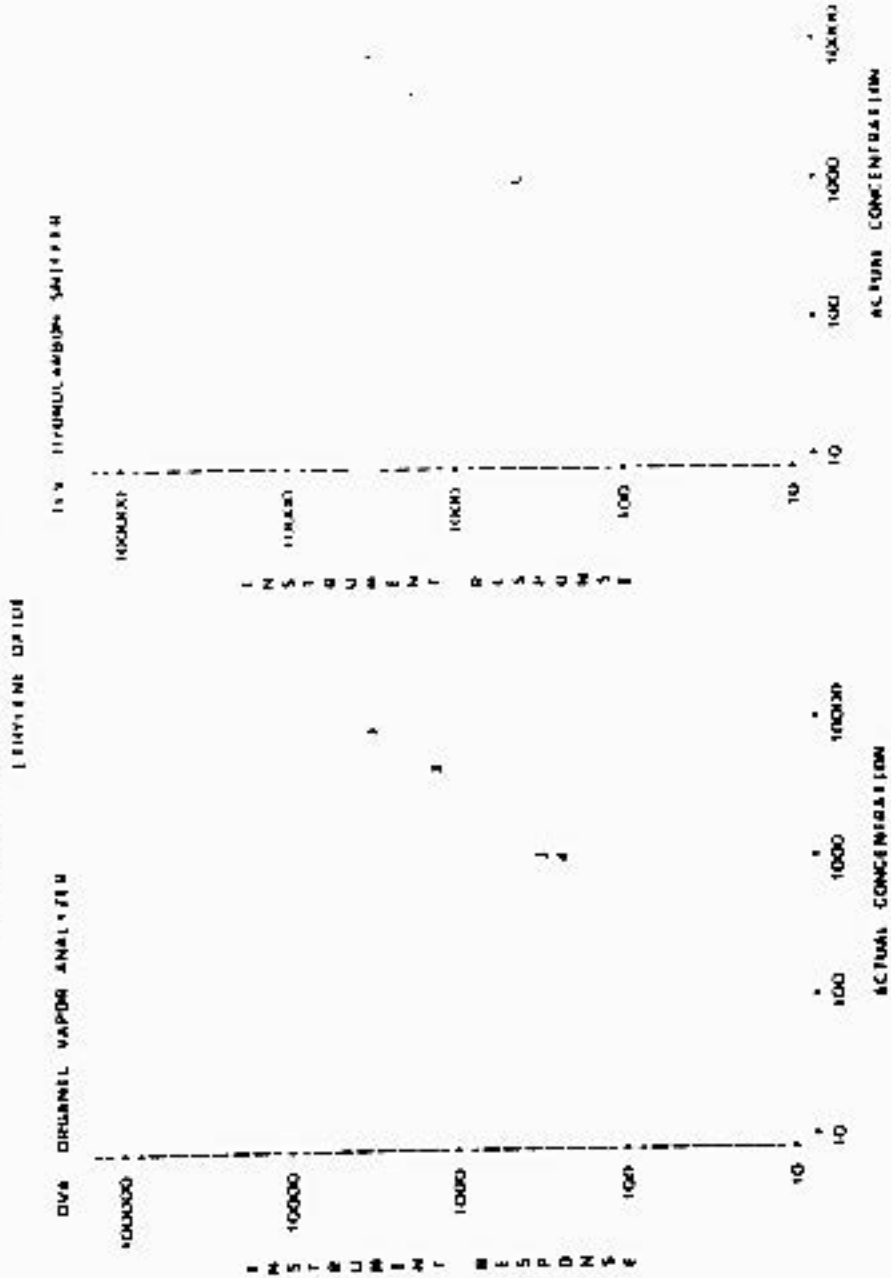

NOTE: 7 OBS. HIDDEN

TABLE 5.9A

RESPONSE TABLE SUMMARY

ETHYLENE DIAMINE

O P N O N S E F A I I O P S  
DMA METERS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		N	SE	N	10SD	SE	N	2SD	SE	N	10SD	SE	
	LOW	HIGH	MEAN	SE												
200	224	224	210.01	2.34	2	2.30	1			1						
1500	1548	1548	1610.02	1.69	2	1.69	1			1						
8000	1636	1636	1600.08	1.91	2	1.91	1			1						
			OVERALL MEANS	1590.01	6	1.51	17	2.08	0.267	1						

ESTIMATED AT 10 000 PPMV 1.78  
95% CONFIDENCE INTERVAL 1.10 2.26

DMV ENSTRUMENTS

M R P O N S F A I I O P S  
DMV METERS


NOMINAL PPMV	ACTUAL PPMV		OVERALL		N	SE	N	10SD	SE	N	2SD	SE	N	10SD	SE	
	LOW	HIGH	MEAN	SE												
200	224	274	1.05		1					1						
1500	1548	1548	1.43		1					1						
8000	1636	1636	2.47		1					1						
			OVERALL MEANS	1.65	1					1						

ESTIMATED AT 10 000 PPMV 2.46  
95% CONFIDENCE INTERVAL 1.18 1.83

Figure 3-9c

INSTRUMENT RESPONSE VS CONCENTRATION

ETHYLENEDIAMINE

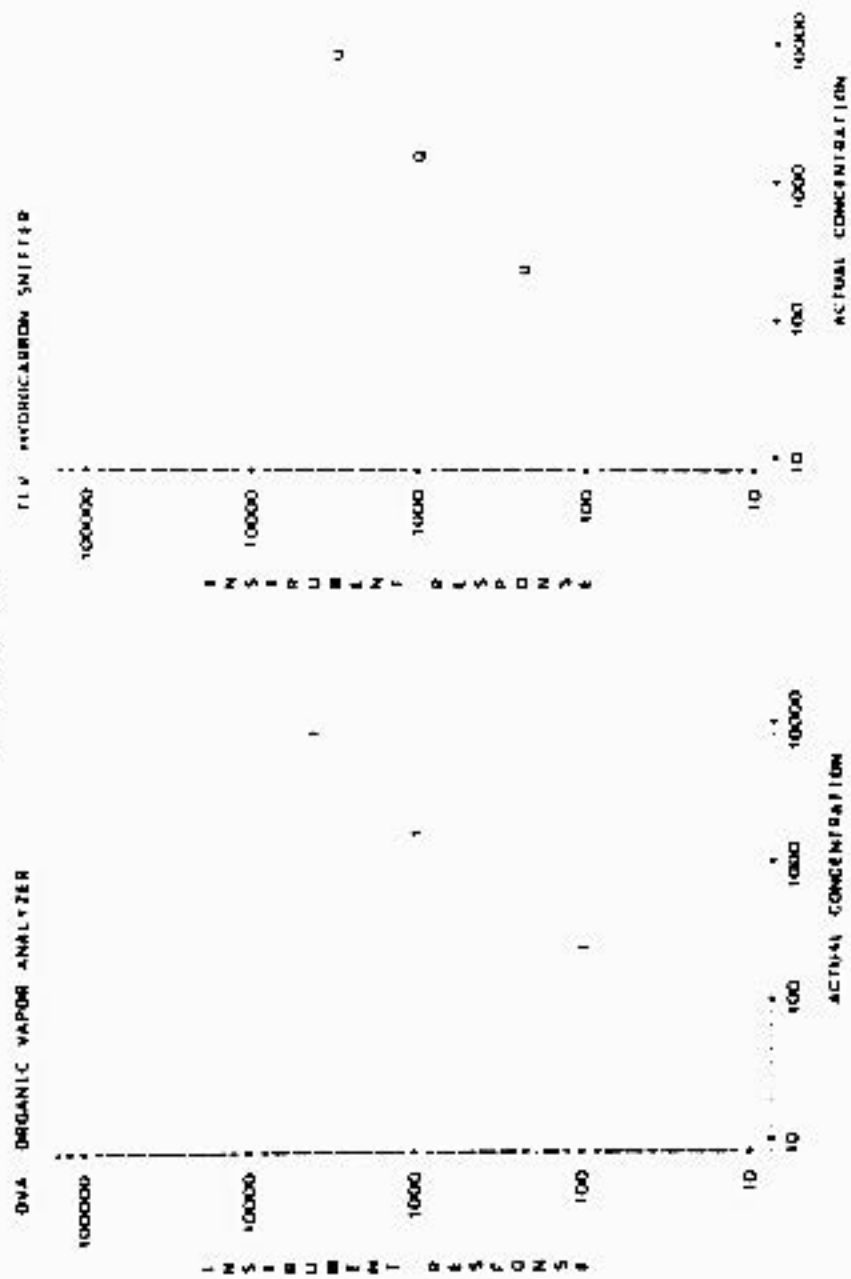

NOTE: 3 OBS. HIGHEN

TABLE 10.

DEFENSE FACTOR SUMMARY

INITIAL ACTS

DEFENSE FACTOR SUMMARY

INITIAL ACTS	DEFENSE FACTOR SUMMARY			
	MEAN	SE	N	OVERALL
ACTUAL PPMV	120.8	1.30	1	120.8
ESTIMATED AT 10 DAYS PPMV	112.8	1.82	1	112.8
OVERALL MEANS	116.8	1.56	2	116.8

INITIAL MEANS IN 10 DAYS PPMV

ESTIMATED AT 10 DAYS PPMV

NEW INSTRUMENTS

DEFENSE FACTOR SUMMARY

NEW INSTRUMENTS	DEFENSE FACTOR SUMMARY			
	MEAN	SE	N	OVERALL
ACTUAL PPMV	24.2	1.10	2	24.2
ESTIMATED AT 10 DAYS PPMV	22.8	1.56	2	22.8
OVERALL MEANS	23.5	1.33	4	23.5

INITIAL MEANS IN 10 DAYS PPMV

ESTIMATED AT 10 DAYS PPMV

OVERALL MEANS

DEFENSE FACTOR SUMMARY

OVERALL MEANS	DEFENSE FACTOR SUMMARY			
	MEAN	SE	N	OVERALL
INITIAL ACTS	116.8	1.56	2	116.8
NEW INSTRUMENTS	23.5	1.33	4	23.5
OVERALL MEANS	70.1	1.45	6	70.1

INITIAL MEANS IN 10 DAYS PPMV

ESTIMATED AT 10 DAYS PPMV


Figure 5-95

INSTRUMENT RESPONSE VS. CONCENTRATION

FORMIC ACID

11V HYDROLABON SWIFTEK

OVA ORGANIC VAPOR ANALYZER

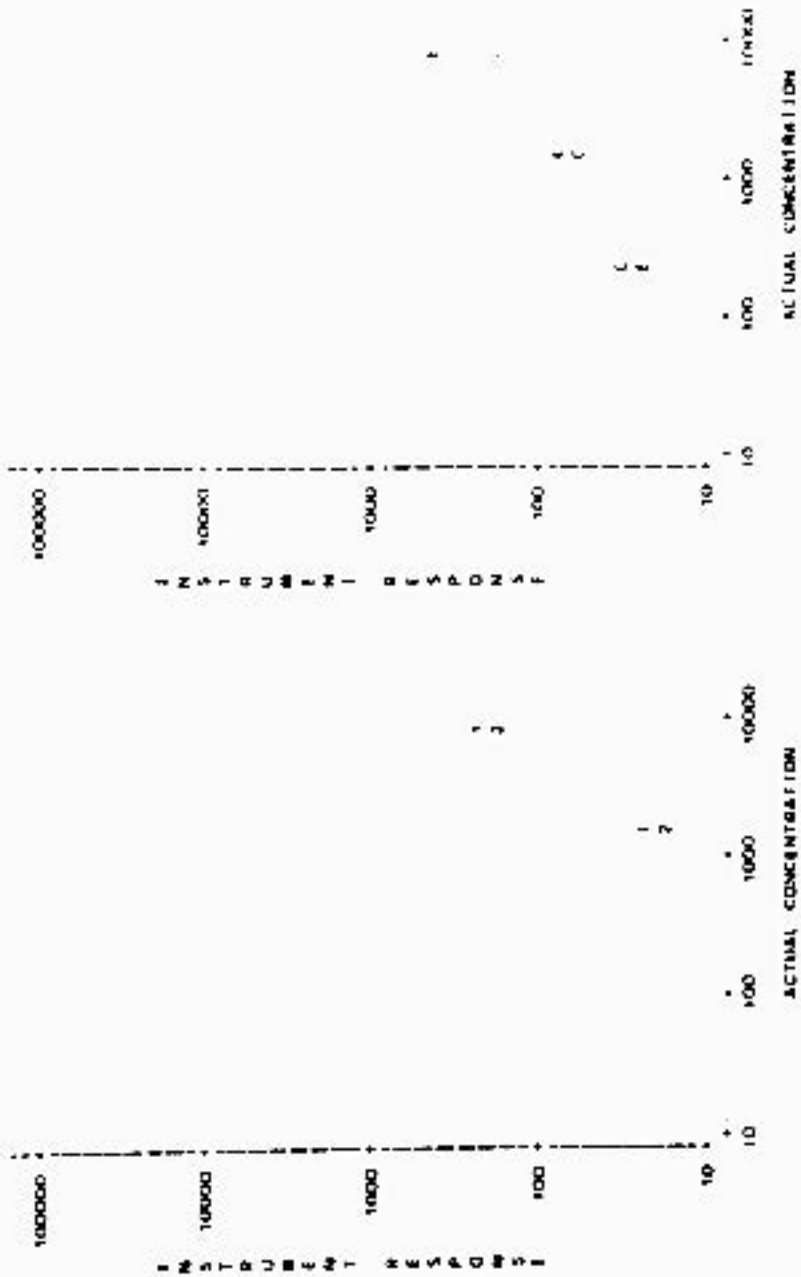

NOTE: 2 DOTS AND MISSING VALUES OR VERY DIRTY

DESIGN SUMMARY

ITEM 12

QVA MEASUREMENTS

MEMBER	ACTUAL PPMV			OVERALL			REPRESENTATIVE ELEMENTS							
	LOW	HIGH	MEAN	SE	N	1200	SE	N	2700	SE	N	3600	SE	N
500	530	530	530	0.00	2	3.06	1	3.06	1	3.06	1	3.06	1	3.06
1500	511	511	511	0.16	2	5.74	1	5.74	1	5.74	1	5.74	1	5.74
8000	7495	7495	7495	1.45	2	41.47	1	41.47	1	41.47	1	41.47	1	41.47
OVERALL MEANS			5.81	0.18	6	8.92	1.17	6	8.92	1.17	6	8.92	1.17	6

ESTIMATED AT 10 0000 PPMV 0.05 MS X 100000000 INTRINSIC ELEMENTS 1.6 10 11 11

QVA MEASUREMENTS

MEMBER	ACTUAL PPMV			OVERALL			REPRESENTATIVE ELEMENTS							
	LOW	HIGH	MEAN	SE	N	1200	SE	N	2700	SE	N	3600	SE	N
500	530	530	530	0.00	2	11.11	1	11.11	1	11.11	1	11.11	1	11.11
1500	511	511	511	0.46	2	17.14	1	17.14	1	17.14	1	17.14	1	17.14
8000	7495	7495	7495	3.47	2	11.13	1	11.13	1	11.13	1	11.13	1	11.13
OVERALL MEANS			10.00	0.66	6	14.22	1.70	6	14.22	1.70	6	14.22	1.70	6

ESTIMATED AT 10 0000 PPMV 1.18 MS X 100000000 INTRINSIC ELEMENTS 1.6 10 11 11

Figure 5-96

INSTRUMENT RESPONSE VS. LUMP CONCENTRATION

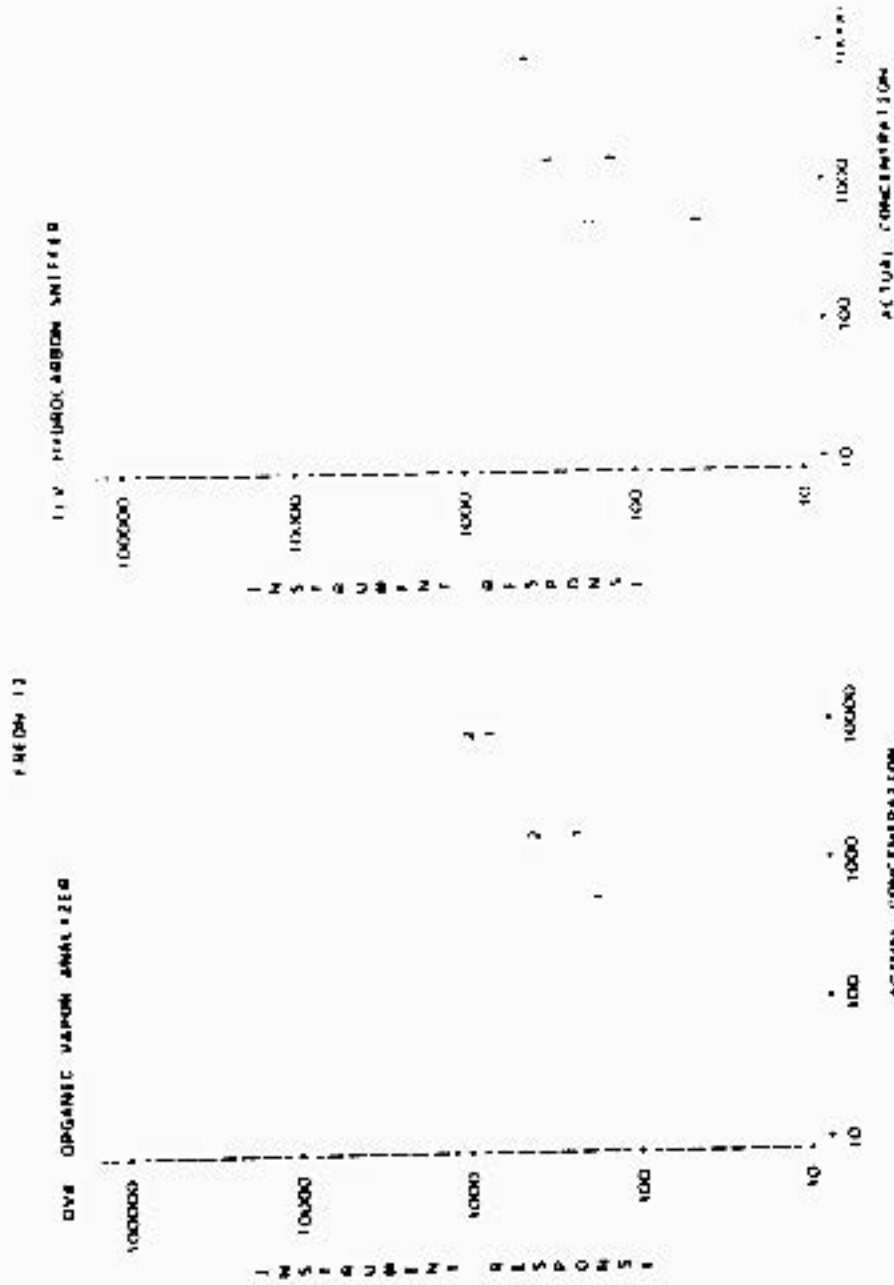




TABLE 5. M  
RESPONSE FACTING SUMMARY

ESTIMATED AT 10 000 PPMV

NOMINAL PPMV	ACTUAL PPMV			OVERALL			95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	MEAN	SE	N	LOW	SE	N	HIGH	SE	N
200	218	218	218	293	0.02	2	2.95		1	2.91		1
1500	1503	1503	1503	272	0.24	3	2.97		1	2.48		1
8000	7662	7662	7662	1083	0.38	2	10.26		1	5.11		1
OVERALL MEANS			542	0.11	8	5.29	3.43		3	5.47		3

ESTIMATED AT 10 000 PPMV

NOMINAL PPMV	ACTUAL PPMV			OVERALL			95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	MEAN	SE	N	LOW	SE	N	HIGH	SE	N
200	218	218	218	293	0.02	2	2.95		1	2.91		1
1500	1503	1503	1503	272	0.24	3	2.97		1	2.48		1
8000	7662	7662	7662	1083	0.38	2	10.26		1	5.11		1
OVERALL MEANS			542	0.11	8	5.29	3.43		3	5.47		3

ESTIMATED AT 10 000 PPMV


NOMINAL PPMV	ACTUAL PPMV			OVERALL			95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	MEAN	SE	N	LOW	SE	N	HIGH	SE	N
200	218	218	218	293	0.02	2	2.95		1	2.91		1
1500	1503	1503	1503	272	0.24	3	2.97		1	2.48		1
8000	7662	7662	7662	1083	0.38	2	10.26		1	5.11		1
OVERALL MEANS			542	0.11	8	5.29	3.43		3	5.47		3

ESTIMATED AT 10 000 PPMV

NOMINAL PPMV	ACTUAL PPMV			OVERALL			95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	MEAN	SE	N	LOW	SE	N	HIGH	SE	N
200	218	218	218	293	0.02	2	2.95		1	2.91		1
1500	1503	1503	1503	272	0.24	3	2.97		1	2.48		1
8000	7662	7662	7662	1083	0.38	2	10.26		1	5.11		1
OVERALL MEANS			542	0.11	8	5.29	3.43		3	5.47		3

FIGURE 3-47

INSTRUMENT RESPONSE VS. CONCENTRATION

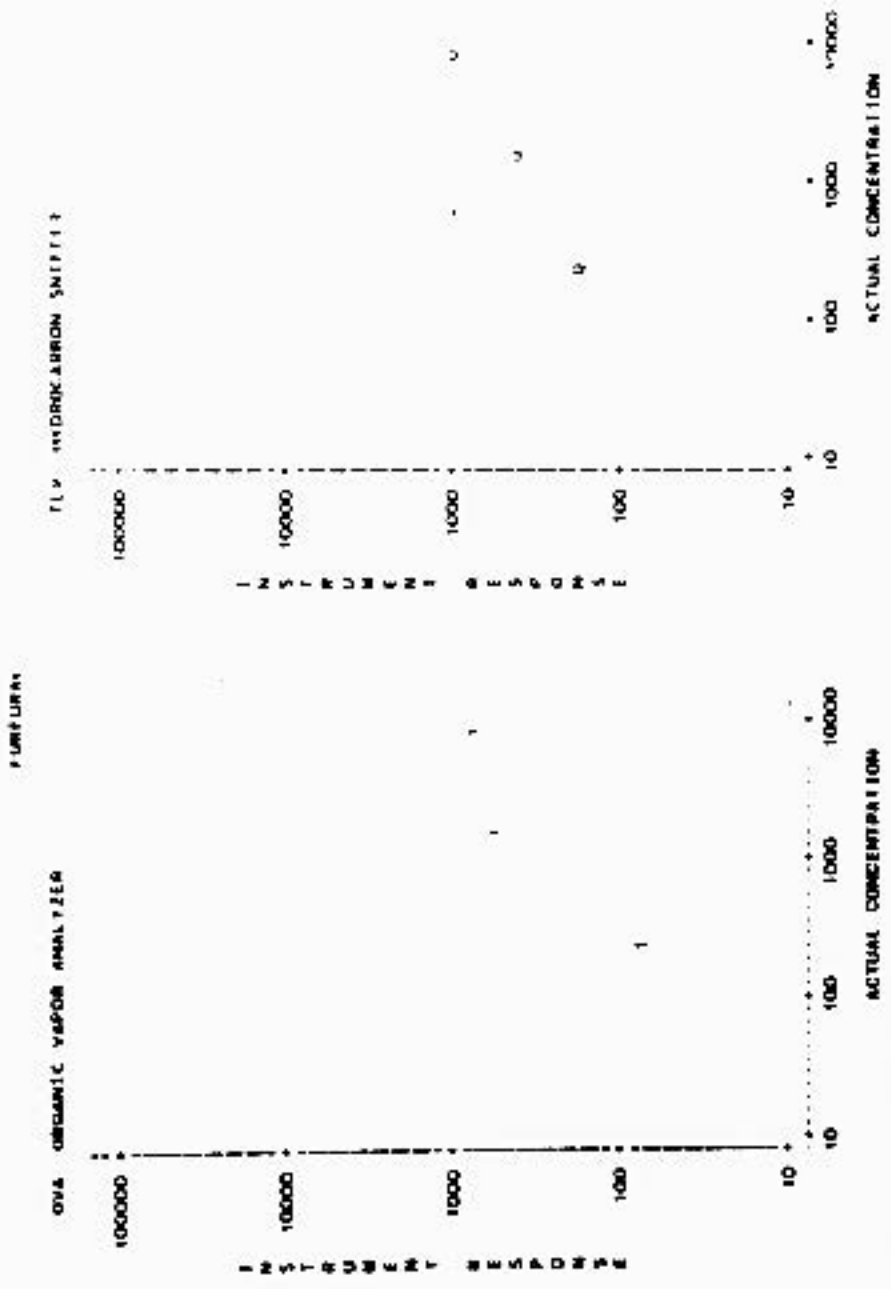

NOTE: 3 OMS HIDDEN

TABLE 5-4B

RESPONSE FACTOR SUMMARY

GLUCIDON

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OVA METERS						
	LOW	HIGH	MEAN	SE	M	U95	SI	M	SI	M	SI	M	SI
200	238	238	738	12.63	2.71	2	10.47	1	18.90	1			
1000	994	994	894	11.55	5.19	2	10.35	1	12.74	1			
2044	2044	2044	2044	9.76	0.12	2	9.05	1	10.48	1			
OVERALL MEANS			31.32	0.43	6	8.92	0.44	1	13.71	28	3		

ESTIMATED AT 10,000 PPMV 8.42

95% CONFIDENCE INTERVAL 5.54-11.61

TV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			TV METERS						
	LOW	HIGH	MEAN	SE	M	U95	SI	M	SI	M	SI	M	SI
200	238	238	738	4.70	0.75	2	5.45	1	1.95	1			
1000	994	994	894	4.56	0.83	2	5.49	1	1.73	1			
2044	2044	2044	2044	6.32	0.91	2	6.21	1	4.42	1			
OVERALL MEANS			4.86	0.14	6	5.44	0.77	1	4.10	20	4		

ESTIMATED AT 10,000 PPMV 5.27

95% CONFIDENCE INTERVAL 3.28-10.27

Figure 3-9B

INSTRUMENT RESPONSE VS. CONCENTRATION

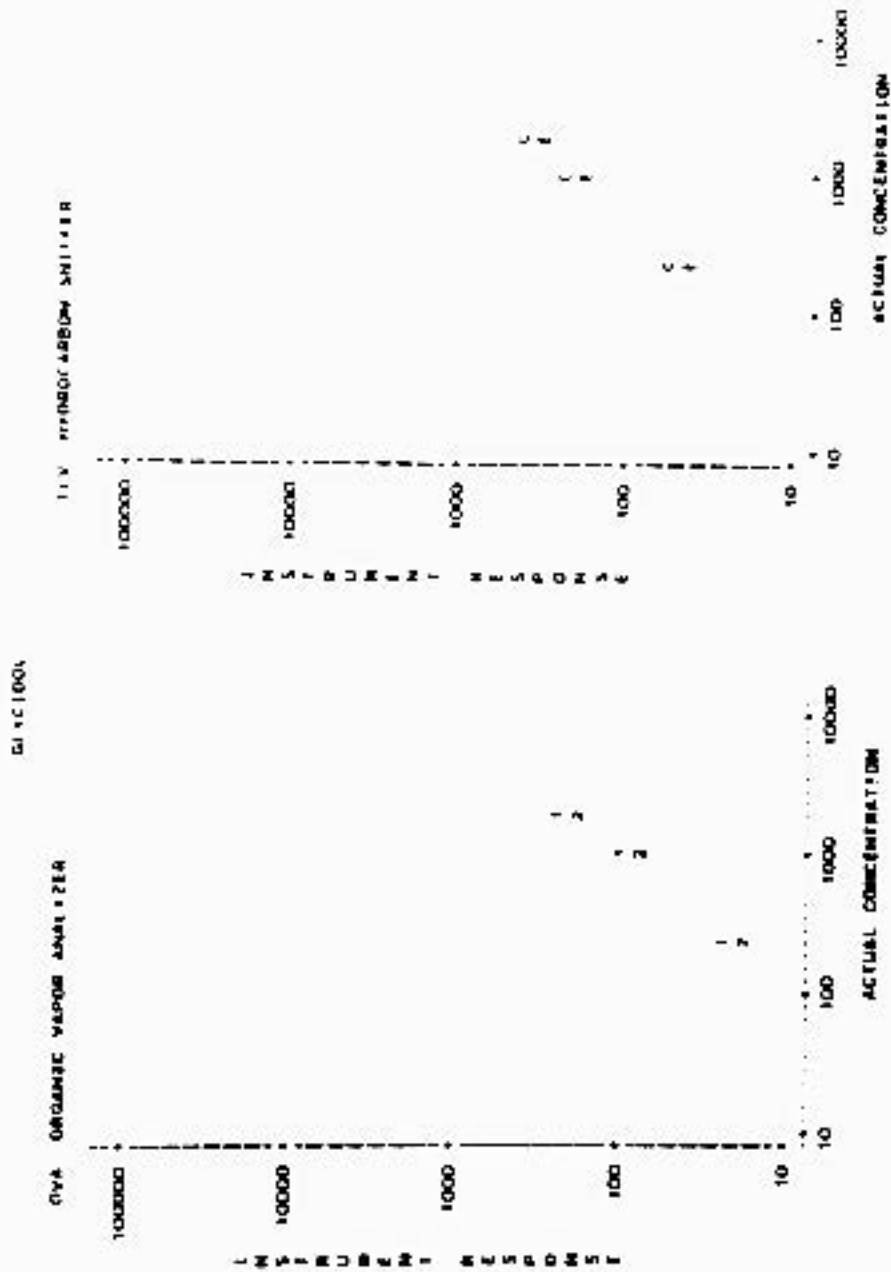


TABLE 5-99

RESPONSE FACTOR SUMMARY

REFUGES

GVA INSTRUMENTS		RESULTS FROM 11 A. C. T. D. R. S.																
NOMINAL PPMV	ACTUAL PPMV		OVERALL		OVER MEANS													
	LOW	HIGH	MEAN	SE	N	1000	51	N	2254	51	N	2159	51	N	1951	51	N	
200	234	234	234	1.00	1													
1500	1602	1602	1602	0.67	1													
4000	3319	3319	3319	0.39	1													
8000	4588	4588	4588		1													
	OVERALL MEANS		0.64		3													

ESTIMATED AT 10 000 PPMV 0.64

95% CONFIDENCE INTERVAL 0.12-0.15

TIV INSTRUMENTS

TIV INSTRUMENTS		RESULTS FROM 5 A. C. T. D. R. S.																
NOMINAL PPMV	ACTUAL PPMV		OVERALL		OVER MEANS													
	LOW	HIGH	MEAN	SE	N	78	51	N	76	51	N	76	51	N	76	51	N	
200	234	234	234	0.87	1													
1500	1602	1602	1602	0.82	1													
4000	3319	3319	3319	0.72	1													
8000	4588	4588	4588		1													
	OVERALL MEANS		0.64		3													

ESTIMATED AT 10 000 PPMV 0.75

95% CONFIDENCE INTERVAL 0.56-1.00

Figure 5-99

INSTRUMENT RESPONSE VS CONCENTRATION

HEPTANE

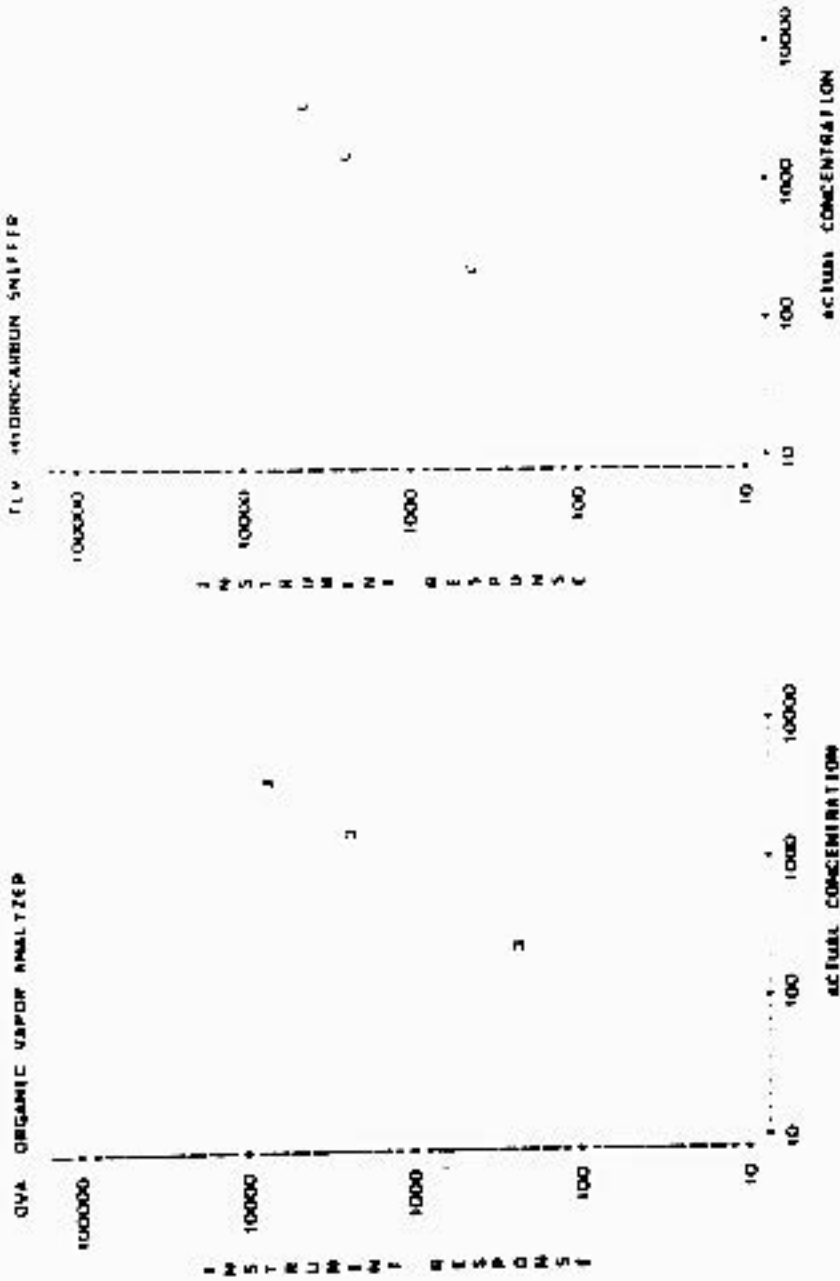


TABLE 5. 10M

RESPONSE FACTOR SUMMARY

40-NAME M

OVA INSTRUMENTS

0 1 2 3 4 5 6 7 8 9

NOMINAL PPMV	ACTUAL PPMV		OVERLAP		OVA METERS				
	LOW	HIGH	MEAN	ST	M	NOISE	SE	ST	ST
150	175	175	175	14	2	0.97	0.97	0.80	0.8
200	148	208	178	0.89	0.08	3	0.97	0.72	0.7
250	259	259	259	1.05	0.22	2	0.97	0.81	0.78
350	394	394	394	1.07	0.22	2	0.97	0.84	0.78
400	436	436	436	1.07	0.00	2	0.97	0.81	0.78
550	556	556	556	0.82	0.14	2	0.97	0.71	0.72
700	702	702	702	0.80	0.00	2	0.97	0.71	0.72
800	837	837	837	0.86	0.04	2	0.97	0.71	0.72
1200	868	1485	1047	0.84	0.02	4	0.97	0.76	0.72
1500	1518	1626	1521	0.76	0.04	3	0.97	0.76	0.72
1600	1720	1720	1720	0.72	0.04	3	0.97	0.76	0.72
2000	2105	2105	2105	0.81	0.01	1	0.97	0.61	0.72
2400	2352	2352	2352	0.47	0.62	1	0.97	0.61	0.72
3800	3020	3020	3020	0.47	0.62	1	0.97	0.45	0.72
3200	3243	3243	3243	0.26	0.60	2	0.97	0.45	0.72
3600	3634	3634	3634	0.38	0.60	2	0.97	0.48	0.72
4000	3645	4083	3870	0.40	0.61	4	0.97	0.48	0.72
5000	5005	5005	5005						
6000	6072	6072	6072						
8000	7266	7266	7266						

OVERALL MEANS

0	1	2	3	4	5	6	7	8	9
0.14	0.26	0.22	0.22	0.16	0.16	0.16	0.16	0.16	0.16

ESTIMATED AT 10 DEX PPMV

0	1	2	3	4	5	6	7	8	9
0.14	0.26	0.22	0.22	0.16	0.16	0.16	0.16	0.16	0.16

TABLE 5-100 (continued)  
RESPONSE FACTOR SUMMARY

HELANE M

REL SPONSE FACTORS

TV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		TV INSTRUMENTS												
	LOW	HIGH	MEAN	SE	N	TE	SE	N	TC	SE	N	TM	SE	N	TO	SE	N
100	176	176	176	0.48	1				0.48	1							
200	148	208	178	0.41	2				0.44	1				0.38			
250	258	258	258	0.52	1				0.53	1							
350	394	394	394	0.63	1				0.63	1							
400	428	428	428	0.65	1				0.65	1							
500	555	555	555	0.77	1				0.77	1							
700	703	703	703	0.47	1				0.47	1							
800	837	837	837	0.45	1				0.45	1							
1200	888	1188	1011	0.45	2				0.45	2				0.56			
1500	1518	1528	1521	0.57	2				0.59	1							
1600	1720	1720	1720	0.85	1				0.85	1							
2000	2108	2108	2108	0.86	1				0.86	1							
2400	2352	2352	2352	0.52	1				0.70	1							
2800	3020	3030	3020	0.70	1				0.70	1							
3200	3249	3243	3243	0.52	1				0.82	1							
3600	3434	3634	3434	0.81	1				0.88	1				0.67			
4000	3846	4008	3870	0.98	1				0.77	1							
5000	5006	5006	5006	0.81	1				0.81	1				0.88			
6000	6073	6073	6073	0.89	1				0.89	1							
8000	7634	7780	7682	0.88	1				0.88	1				0.89			
OVERALL MEANS					0.59	0.00	26										

ESTIMATED AT 10,000 PPMV 0.72 95% CONFIDENCE INTERVAL 1.0 65.0 79.1



Figure 5-100

INSTRUMENT RESPONSE VS CONCENTRATION

10 RANGE IN


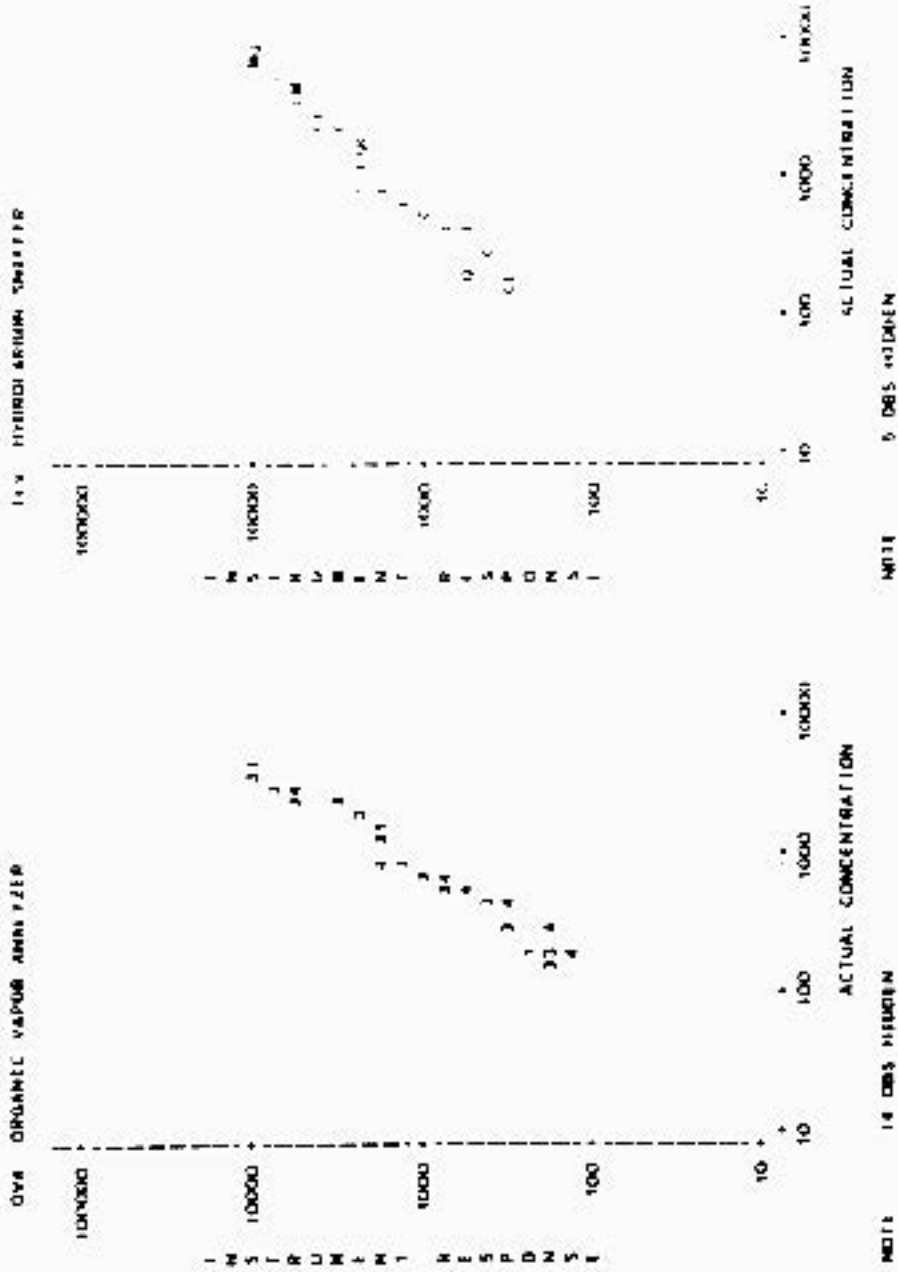




FIGURE 3  
 INSTRUMENT RESPONSE VS. CONCENTRATION  
 MERMEL

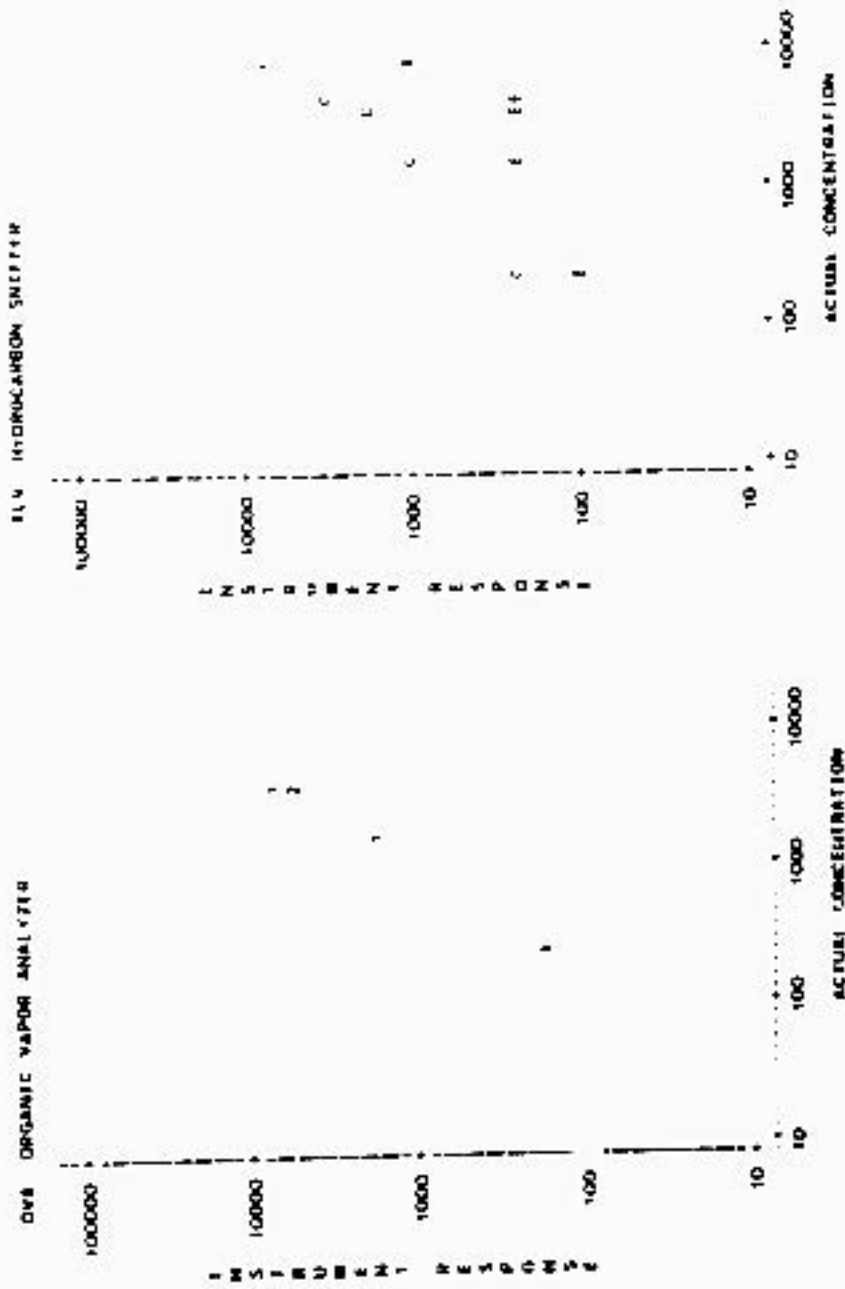

NOTE: 2 OBS. HIGHEN

TABLE 5. 1117

RESPONSE FACTOR SUMMARY

FINISHED ACTION

NOMINAL PPMV	ACTUAL PPMV		OVERALL		O.V.A. MEANS											
	LOW	HIGH	MEAN	SE	N	100BU	N	200A	N	300W	J	4	5	6	7	8
200	229	229	230	1.07	2	11	74	1	13	88	1					
1000	1494	1494	1494	0.31	2	14	79	1	14	16	1					
5000	5161	5561	5561	0.50	2	8	84	1	1	72	1					
8000	8111	8111	8111	0.81	2	10	81	1	8	85	1					

OVERALL MEANS 11 23 0 19 8 11 15 1 29 4 11 11 1 10 4

ESTIMATED AT 10,000 PPMV @ 20

95% CONFIDENCE INTERVAL 1 6 8 11 14

FLY ENCLOSURES

NOMINAL PPMV	ACTUAL PPMV		OVERALL		FLY MEANS											
	LOW	HIGH	MEAN	SE	N	21	24	26	27	28	29	30	31	32	33	34
200	229	229	229	0.44	2	5	28	1	7	70	1					
1000	1494	1494	1494	0.34	2	6	83	1	4	85	1					
5000	5161	5561	5561	0.52	2	13	80	1	6	11	1					
8000	8111	8111	8111	0.79	2	15	61	1	8	11	1					

OVERALL MEANS 7 26 0 24 8 9 11 2 27 4 6 12 1 21 4

ESTIMATED AT 10,000 PPMV @ 34

90% CONFIDENCE INTERVAL 1 6 21 28 33

Figure 3-102

INSTRUMENT RESPONSE VS. CONCENTRATION

HYDROCARBONS

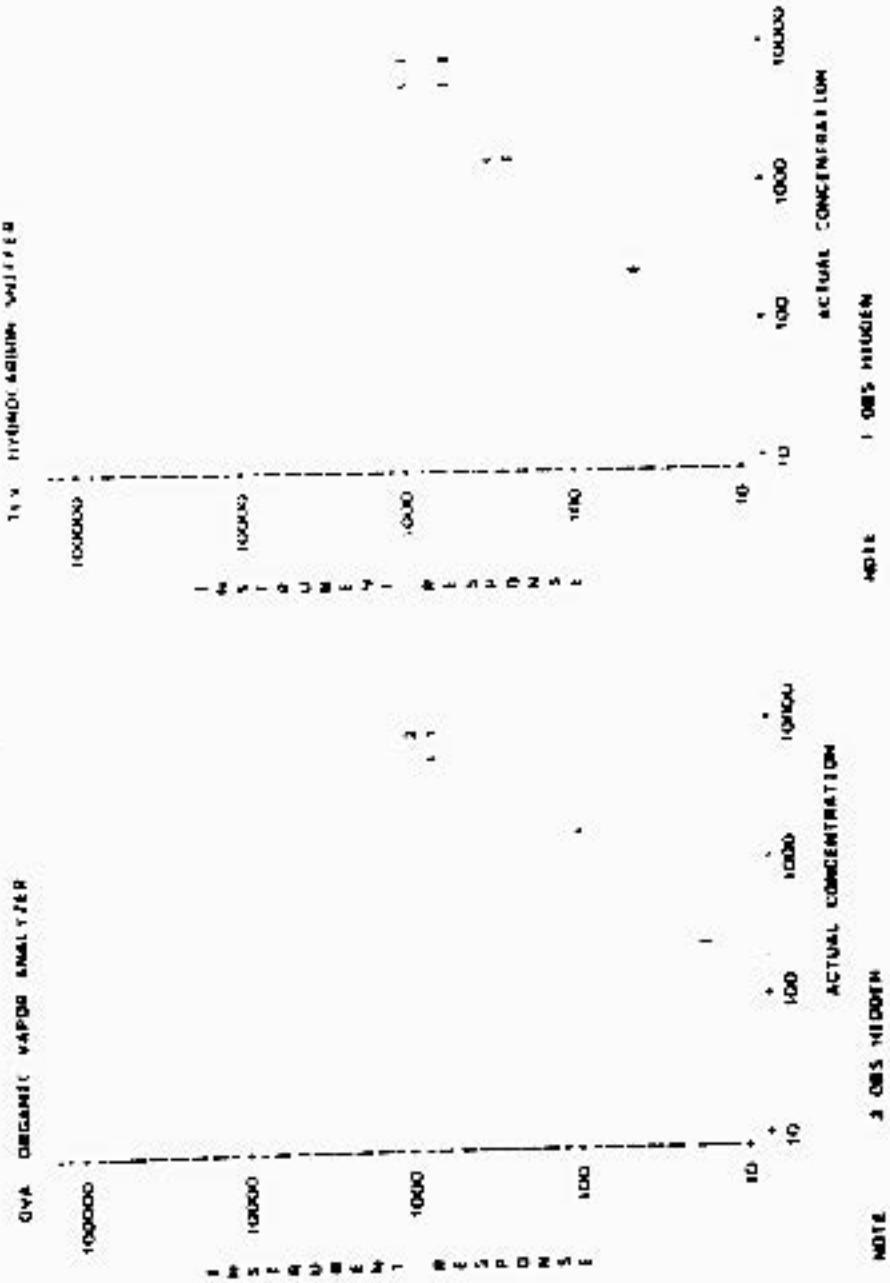


TABLE 1.10

RESPONSE FACTOR SUMMARY

ISOPHTANE

DVA INSTRUMENTS

ADJENAI PPMV	ACTUAL PPMV			OVERALL			R F S P O N S E F A C T O R S												
	LOW	HIGH	MEAN	MEAN	SE	N	LODR	SI	N	FISS	SE	N	FINV	SE	N	IRIT	SI	N	
1000	1223	1723	1223	1.14	0.03	2	1.12		1	1.37		1							
2000	2187	2187	2187	0.27	0.01	2	0.21		1	0.46		1							
4000	4114	4114	4114	0.81	0.02	2	0.61		1	0.63		1							
5000	4967	4967	4967	0.80	0.00	2	0.50		1	0.50		1							
8000	7900	7900	7900																
1383	1383	1383	1383																

OVERALL MEANS 0.67 LOD 4 U 02 D 18 4 0 04 0 0 4

ESTIMATED AT 10 INO PPMV U 00 95 % CONFIDENCE INTERVAL 1 0 19 0 951

FLV INSTRUMENTS

DVA INSTRUMENTS

ADJENAI PPMV	ACTUAL PPMV			OVERALL			R F S P O N S E F A C T O R S												
	LOW	HIGH	MEAN	MEAN	SE	N	LODR	SI	N	FISS	SE	N	FINV	SE	N	IRIT	SI	N	
1000	1223	1223	1223	0.55		1			1	0.15		1							
2000	2187	2187	2187	0.26	0.01	2	0.21		1	0.15		1							
4000	4114	4114	4114	0.64		1													
5000	4967	4967	4967	0.63		1													
8000	7900	7900	7900	0.58		1													
1383	1383	1383	1383	0.65		1													

OVERALL MEANS 0.54 LOD 1 0 11 1 0 36 1

ESTIMATED AT 10 INO PPMV U 61 95 % CONFIDENCE INTERVAL 1 0 44 0 861

Figure 5-103

INSITUUMENT RESPONSE VS CONCENTRATION

ISOBUTANE

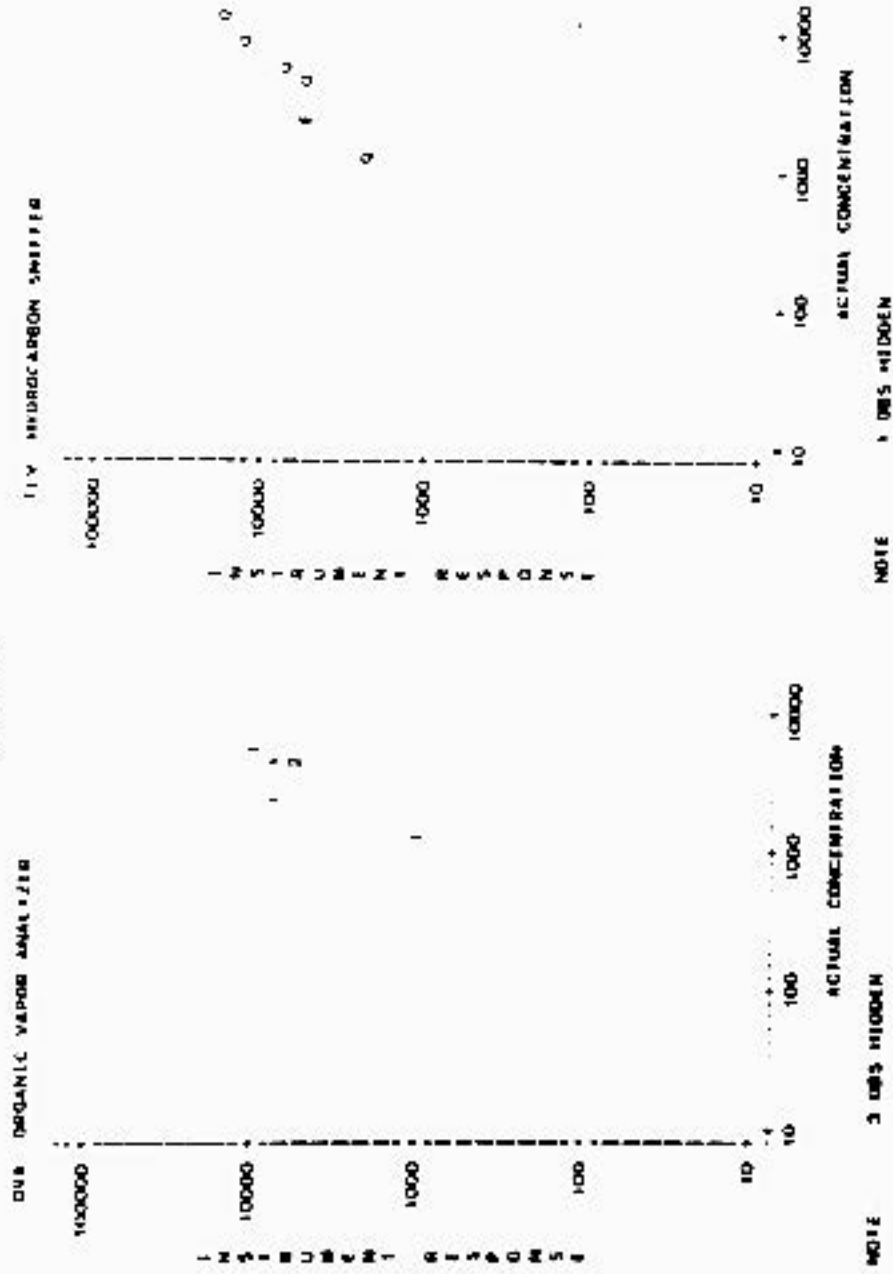


TABLE 1. CONT.

RESPIRATORY PARTICULATE SAMPLERS

3. INSTRUMENTS

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			US 5 CONFIDENCE INTERVAL						
	LOW	HIGH	MEAN	MEAN	SE	SE	LO	HI	SE	LO	HI	SE	SE
100	100	100	100	0.88	0.190	2	0.16	1	0.93	1	0.93	1	0.93
300	294	294	294	1.27	0.082	2	1.10	1	1.26	1	1.26	1	1.26
453	453	453	453	1.11	0.065	2	1.11	1	1.11	1	1.11	1	1.11
OVERALL MEANS			1.08	0.133	6	1.02	0.13	1	1.12	12	1	1.12	12

ESTIMATED AT 10 000 PPMV 7.42

US 5 CONFIDENCE INTERVAL 1 DAY 5 DAY

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			US 5 CONFIDENCE INTERVAL						
	LOW	HIGH	MEAN	MEAN	SE	SE	LO	HI	SE	LO	HI	SE	SE
100	100	100	100	0.87	0.34	2	1.26	1	0.47	1	0.47	1	0.47
300	294	294	294	2.19	1.22	2	3.41	1	0.97	1	0.97	1	0.97
453	453	453	453	1.70	0.80	2	2.50	1	0.86	1	0.86	1	0.86
OVERALL MEANS			1.56	0.14	6	2.41	0.83	3	0.71	15	1	0.71	15

ESTIMATED AT 10 000 PPMV 6.33

US 5 CONFIDENCE INTERVAL 1 DAY 5 DAY 41



FAJREF 5 105

RESPONSE FACTOR SUMMARY

ISOPRENE

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		R E S P O N S E F A C T O R S									
	LOW	HIGH	MEAN	SE	N	100%	SE	N	20%	SE	N	50%	SE	N
200	217	217	217	0.02	2	1.00	0.12	2	1.00	0.11	1	1.00	0.11	1
1000	1042	1043	1042	0.03	2	1.25	0.03	2	1.25	0.22	1	1.25	0.22	1
5000	5209	5209	5209	0.03	2	0.55	0.03	2	0.55	0.52	1	0.55	0.52	1
8000	7771	7771	7771											

OVERALL MEANS 1.26 @ LQ 6 1.24 @ ST 3 1.28 @ H 1

ESTIMATED AT 10,000 PPMV 0.48

95% CONFIDENCE INTERVAL 1.03 @ LQ 1.72 @ H

ILV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		R E S P O N S E F A C T O R S									
	LOW	HIGH	MEAN	SE	N	100%	SE	N	20%	SE	N	50%	SE	N
200	217	217	217											
1000	1042	1043	1042											
5000	5209	5209	5209											
8000	7771	7771	7771											

OVERALL MEANS

ESTIMATED AT 10,000 PPMV

95% CONFIDENCE INTERVAL

TABLE 1 1076

RESPONSE FACTOR SUMMARY

ISOPROPANE

OVA INSTRUMENTS		RESPONSE FACTOR SUMMARY																
ACTUAL PPMV		OVERALL					OVA METERS											
NOMINAL PPMV	LOW	HIGH	MEAN	SE	M	ICMD	SE	N	2254	SE	N	2159	SE	N	1813	SE	N	
200	202	202	202	1.97	0.03	2	1.82	1	2.00	1	2.00	1	1.84	1	1.84	1	1.84	1
1500	1534	1534	1534	1.85	0.10	2	1.75	1	1.84	1	1.84	1	1.84	1	1.84	1	1.84	1
8000	7871	7871	7871	0.87	0.03	2	0.90	1	0.83	1	0.83	1	0.83	1	0.83	1	0.83	1
OVERALL MEANS		1.99		0.01	0	1.53	0.32	3	1.48	0.34	3							

ESTIMATED AT 10,000 PPMV 0.90 95% CONFIDENCE INTERVAL (0.88 1.18)

11V INSTRUMENTS


ACTUAL PPMV		RESPONSE FACTOR SUMMARY																
ACTUAL PPMV		OVERALL					11V METERS											
NOMINAL PPMV	LOW	HIGH	MEAN	SE	M	TF	SE	N	24	SE	N	18	SE	N	14	SE	N	
200	202	202	202	0.85	0.15	2	1.10	1	0.80	1	0.80	1	0.80	1	0.80	1	0.80	1
1500	1534	1534	1534	1.35	0.17	2	1.37	1	1.18	1	1.18	1	1.18	1	1.18	1	1.18	1
8000	7871	7871	7871	1.26	0.11	2	1.31	1	1.14	1	1.14	1	1.14	1	1.14	1	1.14	1
OVERALL MEANS		1.18		0.02	0	1.33	0.12	3	1.04	0.12	3							

ESTIMATED AT 10,000 PPMV 1.35 95% CONFIDENCE INTERVAL (1.08 1.80)

Figure 5-10b

INSTRUMENT RESPONSE VS CONCENTRATION

ISOPROPANOL

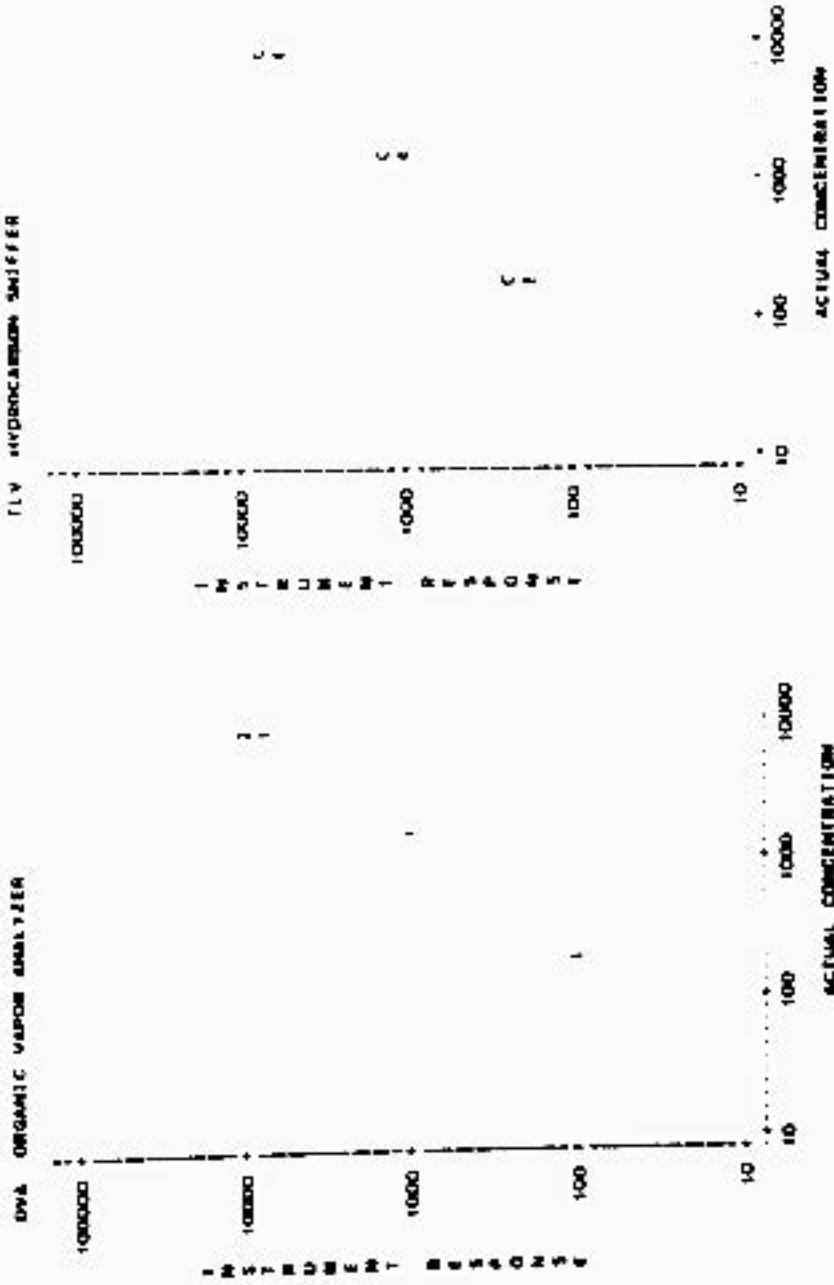

NOTE: 2 ISBS HIDDEN

TABLE 5. 1077

RESPONSE FACTOR SUMMARY

INSTRUMENT AIR FLOW

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			R F S P O M S E F A I S D O S							
	LOW	HIGH	MEAN	MEAN	SE	N	SE	N	SE	N	SE	N	SE	N
2000	188	188	188	1.08	0.02	2	1.18	1	1.18	1				
1500	1512	1512	1512	0.95	0.02	2	1.01	1	1.01	1				
6000	6247	6247	6247	1.06	0.01	2	1.06	1	1.06	1				
8000	7749	7749	7749											

OVERALL MEANS 0.81 0.01 0.00 0.00 0.00 0.00 1

ESTIMATED 95% CONFIDENCE INTERVAL 0.80

ESTIMATED 95% CONFIDENCE INTERVAL 0.80

LIV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			R F S P O M S E F A I S D O S							
	LOW	HIGH	MEAN	MEAN	SE	N	SE	N	SE	N	SE	N	SE	N
200	188	188	188	0.81		1	0.61	1	0.61	1				
1500	1512	1512	1512	0.84		1	0.84	1	0.84	1				
6000	6247	6247	6247	1.21		1	1.21	1	1.21	1				
8000	7749	7749	7749	1.15		1	1.15	1	1.15	1				

OVERALL MEANS 0.85


ESTIMATED 95% CONFIDENCE INTERVAL 0.75

ESTIMATED 95% CONFIDENCE INTERVAL 0.81

Figure 5-107

INSTRUMENT RESPONSE VS CONCENTRATION

ISOPROPYL ACETATE

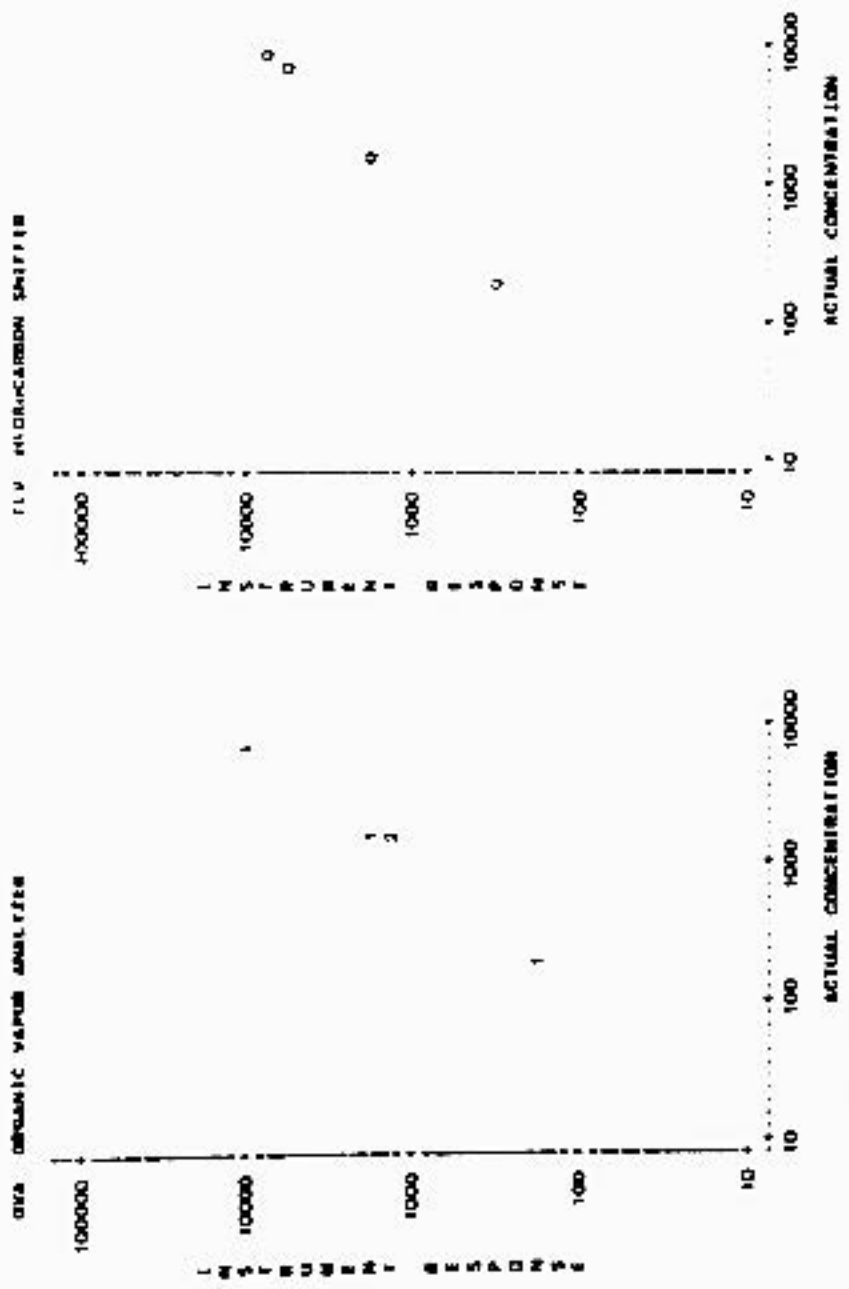

NOTE: 3 OBS MEDIAN

TAB. 5-10B

RESPONSE FACTOR SUMMARY

ISOPROPYL CHLORIDE

DVA INSTRUMENTS

R F S P O N S E F A C T O R S

DVA METERS

OVERALL

NOMINAL PPMV	LOW	HIGH	MEAN	SE	N	10SD	SE	M	2754	SE	M	2199	SE	N	1017	SE	N
700	227	227	227	1.29	0.16	2	1.22	1	1.58	1	1.58	1	1.58	1			
1500	1404	1404	1404	1.12	0.10	2	1.02	1	1.22	1	1.22	1	1.22	1			
3000	4782	4782	4782	0.98	0.01	2	0.68	1	0.70	1	0.70	1	0.70	1			
8000	7878	7878	7878	0.85	0.02	2	0.63	1	0.61	1	0.61	1	0.61	1			
OVERALL MEANS	0.00	0.01	0.00	0.89	0.14	8	1.02	0.21	1.4								

ESTIMATED AT 10,000 PPMV 0.82

95% CONFIDENCE INTERVAL 1.052 0.731

LIV INSTRUMENTS

R F S P O N S E F A C T O R S

LIV METERS

OVERALL


NOMINAL PPMV	LOW	HIGH	MEAN	SE	N	77	SE	N	70	SE	N	74	SE	N
200	227	227	227	1.21	0.06	2	1.28	1	1.15	1	1.15	1	1.15	1
1500	1404	1404	1404	0.85	0.01	2	0.86	1	0.83	1	0.83	1	0.83	1
3000	4782	4782	4782	1.08	0.01	2	1.09	1	1.07	1	1.07	1	1.07	1
8000	7878	7878	7878	1.08	0.02	2	1.05	1	1.08	1	1.08	1	1.08	1
OVERALL MEANS	1.00	0.00	0.00	1.07	0.08	8	1.07	0.08	1.1	0.11	4	1.07	0.11	4

ESTIMATED AT 10,000 PPMV 0.99

95% CONFIDENCE INTERVAL 1.185 1.191

FIGURE 5-108

INSTRUMENT RESPONSE VS CONCENTRATION  
 FENPROPYL CARBONIDE

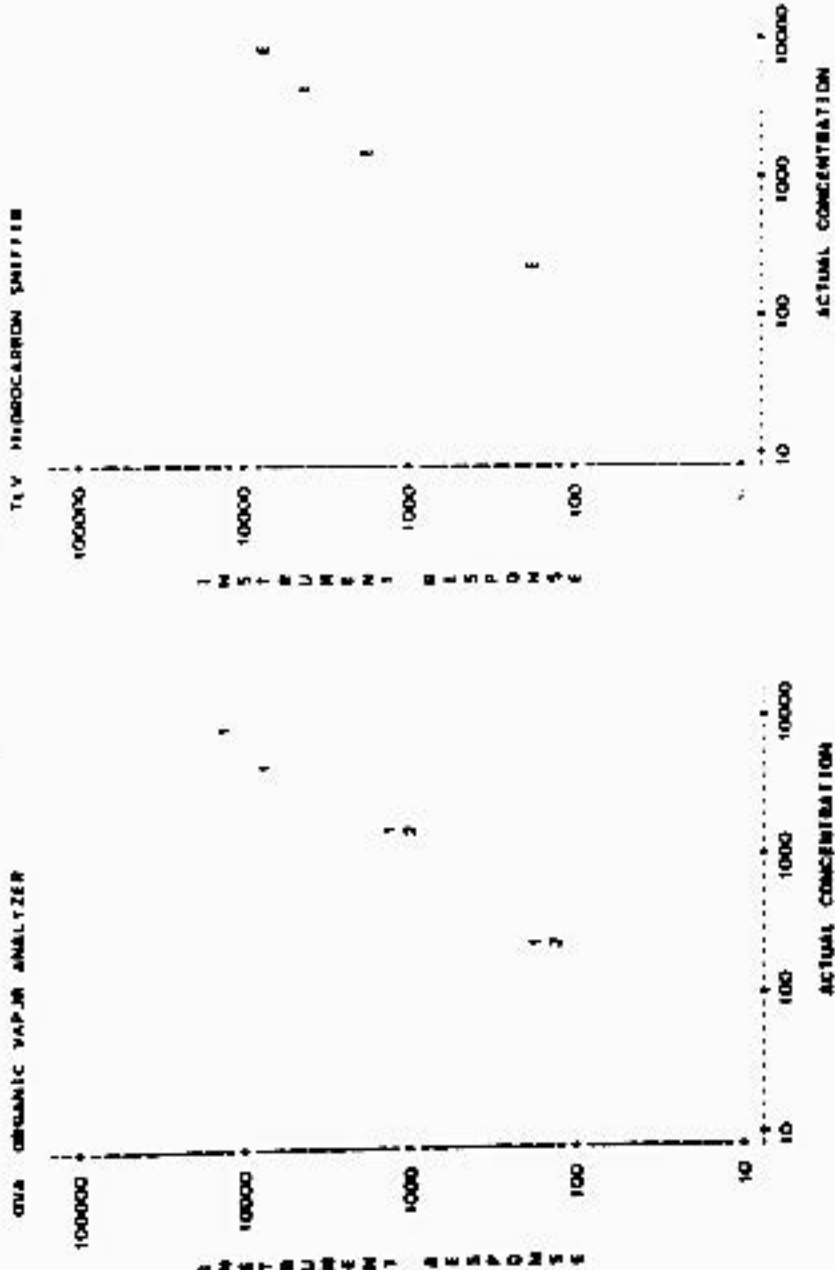

NOTE: 3 CDS HIDDEN

NOTE: 4 CDS HIDDEN

TABLE 5 (Contd)

RESPONSE FACTOR SUMMARY

ESTIMATED AT 10.000 PERM				95% CONFIDENCE INTERVAL					
MEASUREMENT	ACTUAL PERM		OVERALL		OVERALL MEANS				
	LOW	HIGH	MEAN	SE	N	10.000	SE	N	95% CI
PERM	220	220	220	0.00	2	220	0.00	2	220
PERM	1524	1524	1524	0.00	2	1524	0.00	2	1524
PERM	6151	6151	6151	0.00	2	6151	0.00	2	6151
PERM	7806	7806	7806	0.00	2	7806	0.00	2	7806
OVERALL MEANS									
			220	0.00	8	1524	0.00	4	6151
					8	7806	0.00	4	7806
ESTIMATED AT 10.000 PERM									
			0.54			95% CI			0.45 - 1.04

ESTIMATED AT 10.000 PERM				95% CONFIDENCE INTERVAL					
MEASUREMENT	ACTUAL PERM		OVERALL		OVERALL MEANS				
	LOW	HIGH	MEAN	SE	N	10.000	SE	N	95% CI
PERM	220	220	220	0.00	2	220	0.00	2	220
PERM	1524	1524	1524	0.00	2	1524	0.00	2	1524
PERM	6151	6151	6151	0.00	2	6151	0.00	2	6151
PERM	7806	7806	7806	0.00	2	7806	0.00	2	7806
OVERALL MEANS									
			220	0.00	8	1524	0.00	4	6151
					8	7806	0.00	4	7806
ESTIMATED AT 10.000 PERM									
			0.54			95% CI			0.45 - 1.04



Figure 3-109

INSTRUMENT RESPONSE VS CONCENTRATION

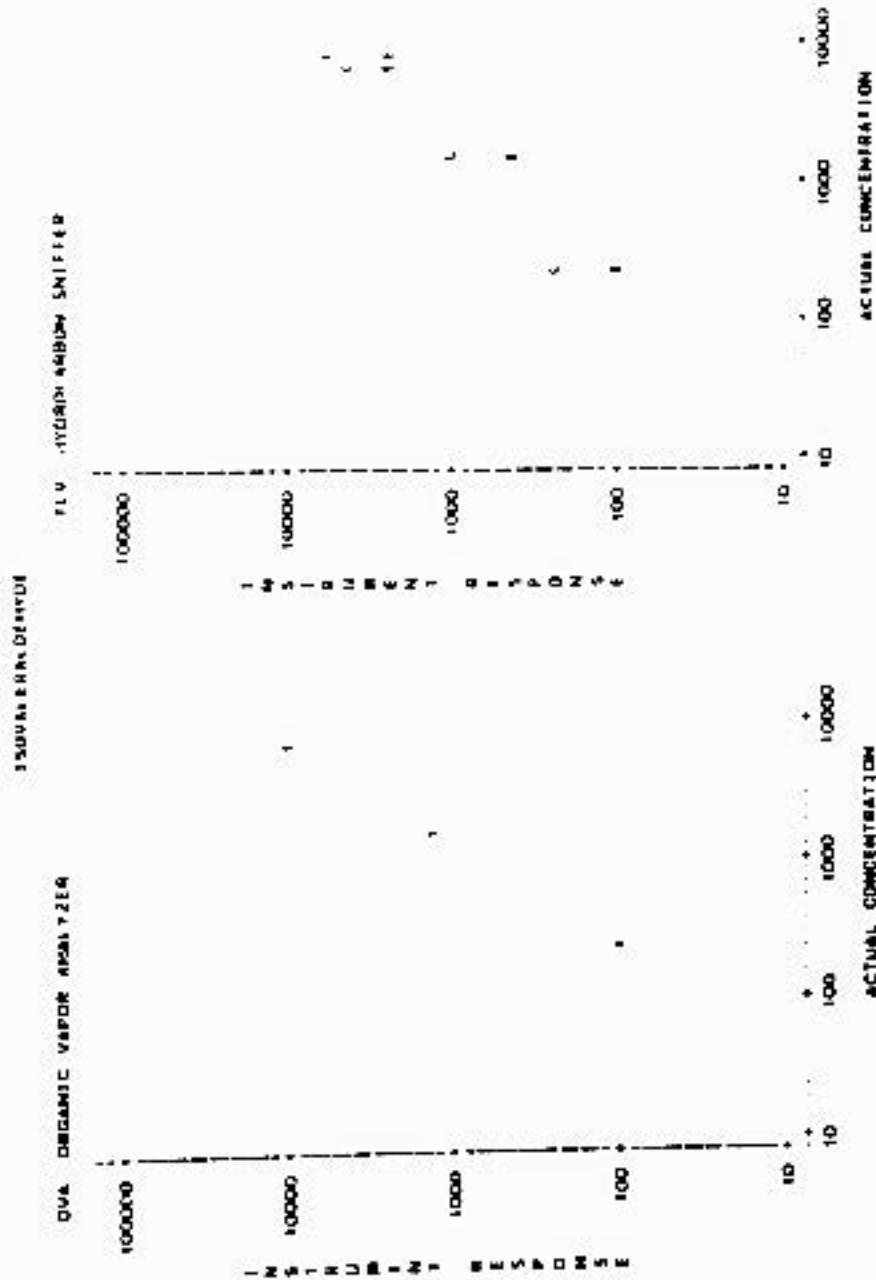


TABLE 1.1111

RESPONSE FACTOR SUMMARY

MSL: 0.104

IVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY								
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2000	SE	N	3000	SE	N
200	214	214	214	2.08	0.21	2	2.81		1	2.24		1	1.63		1
1500	1444	1444	1444	2.08	0.06	2	2.04		1	2.14		1			
8000	7753	7753	7753	1.14	0.03	2	1.11		1	1.18		1			
OVERALL MEANS			2.09	0.02	6	1.09	0.49	3	2.18	0.80	3				
ESTIMATED AT 10 000 PPMV ± 12															
95% CONFIDENCE INTERVAL 1.094 1.321															

IVV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY								
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2000	SE	N	3000	SE	N
200	214	214	214	3.42	0.92	2	4.34		1	2.94		1			
1500	1444	1444	1444	3.37	1.49	2	4.40		1	2.34		1			
8000	7753	7753	7753	2.92	1.01	2	4.54		1	2.51		1			
OVERALL MEANS			3.44	0.18	6	4.43	0.06	3	2.45	0.06	3				
ESTIMATED AT 10 000 PPMV ± 12															
95% CONFIDENCE INTERVAL 1.128 5.791															

Figure 5-110

INSTRUMENT RESPONSE VS. CONCENTRATION

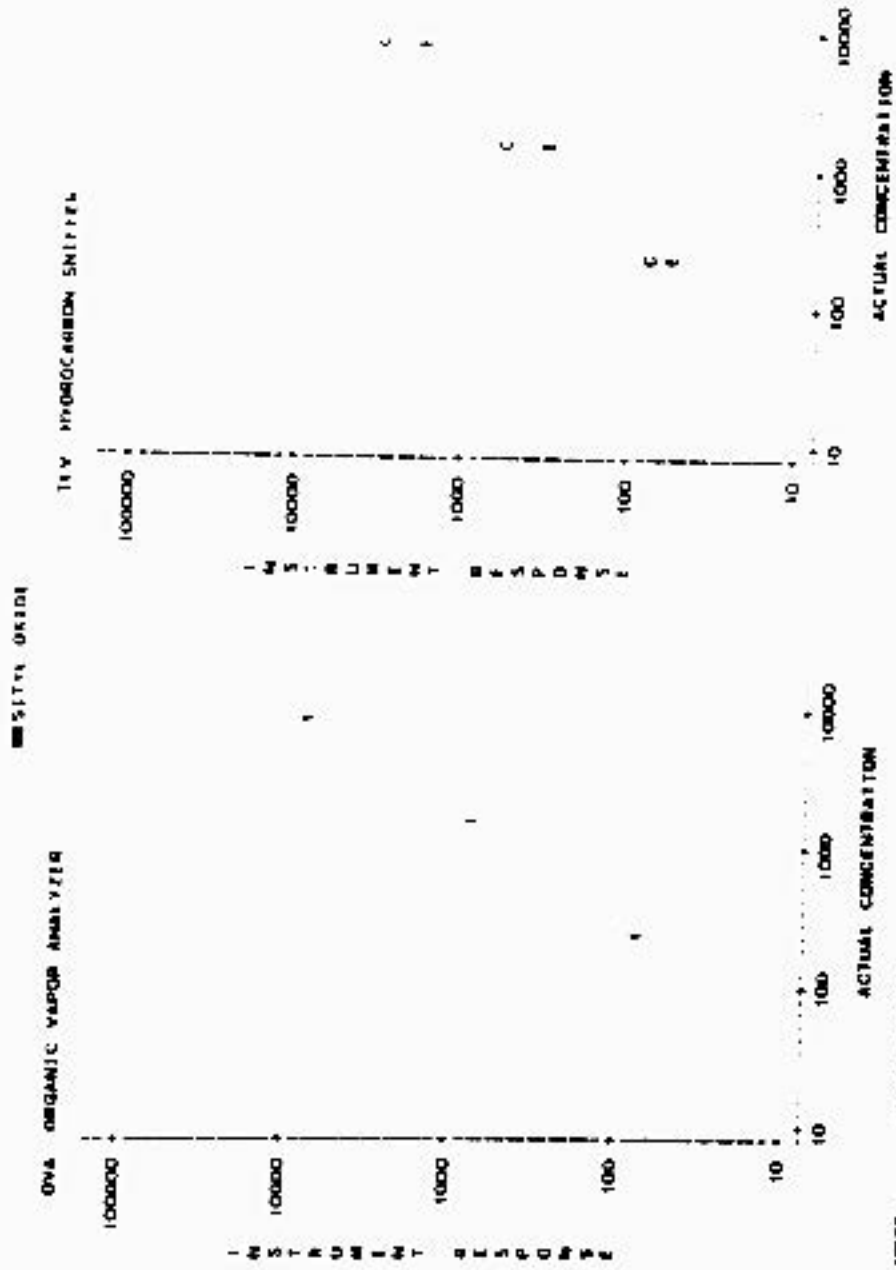


TABLE 5-111

RESPONSE FACTOR SUMMARY

METHACROLEN

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DESIGN FACTORS						
	LOW	HIGH	MEAN	SE	N	100%	SE	M	210%	SE	N
200	300	300	343	0.94	2	2	00	1	3	97	1
4000	4470	4470	198	0.17	2	1	78	1	2	13	1
8000	8608	8608	119	0.18	2	1	01	1	1	27	1
1513	1623	1623									

OVERALL MEANS 220.000 1.00000 2.49000 2

ESTIMATED AT 10,000 PPMV 1.27 95% CONFIDENCE INTERVAL 1.094 1.771

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DESIGN FACTORS						
	LOW	HIGH	MEAN	SE	N	7%	SE	M	7%	SE	N
200	300	300	305	0.84	2	3	60	1	2	51	1
4000	4470	4470	298	1.11	2	4	09	1	1	87	1
8000	8608	8608	388	1.84	2	5	72	1	2	04	1
1513	1623	1623	486	4.58	2	11	45	1	2	28	1


OVERALL MEANS 420.025 0.21100 4.21014 4

ESTIMATED AT 10,000 PPMV 3.10 95% CONFIDENCE INTERVAL 1.195 5.811

Figure 3-111

INSTRUMENT RESPONSE VS CONCENTRATION

METHACROLEIN

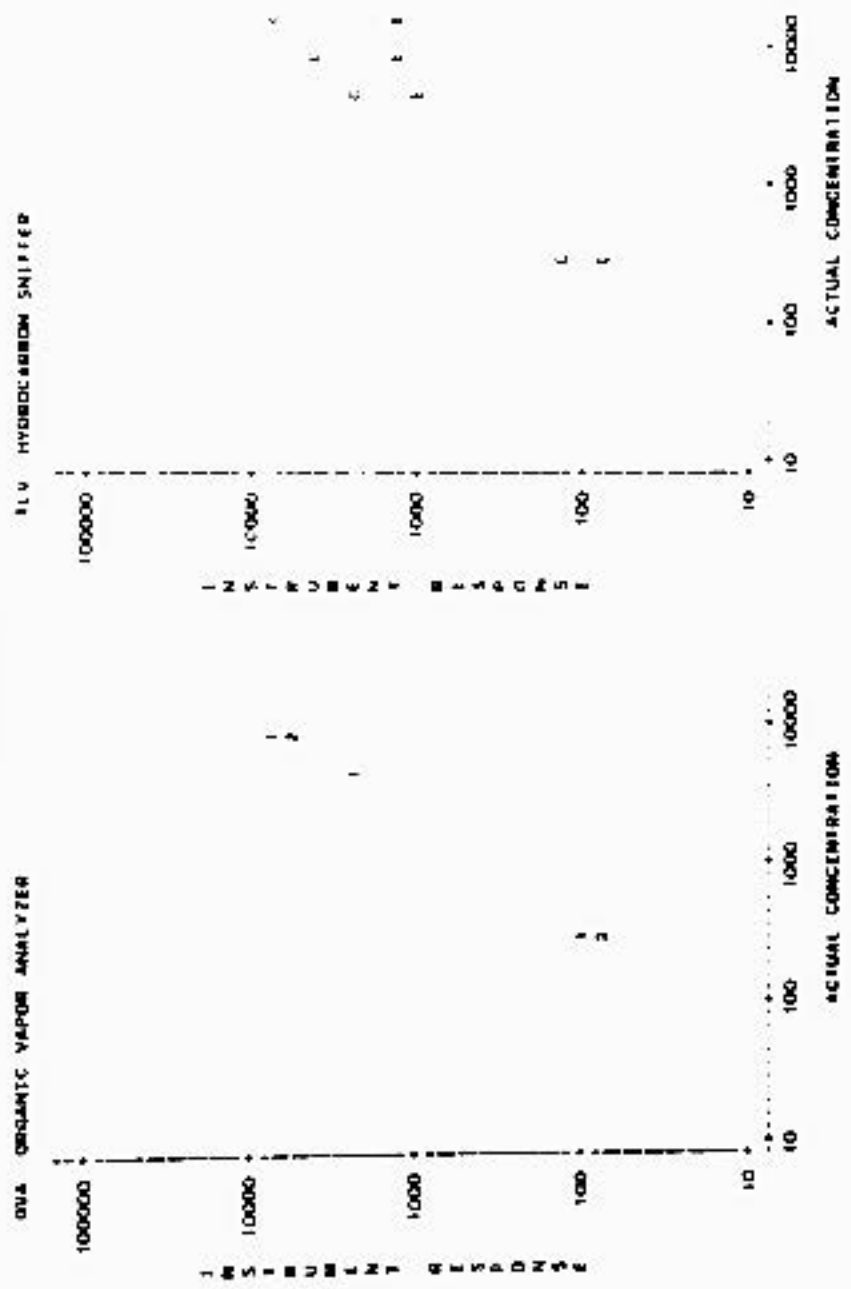

NOTE: 1 OBS. MIDDEN

TABLE 5-117

RESPONSE FACTOR SUMMARY

METHACRYLIC ACID

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			R E S P O N S E F A C T O R S												
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	40	2204	SE	40	2100	SE	N	1013	SE	40	
200	237	237	237	11.27	7.89	2	8.79		1	13.96		1							
500	507	507	507	10.00	1.28	2	8.74		1	11.26		1							
720	754	754	754	4.24	0.80	2	3.84		1	4.83		1							
OVERALL MEANS			6.84	0.25	6	7.06	1.71	3	10.02	2.71	3								

ESTIMATED AT 10,000 PPMV 0.71

95% CONFIDENCE INTERVAL 1.0-06 1.0-01

TLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			R E S P O N S E F A C T O R S												
	LOW	HIGH	MEAN	MEAN	SE	N	71	SE	40	20	SE	40	20	SE	N	30	SE	40	
200	237	237	237	2.17	0.81	2	4.34		1	3.49		1							
500	507	507	507	7.43	1.80	2	8.83		1	6.02		1							
720	754	754	754	2.92	0.86	2	4.80		1	3.07		1							
OVERALL MEANS			5.04	0.16	6	5.90	1.43	3	4.09	0.88	3								


ESTIMATED AT 10,000 PPMV 6.81

95% CONFIDENCE INTERVAL 1.0-17 1.0-01

PLATE 5-112

INSTRUMENT RESPONSE VS CONCENTRATION

METHACRYLIC ACID

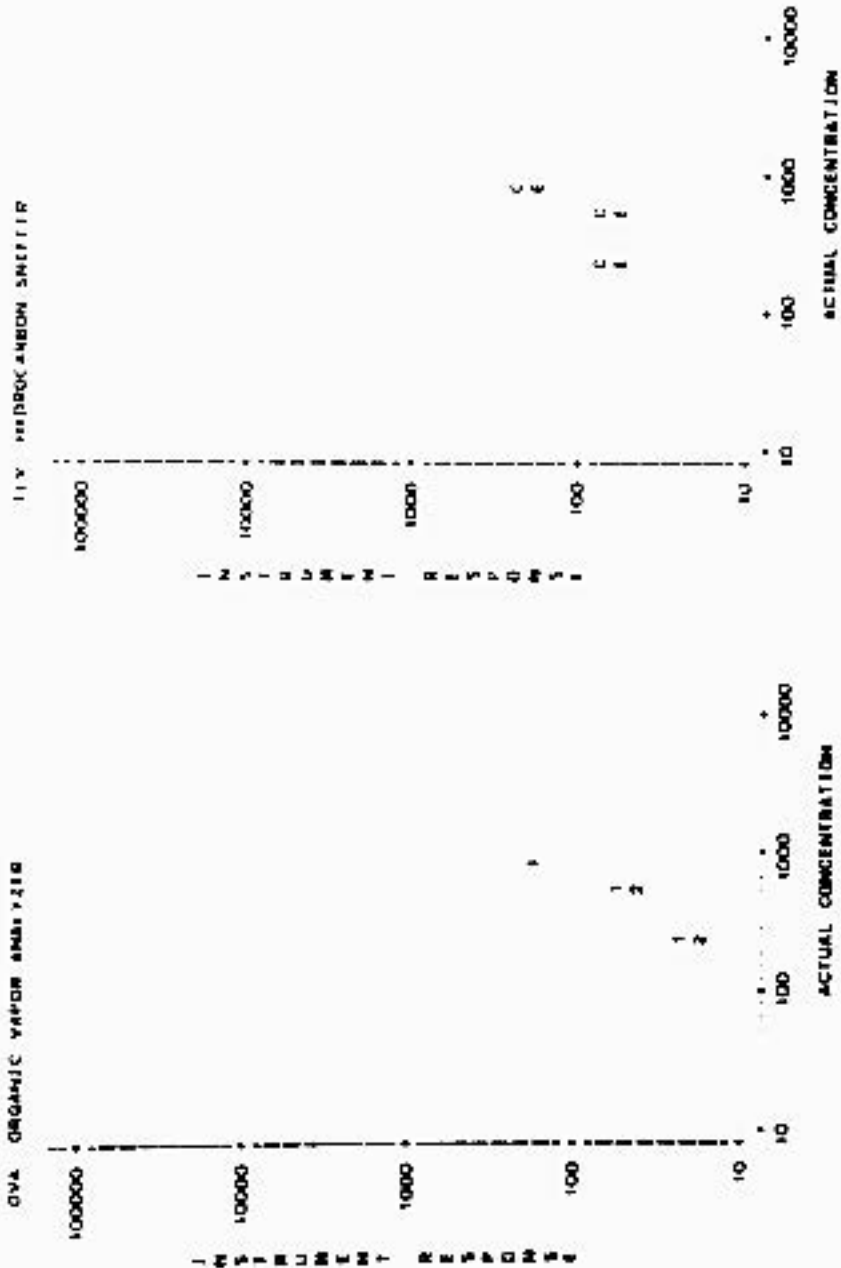

NOTE: 1 OBS 110000

TABLE 5.11.1

RESPONSE FACTOR SUMMARY

METHOD

OVA INSTRUMENTS

RESPONSE FACTOR SUMMARY

NOMINAL PPMV	ACTUAL PPMV			OVERALL		OVA METERS									
	LOW	HIGH	MEAN	MEAN	SE	NO	SE	N	2SD	1.75	1.25	N	1.75	SE	N
50	47	56	50	11.45	0.44	2	12.04	0.64	2	11.75	1.12	2			
150	148	148	148	7.06	1.06	2						2	0.81		1
200	242	242	242	7.00		1						2	0.81		1
500	498	540	521	8.19	0.93	8	8.02	1.21	2	9.08	1.47	2	4.42		1
850	42	42	42	7.17	1.19	2	5.97		1	8.28		1			1
1000	1020	1020	1020	5.75	0.83	2						4	0.93		1
1500	1498	1788	1731	7.80	0.79	3						2	0.81	0.83	2
2000	2141	2141	2141	6.67	0.59	2						2	0.81		1
3500	3409	3409	3409	6.88	0.02	2						1	0.91		1
5000	4772	6106	4854	6.44	0.22	4	6.08		1	6.04		1	6.76		1
7000	7719	7719	7719	6.84	0.28	2						2	0.77		1
8000	8417	8836	8611	7.72	0.70	6	8.97	0.50	2	6.86	0.90	4	7.41		1
10E3	1082	10E3	10E3	5.51	0.37	2						1	0.88		1
15E3	18E3	18E3	18E3	4.98	0.87	2						1	5.66		1
20E3	21E3	21E3	21E3	4.07	0.58	2						1	4.66		1
30E3	30E3	30E3	30E3	3.76		1						1	1.76		1
40E3	45E3	45E3	45E3												
50E3	52E3	52E3	52E3												

OVERALL MEANS 7.24 0.0148 9.01 0.1310 8.88 0.8712 5.79 0.4815 6.08 0.4811  
 ESTIMATED AT 10.000 PPMV 6.69 95% CONFIDENCE INTERVAL 1.496 6.521



TABLE 5-113 (cont'd)  
RESPONSE FACTOR SUMMARY

NOMINAL PPMV	ACTUAL PPMV			RESPONSE FACTORS																			
	LOW	HIGH	MEAN	MEAN	SE	N	ZI	SE	N	ZC	SE	N	ZM	SE	N	ZI	SE	N	ZI	SE	N		
50	42	58	50	1.73	0.06	4	1.87	0.49	2	1.79	0.12	2											
100	146	148	148	0.48																			
200	242	243	242	1.24																			
500	498	540	521	1.38	0.15	8	1.18	0.87	2	1.60	0.10	4											
850	42	42	42	1.02																			
1000	1020	1020	1020	1.98																			
1800	1885	1768	1731	1.88																			
2000	2141	2141	2141	1.32																			
2500	2409	2409	2409	1.48																			
5000	4773	5126	4954	1.82	0.19	3	2.08																
7800	7219	7219	7219	2.09																			
9000	8417	8828	8611	2.11	0.22	7	2.47	0.58	3	1.84	0.08	4											
10K3	10K3	10K3	10K3	2.08																			
18E3	18E3	18E3	18E3	2.46																			
21E3	21E3	21E3	21E3	2.45																			
20K3	20K3	20K3	20K3																				
40K3	40K3	40K3	40K3																				
50K3	52K3	52K3	52K3																				
OVERALL MEANS				1.73	0.00	32	1.80	0.31	8	1.67	0.08	24											
ESTIMATED AT 10,000 PPMV				1.88											95% CONFIDENCE INTERVAL	(1.62, 2.10)							

Figure 5-111

INSTRUMENT RESPONSE VS. CONCENTRATION

METHANE

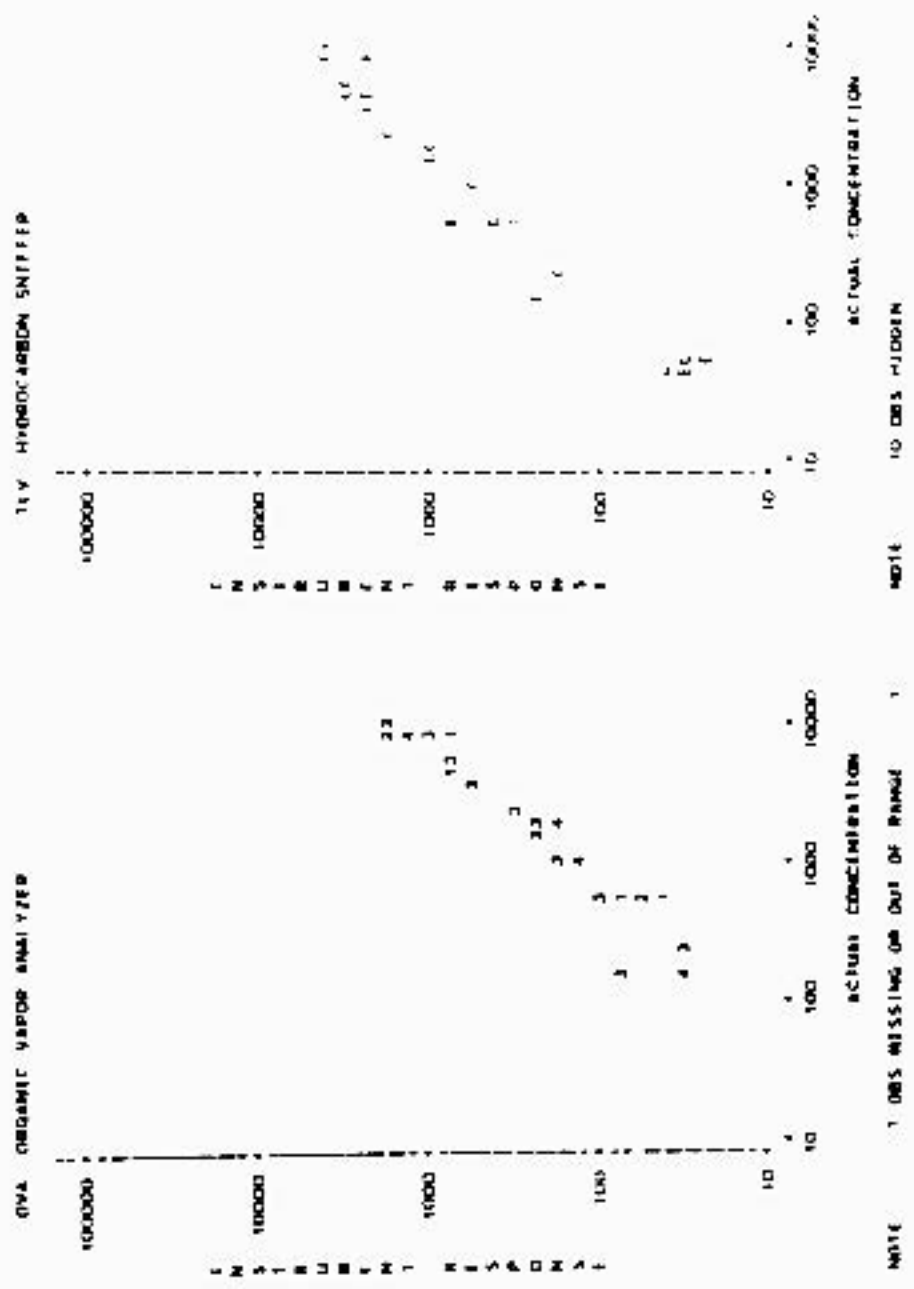


TABLE 5.114

RESPONSE FACTOR SUMMARY

MEASUREMENTS

OVER INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			R A S P I N S E I A C T O R S									
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SF	N	2254	SF	N	2159	SF	N	
200	202	202	202	0.73	0.06	2	5.48		1	7.20		1			1	
1500	1537	1537	1537	4.99	0.26	2	4.70		1	5.28		1			1	
7300	7813	7813	7813	2.88	0.14	2	2.52		1	3.78		1			1	
OVERALL MEANS							4.68	0.07	4	4.22	0.88	2	5.09	1.28	1	
ESTIMATED AT 10,000 PPMV							2.70									

95% CONFIDENCE INTERVAL 1.99 1.671

11V INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			R A S P I N S E I A C T O R S								
	LOW	HIGH	MEAN	MEAN	SE	N	10	SF	N	11	SF	N	24	SF	N
200	202	202	202	0.64		1			1			1			1
1500	1537	1537	1537	1.28		1			1			1			1
7300	7813	7813	7813	1.98		1			1			1			1
OVERALL MEANS							1.30		3						
ESTIMATED AT 10,000 PPMV							2.19								

95% CONFIDENCE INTERVAL 1.85 2.811

Figure 5-11A

INSTRUMENT RESPONSE VS CONCENTRATION

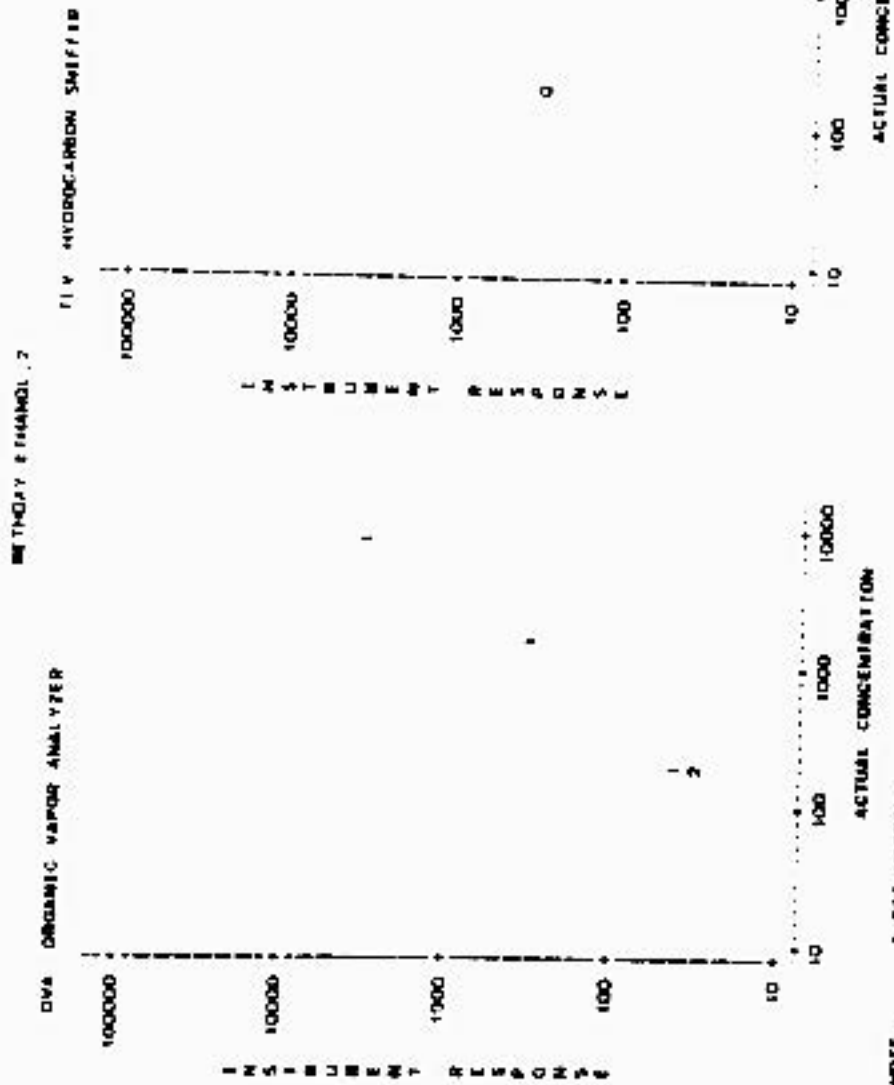


TABLE 7. LYS

MISPLACED FACTOR STANDARD

METHOD ACCE RATE

OVER INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DESIGN VALUE FACTORS										
	LOW	HIGH	MEAN	MEAN	SE	N	100%	5%	1%	0.1%	SE	N	100%	5%	1%	0.1%	
2000	226	228	228	219	0.11	2	2.02	1	2.28	1							
1500	1574	1574	1574	1520	0.14	2	1.98	1	2.28	1							
1000	1197	1197	1197	1177	0.09	2	1.13	1	1.82	1							
OVERALL MEANS			203	0.02	6	1.81	0.09	3	2.28	0.16	2						

ESTIMATED AT 10 000 PPMV 1.80

95% CONFIDENCE INTERVAL 1.35 2.10

OVER INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DESIGN VALUE FACTORS										
	LOW	HIGH	MEAN	MEAN	SE	N	100%	5%	1%	0.1%	SE	N	100%	5%	1%	0.1%	
2000	226	228	228	128	0.11	2	1.18	1	1.15	1							
1500	1574	1574	1574	1470	0.08	2	1.14	1	1.58	1							
1000	1197	1197	1197	1070	0.08	2	1.16	1	1.58	1							
OVERALL MEANS			153	0.02	6	1.48	0.13	3	1.44	0.14	1						

ESTIMATED AT 10 000 PPMV 1.78

95% CONFIDENCE INTERVAL 1.47 2.12

Figure 3-135

INSTRUMENT RESPONSE VS CONCENTRATION

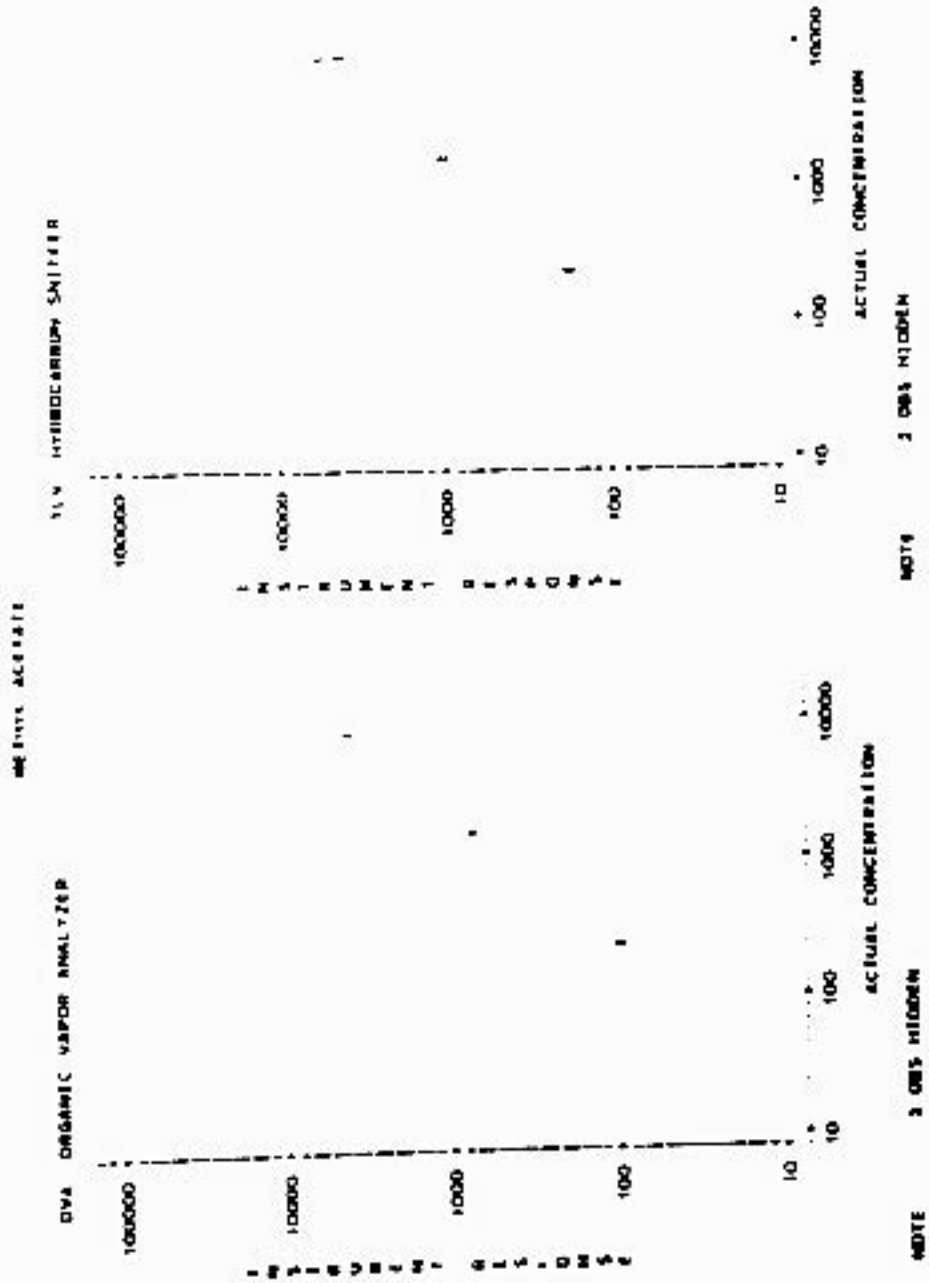


TABLE 5.116

RESPONSE FACTOR SUMMARY

METHYL METHYLENE

OVERALL MEANS AT 10000 PPMV

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPIRATORY FACTORS											
	LOW	HIGH	MEAN	SE	1000	SE	N	2054	SE	N	3450	SE	N	1011	SE	N
1000	987	993	993	1.01	0.04	2	0.97	1	1.04	1						
4000	4073	4073	4073	0.87	0.00	2	0.83	1	0.83	1						
8000	4772	4772	4772	0.68	0.01	2	0.65	1	0.63	1						
12000	5817	5817	5817	1.22	0.03	2	1.22	1	1.22	1						

OVERALL MEANS 0.18 0.00 0.18 0.00 0.18 0.00 0.18 0.00 0.18 0.00 0.18 0.00 0.18 0.00 0.18 0.00 0.18 0.00

ESTIMATE AT 10000 PPMV 0.53

95% CONFIDENCE INTERVAL 0.50 0.57

FLV INSTRUMENTS

OVERALL MEANS AT 10000 PPMV

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPIRATORY FACTORS											
	LOW	HIGH	MEAN	SE	1000	SE	N	2054	SE	N	3450	SE	N	1011	SE	N
1000	987	987	987	2.01												
4000	4073	4073	4073	2.94												
8000	4772	4772	4772	3.18												
12000	5817	5817	5817	3.20												

OVERALL MEANS 3.18


ESTIMATE AT 10000 PPMV 3.92

95% CONFIDENCE INTERVAL 3.50 4.29

Figure S-116

INSTRUMENT RESPONSE VS CONCENTRATION

METHYL ACETALINE

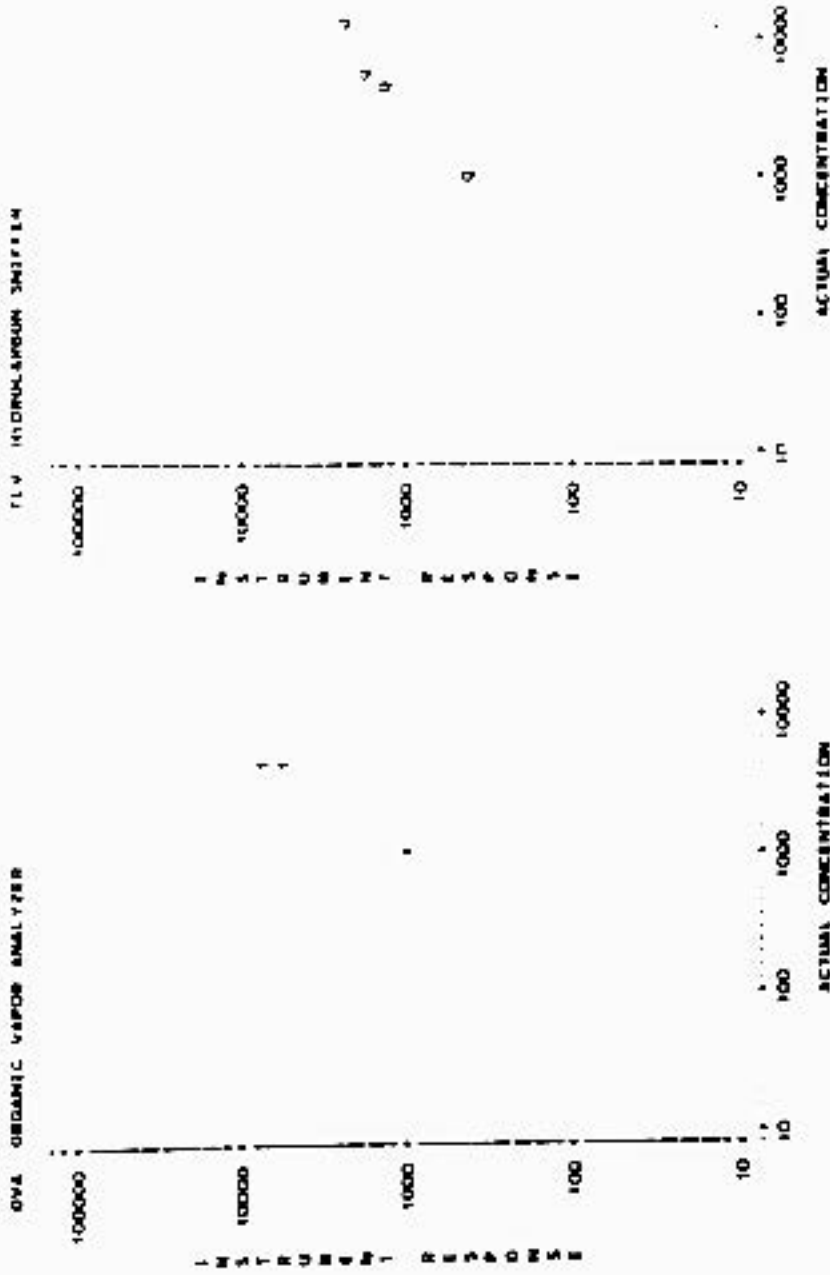

NOTE 3 CM'S H<sub>2</sub>O/CM<sup>3</sup>

NOTE 1 CM'S H<sub>2</sub>O/CM<sup>3</sup>



TABLE 5.117

RESPONSE FACTOR SIMULATED

Well No. C-00104

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DVA METERS													
	LOW	HIGH	MEAN	SE	N	1000	50	N	225A	50	N	215W	50	N	4012	50	N	
1000	1289	1289	1289	5.50	0.80	2						4.70	1		4.31	1		
4000	4828	4828	4828	2.88	0.08	2						2.71	1		2.88	1		
8000	8718	8718	8718	1.82	0.18	2						2.10	1		1.74	1		
			OVERALL MEAN	2.38	0.03	6						3.16	0.18	2	2.74	0.03	2	

ESTIMATED AT 10,000 PPMV 1.75

95% CONFIDENCE INTERVAL 1.44 2.141

ELV INSTRUMENTS


NOMINAL PPMV	ACTUAL PPMV		OVERALL		ELV METERS												
	LOW	HIGH	MEAN	SE	N	74	50	N	74	50	N	74	50	N	74	50	N
1000	1289	1289	1289	8.90	1							6.90	1				
4000	4828	4828	4828	3.19	1							3.19	1				
8000	8718	8718	8718	2.04	1							2.04	1				
			OVERALL MEAN	4.72	2							4.32	0.31	2			

ESTIMATED AT 10,000 PPMV 2.48

95% CONFIDENCE INTERVAL 1.62 3.781

Figure 5-117

INS-800000 RESPONSE VS CONCENTRATION

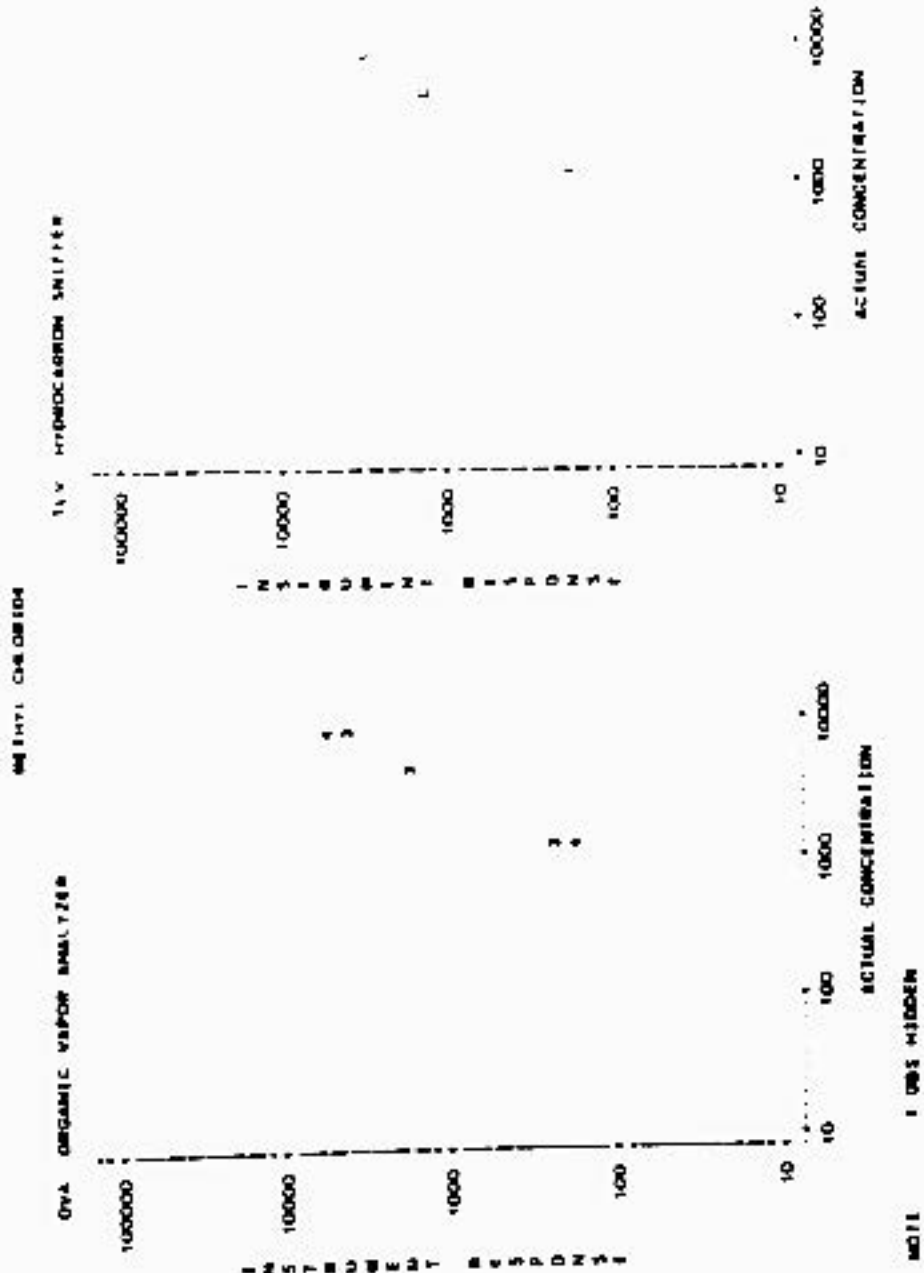

FOR

TABLE 111B

RESPONSE FACTOR SURVEY

METHODS BEYOND

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			METHODS BEYOND												
	LOW	HIGH	MEAN	MEAN	SE	N	COB	SE	N	2284	54	N	2386	54	N	1873	51	N	
50	62	63	62	2.72	0.41	2	2.32		1	3.13		1							
200	187	187	187	1.00		1						1							
500	546	546	546	1.28	0.12	3	1.13		1	1.31		1							
1500	1785	1785	1785	1.00		1						1							
4000	4448	4448	4448	0.74	0.02	3	0.71		1	0.79		1							
8000	8648	8648	8648									1							
OVERALL MEANS			1.30	0.02	9		1.20	0.48	3		1.76	0.11	3		0.61	0.09	1		

ESTIMATED 41 TO 1000 PPMV 0.57

95% CONFIDENCE INTERVAL 1.00 TO 0.81

FLY INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			METHODS BEYOND												
	LOW	HIGH	MEAN	MEAN	SE	N	TE	SE	N	TC	54	N	TM	54	N	TU	54	N	
50	62	63	62	1.28	0.10	2	1.48		1	1.27		1							
200	187	187	187	0.80		1				0.86		1							
500	546	546	546	1.24	0.17	2	1.48		1	1.14		1							
1500	1785	1785	1785	0.98		1				0.38		1							
4000	4448	4448	4448	1.14	0.08	2	1.26		1	1.08		1							
8000	8648	8648	8648	1.24	0.12	2	1.16		1	1.11		1							
OVERALL MEANS			1.19	0.03	11		1.29	0.19	4		1.08	0.06	1						

ESTIMATED 41 TO 1000 PPMV 1.12

95% CONFIDENCE INTERVAL 1.11 TO 1.13

FIGURE 5-11B

INSTRUMENT RESPONSE VS CONCENTRATION

MEASUREMENT SYSTEM

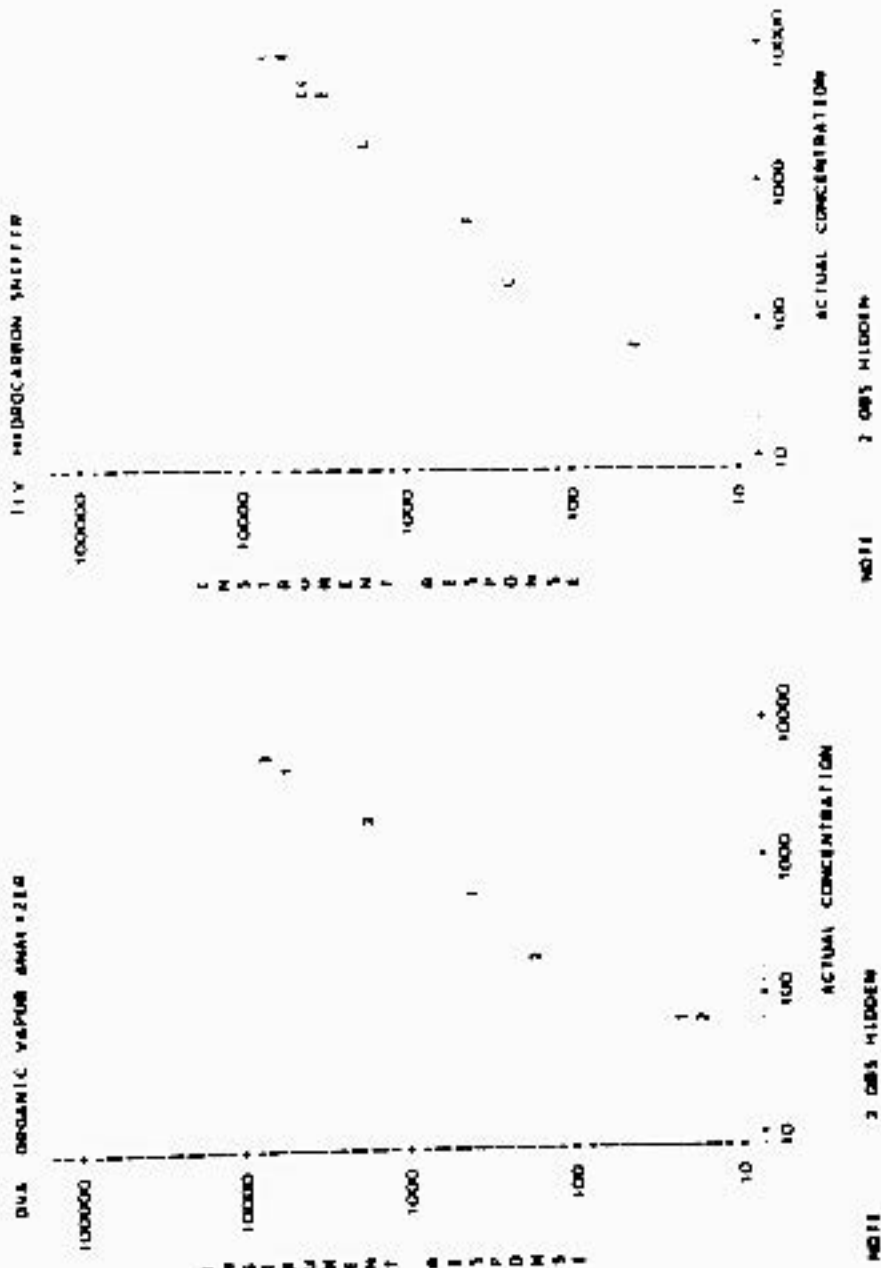


TABLE 5.119

RESPONSE FACTOR SUMMARY

METHYL FORMATE

DVA ENLIGHTENMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DESIGN SPACE FACTORS									
	LOW	HIGH	MEAN	SE	N	1000	SE	N	2150	SE	N	1010	SE	N
200	176	178	0.26	0.70	2	4.57		1	1.98		1			1
1000	1410	1410	4.13	0.36	2	3.27		1	4.49		1			1
8000	1183	1183	3.51	0.23	2	3.29		1	3.14		1			1
OVERALL MEANS					4.30	0.07	4	3.68	0.37	2	4.13	0.65	2	

ESTIMATED AT 10 (KNO) PPMV 3.61

95% CONFIDENCE INTERVAL (2 AT 10)

ILV ENLIGHTENMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DESIGN SPACE FACTORS									
	LOW	HIGH	MEAN	SE	N	71	SE	N	31	SE	N	70	SE	N
200	176	178	1.88	0.01	2	1.88		1	1.90		1			1
1500	1410	1410	1.76	0.02	2	1.81		1	1.77		1			1
8000	1183	1183	1.88	0.10	2	2.09		1	1.88		1			1
OVERALL MEANS					1.88	0.03	6	1.92	0.08	2	1.85	0.16	2	

ESTIMATED AT 10 (KNO) PPMV 1.93

95% CONFIDENCE INTERVAL (2 AT 10)


FIGURE 5-114

IMPLEMENT RESPONSE VS CONCENTRATION

DEF TESTS FORMATE

DVA ORGANIC VAPOR ANALYZER

FLV HYDROCARBON SNIFFER

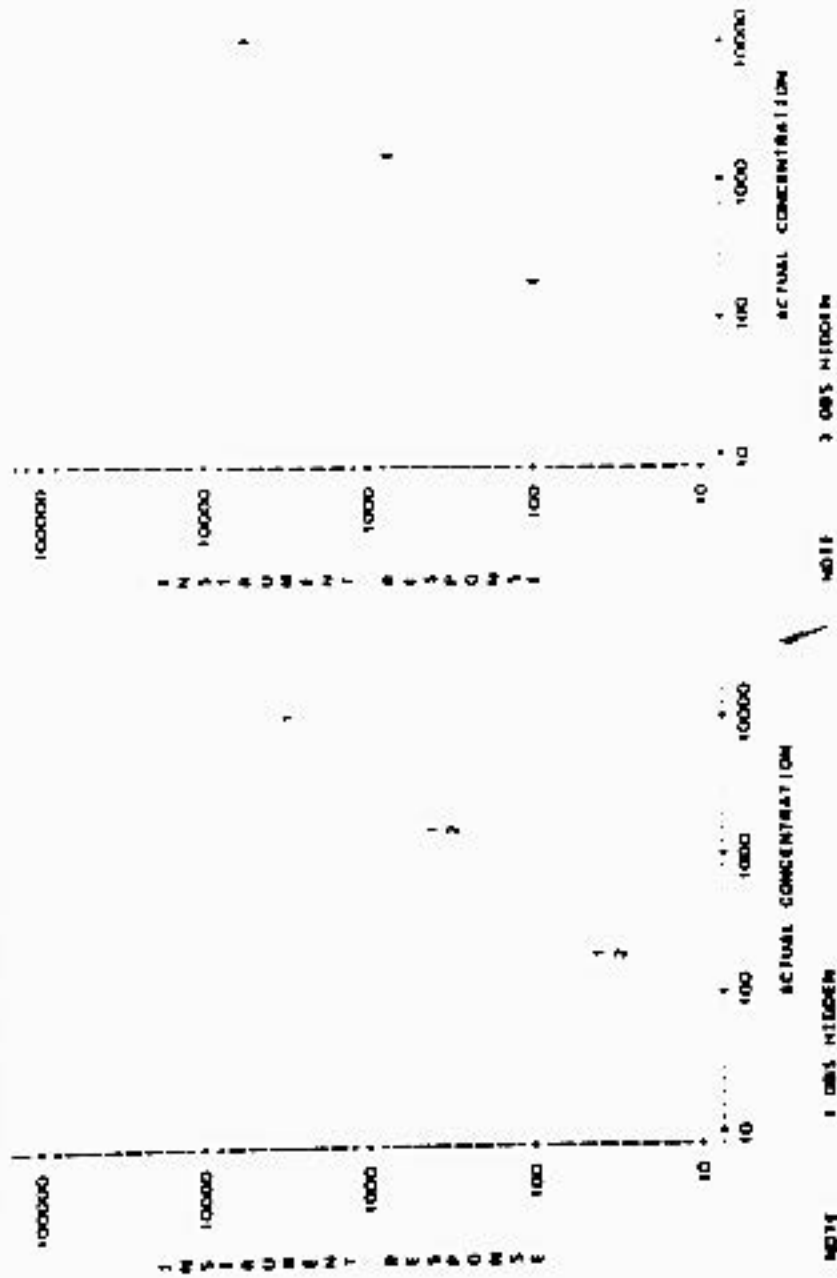

NOTE

1 OBS HIDDEN

2 OBS HIDDEN

TABLE 5.14D

RESPONSE FACTOR SUMMARY

MEANS ON INSTRUMENT

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			MEANS ON INSTRUMENTS									
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2254	SE	N	3158	SE	N	
200	212	212	212	212	0.41	2	2.02			1	2.29					1
1500	1455	1455	1455	1455	0.95	2	1.29			1	1.88					1
8000	7778	7778	7778	7778	0.98	2	0.98			1	1.11					1
OVERALL MEANS							1.84	0.01	8	1.47	0.34	3	1.61	0.31	3	

ESTIMATED AT 10 000 PPMV 0.89

VS % COMPLETION INTERVAL 1.088 1.102

11V INSTRUMENTS

OVA INSTRUMENTS


NOMINAL PPMV	ACTUAL PPMV			OVERALL			MEANS ON INSTRUMENTS									
	LOW	HIGH	MEAN	MEAN	SE	N	21	SE	N	75	SE	N	20	SE	N	
200	212	212	212	212	0.44	2	2.71			1	1.89					1
1500	1455	1455	1455	1455	0.29	2	2.42			1	1.37					1
8000	7778	7778	7778	7778	0.53	2	3.18			1	2.04					1
OVERALL MEANS							2.34	0.07	6	2.38	0.34	3	1.91	0.11	3	

ESTIMATED AT 10 000 PPMV 2.34

VS % COMPLETION INTERVAL 1.58 1.674

FIGURE 5-120

INSTRUMENT RESPONSE VS. CONCENTRATION

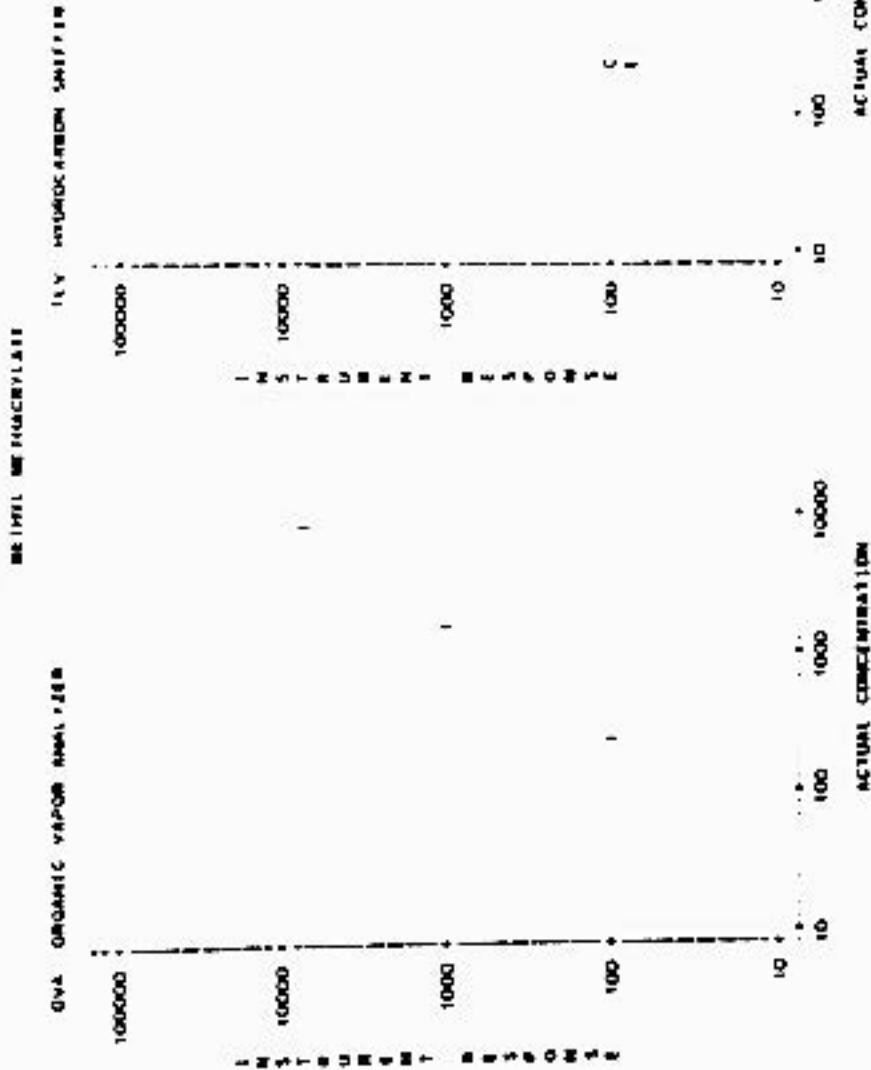

NOTE: 2 OBS HIDDEN



TABLE 5-121

RESPONSE FACTOR SUMMARY

METHOD 2 PERFORMANCE

OVA INSTRUMENTS

NOMINAL PUMP	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY								
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2204	SE	N	2150	SE	N
200	224	224	224	220	0.04	2	2.12								
1000	1460	1460	1460	139	0.04	2	1.34								
5000	5889	5889	5889	154	0.15	2	1.08								
8000	7636	7636	7636	210	0.01	2	2.18								
OVERALL MEANS			188	0.10	4	1.89	0.16	4	1.87	0.21	4				

ESTIMATED AT 10,000 PPMV ± 10

95% CONFIDENCE INTERVAL (1.81) 2.571

11V INSTRUMENTS

NOMINAL PUMP	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY								
	LOW	HIGH	MEAN	MEAN	SE	N	10	SE	N	11	SE	N	10	SE	N
200	224	224	224	190	0.20	2	2.46								
1000	1460	1460	1460	140	0.13	2	1.27								
5000	5889	5889	5889	211	0.20	2	2.29								
8000	7636	7636	7636	210	0.22	2	2.28								
OVERALL MEANS			211	0.02	8	2.09	0.27	4	1.76	0.09	4				

ESTIMATED AT 10,000 PPMV ± 94

95% CONFIDENCE INTERVAL (1.88) 2.581

Figure 3-121  
 INSTRUMENT RESPONSE VS CONCENTRATION

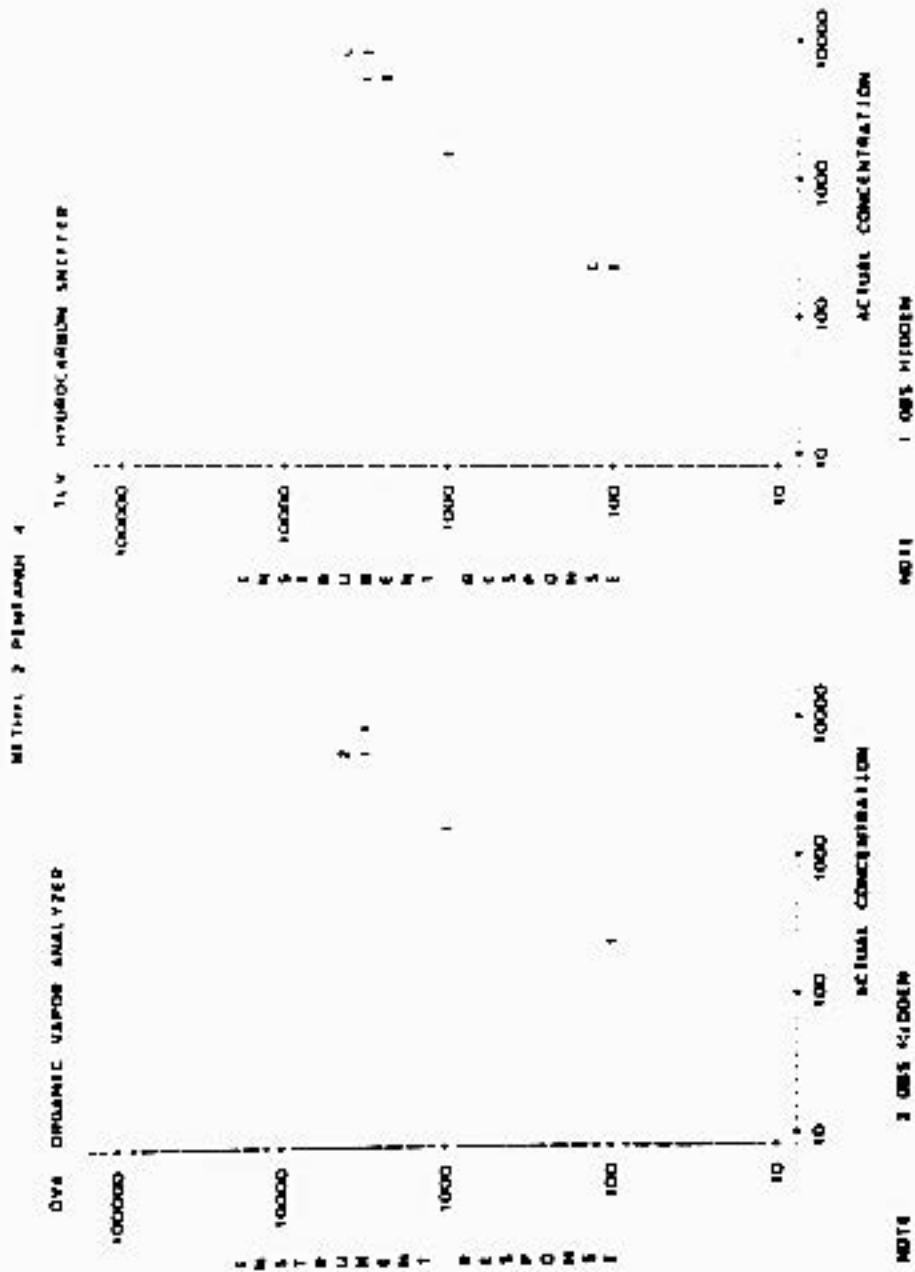


TABLE 5.122

RESPONSE FACTOR SUMMARY

MEANS / MEASUREMENT

OVA CONCENTRATIONS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		M E S U R E M E N T F A C T O R S									
	LOW	HIGH	MEAN	SE	N	100%	5%	N	2.5%	SE	N	10%	SE	N
200	209	209	1.42	0.12	2	1.00		1	1.23		1	1.00		1
1500	1510	1510	0.46	0.05	2	0.80		1	0.49		1	0.80		1
5000	4951	4951	0.54	0.01	2	0.52		1	0.54		1	0.54		1
6000	6268	6268												
6000	7810	7810												

OVERALL MEANS 0.82 0.01 4 1.77 0.14 3 0.86 0.20 4

ESTIMATED AT 10 000 PPMV 0.48

95 % CONFIDENCE INTERVAL 1.02 0.28 1.041

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		M E S U R E M E N T F A C T O R S									
	LOW	HIGH	MEAN	SE	N	100%	5%	N	2.5%	SE	N	10%	SE	N
200	209	209	0.96	0.24	2	1.22		1	0.74		1	1.00		1
1500	1510	1510	1.24	0.25	2	1.54		1	1.40		1	1.00		1
5000	4951	4951	1.78	0.11	2	1.65		1	1.86		1	1.00		1
6000	6268	6268	1.44	0.20	2	1.64		1	1.24		1	1.00		1
6000	1810	7810	1.33	0.11	2	1.90		1	1.16		1	1.00		1

OVERALL MEANS 1.17 0.04 10 1.52 0.08 5 1.23 0.14 5

ESTIMATED AT 10 000 PPMV 1.54

95 % CONFIDENCE INTERVAL 1.12 1.441


Figure 5-122

INSTRUMENT RESPONSE VS CONCENTRATION

MEASURES 2 PENTANE 4

OVA ORGANIC VAPOUR ANALYSER

11V HYDROCARBON SAMPLER

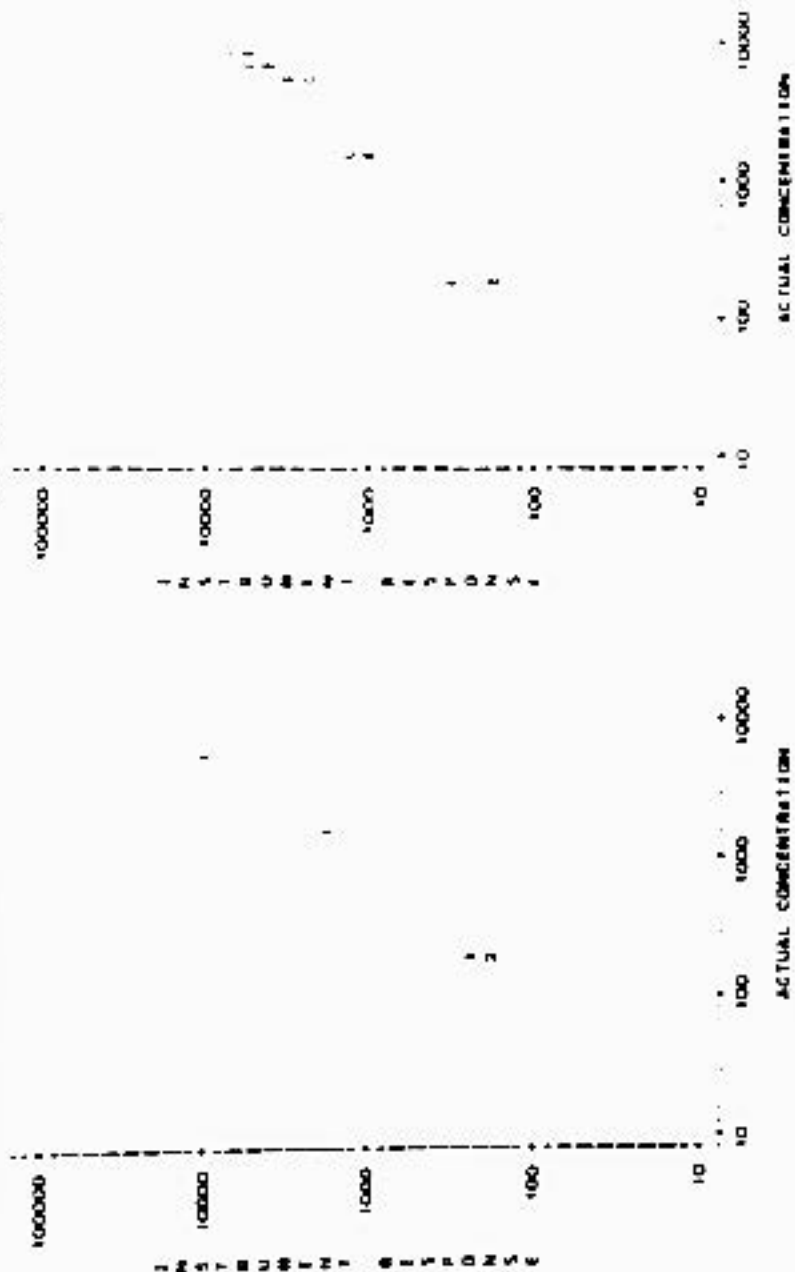

NOTE 2 OBS HIGHEN

TABLE 5.171

RESPONSES FOR THE SUMMARY

MEAN 2 - 4 PERCENTAGE 2

DATA INSTRUMENTS

NUMERICAL POINTS	ACTUAL POINTS		OVERALL	
	LOW	HIGH	MEAN	SD
200	220	220	14.78	0.74
1500	1681	1681	50.80	3.10
4000	4162	4162	80.81	3.11
OVERALL MEANS 68.79 0.72 6				

ESTIMATED 21 TO 4000 POINTS 88.34

DATA INSTRUMENTS

NUMERICAL POINTS	ACTUAL POINTS		OVERALL	
	LOW	HIGH	MEAN	SD
200	220	270	8.28	1.24
1500	1681	1681	31.85	6.12
4000	4162	4162	51.85	14.77
OVERALL MEANS 31.99 1.24 6				

ESTIMATED 41 TO 4000 POINTS 81.07

		N		M		SD	
200	220	2254	54	14.78	0.74	1	0.74
1500	1681	1500	3	50.80	3.10	1	3.10
4000	4162	4000	3	80.81	3.11	1	3.11
OVERALL MEANS 68.79 0.72 6							

ESTIMATED 21 TO 4000 POINTS 88.34

		N		M		SD	
200	220	200	2	8.28	1.24	1	1.24
1500	1681	1500	2	31.85	6.12	1	6.12
4000	4162	4000	2	51.85	14.77	1	14.77
OVERALL MEANS 31.99 1.24 6							

ESTIMATED 41 TO 4000 POINTS 81.07

Figure 5-171

IMPLEMENTED RESPONSE VS CONCENTRATION

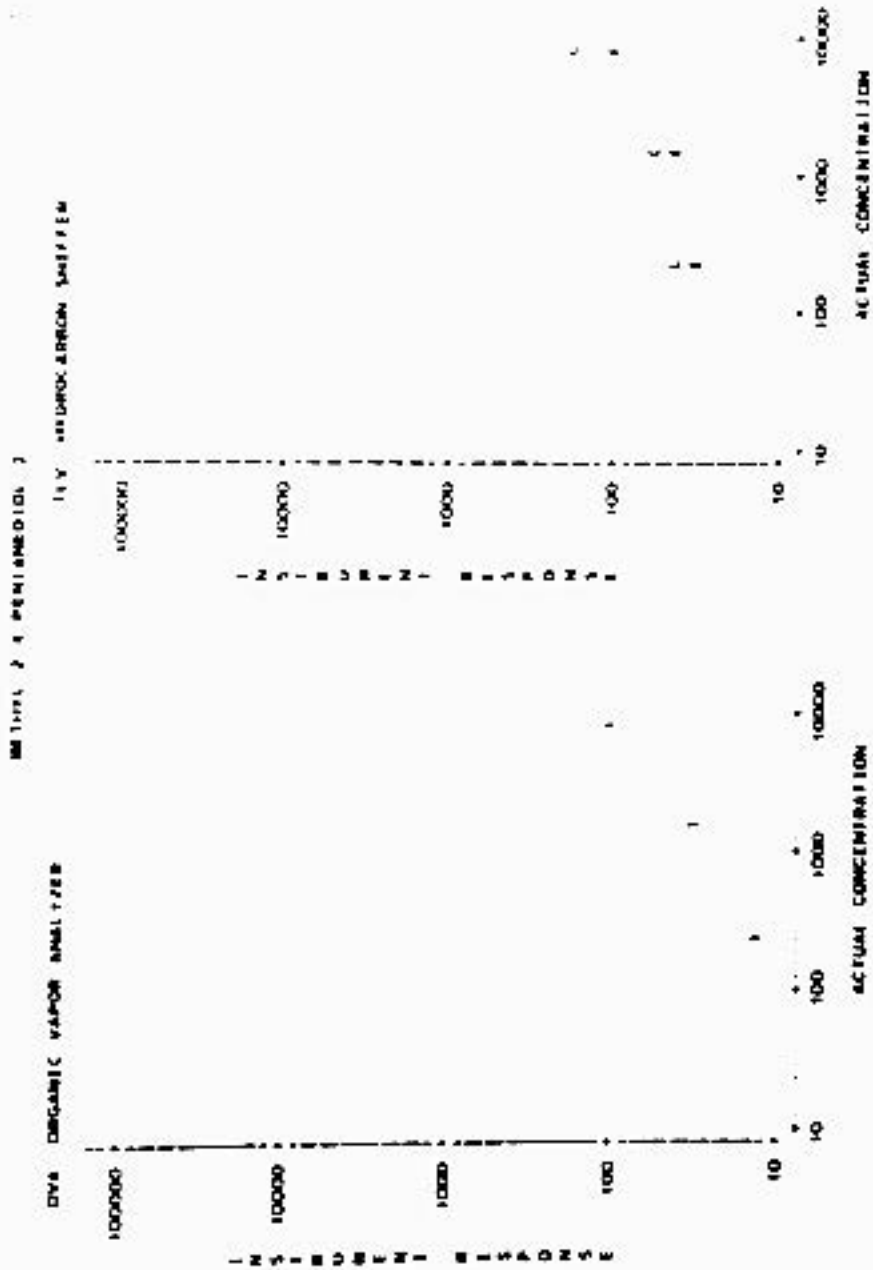


TABLE V 1/74

DESIGN AND FACTOR SUMMARY

METHOD OF MEASUREMENT

DATA INSTRUMENTS

NOMINAL PPMV LOW HIGH MEAN

200 209 209 209  
 1500 1531 1531 1531  
 5000 4914 4914 4914  
 8000 8790 8790 8790  
 9000 8175 8175 8175

OVERALL MEANS

ESTIMATED AT 10,000 PPMV

DESIGN FACTOR

MEAN SE ME HIGH SE ME LOW SE ME

1.40 0.14 2 1.78 1 1.56  
 1.10 0.08 2 1.12 1 1.18  
 0.58 0.04 2 0.48 1 0.61

DATA MEANS

OVERALL MEANS

ESTIMATED AT 10,000 PPMV

DATA INSTRUMENTS

NOMINAL PPMV LOW HIGH MEAN

200 209 209 209  
 1500 1531 1531 1531  
 5000 4914 4914 4914  
 8000 8790 8790 8790  
 9000 8175 8175 8175

OVERALL MEANS

ESTIMATED AT 10,000 PPMV

DESIGN FACTOR

MEAN SE ME HIGH SE ME LOW SE ME

1.40 0.14 2 1.78 1 1.56  
 1.10 0.08 2 1.12 1 1.18  
 0.58 0.04 2 0.48 1 0.61

DATA MEANS

OVERALL MEANS


ESTIMATED AT 10,000 PPMV

Figure 5-124

INSTRUMENT RESPONSE VS CONCENTRATION

METHYL 2 BUTYL 3 OL 2  
 TIV HYDROCARBON UNIT/110

OVA ORGANIC VAPOR ANALYZER

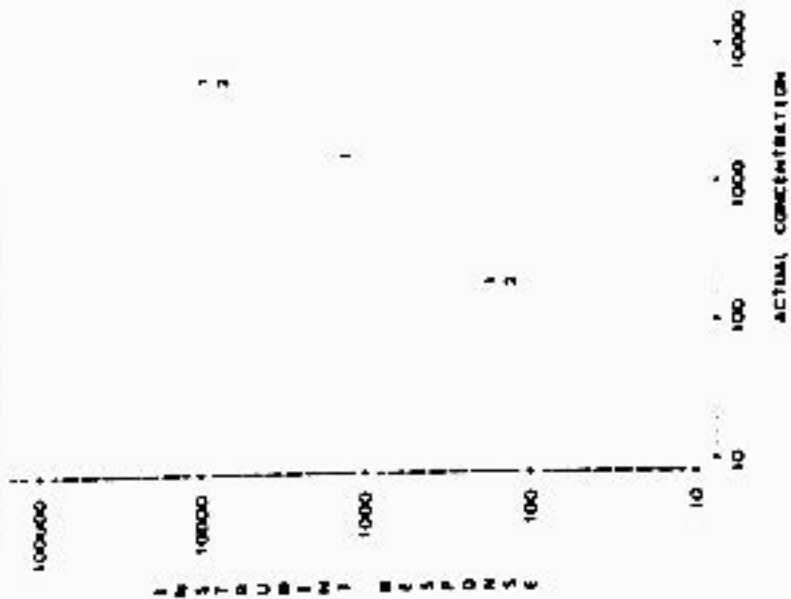

NOTE: 1 OBS. MEDIUM



TABLE 5.25

RESPONSE FACTOR SUMMARY

MEPTLINS

OVA INSTRUMENTS		M E S O D N S R J A R I U M S																	
NOMINAL PPM	ACTUAL PPM			OVERALL			OVS MEANS												
	LOW	HIGH	MEAN	MEAN	ST	%	ME	SE	N	2254	54	N	2109	51	46	1811	58	N	
50	44	57	51	42.3	1.08	4	1.27	0.82	2	0.39	0.97	2							
500	529	531	530	2.10	0.48	4	2.64	0.47	2	0.56	0.22	2							
8000	8308	8500	8400	1.19	0.18	4	1.78	0.08	2	0.64	0.05	2							
OVERALL MEANS				2.97	0.09	12	1.42	0.48	8	2.93	0.13	8							

ESTIMATED AT TO DOO PPMV 1.48

95% CONFIDENCE INTERVAL 1.09 - 1.88

11V INSTRUMENTS

OVA INSTRUMENTS		M E S O D N S R J A R I U M S																	
NOMINAL PPM	ACTUAL PPM			OVERALL			OVS MEANS												
	LOW	HIGH	MEAN	MEAN	ST	%	ME	SE	N	20	70	58	N	198	51	18	19	11	5
50	44	57	51	0.92	0.04	4	0.96	0.17	2	0.87	0.17	2							
500	529	531	530	1.14	0.09	4	1.22	0.08	2	1.05	0.04	2							
8000	8308	8500	8400	1.40	0.08	4	1.48	0.14	2	1.31	0.11	2							
OVERALL MEANS				1.16	0.04	12	1.22	0.10	8	1.08	0.06	8							

ESTIMATED AT TO DOO PPMV 1.41

95% CONFIDENCE INTERVAL 1.12 - 1.63

Figure 5-12b

INSTRUMENT RESPONSE VS CONCENTRATION

11/19/84

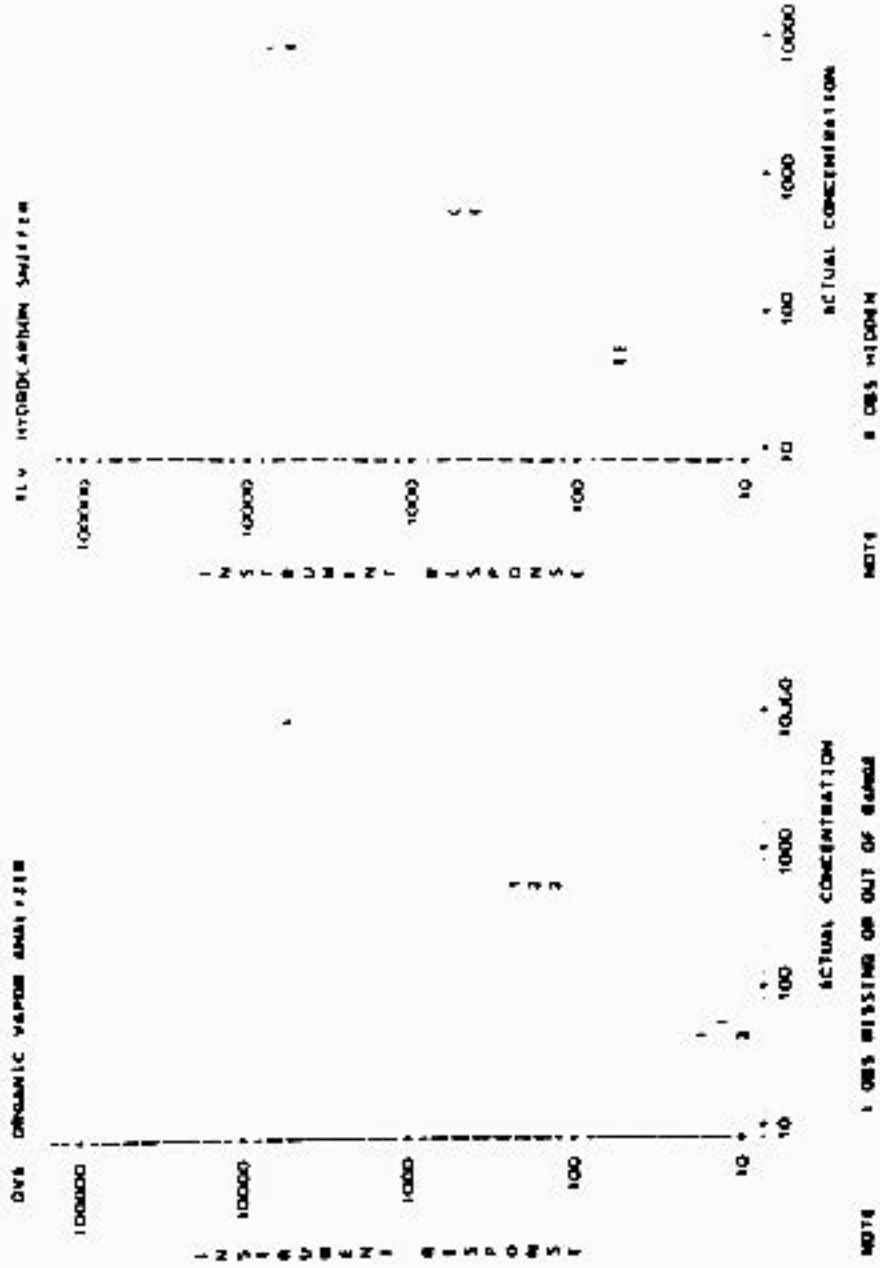


TABLE 5.126

RESPONSE FACTOR SUMMARY

MILLIAMPERE IN

OVER INSTRUMENTS

0 1 2 3 4 5 6 7 8 9

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DVA METERS											
	LOW	HIGH	MEAN	MEAN	SE	N	100%	50%	N	20%	SE	N	50%	N				
200	184	184	184	2 00	0 02	2	3 03	1	3 08	1								
650	664	664	664	3 26	0 08	2	3 28	1	3 48	1								
1100	1076	1076	1076	3 48	0 08	2	3 54	1	3 43	1								
OVERALL MEANS							2 20	0 00	8	3 21	0 15	3	3 12	0 12	1			
ESTIMATED AT 10,000 PPMV							4 13	95% CONFIDENCE INTERVAL									1 1 75	4 743


1-V INSTRUMENTS

0 1 2 3 4 5 6 7 8 9

NOMINAL PPMV	ACTUAL PPMV			OVERALL			1-V METERS											
	LOW	HIGH	MEAN	MEAN	SE	N	100%	50%	N	20%	SE	N	50%	N				
200	184	184	184	1 34		1												
650	664	664	664	2 53		1												
1100	1076	1076	1076	2 23		1												
OVERALL MEANS							2 03	95% CONFIDENCE INTERVAL									1 1 99	2 1 843

Figure 5.12b

INSTRUMENT RESPONSE VS CONCENTRATION

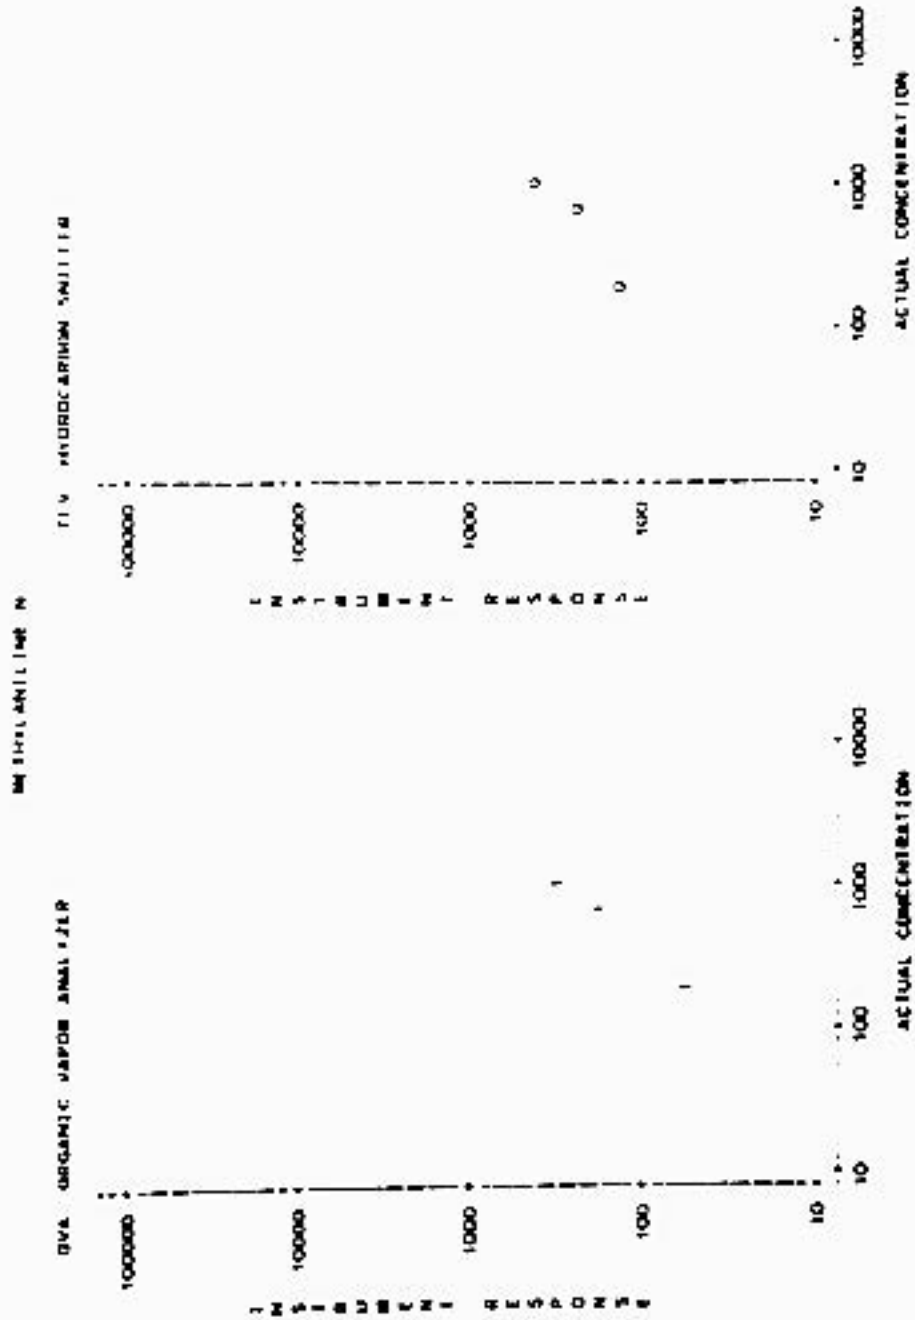

NOTE: 3 OBS HIDDEN

TABLE 3.1.1

RESPONSE FACTOR SUMMARY

HEAVY METALS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		M E S P O N S E F A C T O R S									
	LOW	HIGH	MEAN	SE	N	100%	SE	M	210%	SE	N	100%	SE	N
200	201	201	201	0.00	2	1.95	0.08	2	1.77	1	1.94	1	1.94	1
1500	1498	1498	1498	0.00	2	1.43	0.00	2	1.43	1	1.43	1	1.43	1
3000	3000	3000	3000	0.00	2	0.43	0.00	2	0.43	1	0.44	1	0.44	1
5000	5399	5399	5399	0.00	2	0.43	0.00	2	0.43	1	0.44	1	0.44	1
8000	7788	7788	7788	0.00	2	0.43	0.00	2	0.43	1	0.44	1	0.44	1

OVERALL MEANS 1.43 0.00 6 1.08 0.12 1 1.10 0.15 1

ESTIMATED AT 10 000 PPMV 0.38

95% CONFIDENCE INTERVAL 1.01 1.16 1

TLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		M E S P O N S E F A C T O R S									
	LOW	HIGH	MEAN	SE	N	100%	SE	M	210%	SE	N	100%	SE	N
200	201	201	201	0.00	2	0.72	0.08	2	0.80	1	0.67	1	0.67	1
1500	1498	1498	1498	0.00	2	1.18	0.03	2	1.23	1	1.15	1	1.15	1
3000	3000	3000	3000	0.00	2	0.74	0.05	2	0.78	1	0.89	1	0.89	1
5000	5399	5399	5399	0.00	2	0.89	0.02	2	0.91	1	0.86	1	0.86	1
8000	7788	7788	7788	0.00	2	0.77	0.00	2	0.77	1	0.78	1	0.78	1

OVERALL MEANS 0.80 0.00 10 0.88 0.08 5 0.87 0.08 5

ESTIMATED AT 10 000 PPMV 0.65

95% CONFIDENCE INTERVAL 0.61 0.67 1

Figure 5-12f

INSTRUMENT RESPONSE VS CONCENTRATION

METHYLCECLOHEXANE

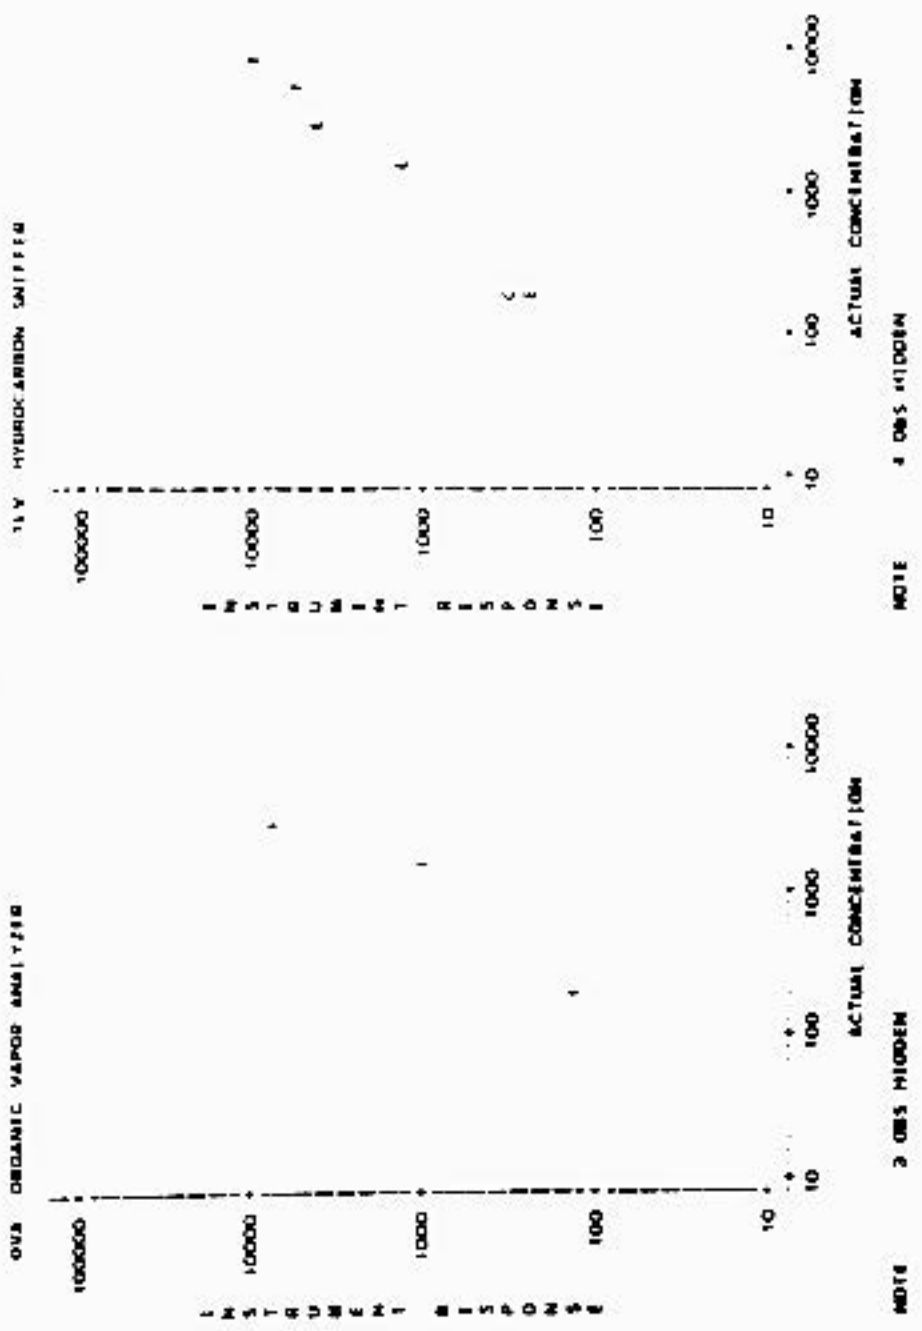


TABLE 5-12M

RESPONSE FACTOR SUMMARY

DEVELOPMENT TIME 1

DEVELOPMENT TIME 1

NOMINAL PPMV	ACTUAL PPMV		OVERALL		NO. OF		95% CONFIDENCE INTERVAL		DEVIATION		STANDARD	
	LOW	HIGH	MEAN	SE	N	SE	N	SE	N	SE	N	SE
200	208	208	1.22	0.04	2	1.18	1	1.26	1	1.26	1	1.26
1500	1547	1547	0.78	0.03	2	0.74	1	0.78	1	0.78	1	0.78
4000	3890	3890	0.41	0.01	2	0.40	1	0.41	1	0.41	1	0.41
8000	8040	8040										

OVERALL MEANS 0.80 0.00 6 0.77 0.27 2 0.82 0.24 1

ESTIMATED AT 10,000 PPMV 0.33 95% CONFIDENCE INTERVAL 1.0 24 0.451

DEVELOPMENT TIME 1

DEVELOPMENT TIME 1

NOMINAL PPMV	ACTUAL PPMV		OVERALL		NO. OF		95% CONFIDENCE INTERVAL		DEVIATION		STANDARD	
	LOW	HIGH	MEAN	SE	N	SE	N	SE	N	SE	N	SE
200	208	208	0.98	0.08	2	0.94	1	0.98	1	0.98	1	0.98
1500	1547	1547	1.48	0.07	2	1.44	1	1.48	1	1.48	1	1.48
4000	3890	3890	2.26	0.08	2	2.22	1	2.26	1	2.26	1	2.26
8000	8040	8040	2.19	0.07	2	2.15	1	2.19	1	2.19	1	2.19


OVERALL MEANS 1.77 0.01 10

ESTIMATED AT 10,000 PPMV 2.22 95% CONFIDENCE INTERVAL 1.5 25 2.053

FIGURE 3-12B

INSTRUMENT RESPONSE VS CONCENTRATION

1,1,1-TRICHLOROETHANE

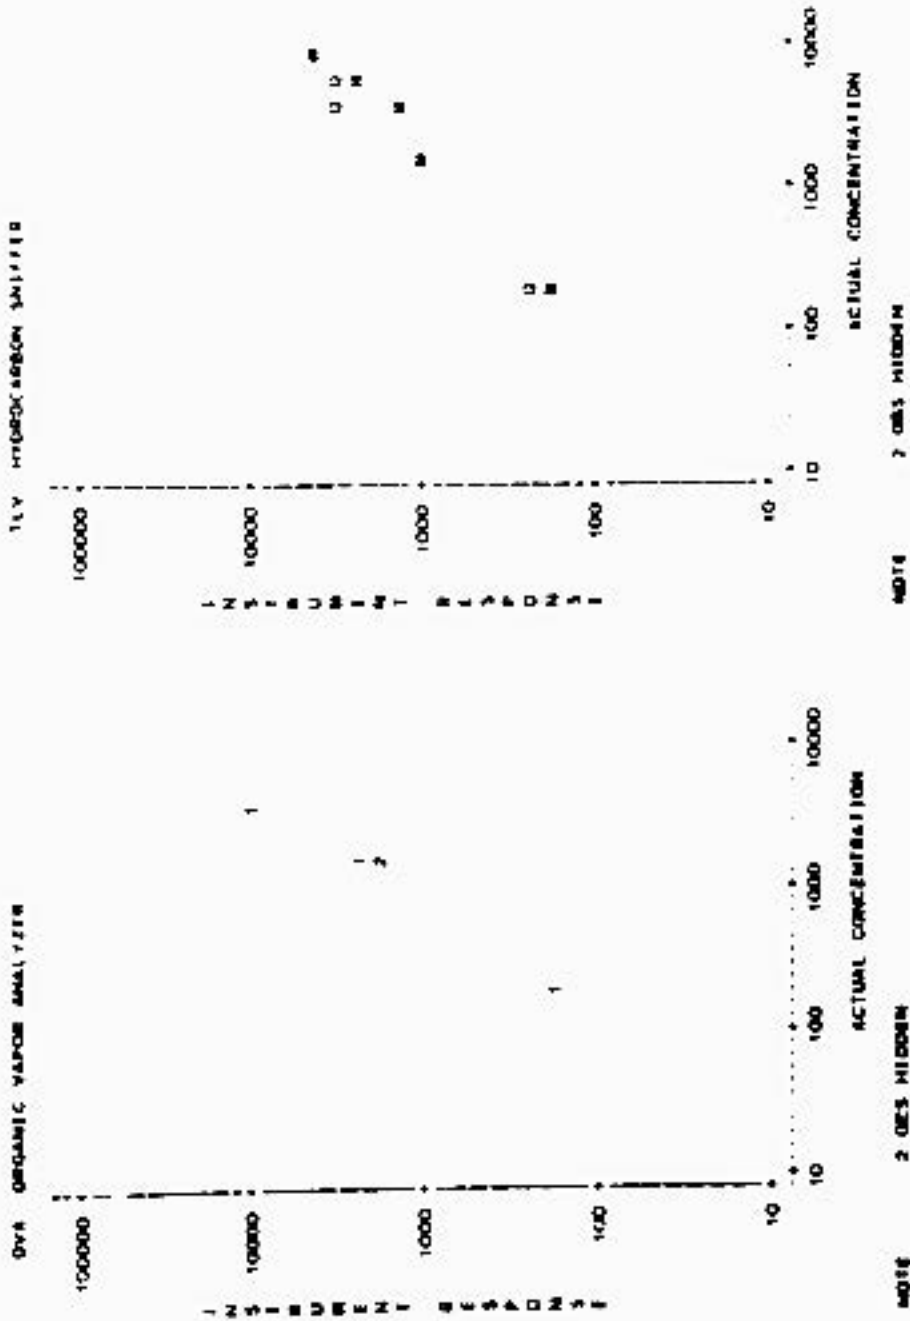

NOTE 2 OBS. HIDDEN

NOTE 2 OBS. HIDDEN



TABLE 5-174

DISPENSE FACTOR SUMMARY

IV INSTRUMENTS


NOMINAL PPMV	ACTUAL PPMV			OVERALL			DESIGN POINTS INTERVALS							
	LOW	HIGH	MEAN	SE	N	MEAN	SE	N	2254	51	N	2199	SE	N
200	218	218	218	1.34	0.00	2	1.30	1	1.39	1	1	1.39	1	1
1000	1487	1487	1487	0.80	0.02	2	0.88	1	0.82	1	1	0.82	1	1
7000	7412	7412	7412	1.46	0.03	2	1.46	1	1.43	1	1	1.43	1	1
OVERALL MEANS			1.22	0.01	6	1.22	0.18	3	1.21	0.19	3			
ESTIMATED AT 90,000 PPMV			1.17	95% CONFIDENCE INTERVAL										

IV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			DESIGN POINTS INTERVALS							
	LOW	HIGH	MEAN	SE	N	MEAN	SE	N	70	SE	N	21	SE	N
200	219	219	219	1.67	0.04	2								
1000	1487	1487	1487	1.98	0.47	2								
7000	7412	7412	7412	2.96	0.44	2								
OVERALL MEANS			2.20	0.08	6									
ESTIMATED AT 90,000 PPMV			2.02	95% CONFIDENCE INTERVAL										

FIGURE 5-129

INSTRUMENT RESPONSE VS CONCENTRATION

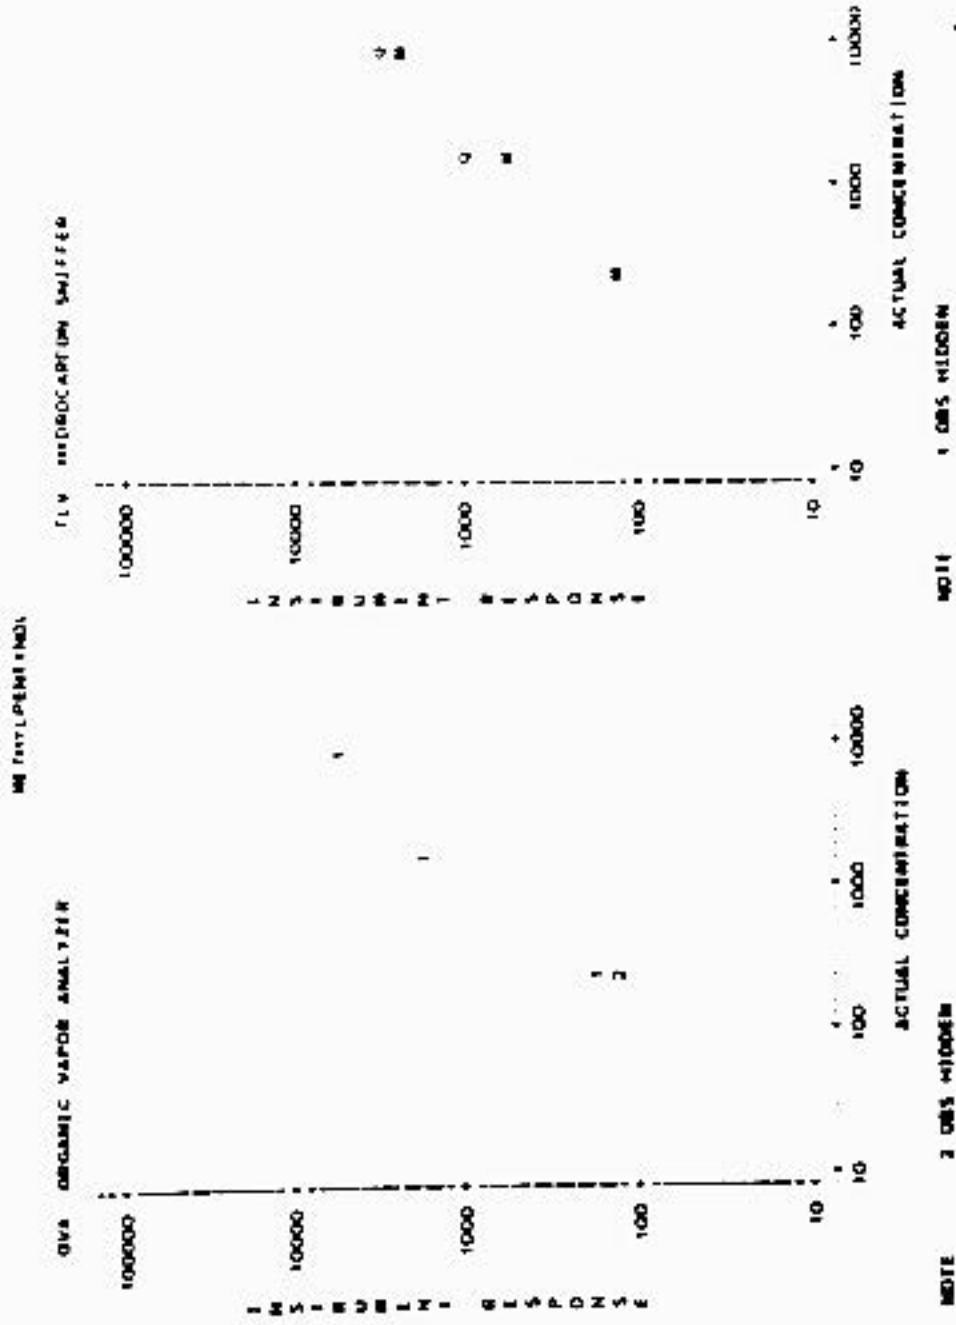

NOTE 2 OBS HI000EM

NOTE 1 OBS HI000EM

TABLE 5.1 (H)

RESPONSE FACTOR SUMMARY

MEASURED DATA

DATA INSTRUMENTS

NOMINAL DEPTH	ACTUAL DEPTH			OVERALL			95% CONFIDENCE INTERVAL								
	LOW	HIGH	MEAN	MEAN	SE	N	LOW	SE	N	LOW	SE	N	HIGH	N	
50	11	08	43	19	0.48	4	9.48	0.50	2	0.47	1	1			
500	534	543	543	6.39	0.28	4	6.11	1.11	2	0.87	2	0.09	2		
5000	5618	5618	5618	12.27	0.92	2	12.18		1	1.35	1				
8000	8817	8896	8896	10.41	0.08	4	10.47	0.02	2	10.35	0.48	2			
OVERALL MEANS			8.22	0.61	14	8.26	1.19	1	6.39	0.07	7				

ESTIMATED AT 10,000 DEPTH 10.24

95% CONFIDENCE INTERVAL 4.8 TO 12.831

TEST INSTRUMENTS

NOMINAL DEPTH	ACTUAL DEPTH			OVERALL			95% CONFIDENCE INTERVAL								
	LOW	HIGH	MEAN	MEAN	SE	N	LOW	SE	N	LOW	SE	N	HIGH	N	
50	31	50	42	1.58	0.22	4	1.80	0.48	2	1.37	0.48	2			
500	524	549	543	12.47	2.41	4	14.88	6.84	2	10.06	4.04	2			
5000	5618	5618	5618	53.16	39.8	2	102.1		1	23.56		1			
8000	8817	8896	8896	37.33	7.4	4	61.81	19.3	2	19.86	0.11	2			
OVERALL MEANS			23.70	0.95	14	36.66	15.3	2	10.46	3.04	7				

ESTIMATED AT 10,000 DEPTH 31.46

95% CONFIDENCE INTERVAL 116.18 TO 61.591


Figure 3-110

ENVIRONMENT RESPONSE VS CONCENTRATION

METHYLSILICONE A

QVA ORGANIC VAPOR ANALYZER

TV HYDROCARBON SNIFFER

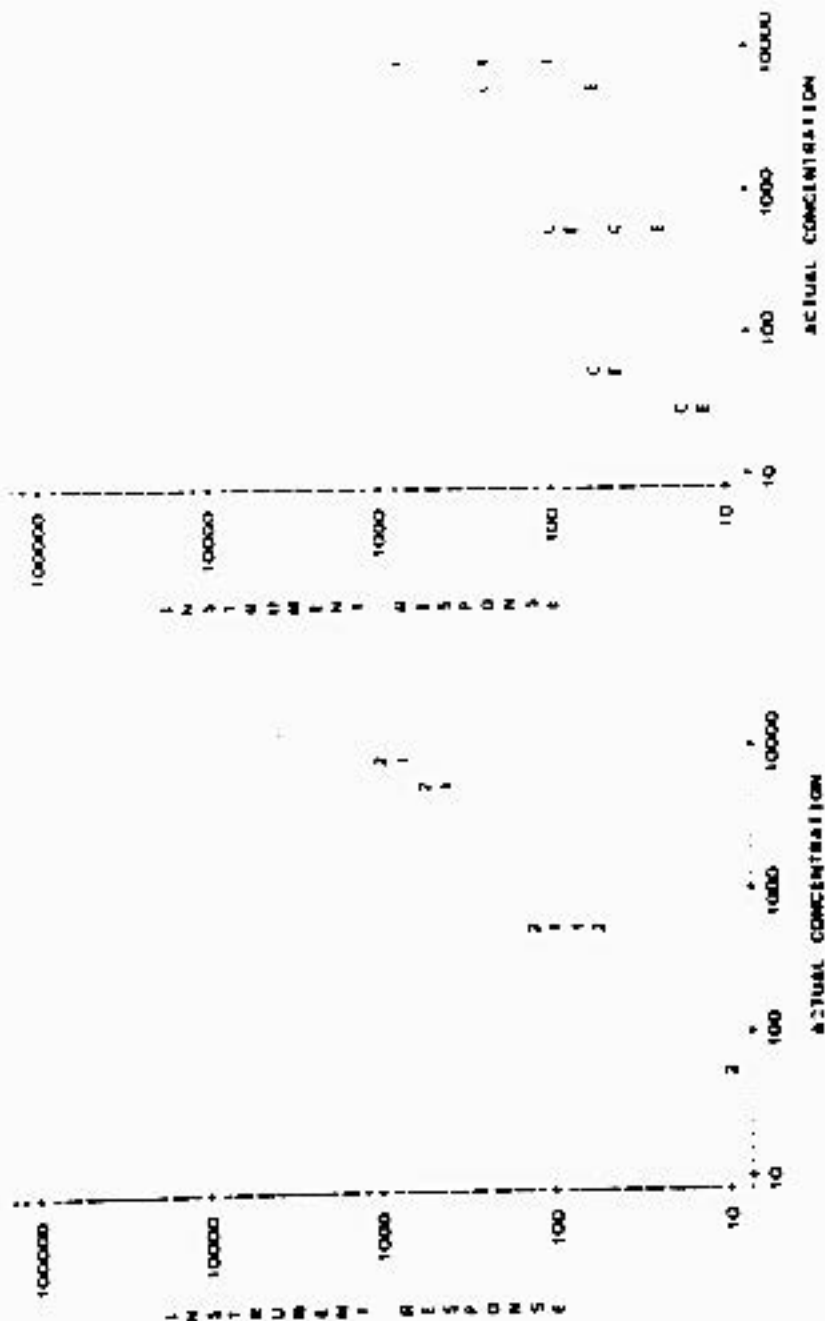

NOTE 3 OBS MISSING OR OUT OF RANGE

NOTE 1 OBS HIDDEN

TABLE 5-111

RESPONSE FACTOR SUMMARY

MINIPIE THERMOCOUPLING

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		P E S P O M S I F A C T O R S											
	LOW	HIGH	MEAN	SE	1000	SE	N	2254	SE	N	3409	SE	N	1818	SE	N
100	92	92	29.74	21.4	2						81.14		7	18.24		1
200	198	198	10.77	2.84	2						1.91		1	13.63		1
400	428	428	28.36	3.98	2						30.34		1	22.36		1
1000	1574	1574	131.8	17.6	2						69.94		1	148.2		1
6000	6024	6024	21.77	0.49	2						16.28		1	27.26		1

OVERALL MEANS AT 24 0 01 10

ESTIMATED AT 10 000 PPMV 28 04

95 % CONFIDENCE INTERVAL 1 6 30 1731

11V INSTRUMENTS

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		P E S P O M S I F A C T O R S											
	LOW	HIGH	MEAN	SE	1000	SE	N	2254	SE	N	3409	SE	N	1818	SE	N
100	92	92	0.87		1						0.87		1			1
200	198	198	1.10		1						1.10		1			1
400	428	428	3.03		1						3.03		1			1
1000	1574	1574	9.26		1						9.26		1			1
6000	6024	6024	13.85		1						13.85		1			1

OVERALL MEANS 7.58

ESTIMATED AT 10 000 PPMV 25 83

95 % CONFIDENCE INTERVAL 1.1 12 96 441

Figure 5-131

INSTRUMENT RESPONSE VS CONCENTRATION

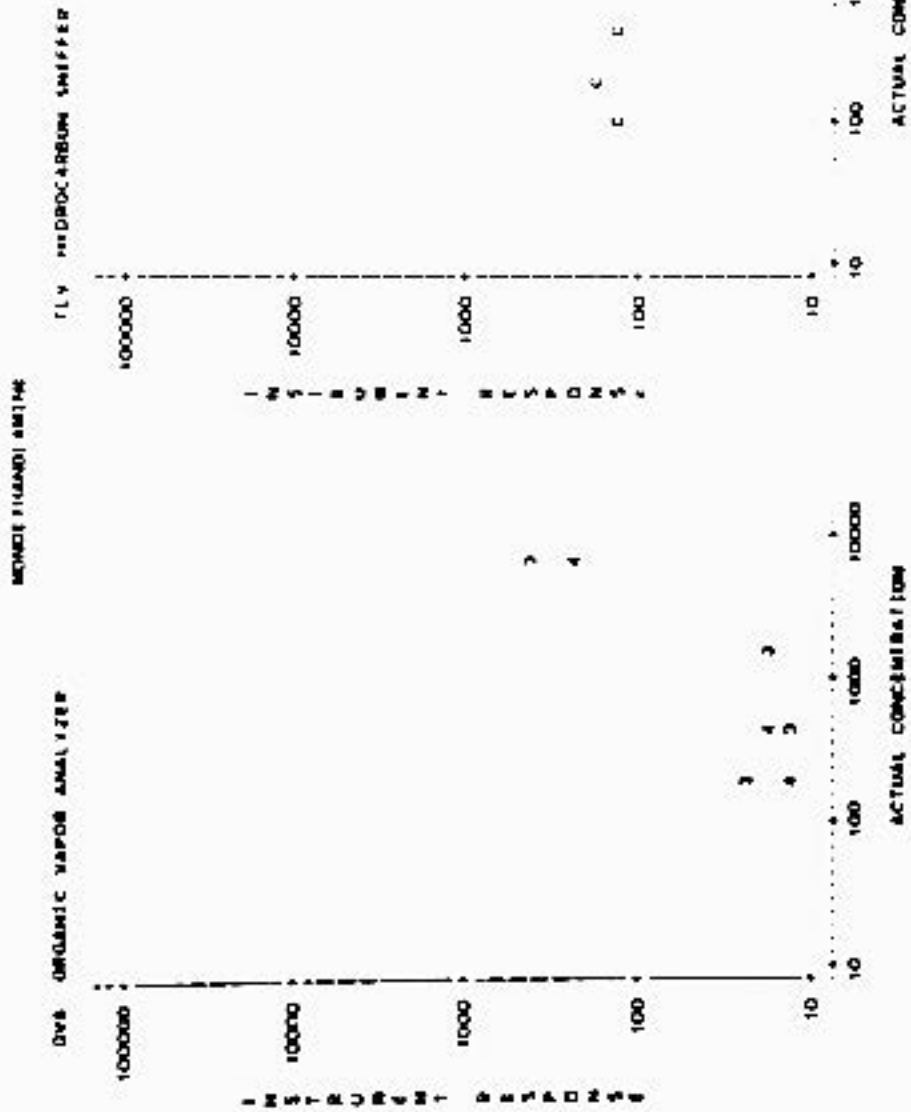


TABLE 1-12

RESPONSE FACTOR SUMMARY

MEMPHIS PM

DVA INSTRUMENTS		M E S P O N S E F A C T O R S																
NOMINAL PPM	ACTUAL PPM			OVERALL			DVA METERS											
	LOW	HIGH	MEAN	MEAN	SE	N	1000	50	25	12.5	6.25	3.125	1.5625	0.78125	0.390625	0.1953125	0.09765625	
200	187	197	192	1.31	0.12	2												
1000	1519	1519	1519	1.45	0.12	2												
8000	7574	7574	7574	0.85	0.01	2												
	OVERALL MEANS			1.70	0.01	6												
ESTIMATED AT 10 CRK PPM			0.92	75 % CONFIDENCE INTERVAL 1 0.64 5.327														

11V INSTRUMENTS


DVA INSTRUMENTS		M E S P O N S E F A C T O R S																
NOMINAL PPM	ACTUAL PPM			OVERALL			DVA METERS											
	LOW	HIGH	MEAN	MEAN	SE	N	10	50	25	12.5	6.25	3.125	1.5625	0.78125	0.390625	0.1953125	0.09765625	
200	197	197	197	1.09		1												
1000	1519	1519	1519	2.71		1												
8000	7574	7574	7574	1.88		1												
	OVERALL MEANS			1.63		3												
ESTIMATED AT 10 CRK PPM			0.99	95 % CONFIDENCE INTERVAL 1 0.36 11.411														

Figure 5-112

INSTRUMENT RESPONSE VS CONCENTRATION

ACETOPHENONE

DVA ORGANIC VAPOR ANALYZER

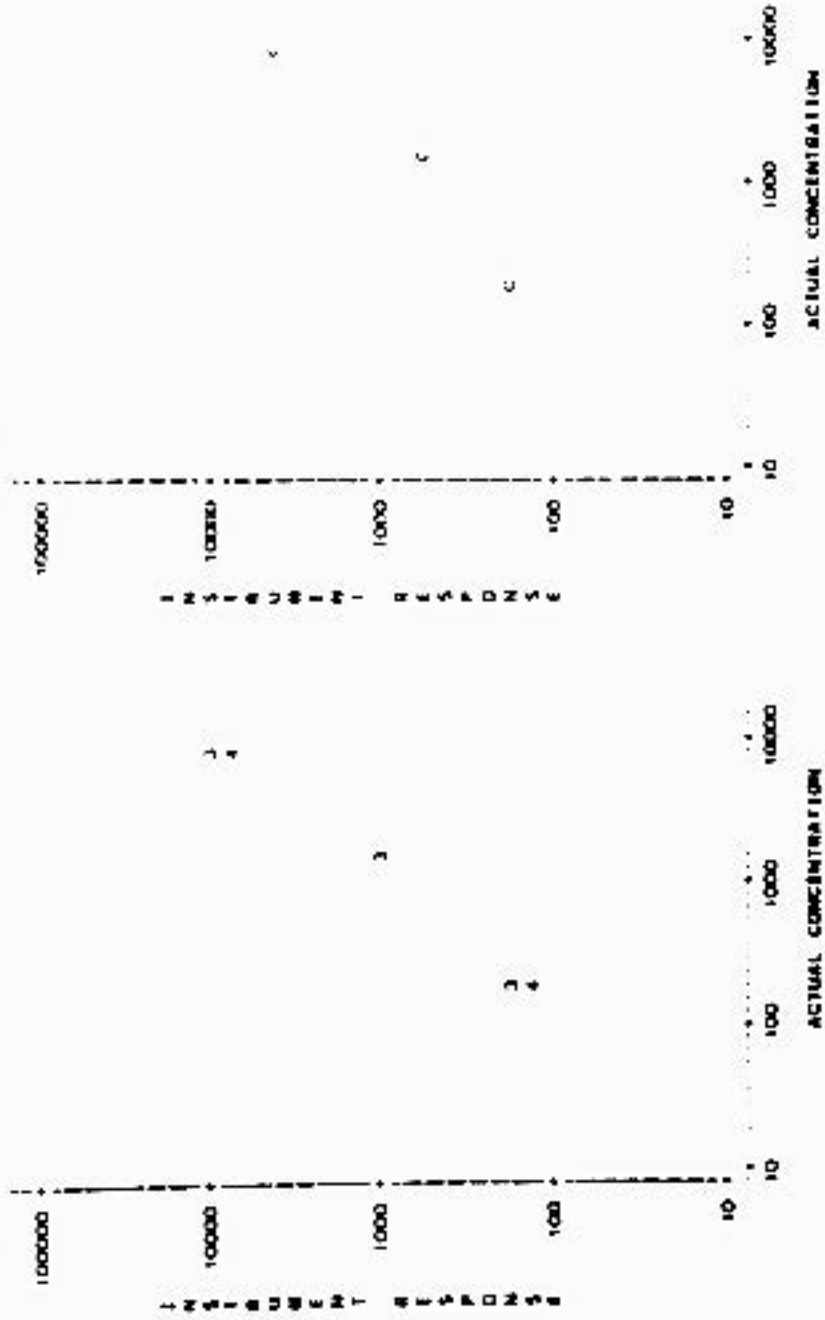

NOTE: OBS. MEDIUM



TABLE 5-133

RESPONSE FACTOR SUMMARY

METHYLENE		RESPONSE FACTOR SUMMARY															
OVR INSTRUMENTS		ACTUAL PPMV				OVERALL				OVR METERS							
NOMINAL PPMV	LOW	HIGH	MEAN	SE	N	100%	SE	N	2204	SE	N	2159	SE	N	95% CI	SE	N
100	103	103	103	0.21	2							1.09	1	1.48			
200	201	201	201	1.02	1							1.02	1				
400	485	485	4.48		1							4.48	1				
1000	920	920	9.22		1							9.22	1				
OVERALL MEANS		2.67		0.12	6	95% CONFIDENCE INTERVAL		1.92		2.40		2.97		1.14	4	1.68	
ESTIMATED AT 10 000 PPMV		2.67		0.12	6	95% CONFIDENCE INTERVAL		1.92		2.40		2.97		1.14	4	1.68	

METHYLENE		RESPONSE FACTOR SUMMARY															
OVR INSTRUMENTS		ACTUAL PPMV				OVERALL				OVR METERS							
NOMINAL PPMV	LOW	HIGH	MEAN	SE	N	100%	SE	N	2204	SE	N	2159	SE	N	95% CI	SE	N
100	103	103	103	0.47	1							0.47	1				
200	201	201	201	0.48	1							0.48	1				
400	485	485	2.09		1							2.09	1				
1000	920	920	3.72		1							3.72	1				
OVERALL MEANS		1.69			4	95% CONFIDENCE INTERVAL		1.08		0.78		1.69		0.78	4	1.48	
ESTIMATED AT 10 000 PPMV		1.69			4	95% CONFIDENCE INTERVAL		1.08		0.78		1.69		0.78	4	1.48	

Figure 5-133  
 INSTRUMENT RESPONSE VS CONCENTRATION

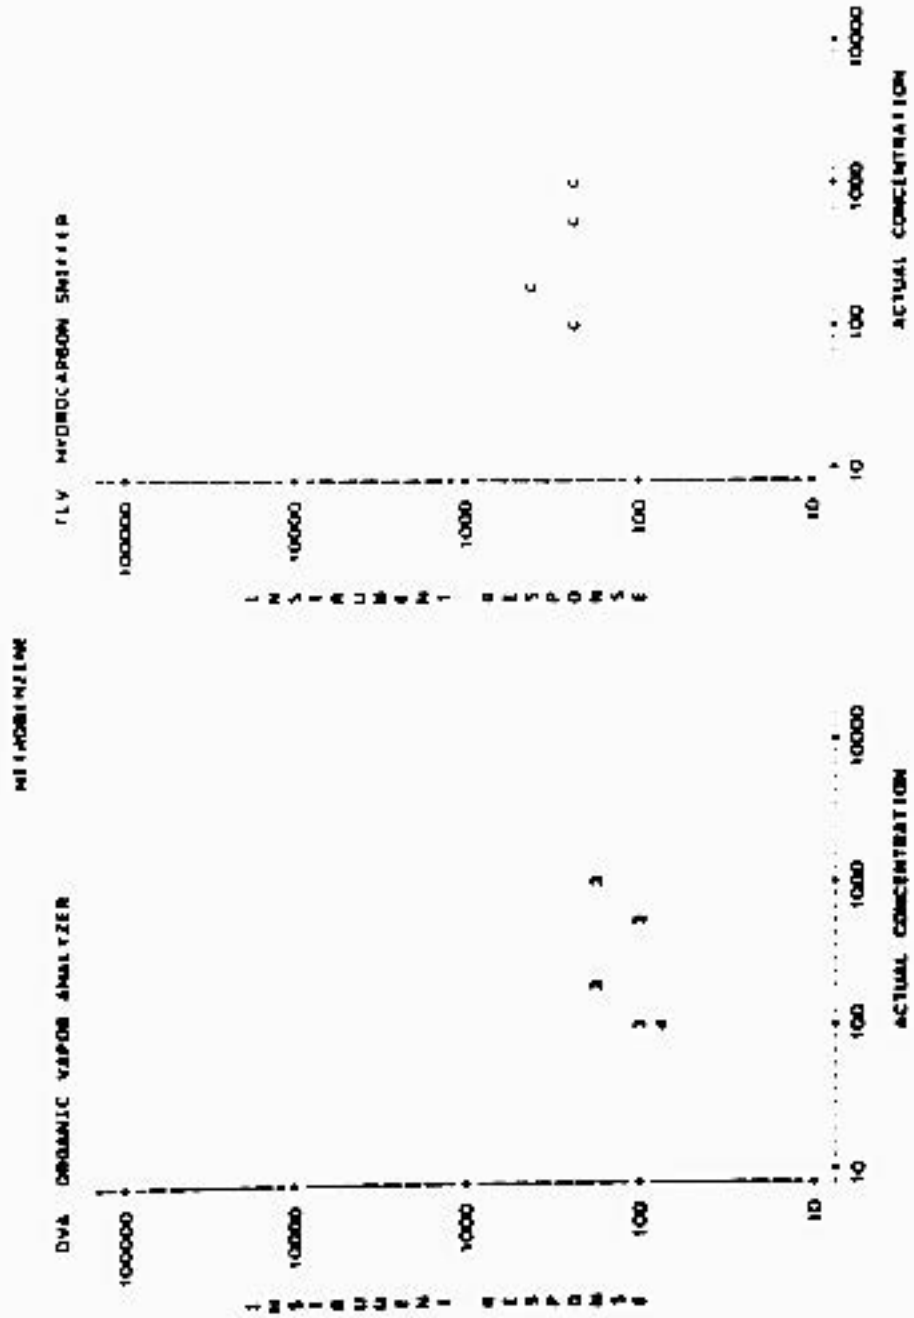


TABLE 5-134

RESPONSE FACTOR SUMMARY

NI FID INSTRUMENT

DIA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTORS									
	LOW	HIGH	MEAN	SE	N	100%	SE	N	225%	SE	N	215%	SE	N
2000	188	188	1.40	0.10	2	1.80		1	1.29		1			
1500	1502	1502	1.51	0.00	2	1.52		1	1.51		1			
8000	1961	1961	1.36	0.01	2	1.34		1	1.36		1			
OVERALL MEANS		1.42	0.01	6	1.40	0.05	3	1.34	0.06	3				
ESTIMATED AT 10,000 PPMV 1.40														
95% CONFIDENCE INTERVAL (1.27 - 1.50)														

DIA METERS

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		RESPONSE FACTORS									
	LOW	HIGH	MEAN	SE	N	100%	SE	N	225%	SE	N	215%	SE	N
2000	188	188	0.98	0.23	2							0.74		
1500	1502	1502	1.88	0.48	2							1.40		
8000	1961	1961	2.30	0.28	2							2.11		
OVERALL MEANS		1.75	0.09	6								1.42	0.10	3
ESTIMATED AT 10,000 PPMV 2.54														
95% CONFIDENCE INTERVAL (1.80 - 3.28)														

FLV METERS


Figure 5-134

INSTRUMENT RESPONSE VS CONCENTRATION

METHYLENE

18 V HYDROCARBON SNIPPER

DVA ORGANIC VAPOR ANALYZER

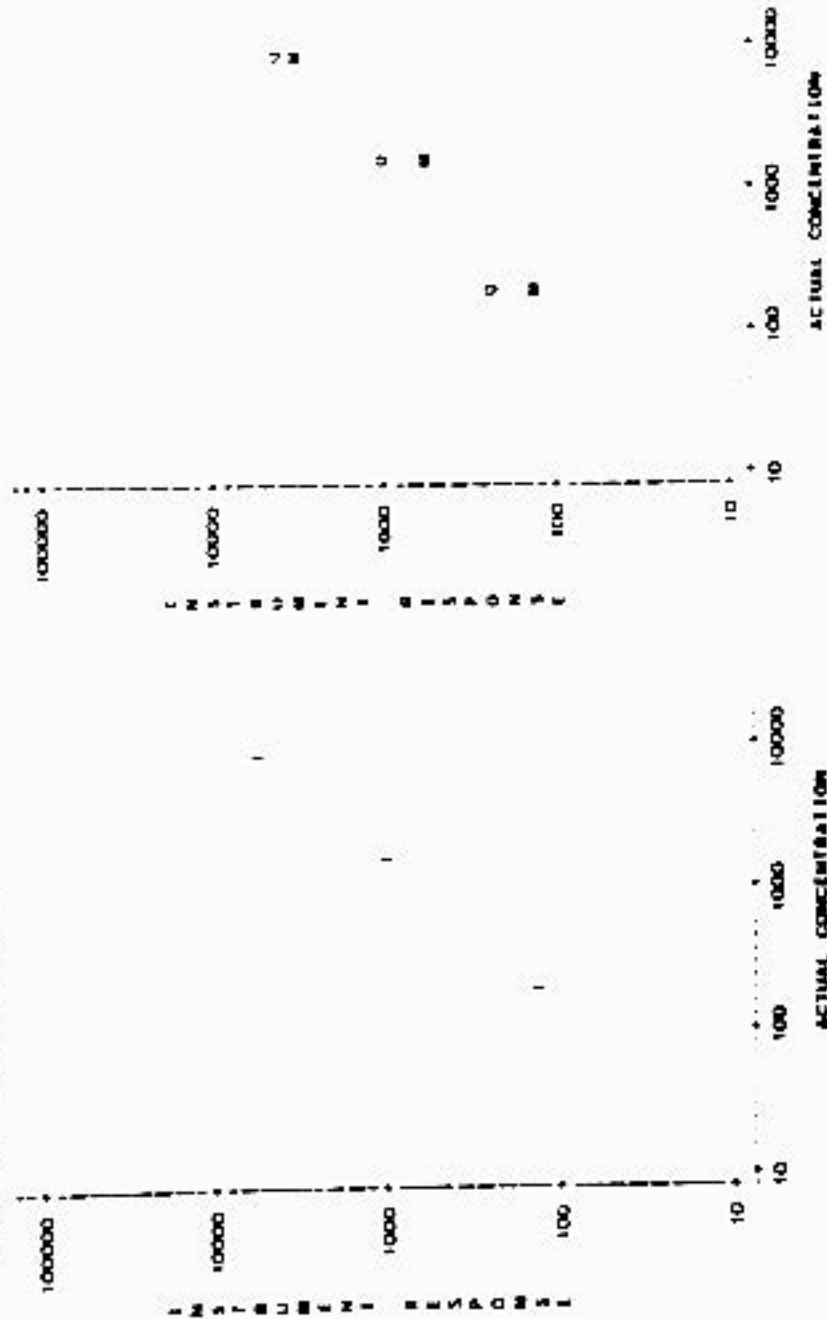

NOTE 3 DBS HYDROGEN

TABLE 5-315

RESPONSE FACTOR SUMMARY

MILLIROMETHANE

R E S P O N S E F A C T O R S

OVA INSTRUMENTS

NOMINAL PPEV	ACTUAL PPEV			OVERALL			OVA METERS												
	LOW	HIGH	MEAN	SE	M	N	1080	SE	N	2254	SE	N	2198	SE	N	1811	SE	N	
200	221	221	221	2 84	0 01	2	2 32		1	2 91		1							
1500	1537	1537	1537	2 95	0 14	2	2 81		1	3 40		1							
8000	8740	8740	8740	3 37	0 32	2	3 24		1	3 50		1							
OVERALL MEANS			3 08	0 02	8	2 84	0 15	3	3 17	0 17	2								

ESTIMATED AT 10,000 PPEV 3 32 95 % CONFIDENCE INTERVAL 1 3 03 3 848

11V INSTRUMENTS


R E S P O N S E F A C T O R S

NOMINAL PPEV	ACTUAL PPEV			OVERALL			11V METERS												
	LOW	HIGH	MEAN	SE	M	N	78	SE	N	16	SE	N	74	SE	N	16	SE	N	
200	221	221	221	3 44	1 39	2				5 22		1	1 65						
1500	1537	1537	1537	4 51	1 32	2				5 83		1	7 18						
8000	8740	8740	8740	5 95	1 67	2				7 84		1	4 18						
OVERALL MEANS			4 63	0 78	6	6 19	0 69	2	6 11	0 14	2								

ESTIMATED AT 10,000 PPEV 5 25 95 % CONFIDENCE INTERVAL 1 2 32 11 867

Figure 5-15

INSTRUMENT RESPONSE VS CONCENTRATION

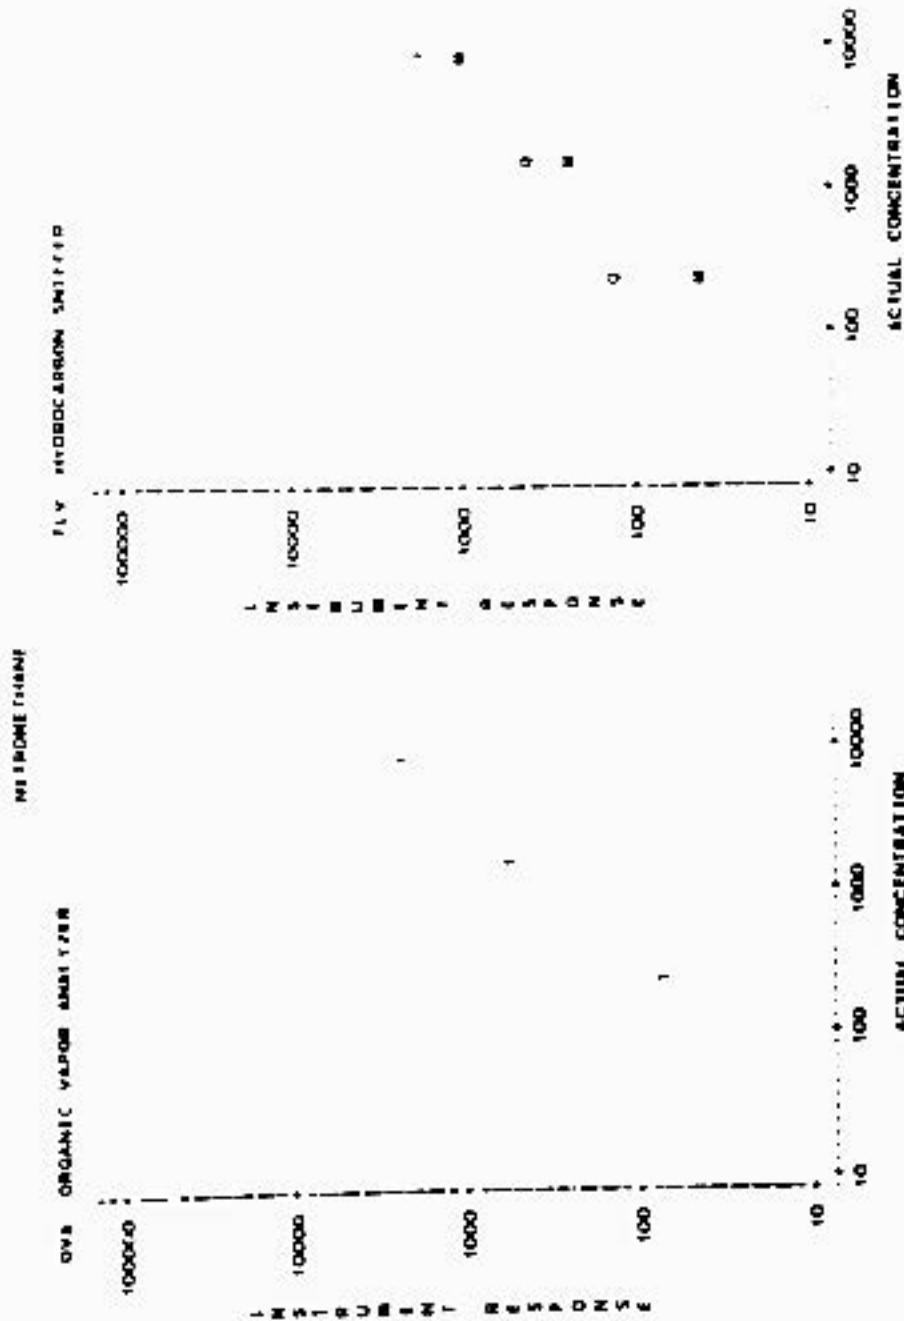

NOTE: 3 OBS HIDDEN

TABLE 5-136

RESPONSE FACTOR SUMMARY

MITROPROPRANE

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY								
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2250	SE	N	1000	SE	N
200	217	217	217	1.51	0.21	2	1.31		1	1.72		1	1.61		1
1000	1564	1564	1564	1.53	0.04	2	1.48		1	1.57		1	1.53		1
8000	8565	8565	8565	1.01	0.09	2	0.92		1	1.10		1	1.05		1
OVERALL MEANS						1.35	0.02	6	1.24	0.17	3	1.46	0.19	3	

ESTIMATED AT 10,000 PPMV 1.06

95% CONFIDENCE INTERVAL 1.07M 1.42I

TEV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY								
	LOW	HIGH	MEAN	MEAN	SE	N	3E	SE	N	70	SE	N	10	SE	N
200	217	217	217	0.90	0.24	2			1	1.11		1	0.69		1
1000	1564	1564	1564	1.32	0.31	2			1	1.54		1	1.05		1
8000	8565	8565	8565	1.75	0.09	2			1	1.85		1	1.68		1
OVERALL MEANS						1.22	0.03	6	1.51	0.21	3	1.14	0.24	3	


ESTIMATED AT 10,000 PPMV 1.77

95% CONFIDENCE INTERVAL 1.22 2.07I

Figure 5-14b

INSTRUMENT RESPONSE VS. CONCENTRATION

NIRODUREPENE

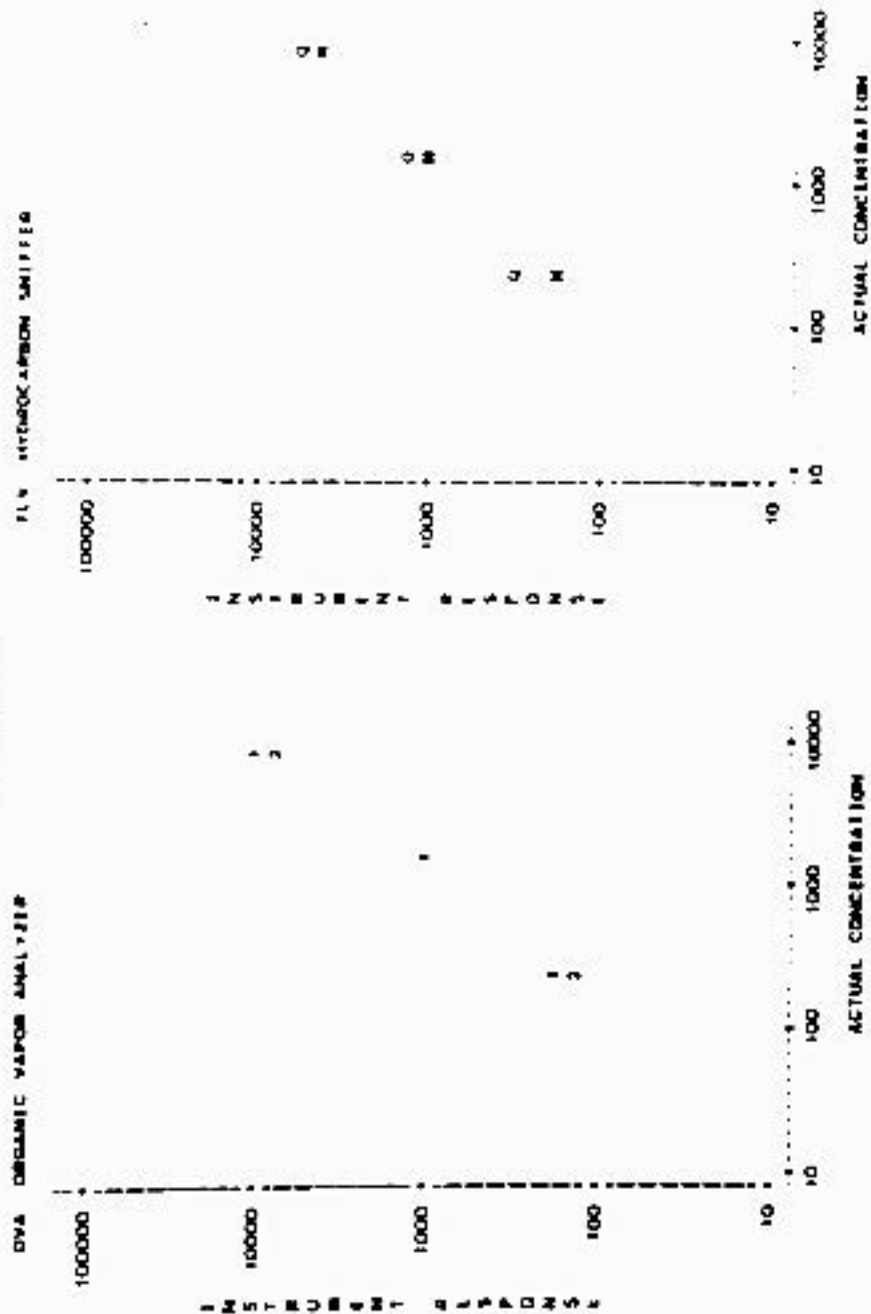

NOTE 1 OBS HIDDEN



TABLE 5.11.

RESPONSE FACTOR SUMMARY

NONANE N

OVA INSTRUMENTS		RESPONSE FACTORS										
NOMINAL PPMV	ACTUAL PPMV	OVERALL					OVA METERS					
		LOW	HIGH	MEAN	SE	N	100%	5%	N	25%	5%	N
50	56	56	56	2.11	0.27	4	2.44	0.22	2	2.08	0.14	2
500	485	490	488	4.04	0.21	4	3.03	0.88	2	4.29	0.94	2
2500	2485	2485	2485	0.87	0.03	2	0.90		1	0.84		1
4000	3923	3926	3944	2.44	0.03	4	2.41	0.44	2	2.47	0.27	2
OVERALL MEANS		2.75	0.01	14	2.61	0.44	2	2.89	0.90	2		

ESTIMATED AT 10 000 PPMV 1.87

95% COMPLIANCE INTERVAL 1.0 93 3.811

11V INSTRUMENTS

ACTUAL PPMV		RESPONSE FACTORS													
NOMINAL PPMV	LOW	HIGH	MEAN	SE	N	OVERALL					11V METERS				
						7%	5%	N	7%	5%	N	7%	5%	N	
50	54	58	56	0.27	0.16	4	1.53	0.22	2	1.21	0.21	2			
500	488	490	488	3.52	0.20	4	3.32	1.19	2	3.21	1.28	2			
2500	2488	2485	2488	12.10	1.77	2	13.87		1	10.34		1			
4000	3923	3926	3944	3.22	0.42	4	1.94	1.12	2	2.80	0.27	2			
OVERALL MEANS		4.05	0.03	14	4.52	1.85	2	3.57	1.22	2					

ESTIMATED AT 10 000 PPMV 5.54

95% COMPLIANCE INTERVAL 1.2 82 10.889


Figure 5-117

INSTRUMENT RESPONSE VS CONCENTRATION

NAME: M

TYPE: HYDROCARBON SAFFER

OVER ORGANIC VAPOR ANALYSIS

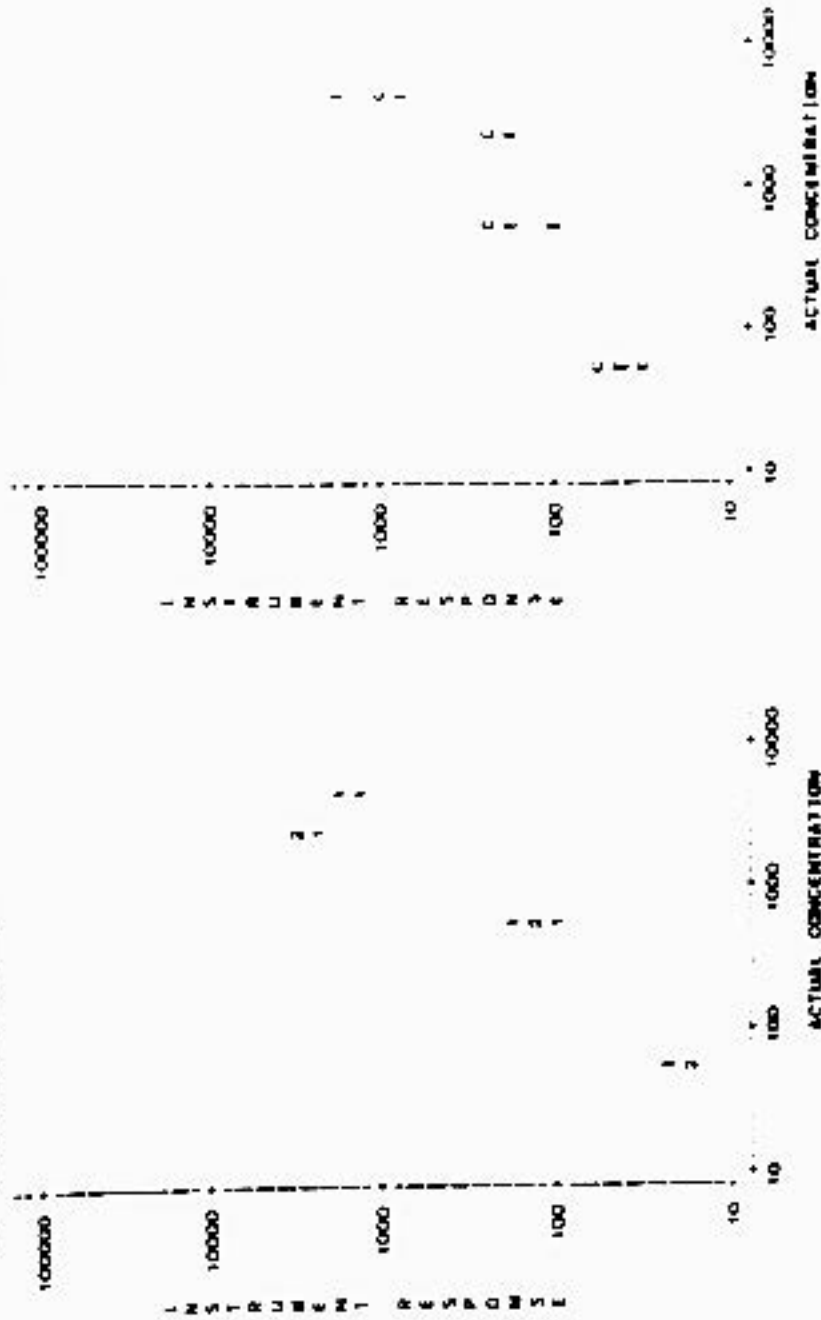

NOTE: 5 OBS HIDDEN

NOTE: 3 OBS HIDDEN

TABLE 5. 11B

RESPONSE FACTOR SUMMARY

DATE: 1/1/74

OUR INSTRUMENTS

RESPIROMETER FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OUR METERS												
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2254	SE	N	2199	SE	N	1811	SE	N	
200	223	223	223	2.27	0.22	2	2.04		1	2.50		1							
1000	1417	1417	1417	1.59	0.11	2	1.48		1	1.71		1							
6000	6508	6508	6508	1.12	0.02	2	1.10		1	1.15		1							
OVERALL MEANS			1.88	0.02	6	1.84	0.27	2	1.78	0.39	3								
ESTIMATED AT 10,000 PPMV			1.04	95% COMPLIANCE INTERVAL															

1.1V INSTRUMENTS

RESPIROMETER FACTORS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OUR METERS												
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2254	SE	N	2199	SE	N	1811	SE	N	
200	223	223	223	1.99	0.07	2	1.92		1	2.08		1							
1000	1417	1417	1417	1.88	0.12	2	2.01		1	1.77		1							
6000	6508	6508	6508	2.18	0.17	2	2.32		1	1.97		1							
OVERALL MEANS			2.01	0.08	6	2.08	0.12	2	1.94	0.09	3								
ESTIMATED AT 10,000 PPMV			2.08	95% COMPLIANCE INTERVAL															

Figure 5-118

INSTRUMENT RESPONSE VS CONCENTRATION

DCBANE

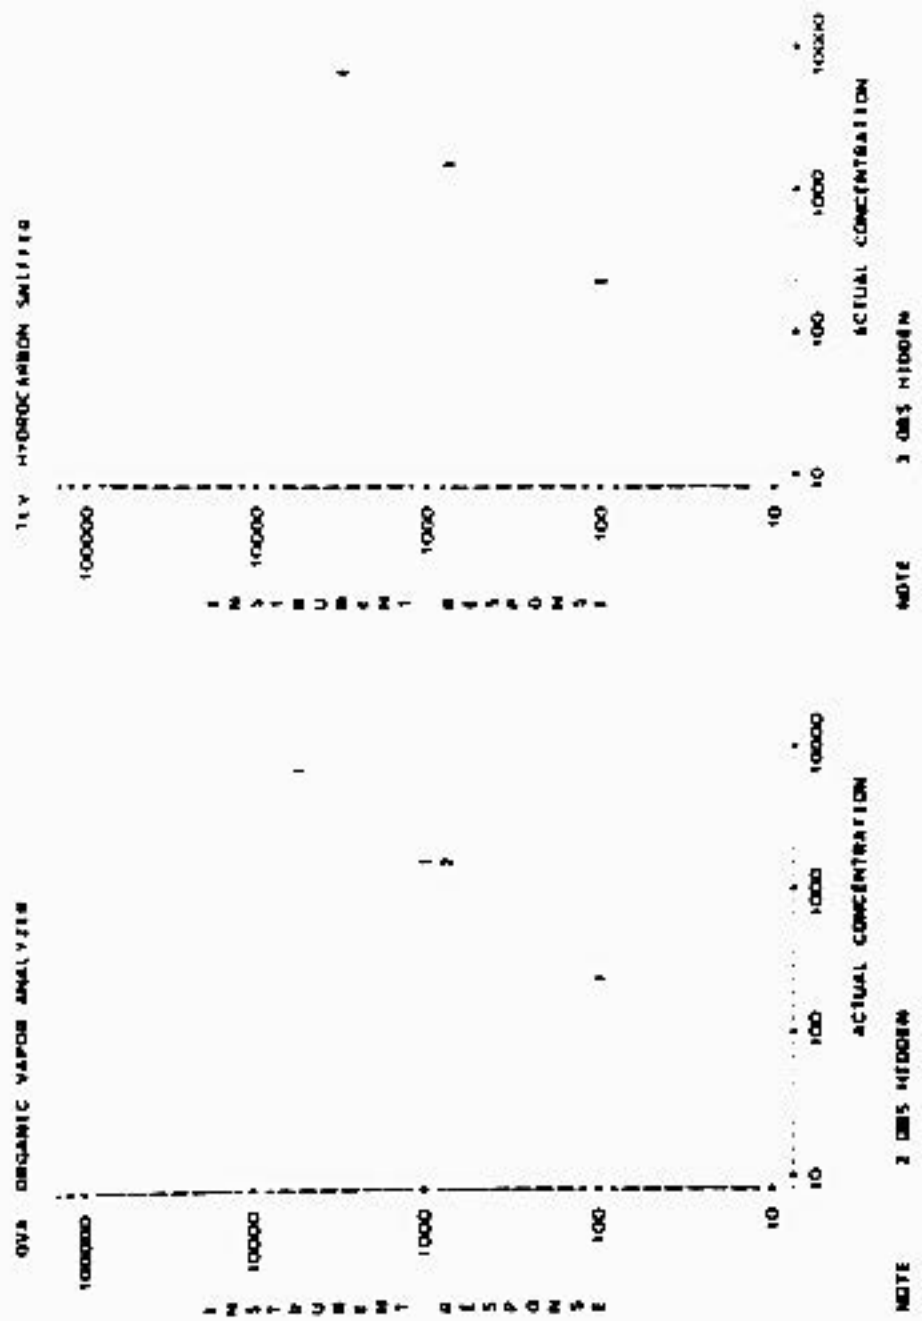


TABLE 5-119


RESPONSE FACTOR SUMMARY

PERFORM	ACTUAL PPMV					OVERALL					RESPONSE FACTOR SUMMARY									
	LOW	HIGH	MEAN	SE	N	MEAN	SE	N	1000	SE	M	225A	SE	M	2100	SE	M	1013	SE	M
IVX INSTRUMENTS																				
NOMINAL PPMV						MEAN	SE	N												
200	220	220	220	1.33	0.08	2	1.41	1	1.78											
1000	1484	1484	1484	0.94	0.03	2	0.97	1	0.91											
5000	4810	4810	4810	0.48	0.00	2	0.48	1	0.48											
8000	7838	7838	7838																	
						OVERALL MEANS	0.92	0.01	6	0.95	0.27	3	0.88	0.22	3					
						ESTIMATED AT 10,000 PPMV	0.42													

PERFORM	ACTUAL PPMV					OVERALL					RESPONSE FACTOR SUMMARY									
	LOW	HIGH	MEAN	SE	N	MEAN	SE	N	TC	SE	M	7M	SE	M	7Q	SE	M			
ILV INSTRUMENTS																				
NOMINAL PPMV						MEAN	SE	N												
200	220	220	220	0.78	0.06	2	0.82	1	0.77											
1000	1484	1484	1484	0.80	0.01	2	0.81	1	0.99											
5000	4810	4810	4810	0.84	0.00	2	0.84	1	0.84											
8000	7838	7838	7838	0.88	0.01	2	0.88	1	0.88											
						OVERALL MEANS	0.87	0.00	8	0.88	0.05	4	0.88	0.01	4					
						ESTIMATED AT 10,000 PPMV	0.87													

Figure 5-119

INSTRUMENT RESPONSE VS CONCENTRATION

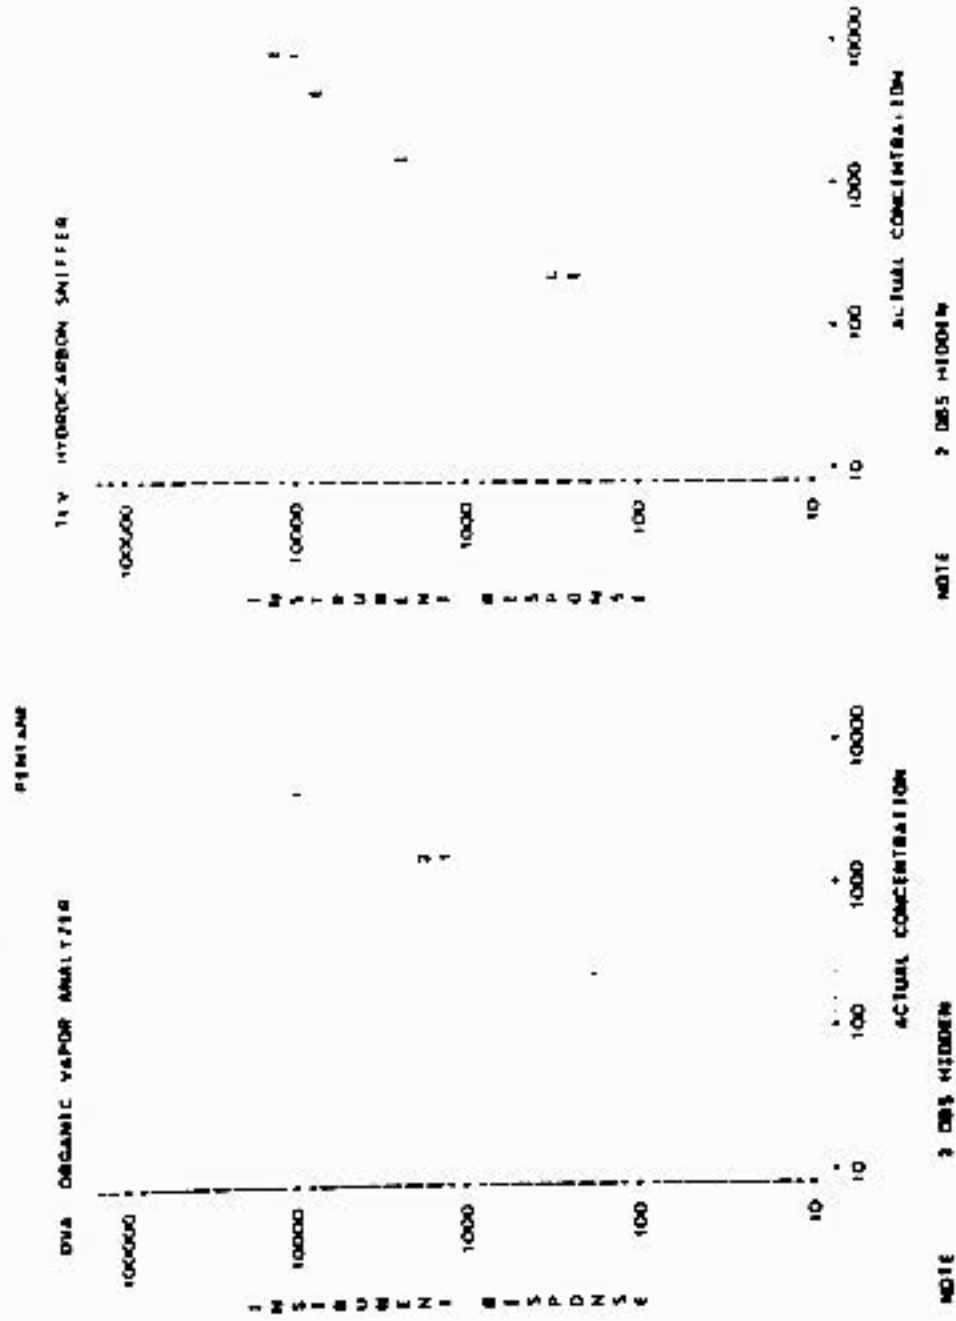

NOTE: 2 DBS H200M

NOTE: 2 DBS H200M

TABLE 5-1AD

RESPONSE FACTOR SUMMARY

PHENOL

OVA INSTRUMENTS DEFIDOMSEI A I T I R U S

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OVA METERS						
	LOW	HIGH	MEAN	SE	M	FC	SE	N	FC	SE	M		
100	72	72	72	0.08	0.28	2					1	1.19	
200	223	223	223	3.83	0.08	2					1	1.73	
300	278	278	278	3.45	0.48	2					1	2.84	
800	857	857	857	3.81	0.37	2					1	3.85	
1000	913	913	913	5.65	0.06	2					1	5.70	
OVERALL MEANS						3.76	0.02	10				3.96	0.57

ESTIMATED AT 10,000 PPMV 11.75

95% CONFIDENCE INTERVAL 1.755 18.291

ILV INSTRUMENTS

A I S P O M S E I A I T I O M S

NOMINAL PPMV	ACTUAL PPMV			OVERALL			ILV METERS				
	LOW	HIGH	MEAN	SE	M	FC	SE	N	FC	SE	M
100	72	72	72	0.57		1			0.57		1
200	223	223	223	1.86		1			1.86		1
300	278	278	278	1.79		1			1.79		1
800	857	857	857	2.17		1			2.17		1
1000	913	913	913	2.92		1			2.92		1
OVERALL MEANS						1.85		5	1.85		5


ESTIMATED AT 10,000 PPMV 12.0

95% CONFIDENCE INTERVAL 1.351 41.431

FIGURE 5-140

INSTRUMENT RESPONSE VS. CONCENTRATION

PM-100

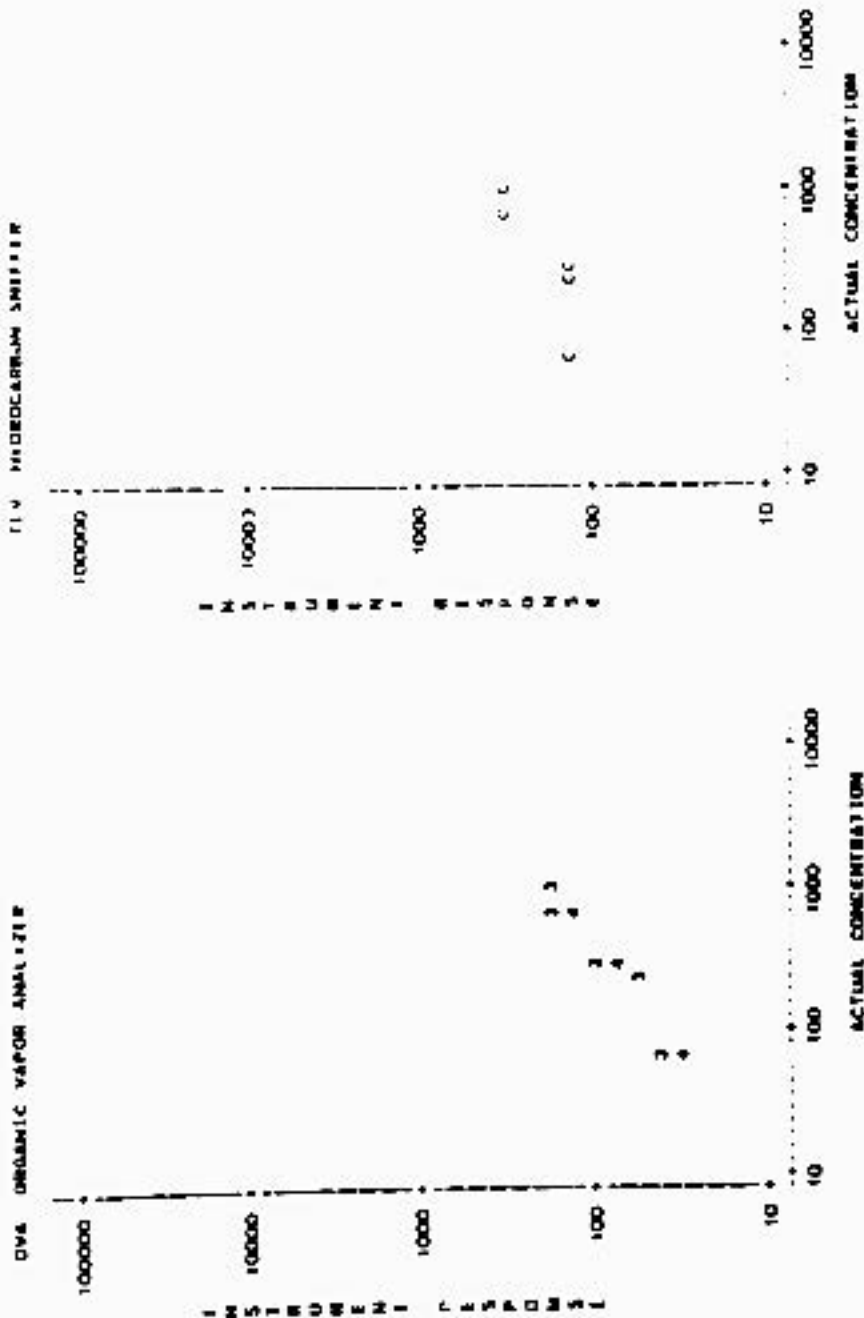

NOTE: 2 OF 11 SHOWN



TABLE 5 (A)

RESPONSE 14 FOR SUBMISSIO

PHENOL PROPANONE 2

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	SE	MEAN	SE
100	223	223	223	9.57	1.60	2
1000	1648	1648	1648	30.48	3.57	2
8000	8383	8383	8383	82.84	4.48	1
OVERALL MEANS 40.96 0.94 6						

ESTIMATED AT 10,000 PPMV 89.86

B I S P O N S E P A C I O N S

DVA METERS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	SE	MEAN	SE
100	1117	1117	1117	11.17	1	1
1000	3405	3405	3405	34.05	1	1
8000	8172	8172	8172	81.72	1	1
OVERALL MEANS 27.74 2.1 3						

ESTIMATED AT 10,000 PPMV 109.84 114.87

ILV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	SE	MEAN	SE
200	223	223	223	4.03	0.78	2
1000	1648	1648	1648	22.61	5.13	2
8000	8383	8383	8383	68.70	18.6	2
OVERALL MEANS 21.78 1.78 6						

ESTIMATED AT 10,000 PPMV 76.57

B I S P O N S E P A C I O N S

ILV METERS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	SE	MEAN	SE
200	223	223	223	4.03	0.78	2
1000	1648	1648	1648	22.61	5.13	2
8000	8383	8383	8383	68.70	18.6	2
OVERALL MEANS 24.7 2.78 5.1 18.6 3						

ESTIMATED AT 10,000 PPMV 146.98 126.41


FIGURE 5-16A

EMULSION RESPONSE VS CONCENTRATION

PHENYL PROPANE, 2

11V HYDROCARBON ANALYZER

DVA ORGANIC VAPOR ANALYZER

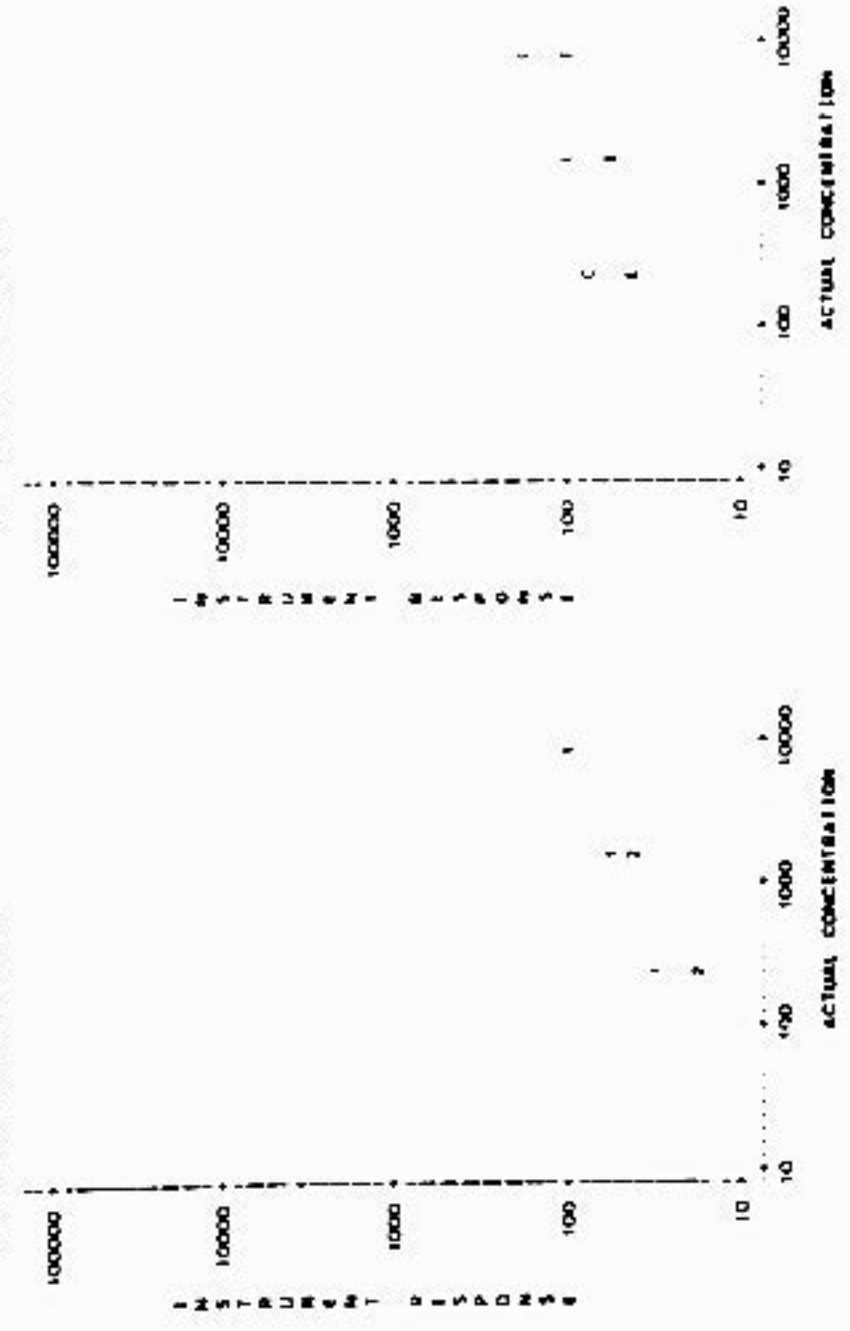

NOTE 1 OBS MEDIUM

TABLE 1-147

OFFSPRING FACTOR SUMMARY

PAGE ONE

OFFSPRING FACTOR SUMMARY

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OFFSPRING FACTOR SUMMARY									
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	99	2100	SE	N	1000	SE	N	
700	217	217	217	1 07 0 00	2	1 01	1	1 12	1							
1800	1809	1809	1809	0 02 0 00	2	0 08	1	0 09	1							
4000	4019	4019	4019	0 42 0 07	2	0 40	1	0 48	1							
9000	9038	9038	9038													
8000	8038	8038	8038													

OVERALL MEANS 0 13 0 01 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06

ESTIMATED AT 10 000 PPMV 0 34 95% CONFIDENCE INTERVAL 1 0 21 0 411

PAGE TWO

OFFSPRING FACTOR SUMMARY

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OFFSPRING FACTOR SUMMARY									
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	99	2100	SE	N	1000	SE	N	
700	217	217	217	1 07 0 00	2	1 01	1	1 12	1							
1800	1809	1809	1809	0 02 0 00	2	0 08	1	0 09	1							
4000	4019	4019	4019	0 42 0 07	2	0 40	1	0 48	1							
9000	9038	9038	9038													
8000	8038	8038	8038													

OVERALL MEANS 0 13 0 01 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06 0 06

ESTIMATED AT 10 000 PPMV 0 34 95% CONFIDENCE INTERVAL 1 0 21 0 411

Figure 5-142

INSTRUMENT RESPONSE VS CONCENTRATION

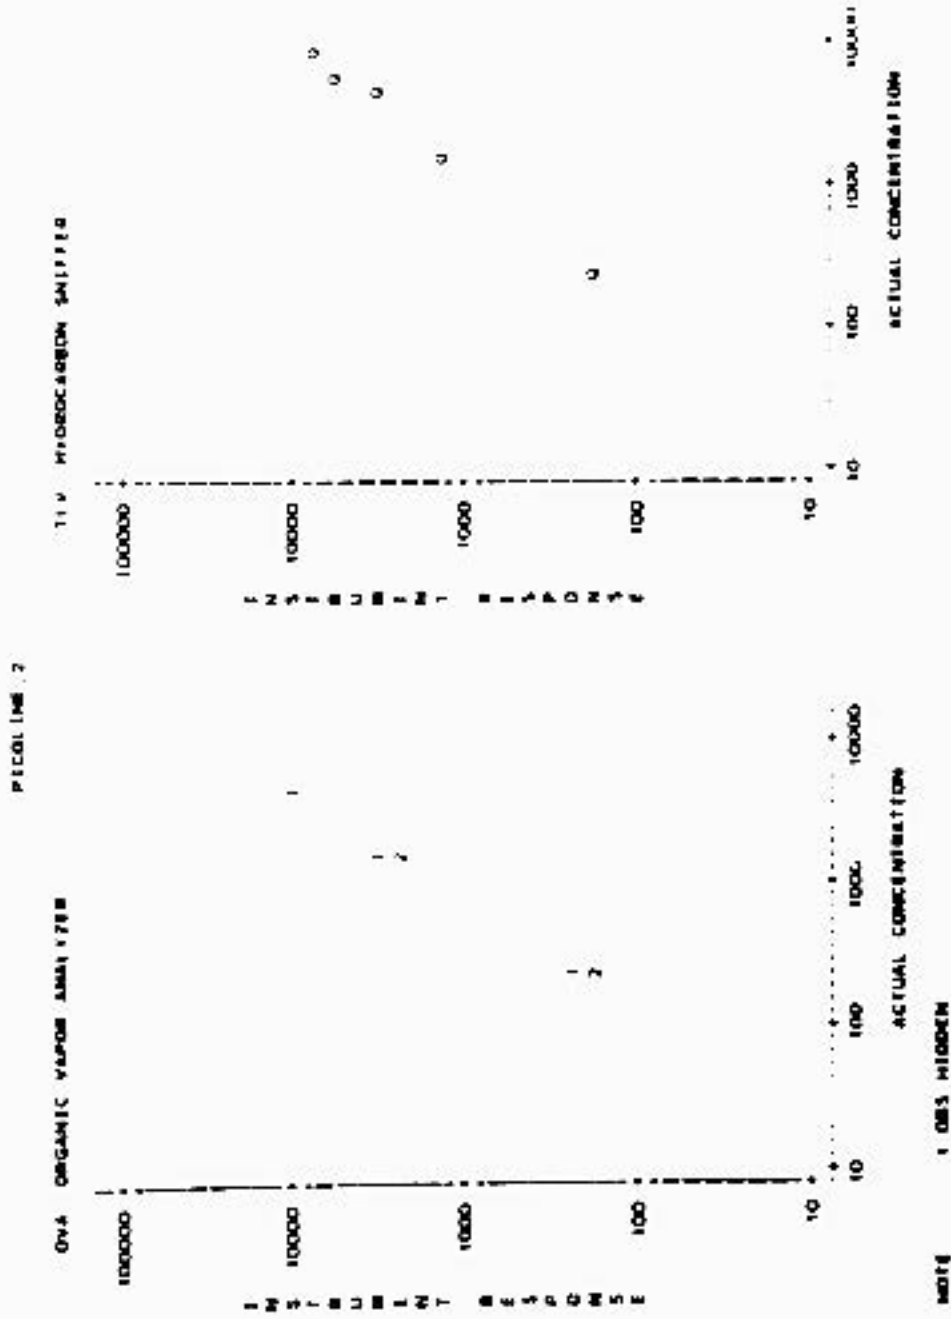


TABLE 1

DISPERSED FACTOR STUDIES

PROGRAM

DVA INSTRUMENTS

MINIMAL PPMV	ACTUAL PPMV		OVERALL		DISPERSED FACTOR STUDIES						
	LOW	HIGH	MEAN	ST	MEAN	ST	N	SE	M	N	
1000	896	1039	967	0.84	0.71	4	0.87	0.39	2	1.85	4
2000	2029	2150	2089	3.12	0.04	4	3.16	0.08	2	3.70	4
4000	4323	4323	4323	0.59	0.05	2	0.63	0.01	1	0.64	2
8000	8450	8450	8450	1.82	1.82	1	1.82	0.00	1	1.82	1

OVERALL MEANS

ESTIMATED AT 10,000 PPMV 0.68

95% LOWER CONFIDENCE INTERVAL 0.54

DVA INSTRUMENTS

MINIMAL PPMV	ACTUAL PPMV		OVERALL		DISPERSED FACTOR STUDIES						
	LOW	HIGH	MEAN	ST	MEAN	ST	N	SE	M	N	
1000	896	1039	967	0.41	0.41	2	0.41	0.00	1	0.41	2
2000	2029	2150	2089	1.31	1.31	2	1.31	0.00	1	1.31	2
4000	4323	4323	4323	0.63	0.63	1	0.63	0.00	1	0.63	1
8000	8450	8450	8450	2.63	2.63	1	2.63	0.00	1	2.63	1

OVERALL MEANS

ESTIMATED AT 10,000 PPMV 0.43

95% LOWER CONFIDENCE INTERVAL 0.34

Figure 5-16

INSTRUMENT RESPONSE VS CONCENTRATION

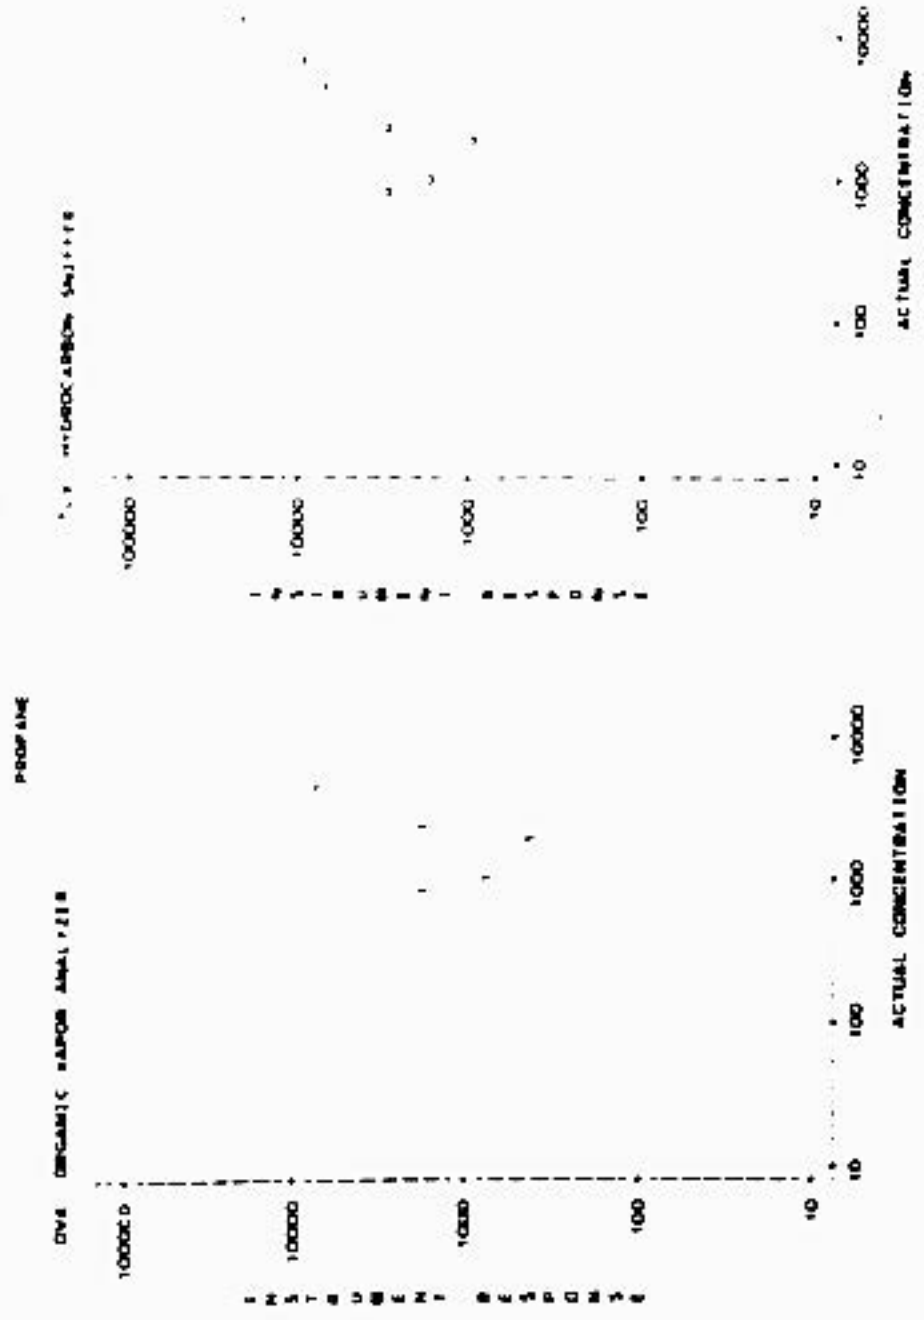


TABLE 5. 15a

DISPERSED FLYCATCHER SUMMARY

PROPORTIONAL DEFENSE

NOMINAL PPMV	ACTUAL PPMV			OVERALL			M I S P O N S E F A I I O M S											
	LOW	HIGH	MEAN	MEAN	SE	N	100U	SE	N	25U	SE	N	75U	SE	N			
400	223	223	223	2 40	0 00	2	1 48		1	1 48		1						
1500	1505	1505	1505	2 30	0 03	2	2 33		1	2 21		1						
8000	7888	8101	7884	1 20	0 05	2	1 24		1	1 15		1						
OVERALL MEANS							2 33	0 00	6	2 28	0 44	1	2 30	0 61	2			
ESTIMATED AT 10,000 PPMV							1 19	95% CONFIDENCE INTERVAL									1 11	1 30

FLY INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			M I S P O N S E F A I I O M S											
	LOW	HIGH	MEAN	MEAN	SE	N	100U	SE	N	25U	SE	N	75U	SE	N			
200	223	223	223	1 24	0 24	2	1 48		1	0 99		1						
1500	1505	1505	1505	1 95	0 31	2	2 22		1	1 54		1						
8000	7888	8101	7884	1 56	0 03	3	1 60		1	1 54	0 21	2						
OVERALL MEANS							1 58	0 03	7	1 80	0 26	2	1 41	0 14	4			
ESTIMATED AT 10,000 PPMV							1 65	95% CONFIDENCE INTERVAL									1 15	1 36

Figure 5-144  
 INSTRUMENT RESPONSE VS CONCENTRATION  
 PROPIONALDEHYDE

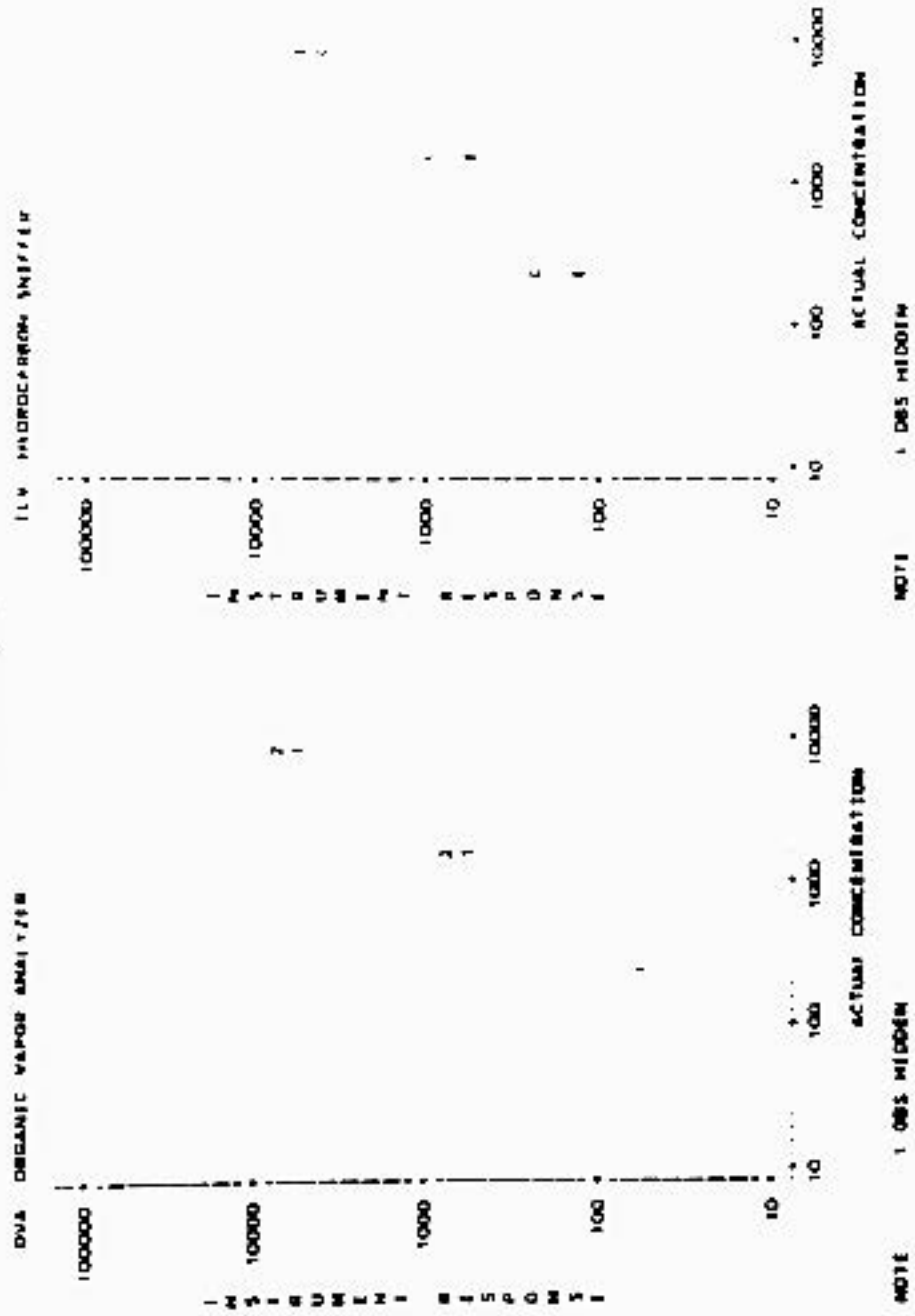




TABLE 2 (cont.)

RESPONSE FACTOR SUMMARY

PROPIONIC ACID

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			R F S P O N S E F A C T O R S									
	LOW	HIGH	MEAN	MEAN	SE	N	MEAN	SE	N	MEAN	SE	N	MEAN	SE	N	
200	212	212	212	220	0.23	2	2.01			2.48		1				
1500	1552	1552	1552	1.66	0.11	2	1.56			1.71		1				
2700	2903	2903	2903	1.62	0.08	2	1.52			1.71		1				
OVERALL MEANS			1.84	0.02	6	1.90	0.16	3	1.80	0.25	1					
ESTIMATED AT 10 000 PPMV			1.74	95% CONFIDENCE INTERVAL												

TIV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			R F S P O N S E F A C T O R S									
	LOW	HIGH	MEAN	MEAN	SE	N	MEAN	SE	N	MEAN	SE	N	MEAN	SE	N	
200	212	212	212	1.97	0.04	2				2.91		1				
1500	1552	1552	1552	2.05		1				2.05		1				
2700	2903	2903	2903	3.52	1.09	2				4.61		1				
OVERALL MEANS			2.60	0.19	5					3.79	0.85	1				
ESTIMATED AT 10 000 PPMV			3.51	95% CONFIDENCE INTERVAL												

Figure 3-165

ENVIRONMENT RESPONSE VS CONCENTRATION

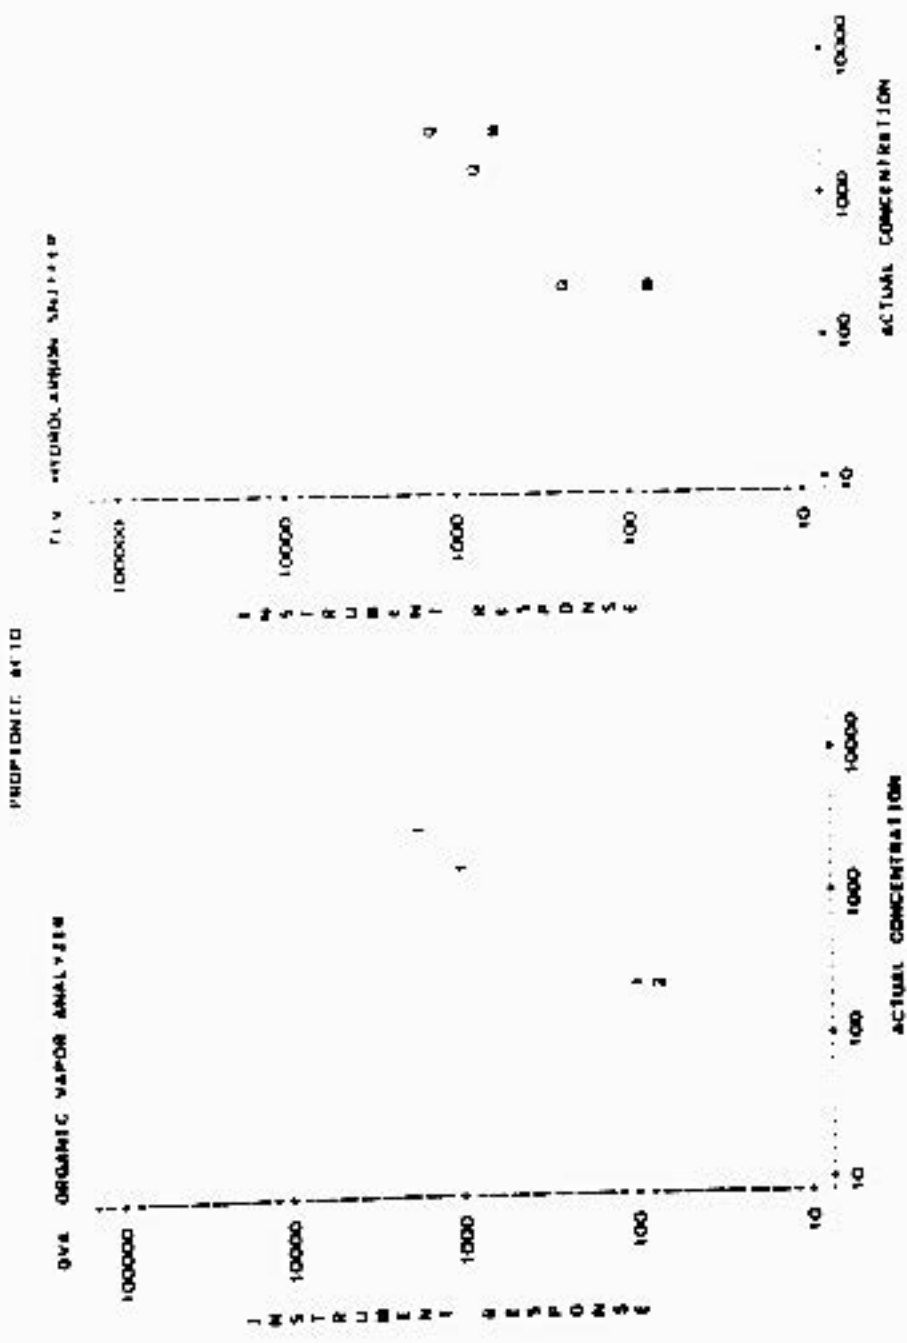


TABLE 5-144

RESPONSE RATING SUMMARY

PROPERTY ALCOHOL

DVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	SE	N	ST
200	201	201	201	0.12	2	2.36
1500	1538	1538	1538	0.06	2	1.19
8000	8487	8487	8487	0.03	2	0.88
	Overall MEANS			0.04	6	1.88
ESTIMATED AT 10,000 PPMV 0.91						

95% CONFIDENCE INTERVALS 1.12 1.91

TIV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	SE	N	ST
200	201	201	201	0.69	1	0.69
1500	1538	1538	1538	1.02	1	1.02
8000	8487	8487	8487	1.52	1	1.52
	Overall MEANS			1.08	3	1.08
ESTIMATED AT 10,000 PPMV 1.80						

95% CONFIDENCE INTERVALS 1.47 3.20

DVA METERS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	SE	N	ST
200	201	201	201	0.44	1	0.44
1500	1538	1538	1538	0.88	1	0.88
8000	8487	8487	8487	1.32	1	1.32
	Overall MEANS			1.12	3	1.12
ESTIMATED AT 10,000 PPMV 1.91						

95% CONFIDENCE INTERVALS 1.12 1.91


TIV METERS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	SE	N	ST
200	201	201	201	0.44	1	0.44
1500	1538	1538	1538	0.88	1	0.88
8000	8487	8487	8487	1.32	1	1.32
	Overall MEANS			1.12	3	1.12
ESTIMATED AT 10,000 PPMV 1.91						

95% CONFIDENCE INTERVALS 1.12 1.91

Figure 5-14b

INSTRUMENT RESPONSE VS CONCENTRATION

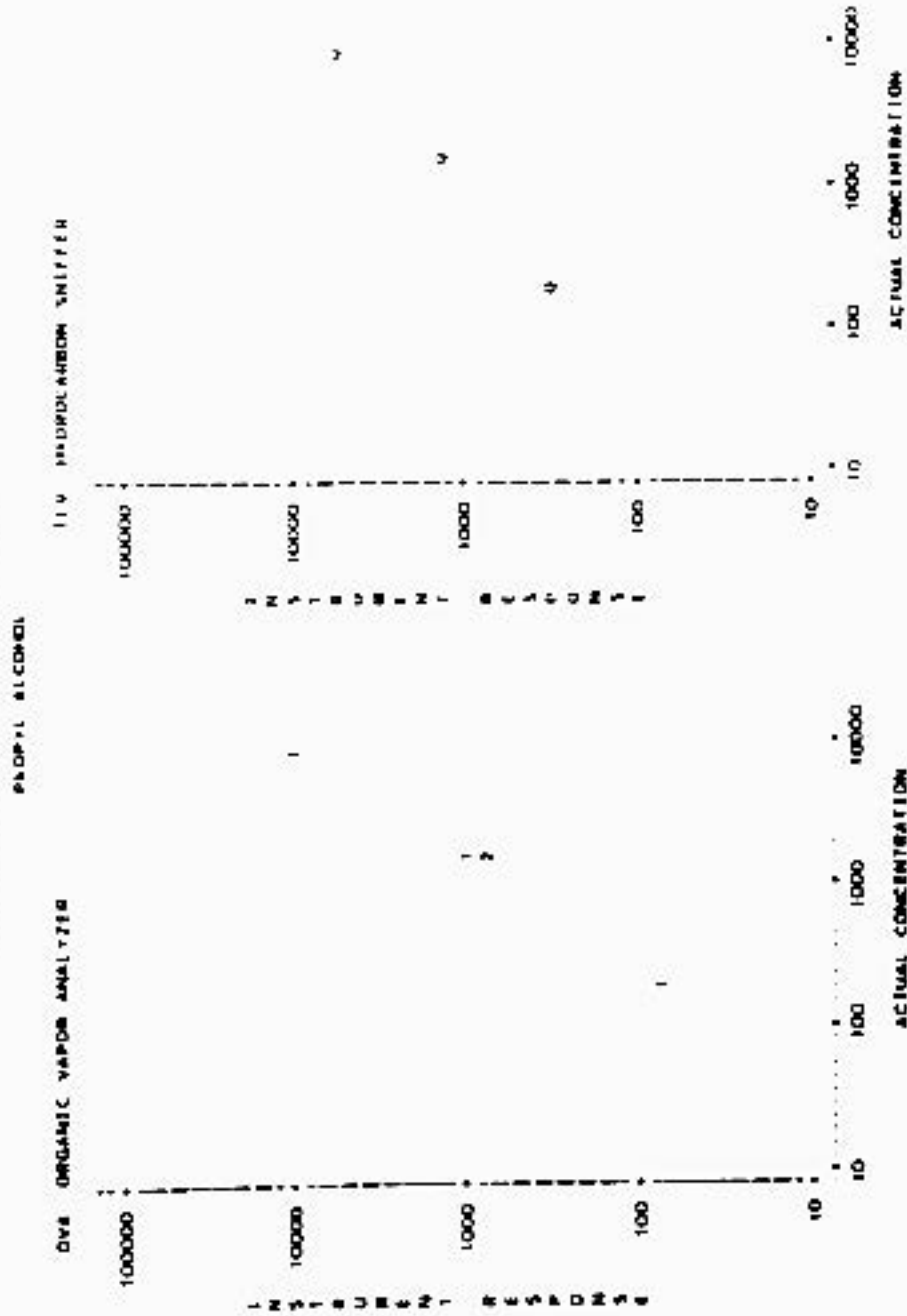

NOTE: 3 CBS HIGHWAY

TABLE 5.14.1

RESPONSE FACTOR SUMMARY

PROPELLANT M

IVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY						
	LOW	HIGH	MEAN	MEAN	SE	N	1000	50	25	10	5	1	0.1
200	217	217	217	1.03	0.08	2	0.98	1	1.11				
1500	1837	1837	1837	0.72	0.02	2	0.10	1	0.79				
8000	3243	3243	3243	0.95	0.04	2	0.93	1	0.96				
OVERALL MEANS						0.77	0.04	6	0.81	0.27	0.80	0.18	0
ESTIMATED AT 10,000 PPMV						0.64							
						95% CONFIDENCE INTERVAL							


FIV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTOR SUMMARY						
	LOW	HIGH	MEAN	MEAN	SE	N	20	10	5	2.5	1	0.5	0.1
200	217	217	217	1.97	0.08	2	2.98	1	1.18				
1500	1837	1837	1837	9.06	1.00	2	16.00	1	2.07				
8000	3243	3243	3243	10.64	0.15	2	31.03	1	1.85				
OVERALL MEANS						0.22	0.26	6	16.00	0.37	1.87	0.22	0
ESTIMATED AT 10,000 PPMV						5.97							
						95% CONFIDENCE INTERVAL							

FIGURE 5-147

INSTUMENT RESPONSE VS CONCENTRATION

PROPYLENEBENZENE M

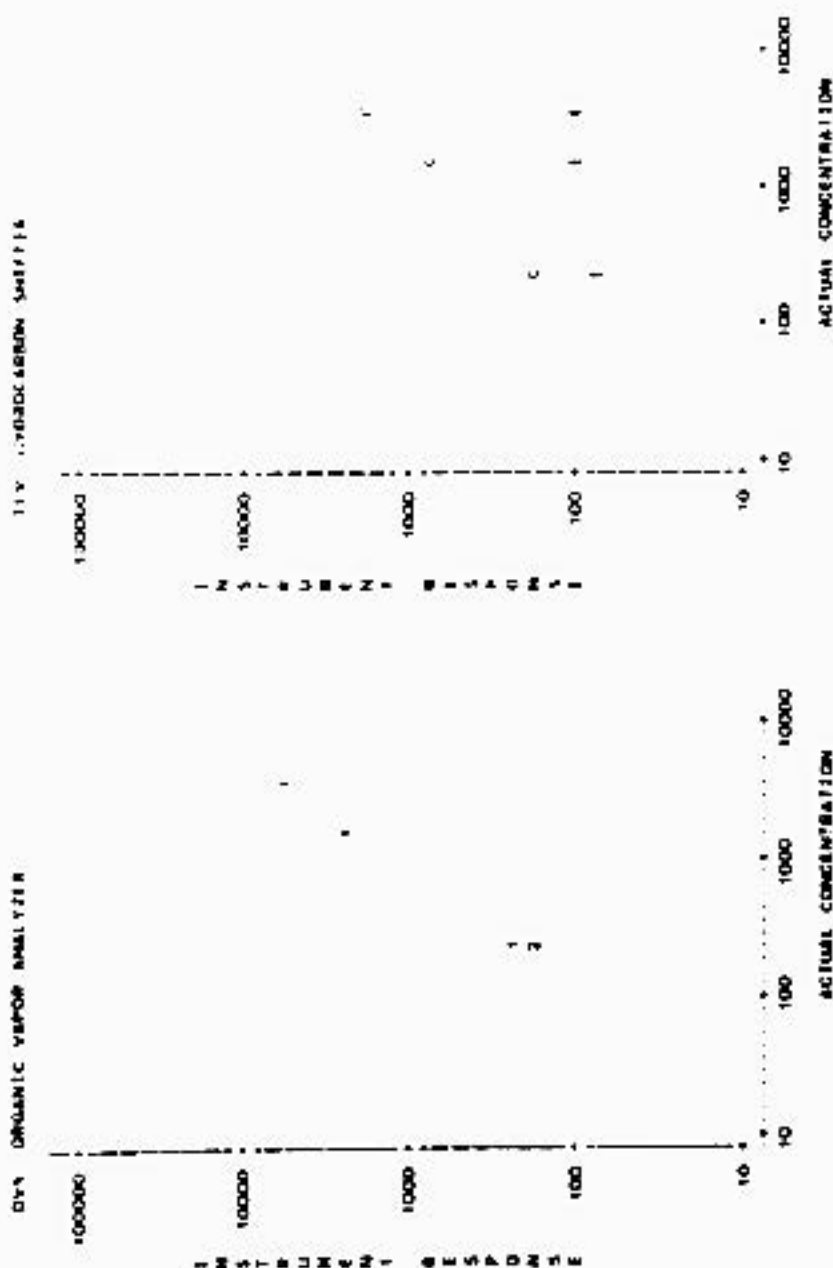

NOTE 2 OBS HIDDEN

TABLE 3.14M

RESPONSE FACTOR SUMMARY

PROBLEMS

UVA INSTRUMENTS

W P S P O N S E F A C T O R S

MINIMAL PPMV	ACTUAL PPMV		OVERALL		UVA METERS									
	LOW	HIGH	MEAN	SE	N	10000	SE	N	2100	SE	N	1010	SE	N
5000	0.33	5.37	0.33	0.00	0.92	2	0.00	1	0.57	1				
2000	2.19	2.19	2.19	1.00	0.00	2	1.00	1	1.12	1				
5000	4.48	4.48	4.48	0.47	0.00	2	0.47	1	0.85	1				
5000	0.00	0.00	0.00											

OVERALL MEANS OF THE DATA IS 0.17

ESTIMATED AT 10,000 PPMV IS 0.70

95% CONFIDENCE INTERVAL IS 0.19 TO 0.17

TLS INSTRUMENTS

W P S P O N S E F A C T O R S

MINIMAL PPMV	ACTUAL PPMV		OVERALL		TLS METERS									
	LOW	HIGH	MEAN	SE	N	20	SE	N	20	SE	N	20	SE	N
5000	5.37	5.37	5.37	0.50	0.47	2	0.47	1	1.44	1				
2000	2.19	2.19	2.19	2.07	1.18	2	2.07	1	0.93	1				
5000	4.48	4.48	4.48	2.72	2.30	2	2.72	1	1.33	1				
5000	0.00	0.00	0.00	1.00	3.40	2	1.00	1	1.44	1				


OVERALL MEANS OF THE DATA IS 0.23

ESTIMATED AT 10,000 PPMV IS 0.80

95% CONFIDENCE INTERVAL IS 0.06 TO 0.40

Figure 5-148

INSTRUMENT RESPONSE VS CONCENTRATION

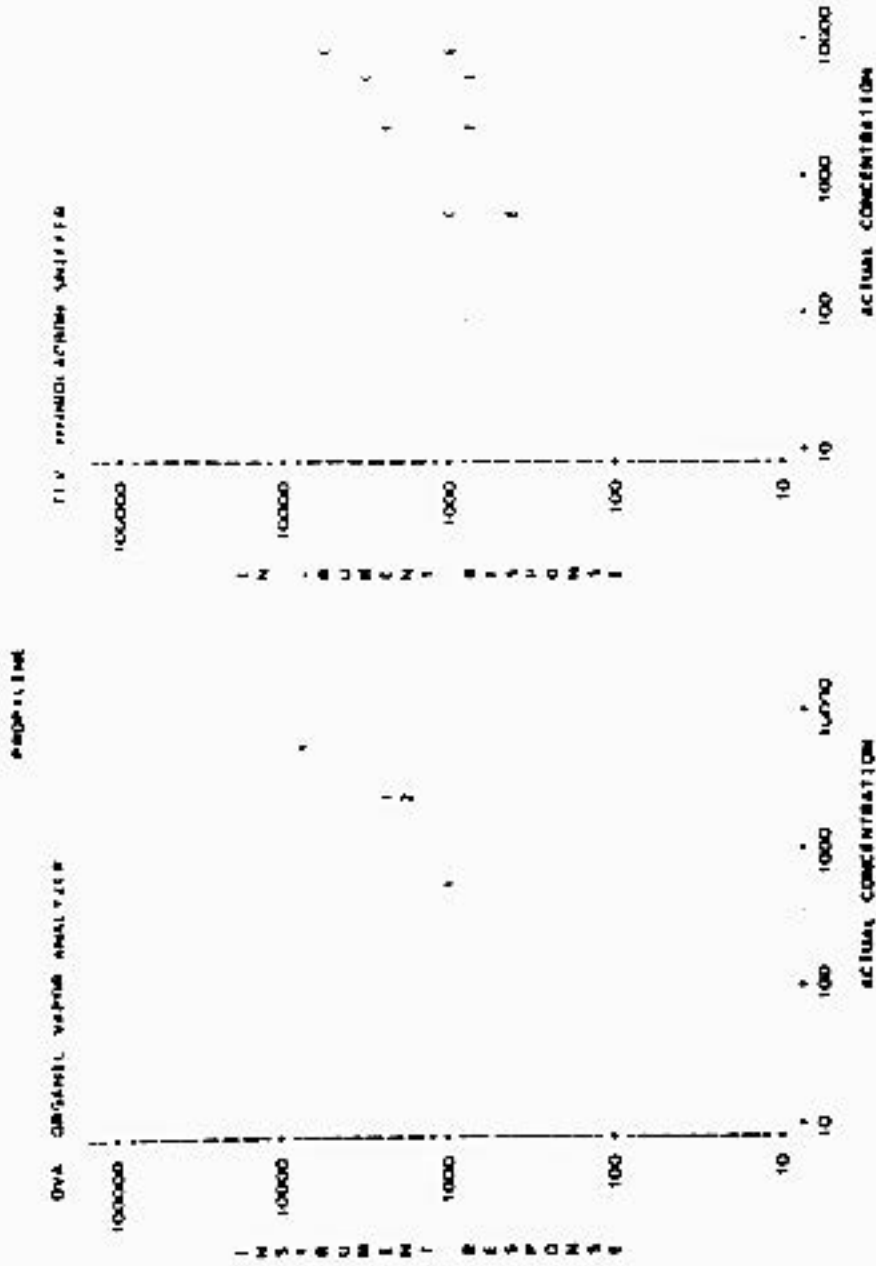

NOTE: 3 OBS. HIDDEN



TABLE 5.149

RESPONSE FACTOR SUMMARY

PROPYLENE OXIDE

DVA INSTRUMENTS

D E S I G N S I - E - I D R S

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DVA METERS							
	LOW	HIGH	MEAN	SE	10000	5000	2500	500	100	10	N	
200	227	227	227	1.59	0.15	2	1	1	1	1	1	1
1000	1467	1467	1467	1.26	0.03	2	1	1	1	1	1	1
10000	8558	8558	8558	0.89	0.04	2	1	1	1	1	1	1
80000	7633	7633	7633	0.78		1	1	1	1	1	1	1

OVERALL MEANS 1.17 0.01 1.28 0.24 1.41 0.54

ESTIMATED 95 TO 99% PPMV 0.80

95% CONFIDENCE INTERVAL 1.00 0.00 0.93

DVA INSTRUMENTS

D E S I G N S I - F - I D R S

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DVA METERS							
	LOW	HIGH	MEAN	SE	10000	5000	2500	500	100	10	N	
200	227	227	227	1.60	0.05	2	1	1	1	1	1	1
1000	1467	1467	1467	1.09	0.25	2	1	1	1	1	1	1
10000	8558	8558	8558	0.78		1	1	1	1	1	1	1
80000	7633	7633	7633	0.79	0.12	2	1	1	1	1	1	1

OVERALL MEANS 1.28 0.04

ESTIMATED 95 TO 99% PPMV 1.10

95% CONFIDENCE INTERVAL 1.00 0.00 0.93


Figure 5-149

INSTRUMENT RESPONSE VS. CONCENTRATION

PREPILAME DATA

FLY HYDROCARBON ANALYSIS

DATA ORGANIC VAPOR ANALYSIS

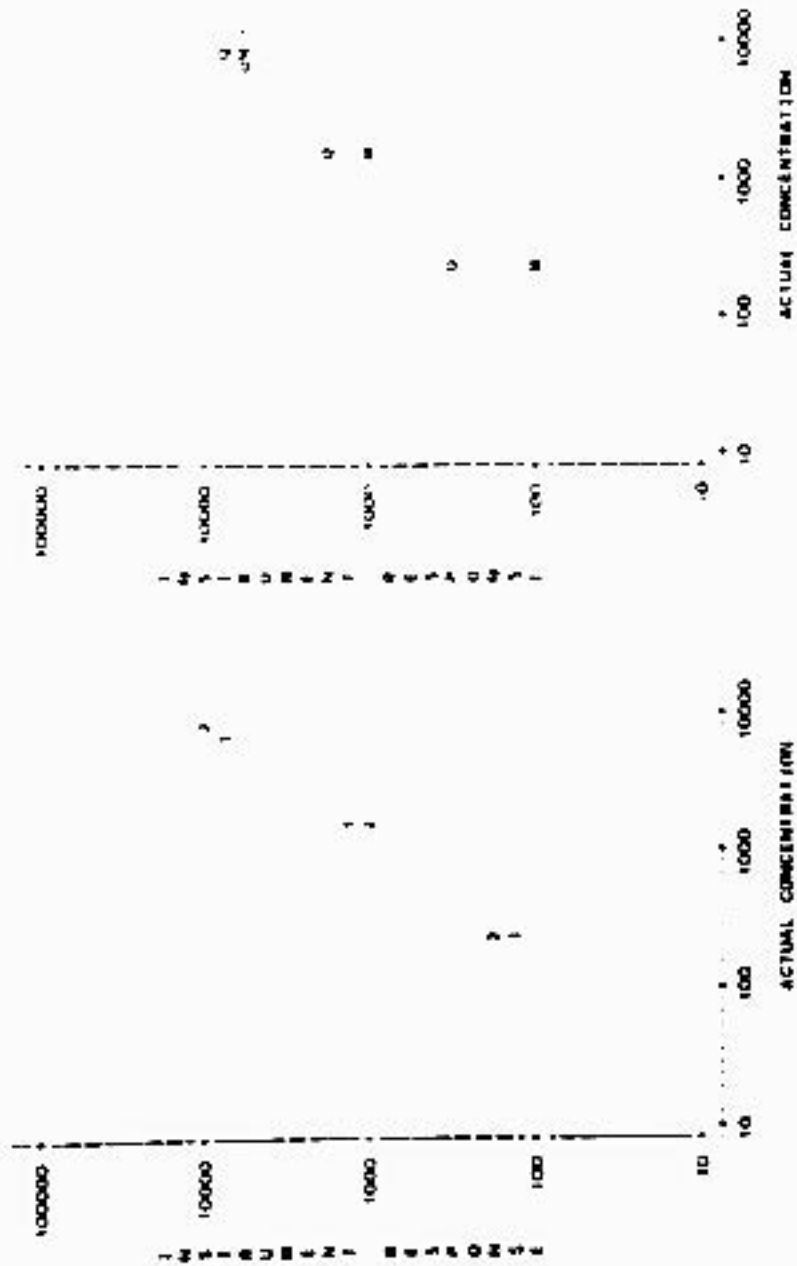

NOTE: OBS. HIDDEN

TABLE 5-150

RESPONSE FACTOR SUMMARY

PROBING

OVA INSTRUMENTS

0 4 5 P D N S T P A C T O M S

NOMINAL PPMV	ACTUAL PPMV			OVERALL			OVA METERS									
	LOW	HIGH	MEAN	MEAN	SE	N	1100	SE	N	2204	SE	N	2100	SE	N	
200	226	226	226	0.73	0.04	2	0.70		1	0.71		1				
1000	1308	1308	1308	0.84	0.05	2	0.84		1	0.84		1				
4000	4070	4070	4070	0.48	0.03	2	0.44		1	0.48		1				
8000	8078	8078	8078													
8000	8078	8078	8078													

OVERALL MEANS 0.61 0.00 4 0.59 0.00 2 0.87 0.00 2

ESTIMATED AT 10 0000 PPMV 0.41

95 % CONFIDENCE INTERVAL 1.0 0.0 0.512

11V INSTRUMENTS

NOMINAL PPMV

0 1 5 P D N S T P A C T O M S

NOMINAL PPMV	ACTUAL PPMV			OVERALL			11V METERS								
	1.0P	10.0P	MEAN	MEAN	SE	N	71	SE	N	71	SE	N	74	SE	N
200	226	226	226	1.17	0.14	2							1.41		1
1000	1308	1308	1308	1.34	0.16	2							1.52		1
4000	4070	4070	4070	1.20	0.04	2							1.27		1
5000	5088	5088	5088	1.17	0.03	2							1.25		1
6000	5812	5812	5812	1.18	0.03	2							1.21		1
8000	8078	8078	8078	1.12	0.03	2							1.18		1

OVERALL MEANS 1.20 0.01 12

ESTIMATED AT 10 0000 PPMV 1.17

95 % CONFIDENCE INTERVAL 1.1 0.1 1.871

FIGURE 5-15D  
 INSTRUMENT RESPONSE VS CONCENTRATION  
 PYRIDINE

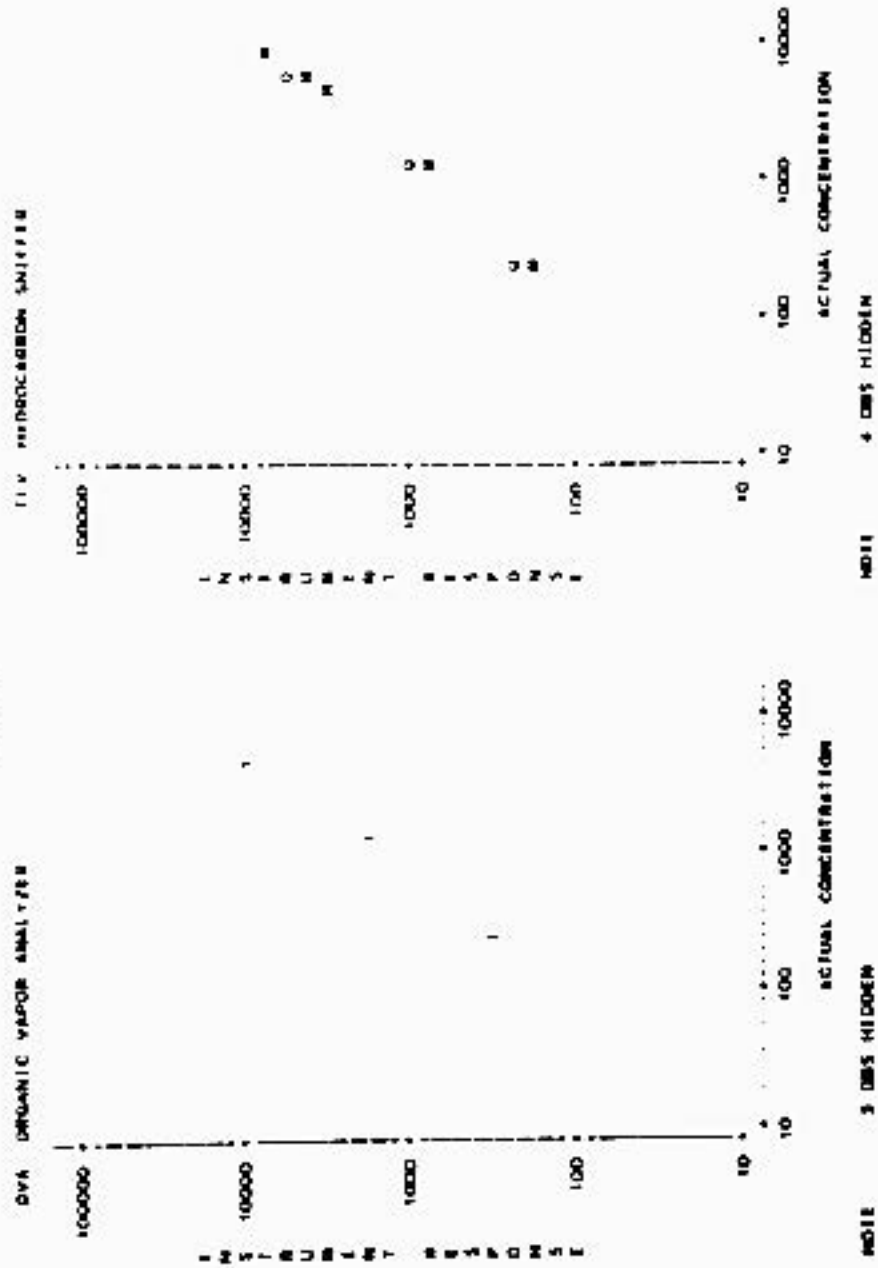


TABLE 5.151

RESPONSE FACTOR SUMMARY

SYSTEM

DVA INSTRUMENTS

W E S P O N S E F A C T O R S

NOMINAL PIPE	ACTUAL PPMV				OVERALL				DVA METERS					
	LOW	HIGH	MEAN	SE	SE	SE	SE	SE	SE	SE	SE	SE	SE	
200	212	212	212	4.14	0.28	1	2.88	1	4.42	1	4.42	1	4.42	
1500	1471	1471	1471	3.87	0.18	1	3.71	1	4.13	1	4.13	1	4.13	
8000	8889	8889	8889	4.28	0.09	1	4.24	1	4.35	1	4.35	1	4.35	
OVERALL MEANS				4.10	0.17	8	3.84	0.14	3	4.28	0.12	3	4.28	0.12

ESTIMATED AT 10 000 PPMV 4.10

95 % CONFIDENCE INTERVAL 3.88 4.11

LIV INSTRUMENTS

W E S P O N S E F A C T O R S

NOMINAL PIPE	ACTUAL PPMV				OVERALL				LIV METERS					
	LOW	HIGH	MEAN	SE	SE	SE	SE	SE	SE	SE	SE	SE	SE	
200	212	212	212	5.12	1.09	2	8.21	1	4.03	1	4.03	1	4.03	
1500	1471	1471	1471	16.22	3.98	2	20.30	1	12.33	1	12.33	1	12.33	
8000	8889	8889	8889	116.7	103.2	2	218.2	1	14.74	1	14.74	1	14.74	
OVERALL MEANS				48.04	9.98	4	81.23	4.88	3	111.16	9.24	3	111.16	9.24

ESTIMATED AT 10 000 PPMV 48.04

95 % CONFIDENCE INTERVAL 11.12 185.81

Figure 3-151  
 INSTRUMENT RESPONSE VS CONCENTRATION

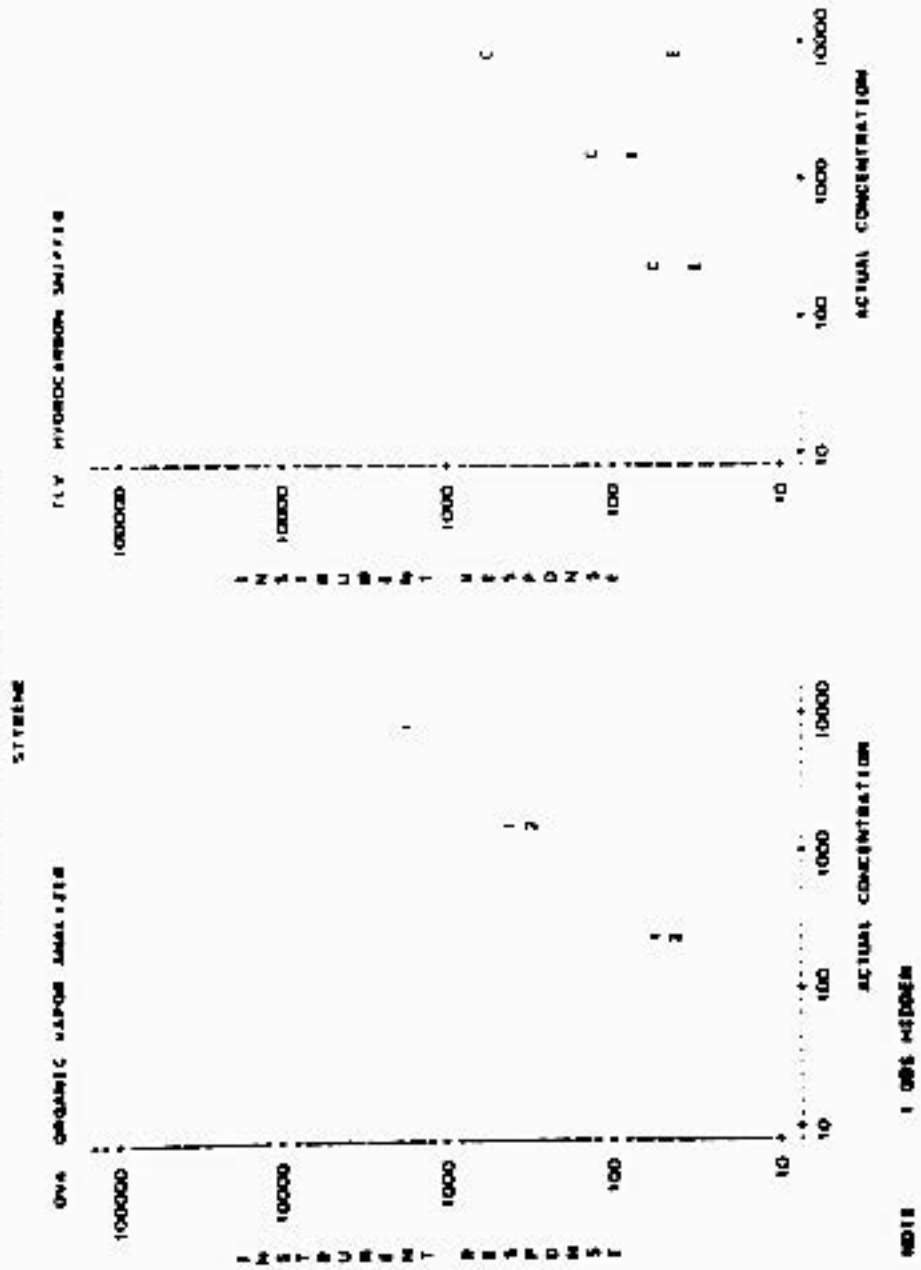


TABLE 5. 152

RESIDENCE FACILITY SUMMARY

PERMITS/INSTRUMENTS 1 1 1 2

OVA INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	MEAN	SE	N
200	228	227	227	1.32	0.01	4
1000	1123	1123	1123	2.41	0.10	2
1800	1487	1487	1487	2.48	0.02	2
8000	7835	7835	7835	2.82	0.08	2

OVERALL MEANS 2.03 0.10 10 2.06 0.41 5 2.01 0.29 5

ESTIMATED AT 10 000 PPMV 3.00

95 % CONFIDENCE INTERVAL 1.27 1.011

RESIDENCE FACILITY

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	MEAN	SE	N
200	228	227	227	1.32	0.01	4
1000	1123	1123	1123	2.41	0.10	2
1800	1487	1487	1487	2.48	0.02	2
8000	7835	7835	7835	2.82	0.08	2

FLV INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV			OVERALL		
	LOW	HIGH	MEAN	MEAN	SE	N
200	228	227	227	7.53	2.62	4
1000	1123	1123	1123	5.11	0.88	2
1500	1487	1487	1487	4.82	0.26	2
8000	7835	7835	7835	8.91	0.06	2

OVERALL MEANS 6.86 0.12 10 6.11 1.09 5 5.81 0.86 5

ESTIMATED AT 10 000 PPMV 6.92

95 % CONFIDENCE INTERVAL 3.82 11.911

Figure 5-152

INSTRUMENT RESPONSE VS CONCENTRATION

TETRAACHLOROETHANE 1 1 1 2

OVA ORGANIC VAPOR ANALYZER

FID HYDROCARBON ANALYZER

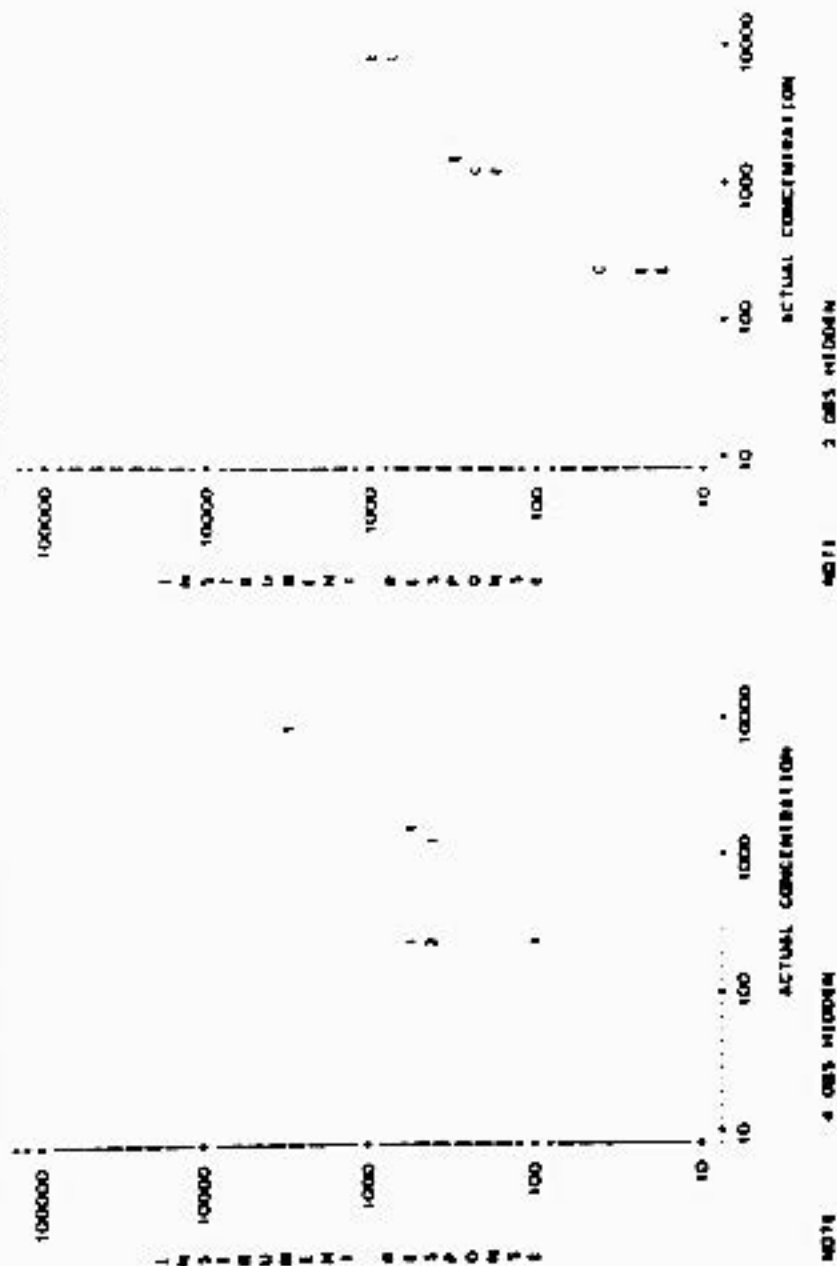






Figure 5-153

INSTRUMENT RESPONSE VS CONCENTRATION

1,1,1-TRICHLOROETHANE 1,1,1,2,2,2

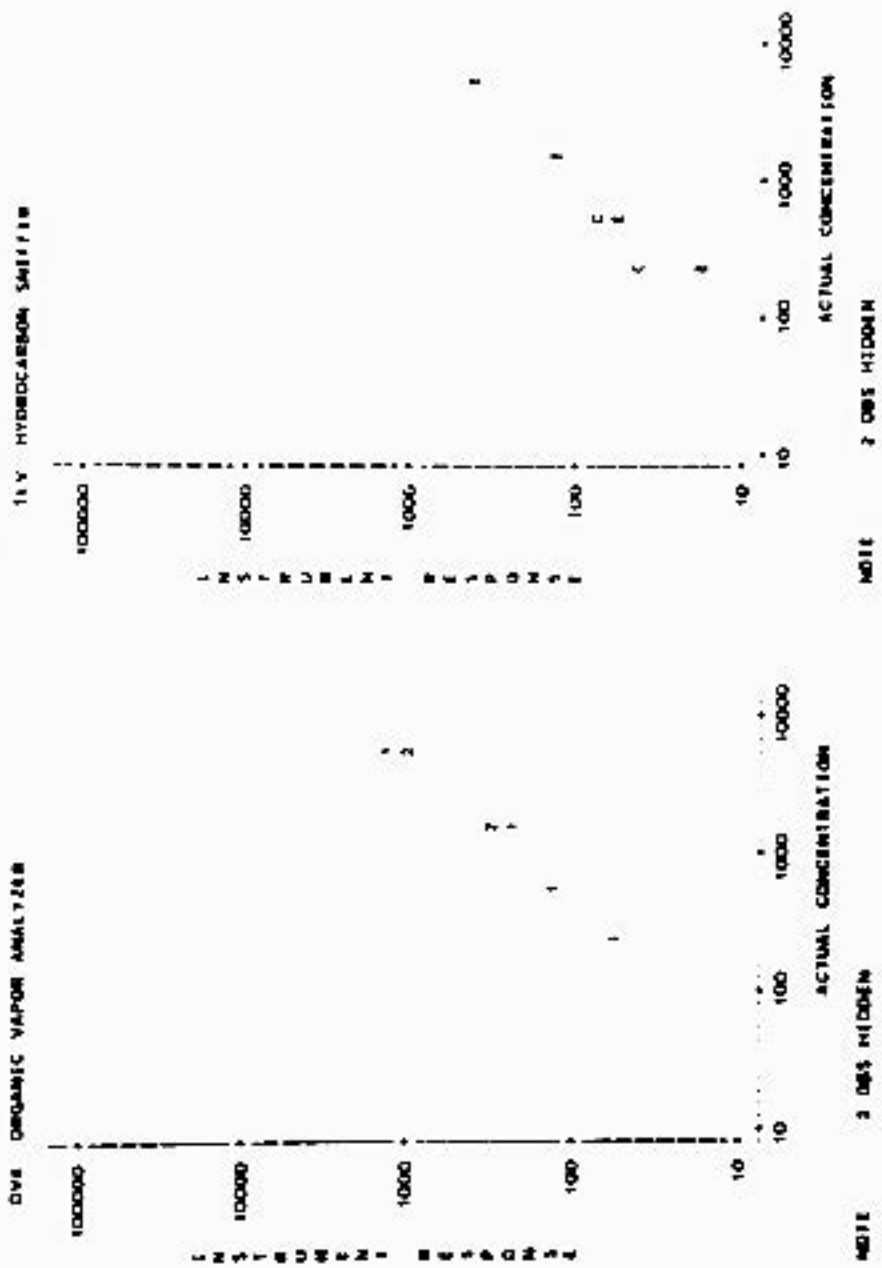


TABLE 3. 154

RESPONSE FACTOR SUMMARY

TERMINAL DOSE INTERVAL

DVA INSTRUMENTS	ACTUAL PPMV			OVERALL			RESPONSE FACTORS									
	LOW	HIGH	MEAN	MEAN	SE	N	1000	SE	N	2200	SE	N	1000	SE	N	
SCHEMATA																
PPMV																
50	23	42	48	8.20	0.43	7	6.29	0.40	2	9.92	1.70	4				
500	526	948	540	2.28	0.48	8	2.84	2.17	4	4.92	1.10	4				
5000	5371	5371	5371	1.23	0.00	2	1.73		1	1.34		1				
8000	8283	8888	8545	7.25	1.28	5	8.07	2.88	5	6.19	1.91	5				
				OVERALL MEANS	8.21	0.03	26	1.38	1.46	12	8.98	0.91	14			
				ESTIMATED AT 10 000 PPMV	3.18											

95% CONFIDENCE INTERVAL 1.5 92 8.217

11V INSTRUMENTS


NOMINAL PPMV	ACTUAL PPMV			OVERALL			RESPONSE FACTORS									
	LOW	HIGH	MEAN	MEAN	SE	N	78	SE	N	11	SE	N	200	SE	N	
50	23	42	48	1.94	0.28	7	2.21	0.44	4	1.62	0.27	2				
500	526	948	540	8.87	0.80	8	8.27	1.40	4	8.27	1.58	4				
5000	5371	5371	5371	8.17	0.02	2	8.19		1	8.15		1				
8000	8283	8888	8545	10.85	0.81	5	11.21	1.29	5	10.27	1.86	4				
				OVERALL MEANS	7.84	0.01	26	1.93	1.20	14	7.81	1.23	12			
				ESTIMATED AT 10 000 PPMV	11.48											

95% CONFIDENCE INTERVAL 1.8 04 15.201

FIGURE 5-15A

ENVIRONMENT RESPONSE VS CONCENTRATION

TETRACHLOROETHYLENE

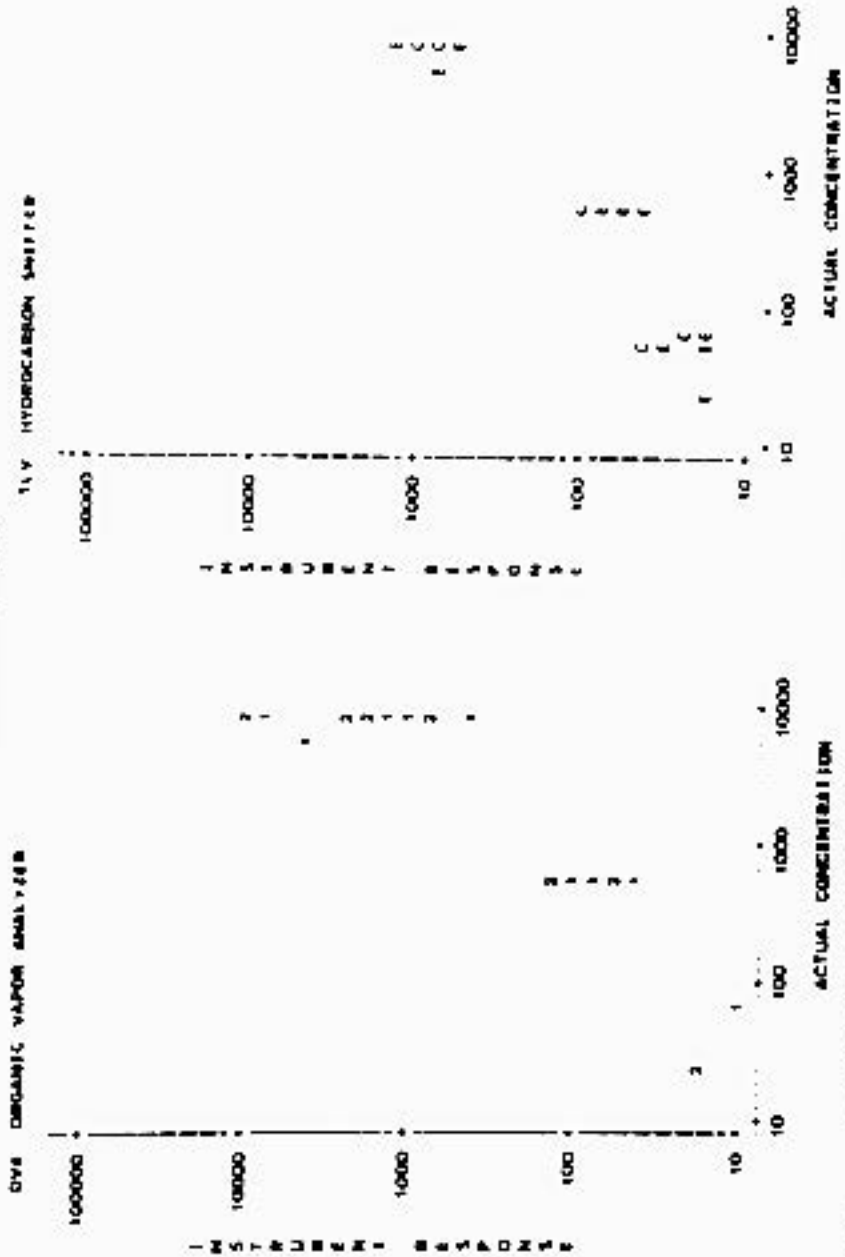

NOTE 4 OBS MISSING OR OUT OF RANGE

NOTE 11 OBS MISSING

TABLE 1.15

RESPONSE FACTOR SUMMARY

FOR USE

OVA INSTRUMENTS		RESPONSE FACTOR FACTORS											
NOMINAL PPMV	ACTUAL PPMV	OVERALL					OVA MEANS						
		LOW	HIGH	MEAN	ST	SE	1000	50	25	10	5		
2000	192	192	192	0.87	0.02	2	0.45	1	0.44	1			
1500	1824	1824	1824	0.49	0.02	2	0.48	1	0.51	1			
3000	3285	3285	3285	0.39	0.02	2	0.38	1	0.44	1			
4000	4344	4344	4344										
8000	7830	7830	7830										

OVERALL MEANS: 0.81 0.02 0.49 0.02 0.45 0.02 0.44 0.02

ESTIMATED AT 10,000 PPMV: 0.33 0.33 0.33 0.33 0.33 0.33 0.33 0.33

FOR INSTRUMENTS

ACTUAL PPMV		RESPONSE FACTOR FACTORS											
NOMINAL PPMV	LOW	HIGH	MEAN	OVERALL					OVA MEANS				
				ST	SE	1000	50	25	10	5			
2000	192	192	192	2.04	0.05	2	1.00	1	1.10	1			
1500	1824	1824	1824	4.49	0.08	2	0.97	1	2.04	1			
3000	3285	3285	3285	1.29		1		1	1.29	1			
4000	4344	4344	4344	4.72	0.43	2	0.15	1	1.29	1			
8000	7830	7830	7830	5.33	0.94	2	0.24	1	1.44	1			


OVERALL MEANS: 3.03 0.30 0.49 0.36 0.42 0.36 0.42

ESTIMATED AT 10,000 PPMV: 1.32 0.32 0.32 0.32 0.32 0.32 0.32 0.32

FIGURE 5-153

INSTRUMENT RESPONSE VS CONCENTRATION

EDURENE

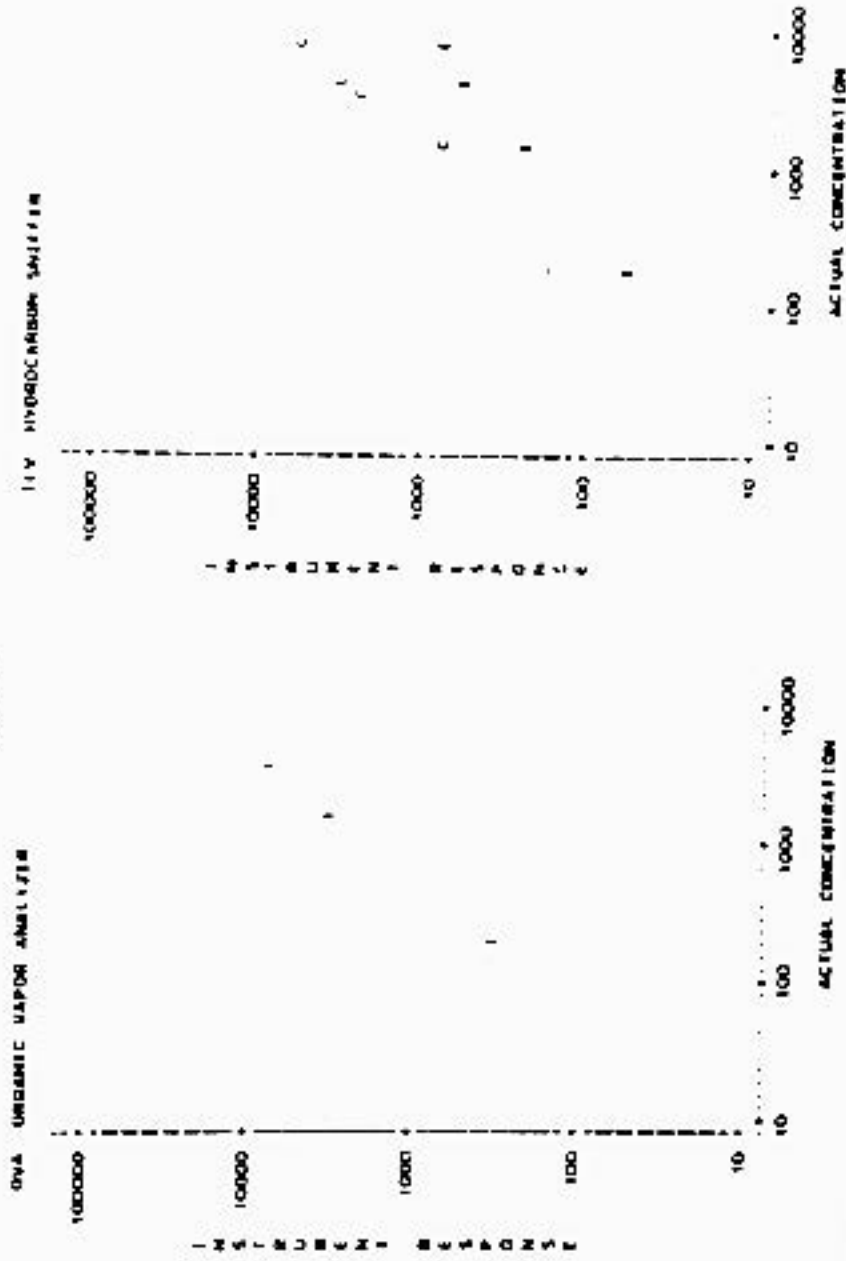

NOTE: 2 OBS. HIGHEN

TABLE 5.15b

RESPONSE FACTOR SUMMARY

TRICHLOROBENZENE - 7.4

OVA INSTALLMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL	
	LOW	HIGH	MEAN	SE
200	208	208	1.41	1
400	588	588	1.08	1
1000	878	878	1.85	1
OVERALL MEANS			1.20	3

ESTIMATED AT 10,000 PPMV = 15

95% CONFIDENCE INTERVAL = 0.13-14.0011

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV		OVERALL	
	LOW	HIGH	MEAN	SE
200	208	208	1.41	1
400	588	588	1.08	1
1000	878	878	1.85	1
OVERALL MEANS			1.20	3

TUV INSTALLMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL	
	LOW	HIGH	MEAN	SE
200	208	208	1.07	1
400	588	588	0.70	1
1000	878	878	0.37	1
OVERALL MEANS			0.84	3

ESTIMATED AT 10,000 PPMV = 30

95% CONFIDENCE INTERVAL = 0.40-1.571

RESPONSE FACTORS

NOMINAL PPMV	ACTUAL PPMV		OVERALL	
	LOW	HIGH	MEAN	SE
200	208	208	1.07	1
400	588	588	0.70	1
1000	878	878	0.37	1
OVERALL MEANS			0.84	3

Figure 5-156

INSTRUMENT RESPONSE VS CONCENTRATION

TELECHEMICALS INC. 1.2.4.

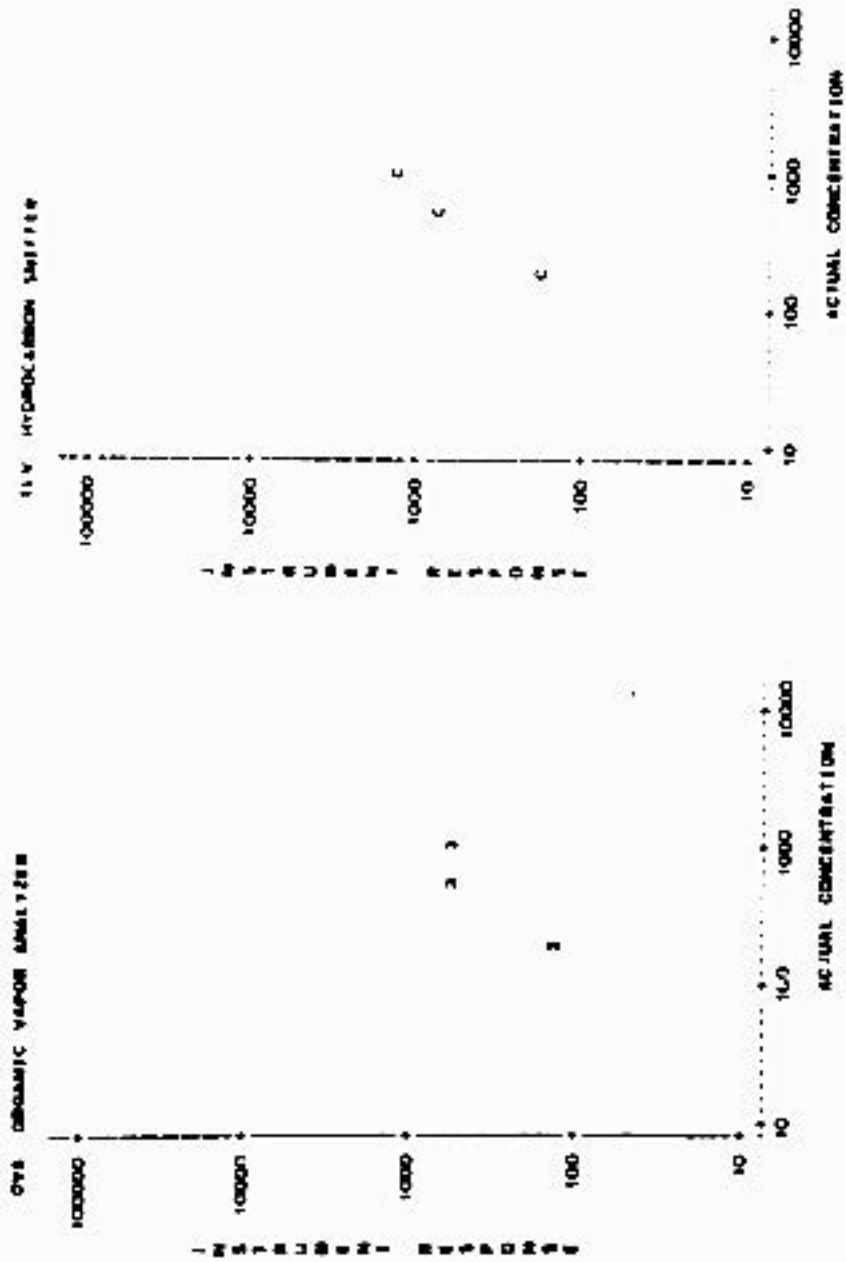




TABLE 5.25

RESPONSE FACTOR SUMMARY

TELECOMMUNICATIONS

DATA INSTRUMENTS

MEMBER	ACTUAL PPMV		OVERALL		95% CONFIDENCE INTERVAL									
	LOW	HIGH	MEAN	SE	1	2	3	4	5	6	7	8	9	10
JOKO	218	218	1.11	0.05	2	1.08	1	1.16	1	1.02	1	1.12	1	1.04
18KO	1380	1380	0.98	0.08	2	0.87	1	1.02	1	0.82	1	1.02	1	0.82
80KO	2708	2708	0.83	0.13	2	0.70	1	0.92	1	0.62	1	0.82	1	0.62
OVERALL MEANS		0.97	0.07	6	0.81	0.68	1	0.91	1	0.70	1	0.81	1	0.70

ESTIMATED AT 10,000 PPMV 0.70

DATA INSTRUMENTS

MEMBER	ACTUAL PPMV		OVERALL		95% CONFIDENCE INTERVAL									
	LOW	HIGH	MEAN	SE	1	2	3	4	5	6	7	8	9	10
JOKO	218	218	2.02	0.17	2	2.00	1	2.18	1	1.86	1	2.10	1	1.86
18KO	1380	1380	2.37	0.17	2	2.54	1	2.20	1	2.41	1	2.41	1	2.41
80KO	2708	2708	2.47	0.08	2	2.53	1	2.41	1	2.41	1	2.41	1	2.41
OVERALL MEANS		2.46	0.08	6	2.68	0.72	1	2.28	1	2.28	1	2.28	1	2.28

ESTIMATED AT 10,000 PPMV 2.47

Figure 5-33

INSTRUMENT RESPONSE VS. CONCENTRATION

TRICHLOROETHANE

OV4 ORGANIC VAPOR ANALYZER

F1V HYDROCARBON ANALYZER

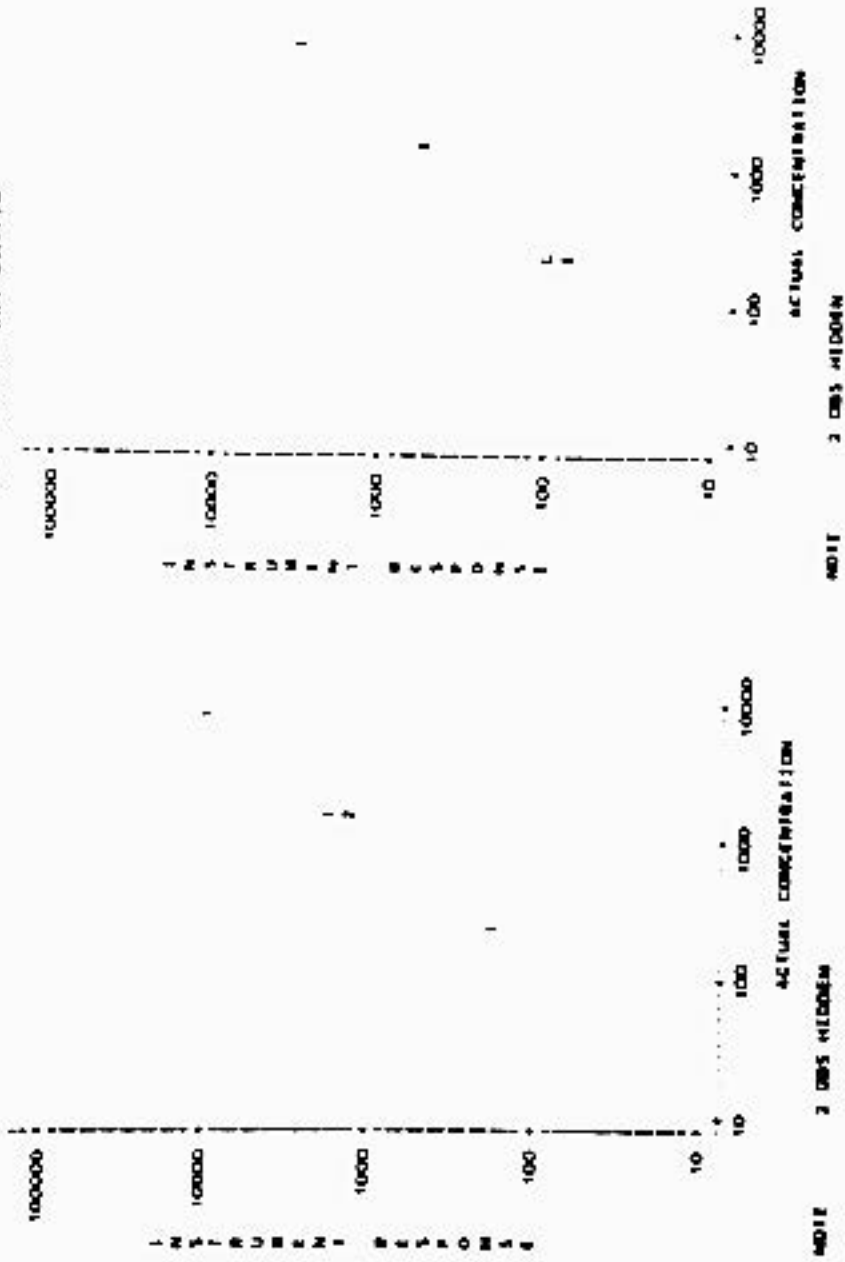


TABLE 5. 111

of surface water samples

1970-1971

ACTUAL DATA

NOMINAL PPMV	ACTUAL PPMV		OVERALL	
	LOW	HIGH	MEAN	SE
200	220	220	1.80	0.18
1500	1410	1410	1.82	0.11
8000	7817	7817	3.28	0.05
OVERALL MEANS	1.44	0.02	1.44	0.02

ESTIMATED AT 10,000 PPMV = 24

ESTIMATED DATA

NOMINAL PPMV	ACTUAL PPMV		OVERALL	
	LOW	HIGH	MEAN	SE
200	220	220	3.75	0.48
1500	1410	1410	3.61	0.28
8000	7817	7817	3.28	0.05
OVERALL MEANS	3.70	0.06	3.70	0.06

ESTIMATED AT 10,000 PPMV = 68

W E S P O N S E I N T E R V A L S

DATA MEANS

W	E	S	P	O	N	S	E	I	N	T	E	R	V	A	L	S
200	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1
1500	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1
8000	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1
OVERALL MEANS	1.34	0.08	1.34	0.08	1.34	0.08	1.34	0.08	1.34	0.08	1.34	0.08	1.34	0.08	1.34	0.08

95% CONFIDENCE INTERVAL = 1.08 - 1.61

W E S P O N S E I N T E R V A L S

DATA MEANS

W	E	S	P	O	N	S	E	I	N	T	E	R	V	A	L	S
200	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1
1500	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1
8000	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1
OVERALL MEANS	3.98	0.11	3.98	0.11	3.98	0.11	3.98	0.11	3.98	0.11	3.98	0.11	3.98	0.11	3.98	0.11

95% CONFIDENCE INTERVAL = 1.175 - 6.821


Figure 3-15A

INSTRUMENT RESPONSE VS CONCENTRATION

TRICHLOROETHANE 1,1,2

DVA ORGANIC VAPOR ANALYZER

14V HYDROGEN FLAME IONIZATION

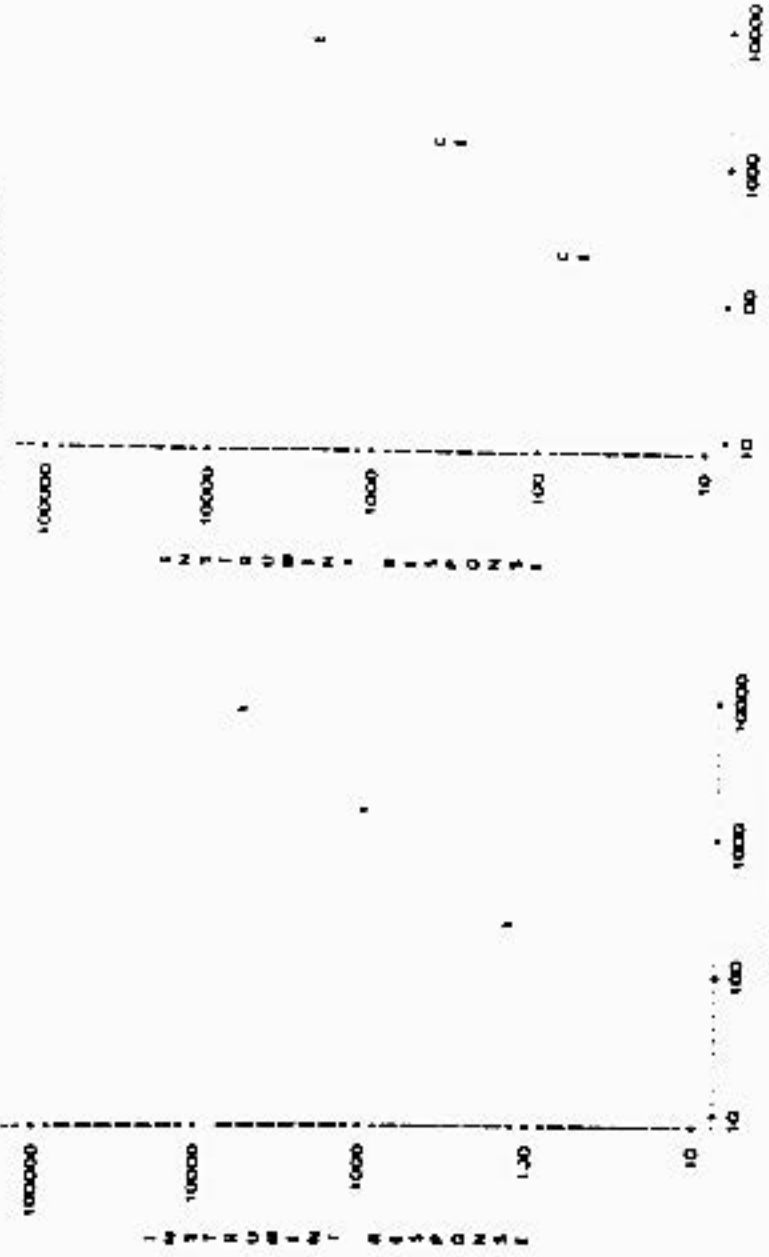

NOTE 3 OBS HIDDEN

NOTE 1 OBS HIDDEN

TABLE 3-154

RESPONSE FACTOR SUMMARS

TRICHLOROETHYLENE

DVB INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		R E S P O N S E F A C T O R S														
	LOW	HIGH	MEAN	SE	N	1000	SE	N	2000	SE	N	2100	SE	N	2110	SE	N		
200	206	206	206	1.87	0.08	2	1.78	1	1.90	1	1.88	1	1.88	1	1.88	1	1.88	1	
1500	1548	1548	1548	1.93	0.09	2	1.88	1	1.88	1	1.88	1	1.88	1	1.88	1	1.88	1	
8000	7987	7987	7987	0.94	0.04	2	0.80	1	1.01	1	1.01	1	1.01	1	1.01	1	1.01	1	
OVERALL MEANS			1.41	0.03	6	1.20	0.20	3	1.88	0.28	3	1.88	0.28	3	1.88	0.28	3	1.88	0.28

ESTIMATED AT 10,000 PPMV 0.94

95% CONFIDENCE INTERVALS 1.01 1.50

DVB INSTRUMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		R E S P O N S E F A C T O R S														
	LOW	HIGH	MEAN	SE	N	78	SE	N	76	SE	N	76	SE	N	76	SE	N		
200	206	206	206	2.18	0.40	2	2.58	1	1.78	1	1.78	1	1.78	1	1.78	1	1.78	1	
1500	1548	1548	1548	2.73	0.10	2	2.83	1	2.03	1	2.03	1	2.03	1	2.03	1	2.03	1	
8000	7987	7987	7987	3.28	0.04	2	3.11	1	3.26	1	3.26	1	3.26	1	3.26	1	3.26	1	
OVERALL MEANS			2.73	0.03	6	2.87	0.22	3	2.58	0.42	3	2.58	0.42	3	2.58	0.42	3	2.58	0.42

ESTIMATED AT 10,000 PPMV 3.35

95% CONFIDENCE INTERVALS 2.68 4.10

Figure 5-159

INSTRUMENT RESPONSE VS. CONCENTRATION

TRICHLOROETHYLENE

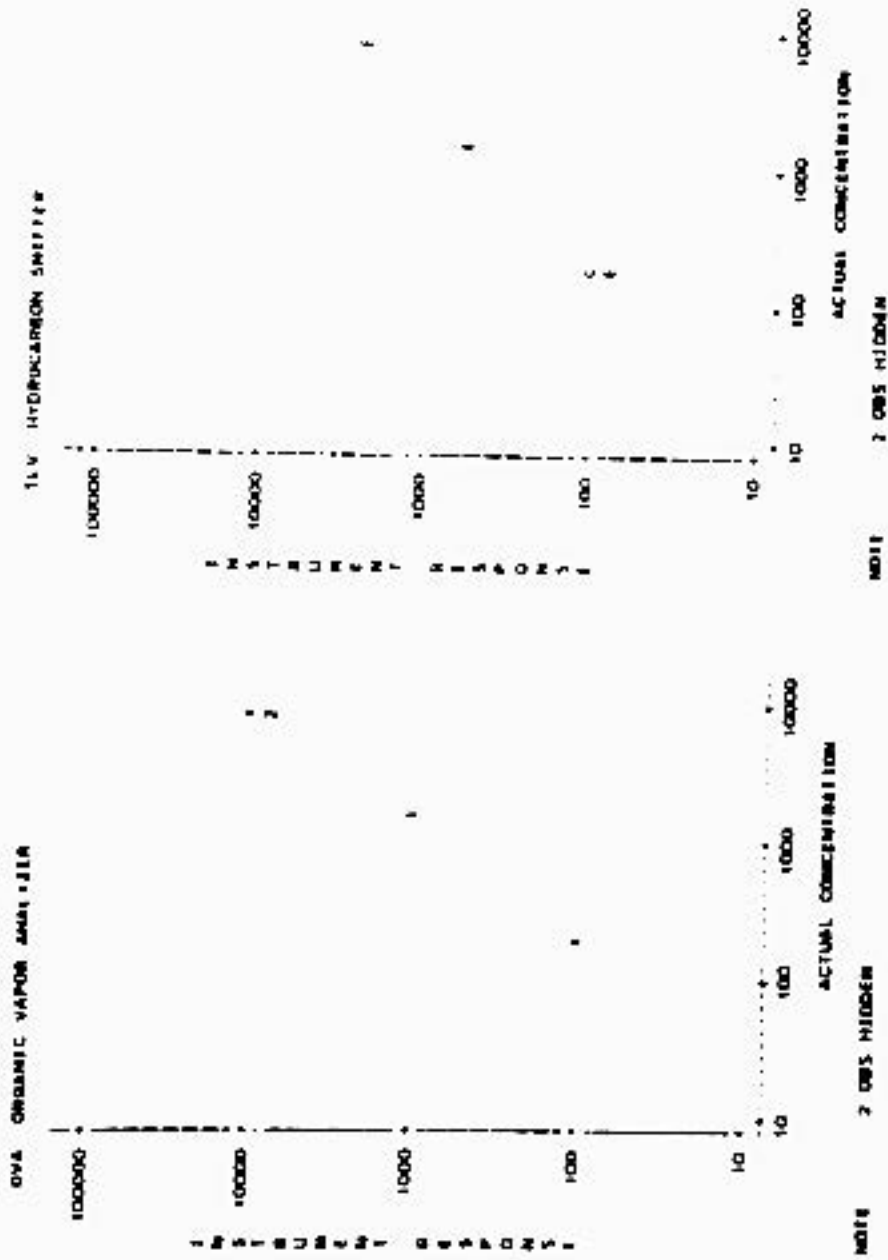


TABLE 1, CONT.

RESPONSE FREQUENCY SUMMARY

FRICION DRUMS-PPHNS 1 2 3

OVA INSTRUMENTS

NOMINAL PPHN	ACTUAL PPHN			OVERALL			DESIGN POINTS							
	LOW	HIGH	MEAN	MEAN	SD	N	1000	50	2700	50	2700	50	2700	50
200	522	522	522	3 19 0 48		2	2 12		1	3 07				
1000	1518	1518	1518	1 20 0 18		2	1 11		1	1 03				
8000	8000	8000	8000	1 22 0 07		2	1 45		1	1 20				
OVERALL MEANS						3 92 0 04	6	1 08 0 52	2	2 18 0 26	2			
ESTIMATED AT 10,000 PPHN						0 89		95% CONFIDENCE INTERVAL 1 0 50 1 001						

FLY INSTRUMENTS

NOMINAL PPHN	ACTUAL PPHN			OVERALL			DESIGN POINTS							
	LOW	HIGH	MEAN	MEAN	SD	N	100	50	2700	50	2700	50	2700	50
200	522	522	522	4 41 0 28		2	4 59		1	4 42				
1000	1518	1518	1518	2 43 0 10		2	2 52		1	2 33				
8000	8000	8000	8000	2 82 0 00		2	2 63		1	2 61				
OVERALL MEANS						3 15 0 02	6	3 28 0 10	2	3 12 0 50	2			
ESTIMATED AT 10,000 PPHN						2 22		95% CONFIDENCE INTERVAL 1 1 43 1 401						

Figure 5-160

INSTRUMENT RESPONSE VS CONCENTRATION

TRICHLOROPROPANE 1,2,3

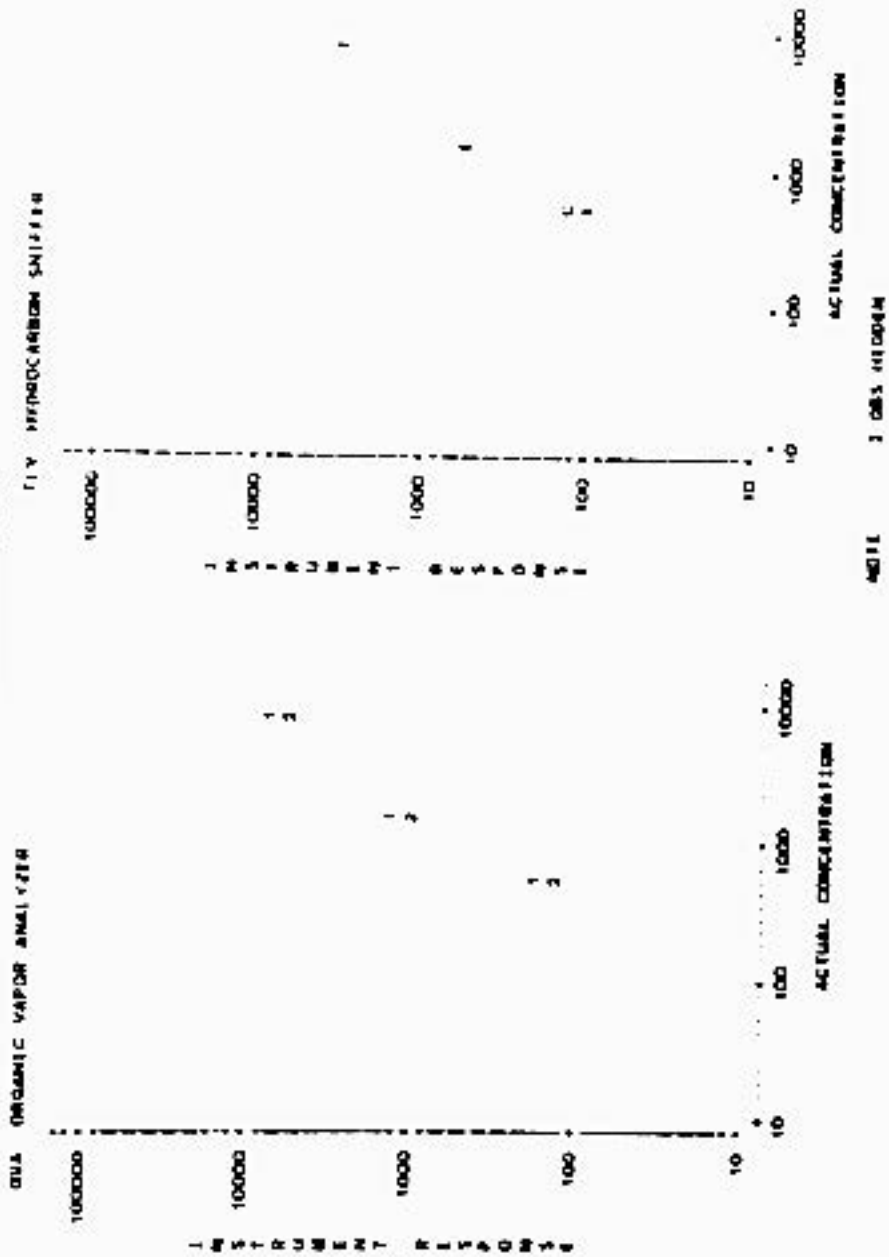




TABLE 5 (a)

RESPONSE FACTOR SUMMARY

TRIBUTYLAMINE

DVA IMPROVEMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DVA IMPROVEMENTS													
	LOW	HIGH	MEAN	SE	N	1000	SE	N	2250	SE	N	4100	SE	N	6000	SE	N	
200	198	198	198	0.82	2	0.82	0.40	2	0.82	1	0.82	1	0.82	1	0.82	1	0.82	1
1000	1023	1023	1023	0.71	2	0.71	0.31	2	0.71	1	0.71	1	0.71	1	0.71	1	0.71	1
4000	3844	3844	3844	0.58	2	0.58	0.20	2	0.58	1	0.58	1	0.58	1	0.58	1	0.58	1
8000	7967	7967	7967	0.66	2	0.66	0.33	2	0.66	1	0.66	1	0.66	1	0.66	1	0.66	1
OVERALL MEANS					0.66	0.66	0.66	0.66	0.66	0.66	0.66	0.66	0.66	0.66	0.66	0.66	0.66	0.66
ESTIMATED AT 10000 PPMV					0.44	0.44	0.44	0.44	0.44	0.44	0.44	0.44	0.44	0.44	0.44	0.44	0.44	0.44

ESTIMATED AT 10000 PPMV

OVERALL MEANS

95% CONFIDENCE INTERVAL

FLV IMPROVEMENTS

DVA IMPROVEMENTS

NOMINAL PPMV	ACTUAL PPMV		OVERALL		DVA IMPROVEMENTS														
	LOW	HIGH	MEAN	SE	N	75	SE	N	200	SE	N	400	SE	N	600	SE	N		
200	198	198	198	0.78	1	0.78	0.39	1	0.78	1	0.78	1	0.78	1	0.78	1	0.78	1	
1000	1023	1023	1023	1.31	1	1.31	0.66	1	1.31	1	1.31	1	1.31	1	1.31	1	1.31	1	
4000	3844	3844	3844	1.36	1	1.36	0.68	1	1.36	1	1.36	1	1.36	1	1.36	1	1.36	1	
8000	7967	7967	7967	1.41	1	1.41	0.71	1	1.41	1	1.41	1	1.41	1	1.41	1	1.41	1	
OVERALL MEANS					1.21	1.21	1.21	1.21	1.21	1.21	1.21	1.21	1.21	1.21	1.21	1.21	1.21	1.21	
ESTIMATED AT 10000 PPMV					1.41	1.41	1.41	1.41	1.41	1.41	1.41	1.41	1.41	1.41	1.41	1.41	1.41	1.41	1.41

ESTIMATED AT 10000 PPMV

95% CONFIDENCE INTERVAL

Figure 3-16)

INSTRUMENT RESPONSE VS CONCENTRATION

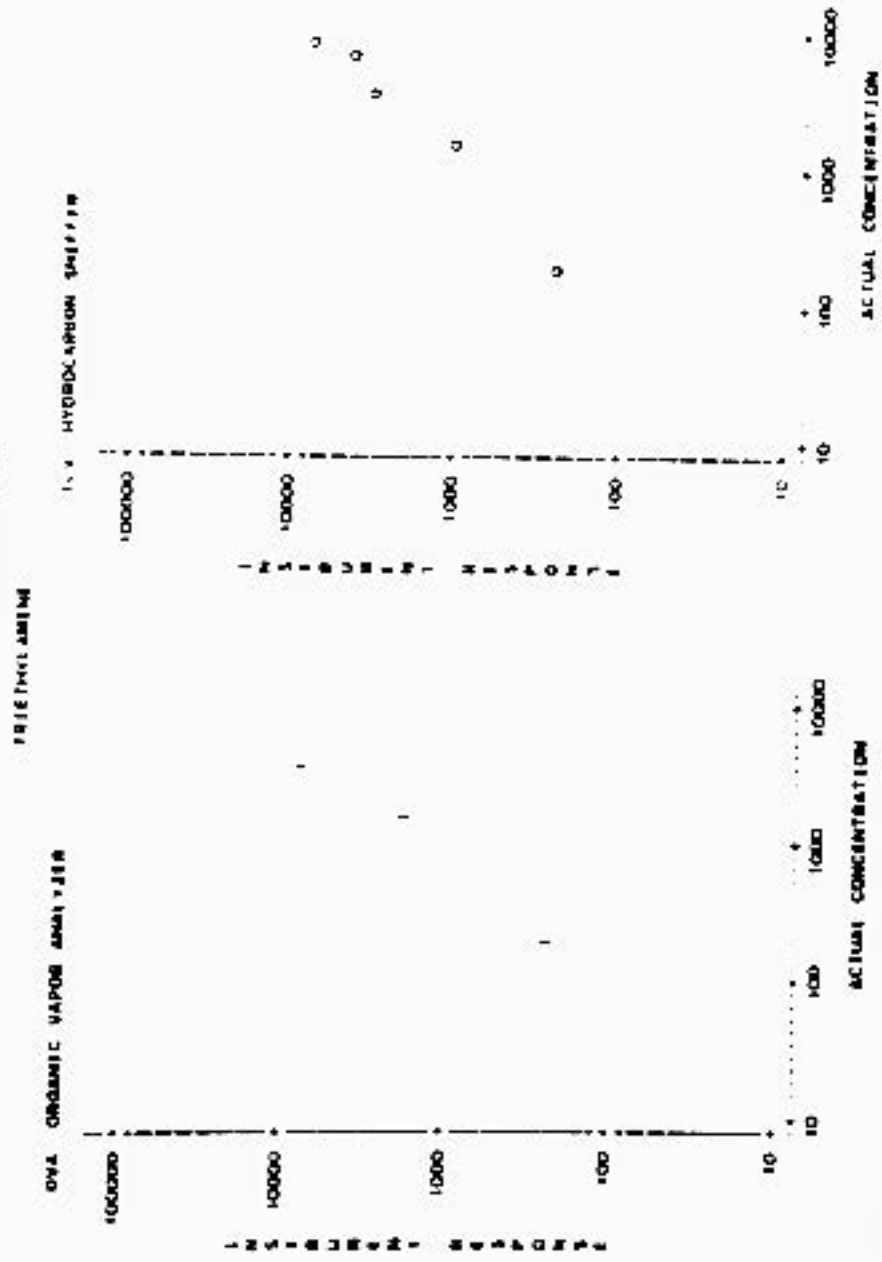


TABLE 5. 14.7

MEASUREMENT FREQUENCY SUMMARY

VENTI ACULATE

DVA INSTRUMENTS

NOMINAL PUMP	ACTUAL PUMP			OVERALL			M E A S U R E M E N T F R E Q U E N C Y												
	LOW	MID	HIGH	MEAN	SE	N	1	2	3	4	5	6	7	8	9	10	11	12	
2000	214	214	214	1.97	0.10	2													
1500	1547	1547	1547	2.06	0.13	2													
8000	8154	8154	8154	1.73	0.03	2													
OVERALL MEANS							1.70	0.04	6										
ESTIMATED AT 10 000 RPM							1.71												


95% CONFIDENCE INTERVAL 1.10 2.76

DVA INSTRUMENTS

NOMINAL PUMP	ACTUAL PUMP			OVERALL			M E A S U R E M E N T F R E Q U E N C Y												
	LOW	MID	HIGH	MEAN	SE	N	1	2	3	4	5	6	7	8	9	10	11	12	
2000	214	214	214	2.14	0.17	2													
1500	1547	1547	1547	2.27	0.22	2													
8000	8154	8154	8154	5.90	1.51	2													
OVERALL MEANS							3.75	0.24	6										
ESTIMATED AT 10 000 RPM							3.60												

95% CONFIDENCE INTERVAL 1.74 5.79

Figure 5-16.2  
 INSTRUMENT RESPONSE VS CONCENTRATION

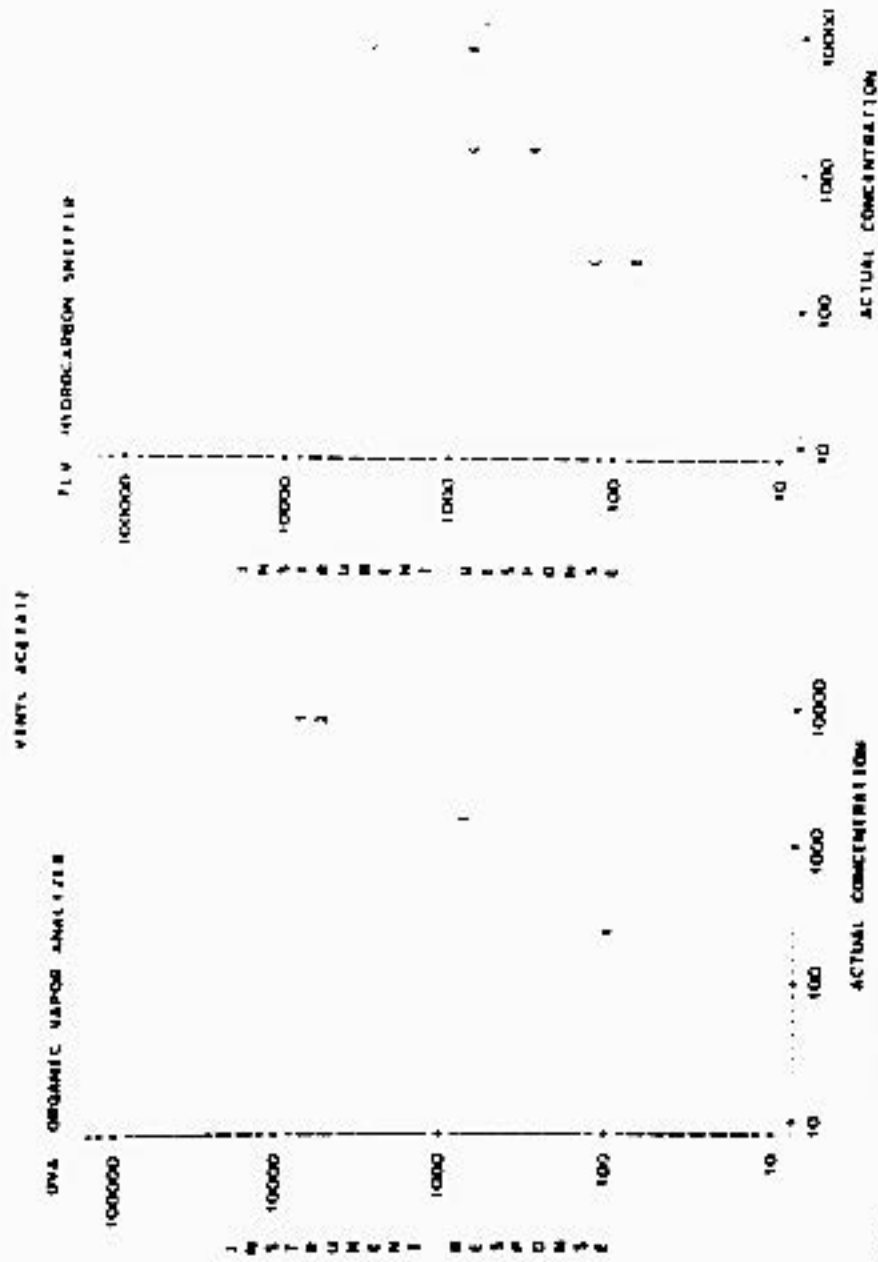

NOTE: 1 OBS. HIDDEN

TABLE 5 (Cont.)

ACTIVELY ENGAGED

FINANCIAL INSTITUTIONS

OVERALL MEANS

ACTIVELY ENGAGED FINANCIAL INSTITUTIONS	ACTUAL PERCENTAGE		OVERALL		U.S. COMPANIES						
	LOW	HIGH	MEAN	SD	1980	81	82	83	84	85	86
1000	884	804	804	27.40							
4000	4283	4283	4283	2.09						27.40	
8000	1227	1227	1227	1.10						2.10	
	OVERALL MEANS		804							1.91	
ESTIMATED AT 50 PERCENT											
	OVERALL MEANS		804							8.54	

FINANCIAL INSTITUTIONS

OVERALL

FINANCIAL INSTITUTIONS	ACTUAL PERCENTAGE		OVERALL		U.S. COMPANIES						
	LOW	HIGH	MEAN	SD	1980	81	82	83	84	85	86
1000	884	804	804	27.40							
4000	4283	4283	4283	1.94						27.40	
8000	1227	1227	1227	1.51						1.94	
	OVERALL MEANS		804							1.91	
ESTIMATED AT 50 PERCENT											
	OVERALL MEANS		804							1.91	

FIGURE 5-161

INSTRUMENT RESPONSE VS CONCENTRATION

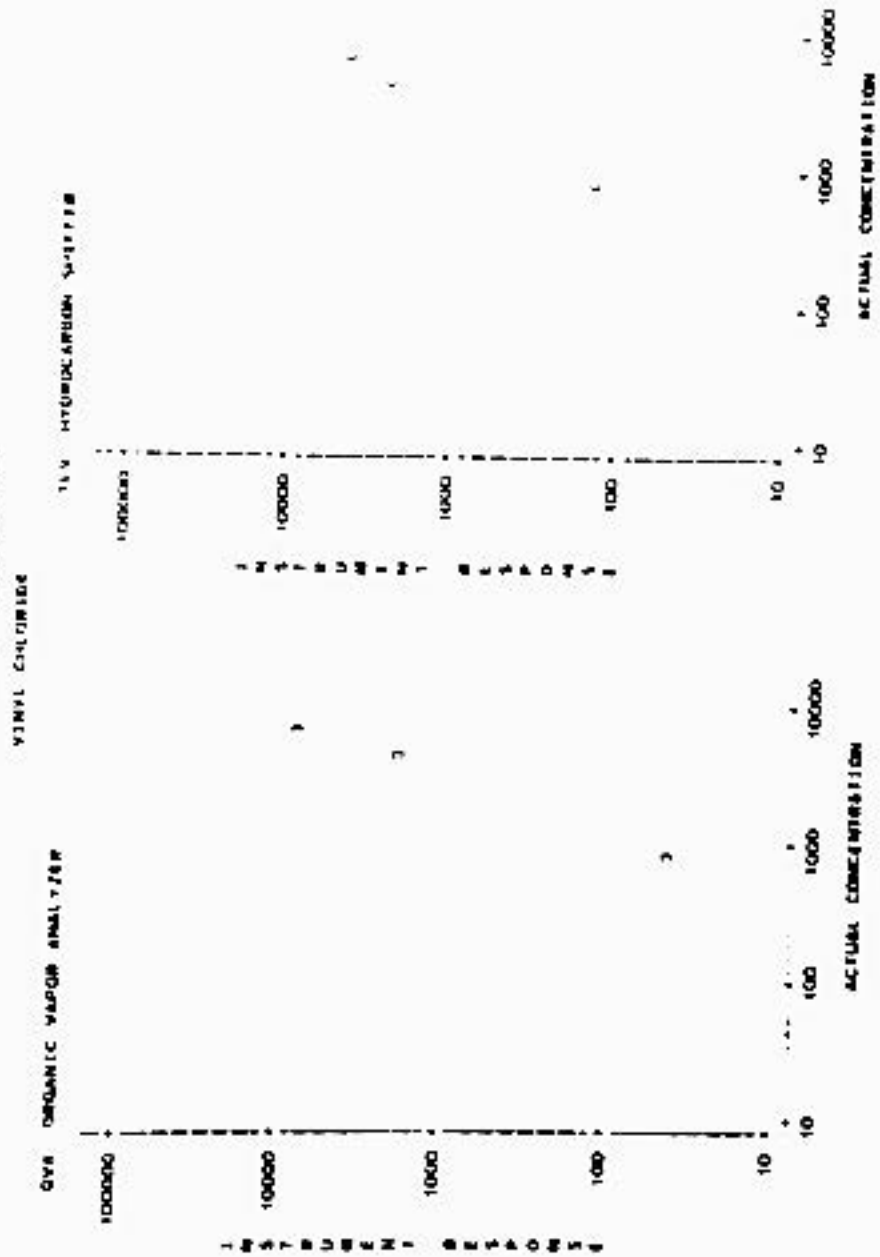




FIGURE 5-164

INSTRUMENT RESPONSE VS CONCENTRATION

VINYL PROPIONATE

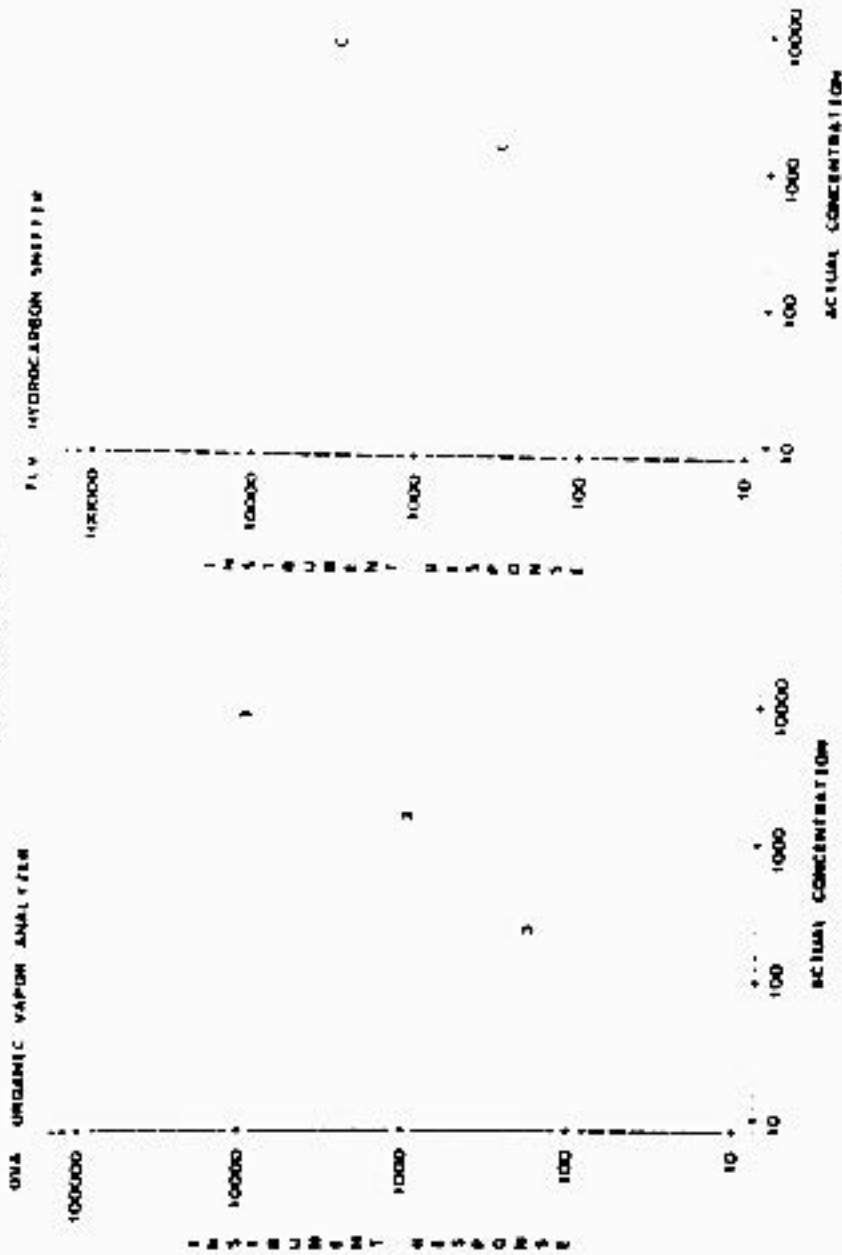




TABLE 5. 165

RESPONSE ACTION SUMMARY

VINYL CHLORIDE CUMULATIVE

OVERALL MEASUREMENTS

NOMINAL DEPTH	ACTUAL DEPTH		OVERLAP		PERCENTAGE OF OVERLAP					
	LOW	HIGH	MEAN	STDEV	0	10	20	30	40	50
2000	270	270	270	0.00	2	0	0	0	0	0
15000	1827	1827	1827	0.00	2	0	0	0	0	0
80000	8181	8181	8181	0.00	2	0	0	0	0	0
OVERALL MEASUREMENTS					2	0	0	0	0	0

ESTIMATED AT 10000 DEPTH 1.00

FLY MEASUREMENTS

NOMINAL DEPTH	ACTUAL DEPTH		OVERLAP		PERCENTAGE OF OVERLAP					
	LOW	HIGH	MEAN	STDEV	0	10	20	30	40	50
2000	270	270	270	0.00	2	0	0	0	0	0
15000	1827	1827	1827	0.00	2	0	0	0	0	0
80000	8181	8181	8181	0.00	2	0	0	0	0	0
OVERALL MEASUREMENTS					2	0	0	0	0	0

ESTIMATED AT 10000 DEPTH 2.00

PERCENTAGE OF OVERLAP

PERCENTAGE OF OVERLAP										
0	10	20	30	40	50	60	70	80	90	100
2	0	0	0	0	0	0	0	0	0	0

ESTIMATED AT 10000 DEPTH 1.00

FLY MEASUREMENTS

PERCENTAGE OF OVERLAP										
0	10	20	30	40	50	60	70	80	90	100
2	0	0	0	0	0	0	0	0	0	0

ESTIMATED AT 10000 DEPTH 2.00

Figure 5-16a

INSTRUMENT RESPONSE VS CONCENTRATION

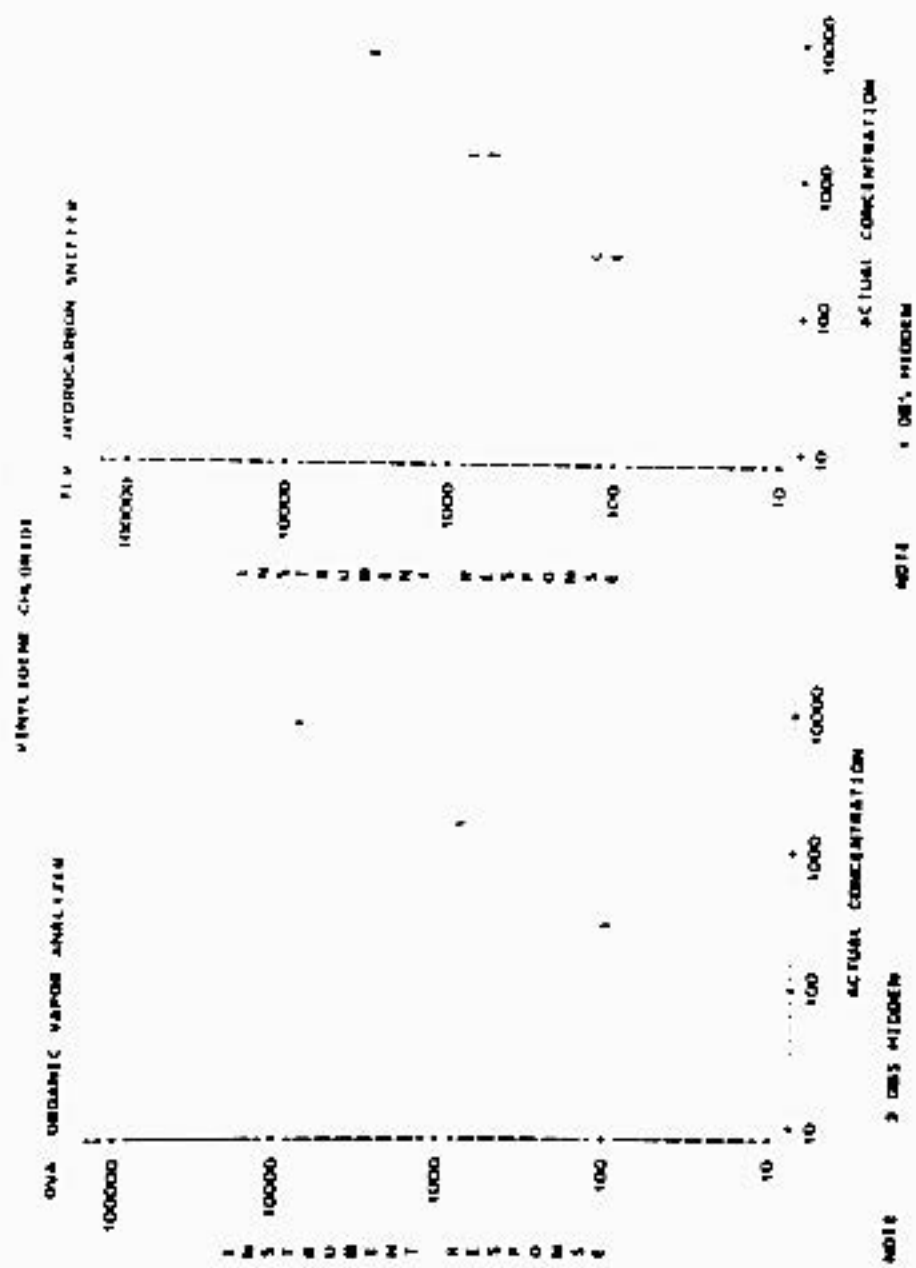


TABLE 4 (Cont.)

RESPONSE FACTOR SUMMARY

TABLE 4

Overall Instrument 1

NOMINAL POWER	ACTUAL POWER		OVERALL		95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	SD	LO	HI	LO	HI	LO	HI
300	45	55	3.48	0.42	2.70	4.26	2.70	4.26	2.70	4.26
600	94	106	3.70	0.34	3.20	4.20	3.20	4.20	3.20	4.20
1200	181	212	3.77	0.40	3.20	4.34	3.20	4.34	3.20	4.34
OVERALL MEAN			3.49	0.39	3.03	3.95	3.03	3.95	3.03	3.95
ESTIMATED AT 10000 POWER			3.27		2.83	3.70	2.83	3.70	2.83	3.70

Overall Instrument 2

NOMINAL POWER	ACTUAL POWER		OVERALL		95% CONFIDENCE INTERVAL					
	LOW	HIGH	MEAN	SD	LO	HI	LO	HI	LO	HI
300	45	51	1.99	0.48	1.00	2.98	1.00	2.98	1.00	2.98
600	94	106	2.71	0.33	2.00	3.42	2.00	3.42	2.00	3.42
1200	181	212	3.00	0.43	2.00	4.00	2.00	4.00	2.00	4.00
OVERALL MEAN			2.57	0.43	1.67	3.47	1.67	3.47	1.67	3.47
ESTIMATED AT 10000 POWER			2.26		1.67	2.85	1.67	2.85	1.67	2.85

Figure 5-10b  
 INSTRUMENT RESPONSE VS CONCENTRATION

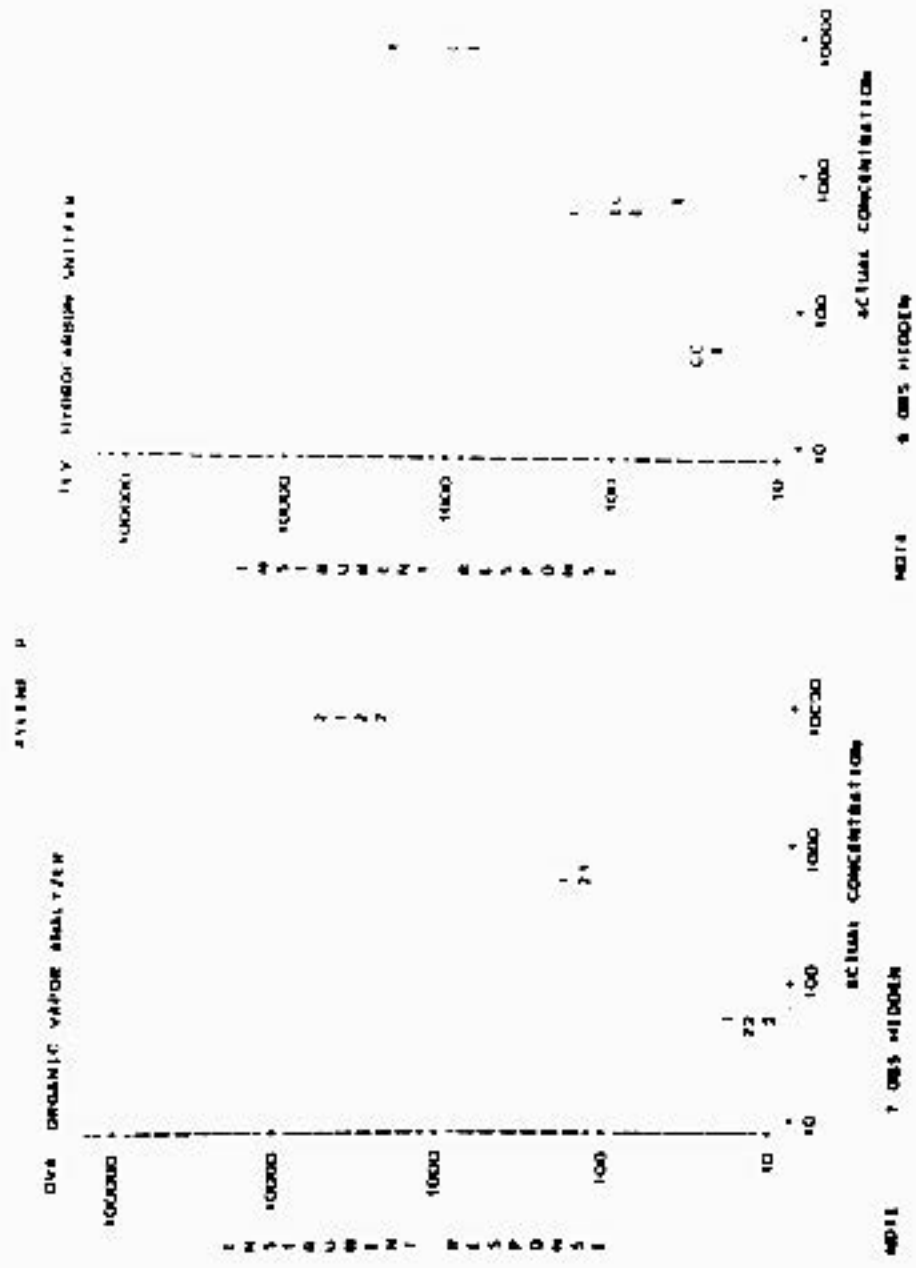


TABLE 5 (cont.)

RESPONSE FACTOR SUMMARS

TYPE III

OVA ESTIMATES

MEAN SQUARES

OVERALL

NOMINAL PPMV	LOW	HIGH	MEAN	MEAN	SE	N	SS	DF	M	SS	DF	M	SS	DF
200	203	207	203	1.04	0.198	2	1.98	1	0.09	1	0.09	1	0.09	1
1500	1548	1548	1548	0.60	0.492	2	0.57	1	0.07	1	0.07	1	0.07	1
3000	2984	2984	2984	0.47	0.091	2	0.47	1	0.07	1	0.07	1	0.07	1
4500	4513	4513	4513											
6000	5762	5762	5762											

OVERALL MEANS

ESTIMATED AT 10 000 PPMV

95% CONFIDENCE INTERVAL

TYPE III

OVA ESTIMATES

MEAN SQUARES

OVERALL

NOMINAL PPMV	LOW	HIGH	MEAN	MEAN	SE	N	SS	DF	M	SS	DF	M	SS	DF
200	203	203	203	2.03	0.091	2	1.53	1	0.07	1	0.07	1	0.07	1
1500	1548	1548	1548	5.72	0.72	2	0.44	1	2.00	1	2.00	1	2.00	1
3000	2984	2984	2984	7.24	0.80	2	12.84	1	1.84	1	1.84	1	1.84	1
4500	4513	4513	4513	8.21	0.74	2	15.01	1	1.51	1	1.51	1	1.51	1
6000	5762	5762	5762	18.76	0.81	2	37.86	1	1.51	1	1.51	1	1.51	1

OVERALL MEANS

ESTIMATED AT 10 000 PPMV

95% CONFIDENCE INTERVAL

Figure 3-16?

INSTRUMENT RESPONSE VS CONCENTRATION

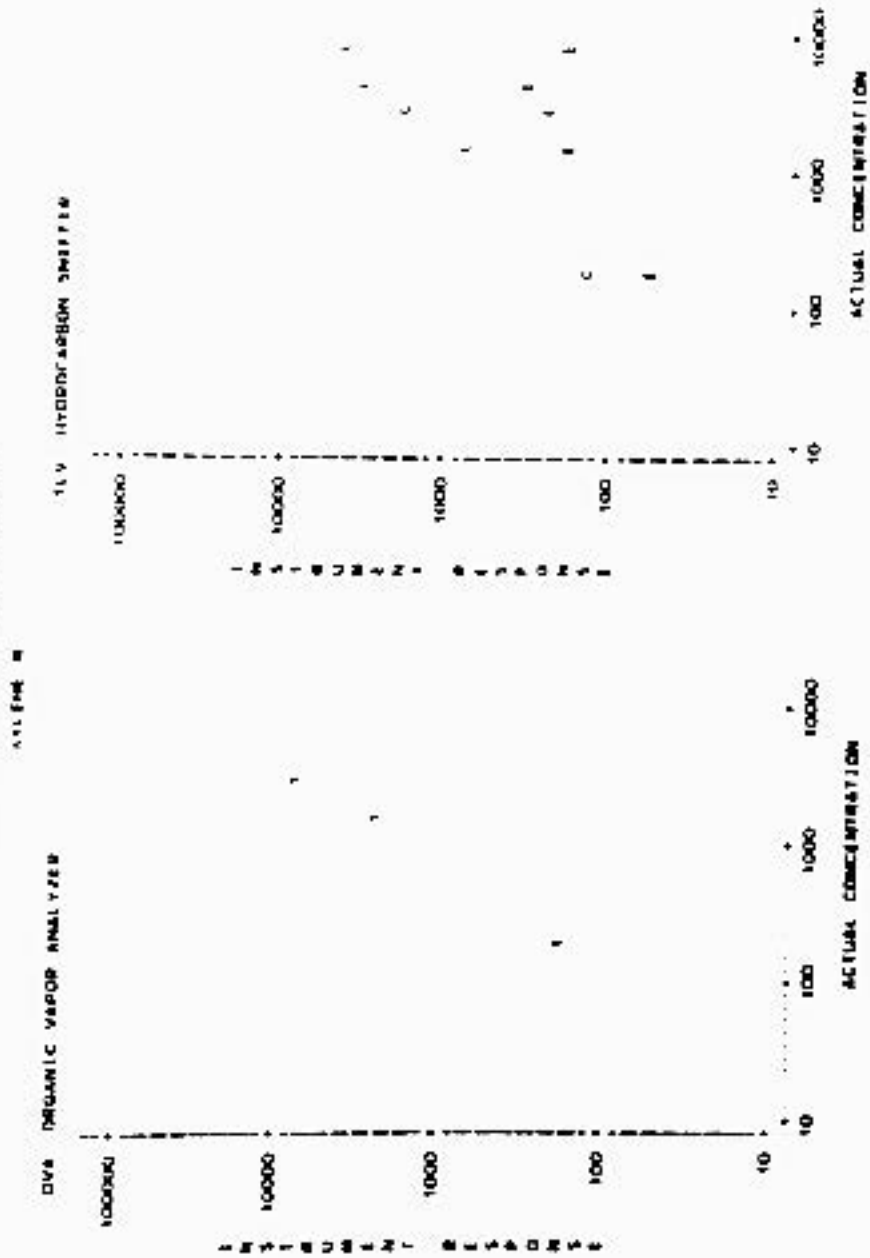


TABLE 5. 1948

RESIDUAL FACTORIAL SUMMARS

TABLE 6

OVA INSTRUMENTS

NOMINAL PIPV	ACTUAL PIPV		OVERALL		M E S P D M S I P A . I I R S															
	LOW	HIGH	MEAN	SE	M	1000	SE	M	2750	SE	M	4500	SE	M	6250	SE	M	8000	SE	
200	205	205	205	0.89	0.08	2	0.83	1	0.94	1	0.94	1	0.94	1	0.94	1	0.94	1	0.94	1
1500	1523	1523	1523	0.86	0.08	2	0.81	1	0.91	1	0.91	1	0.91	1	0.91	1	0.91	1	0.91	1
3000	2968	2968	2968	0.38	0.04	2	0.35	1	0.47	1	0.47	1	0.47	1	0.47	1	0.47	1	0.47	1
5000	6268	6268	6268																	

OVERALL MEANS 0.11 0.01 0.08 0.16 0.10 0.11 0.13

ESTIMATED AT 10 000 PIPV 0.10

95% CONFIDENCE INTERVALS 0.01 0.16 0.21

FLV INSTRUMENTS

NOMINAL PIPV	ACTUAL PIPV		OVERALL		M E S P D M S I P A . I I R S															
	LOW	HIGH	MEAN	SE	M	10	SE	M	25	SE	M	50	SE	M	75	SE	M	100	SE	
200	205	205	205	1.78	1	1.78	1	1.78	1	1.78	1	1.78	1	1.78	1	1.78	1	1.78	1	1.78
1500	1523	1523	1523	1.08	1	1.08	1	1.08	1	1.08	1	1.08	1	1.08	1	1.08	1	1.08	1	1.08
3000	2968	2968	2968	1.57	1	1.57	1	1.57	1	1.57	1	1.57	1	1.57	1	1.57	1	1.57	1	1.57
5000	6268	6268	6268	1.71	1	1.71	1	1.71	1	1.71	1	1.71	1	1.71	1	1.71	1	1.71	1	1.71

OVERALL MEANS 1.51

ESTIMATED AT 10 000 PIPV 1.40

95% CONFIDENCE INTERVALS 1.01 1.71





TABLE 5.107

STATISTICS FOR COMPUTING ESTIMATES AND CONFIDENCE INTERVALS

COMPOUND ID NO	COMPOUND NAME	CLASS	Q	R	S	T	U	V	W	X	Y	Z
70	ACETIC ACID	11	2.8794	1.22143	21	0.811209	44.0588	1.011	1.011	1.011	1.011	1.011
80	ACETIC ANHYDRIDE	11	3.75286	925664	8	0.74500	8.19851	1.011	1.011	1.011	1.011	1.011
90	ACETONE	11	4.2801	1166086	14	0.44568	56.4433	1.011	1.011	1.011	1.011	1.011
100	ACETONE CHLORHYDRIN	11	1.0124	9805873	6	0.216118	1.011	1.011	1.011	1.011	1.011	1.011
110	ACETONITRILE	11	8.0887	3.09808	8	0.182116	12.5478	1.011	1.011	1.011	1.011	1.011
120	ACETOPHENONE	11	1.011	811851	4	0.268281	42.011	1.011	1.011	1.011	1.011	1.011
125	ACETYL CHLORIDE	11	88504	984411	4	0.177841	14.8944	1.011	1.011	1.011	1.011	1.011
130	ACETYL PROPANOL 3	11	1.011	811182	2	0.476851	40.2071	1.011	1.011	1.011	1.011	1.011
130	ACETYLENE	11	485845	1.05433	6	0.110139	44.011	1.011	1.011	1.011	1.011	1.011
140	ACRYLIC ACID	11	1.011	1.011	6	0.111844	1.011	1.011	1.011	1.011	1.011	1.011
110	ACRYLONITRILE	11	5.1242	1.05339	8	0.118828	14.844	1.011	1.011	1.011	1.011	1.011
110	ALLENE	11	2.8183	1.37159	8	0.191886	4.422	1.011	1.011	1.011	1.011	1.011
200	ALLYL ALCOHOL	11	3.6	1.05334	8	0.12788	1.011	1.011	1.011	1.011	1.011	1.011
250	AMYL ALCOHOL N	11	2.1531	1.29529	6	0.114876	5.09458	1.011	1.011	1.011	1.011	1.011
310	ANILINE	11	2.0918	1.41493	8	0.116619	4.28984	1.011	1.011	1.011	1.011	1.011
310	ANISOLE	11	1.011	918952	6	0.188868	4.64885	1.011	1.011	1.011	1.011	1.011
340	ANTRACENE	11	4.4202	911919	6	0.114713	4.55056	1.011	1.011	1.011	1.011	1.011
340	ANTRACENE	11	8.111	1.26135	11	0.148218	51.4347	1.011	1.011	1.011	1.011	1.011
380	BENZENE	11	1.05512	1.85448	12	0.226988	6.18245	1.011	1.011	1.011	1.011	1.011
450	BENZONITRILE	11	1.4641	989853	6	0.410189	13.7681	1.011	1.011	1.011	1.011	1.011
490	BENZYL CHLORIDE	11	3.1671	528181	12	0.151811	17.1481	1.011	1.011	1.011	1.011	1.011
530	BENZYL CHLORIDE	11	14.983	1.11851	8	0.11160	1.011	1.011	1.011	1.011	1.011	1.011
540	BROMOBENZENE	11	5.1128	1.2811	8	0.14647	1.011	1.011	1.011	1.011	1.011	1.011
540	BROMOBENZENE	11	2.9032	1.42016	1	0.180245	1.011	1.011	1.011	1.011	1.011	1.011
540	BUTADIENE	11	9411	4.262	1	0.133644	6.111	1.011	1.011	1.011	1.011	1.011
540	BUTADIENE	11	1.011	1.011	6	0.11518	5.651	1.011	1.011	1.011	1.011	1.011
580	BUTANOL SEC	11	1.011	1.011	6	0.248818	4.5818	1.011	1.011	1.011	1.011	1.011
580	BUTANOL TER	11	1.011	1.011	6	0.088523	4.9818	1.011	1.011	1.011	1.011	1.011
592	BUTENE	11	1.011	1.011	6	0.149189	1.011	1.011	1.011	1.011	1.011	1.011
600	MULTI ACETATE N	11	1.011	1.011	6	0.07847	6.9845	1.011	1.011	1.011	1.011	1.011
610	MULTI ACETATE N	11	1.011	1.011	6	0.07847	6.9845	1.011	1.011	1.011	1.011	1.011

ORGANIC CHEMICAL FINDER, DATA BASE

U.S. G. PAT. OFF. (Cont.)



TABLE 5-269 (Contd. Unref.)

STATISTICS FOR COMPUTING ESTIMATES AND CONFIDENCE INTERVALS

OCPOB* 10 80	COMPOUND NAME	MOLECULAR CLASS	A	B	N	M	SS	SDM
1270	DICHLORO-1-PROPANOL-2,3	LL	1 8734	1 1852	13	0 204878	49 1017	6 66117
-	DICHLORO-1-PROPANOL-3,3	LL	3 0524	873976	6	0 432834	13 8007	7 28779
-	DICHLORO-2-PROPANOL-1,3	LL	1 8418	1 24873	6	0 212282	11 2691	7 10441
1218	DICHLOROBENZENE-M	LL	79172	0 70998	6	0 410298	15 4888	1 55414
1216	DICHLOROBENZENE-O	ML	988273	937683	6	0547624	7 4863	6 58817
-	DICHLOROBENZENE-1,1	ML	1 10876	9 7648	6	0947498	1 19818	6 22962
1248	DICHLOROBETHANE-1,1	LL	00708	1 02619	6	0 130118	10 5488	7 11116
1238	DICHLOROBETHANE-1,2	LL	30877	1 02345	6	0 131104	14 1446	1 2061
1236	DICHLOROBETHYLENE-CIS-1,2	LL	1 4818	1 2855	6	0 2006	15 275	1 54257
1236	DICHLOROBETHYLENE-TRANS-1,2	LL	2 0189	1 20515	6	0 0863401	13 1057	7 02026
1670	DICHLOROBETHANE	LL	1 0824	182173	6	0915883	13 1072	7 23489
3110	DICHLOROPROPANE-1,2	LL	88509	1 09215	6	0 123324	10 8605	1 271
1448	DICHLOROPROPANE-1,3	LL	2 0148	1 37178	6	0 165223	7 56682	6 9367
-	DICHLOROPROPYL BENZENE-1,3	LL	1 76489	547649	6	0 861938	26 5679	6 21642
1470	DIMETHOXY ETHANE-1,2	LL	2 928	1 27573	6	0 483998	13 2136	1 19273
1480	DIMETHYLFORMAMIDE-M	LL	87443	947137	6	0 108855	9 19506	1 02813
1655	DIMETHYLHYDRAZINE-1,1	LL	3 7521	1 40074	6	0 220874	13 1961	1 24392
-	DIMETHYLSTYRENE-2,4	LL	1 5247	771285	6	0 224822	13 6858	1 24061
1570	DIMETHYLSULFONIDE	ML	14 573	3 43602	6	1 0923	409861	5 66174
1480	DIBLAME	LL	3 0831	1 1043	6	0 215831	13 0262	7 20204
1850	ETHANOL	LL	78038	1 02734	6	0 276406	13 396	1 2068
-	ETHANOL	LL	2 0458	1 27848	6	0 279301	7 31961	1 8883
1870	ETHOXY ETHANOL-2	LL	2 9244	1 27973	6	0 096231	19 4173	1 5670
1870	ETHYL ACETATE	LL	2 3244	1 19637	6	0 101064	9 75276	1 07472
1880	ETHYL ACETOACETATE	ML	1 2248	1 18192	6	0 18188	85 2741	6 71408
1890	ETHYL ACRYLATE	LL	404514	875583	6	0 107831	7 5844	6 28103
1750	ETHYL CARBOACETATE	LL	2 1188	1 26487	6	0 144231	11 6226	7 1427
1890	ETHYL CARBOACETATE	LL	80489	0 99184	6	0531139	8 85726	6 99629
1710	ETHYL ETHER	LL	1 8881	1 20484	6	0 155052	11 8344	7 12179
1710	ETHYLENE	LL	1 0274	1 2088	20	0 587092	68 947	6 80288
1710	ETHYLENE	C	8 0864	1 98341	6	0 121488	7 84823	6 01314

\* ORGANIC CHEMICAL PRODUCERS DATA BANK

\*\* G = GAS; LL = LIGHT LIQUID; ML = MEDIUM LIQUID



TABLE 3-169 (continued)  
 STATISTICS FOR COMPUTING ESTIMATES AND CONFIDENCE INTERVALS

OCPOB* ID NO.	COMPOUND NAME	VOLATILITY CLASS**	TYPE DATA									
			A	R	M	N	SS*	SRAD				
2550	METHYL-2-BUTYL-2-OL-2	LL	1 8074	1 27615	6	0 23082	10 1905	7 12895				
	METHYLAL	LL	2 2406	1 10782	12	0 28504	52 8818	6 4111				
2560	METHYLBENZENE-N	ML	1 1209	927574	6	0227429	2 11941	6 24884				
2570	METHYLCYCLOHEXANE	LL	2 2603	1 16952	6	0 48889	1 87591	6 87425				
	METHYLCYCLOHEXENE	LL	3 1159	1 24919	6	0 153802	8 95189	6 98321				
2620	METHYLPENTHOL	LL	0 8938	845945	6	0 280771	12 5573	6 93418				
2630	METHYLSULFONE	LL	1 2814	884734	14	0 240238	66 6129	6 93418				
1660	METHYLTANOLAMINE	LL	2 4781	959184	10	0 318058	21 2589	6 18121				
2700	METHYLOXINE	LL	0 9405	1 10892	6	0 215556	13 2898	1 8111				
2770	NITROBENZENE	ML	2 27819	255851	7	0 403458	3 1675	7 5170				
2790	METHOXYBENZENE	LL	3 8824	1 00525	6	0 168138	14 162	2 1121				
2791	METHOXYBENZENE	LL	1 7991	954076	6	0 109273	11 5221	2 2112				
2795	METHOXYBENZENE	LL	1 0828	1 10518	6	0 178504	13 9435	1 26288				
	METHOXYBENZENE	LL	1 0402	1 10603	14	0 961526	41 1108	8 1997				
	METHOXYBENZENE	LL	1 0402	1 10603	14	0 961526	41 1108	8 1997				
2851	METHOXYBENZENE	LL	2 0550	1 31598	6	0 165283	9 88585	1 05104				
2910	METHOXYBENZENE	LL	1 0423	1 10518	6	0 155262	1 90326	5 24517				
	METHOXYBENZENE	LL	1 0402	1 10603	14	0 961526	41 1108	8 1997				
2911	METHOXYBENZENE	LL	1 7778	1 20562	6	0 160041	8 91212	2 2075				
	METHOXYBENZENE	LL	0 28146	802834	10	0 849772	3 20321	2 88011				
3061	METHOXYBENZENE	LL	2 8877	1 29443	6	0 279661	12 9242	1 24108				
3066	METHOXYBENZENE	LL	1 4819	1 12962	6	0 295821	1 82093	6 89446				
3070	METHOXYBENZENE	LL	2 4127	1 27118	6	0 142748	14 0456	1 22123				
	METHOXYBENZENE	LL	1 2592	1 2127	6	0 165543	1 18821	6 93889				
3090	METHOXYBENZENE	G	8 6818	9 6567	6	0 225082	4 94104	2 41693				
3170	METHOXYBENZENE	LL	1 5249	1 1886	7	0 103187	13 8051	2 43403				
3210	METHOXYBENZENE	LL	9 123	1 4018	8	0 2900446	8 47388	6 91011				
3230	METHOXYBENZENE	LL	1 2382	990213	6	0 151181	13 177	2 21099				
3291	METHOXYBENZENE	LL	1 50932	697922	10	0 589879	11 5223	6 62611				
	METHOXYBENZENE	LL	8 3198	872029	8	0 137087	12 074	6 91454				
3369	METHOXYBENZENE	LL	2 0128	1 05646	26	0 811876	117 642	6 27884				

\* ORGANIC CHEMICAL PRODUCTION DATA BASE  
 \*\* G - GAS, L - LIQUID, ML - MELT LIQUID, PL - PLAST LIQUID





TABLE 5 (20) (CONTINUED)

STATISTICS FOR COMPUTING ESTIMATES FOR TEMPERATURE INDEXTES

COMP- ID NO	COMPOUND NAME	WTA CLASS	4	8	9	10	11	12	13	14	15	16	17	18	19	20
670	BUTYL ETHER, SEC	11	474.186	800.527	7	11.24208	8	9.1922	1	1.24						
680	BUTYLAMINE, N	15	109.161	921.84	4	11.19514	4	11.19514	4	1.24						
690	BUTYLAMINE, TER	15	104.394	916.167	1	11.19514	1	11.19514	1	1.24						
700	BUTYLAMINE, TER	11	514.193	881.811	4	11.19514	4	11.19514	4	1.24						
710	BUTYLBENZENE, TER	10	2.81474	515.112	6	11.26441	6	11.26441	6	1.24						
720	BUTYRIC ACID	11	1.53201	11.26441	1	11.26441	1	11.26441	1	1.24						
730	BUTYNYLBENZENE, N	15	1.00008	403.185	1	11.26441	1	11.26441	1	1.24						
740	BUTYNYLBENZENE, N	15	403.185	410.116	4	11.26441	4	11.26441	4	1.24						
750	CARBON DIBAZIDE	11	100.447	193.281	1	11.26441	1	11.26441	1	1.24						
760	CARBON TETRACHLORIDE	11	4.85988	193.281	1	11.26441	1	11.26441	1	1.24						
770	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
780	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
790	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
800	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
810	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
820	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
830	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
840	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
850	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
860	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
870	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
880	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
890	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
900	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
910	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
920	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
930	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
940	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
950	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
960	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
970	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
980	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
990	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1000	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1010	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1020	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1030	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1040	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1050	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1060	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1070	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1080	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1090	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1100	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1110	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1120	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1130	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1140	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1150	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1160	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1170	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1180	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1190	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1200	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1210	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1220	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1230	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1240	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1250	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1260	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1270	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1280	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1290	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1300	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1310	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1320	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1330	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1340	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1350	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1360	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1370	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1380	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1390	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1400	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1410	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1420	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1430	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1440	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1450	CHEMICAL FALSHOLD	11	1.00008	193.281	1	11.26441	1	11.26441	1	1.24						
1460	CHEMICAL FALSHOLD	11	1													



TABLE 5-170 (Cont. from Table 5-170)

STATISTICS FOR COMPUTING ESTIMATES AND CONFIDENCE INTERVALS

CPDB* LU NO	COMPOUND NAME	VELOCITY CLASS	Z	II	N	SA	SS*	IRMS
1270	DICHLORO-1-PROPANE, 1,2	11	2.10204	719556	6	0.22282	13.6007	7.23079
	DICHLORO-1-PROPENE, 2,3	11	1.19248	845593	2	0.50888	9.26572	7.94771
	DICHLORO-2-PROPANOL, 1,3	11	3.58176	638059	4	0.286148	15.4488	7.55174
1285	DICHLOROBENZENE, M	14	1.75138	740894	2	0.988518	7.74215	6.59811
1216	DICHLOROBENZENE, O	14	1.02102	896847	3	0.970792	1.59808	4.33962
	DICHLORODITHANE, 1,1	11	1.5658	952454	4	0.109848	16.1125	7.51504
1244	DICHLORODITHANE, 1,2	11	3.4942	951121	6	0.16588	14.1446	7.2801
1235	DICHLORODITHYLENE, C1S, 2	11	2.9113	1.2388	8	0.560384	16.325	7.44251
1236	DICHLORODITHYLENE, TRANS, 1,2	11	2.9989	1.22145	8	0.152501	13.1025	7.13025
2620	DICHLOROMETHANE	11	8.102	955288	8	0.173046	13.1072	7.24949
3170	DICHLOROPROPANE, 1,2	11	2.2412	1.1229	8	0.380407	15.9587	7.58131
1440	DIBROMETHYLENE	11	0.9480	969101	10	0.318279	19.3086	7.61106
	DIBROMOPYR, BENZENE, 1,2	11	2.04893	287379	6	0.843052	28.2839	6.21842
1870	DIMETHOXY ETHANE, 1,2	11	1.0282	849494	3	0.663082	6.80678	7.19222
1890	DIME THYLFORMAMIDE, N, N	11	2.15791	648372	3	0.071422	4.59188	7.02873
1495	DIME THYLPROPYLENE, 1,1	11	1.1638	1.01568	2	0.17982	6.59824	7.26292
	DIME THYLSTYRENE, 2,4	11	8.4209	718972	6	0.429489	13.8828	7.28047
1570	DIME THYL SULFONIDE	14	1.19048	828461	3	0.048848	20.481	5.66978
1480	DIOXANE	11	1.80448	70596	2	0.435819	6.5421	7.20306
1450	DIOXANE, DIBROMOETHANE	11	8.3162	992322	6	0.962992	13.756	7.22046
	DIOXANE, DIBROMOETHANE	11	1.87054	649187	3	0.28197	1.15981	7.64885
1910	DIOXYL ETHANOL, 2	11	1.34791	798003	3	0.354329	4.81638	7.00472
1870	DIOXYL ACETATE	11	4.71462	887545	10	0.308859	94.2747	6.71408
1480	DIOXYL ACETOACETATE	14	1.98467	0.66266	3	0.202922	1.7222	6.29101
1750	DIOXYL CHLOROACETATE	11	1.0023	832749	2	0.108622	4.47882	6.99629
1990	DIOXYL ETHER	11	1.00083	814314	4	0.494927	6.56318	7.50805
1740	DIOXYLBENZENE	11	6.65879	235574	19	1.11787	88.9271	6.97745
1720	DIOXYLENE	11	9.04102	801124	6	0.148848	6.28961	6.8141
1980	DIOXYLENE OXIDE	11	1.0088	1.01284	3	0.811012	7.39808	8.17482
1800	DIOXYLENE DIBROMIDE	11	1.20845	764067	3	0.990440	8.24219	7.23273
2080	DIOXYLIC ACID	11	2.7908	641273	6	0.39844	12.0961	7.24228

\* ORGANIC CHEMICAL PRODUCERS DATA BANK

\*\* C. CAS 11 - IUPAC LIQUID, M - MAYER LIQUID





TABLE V. (21) (cont'd) (cont'd)  
 STATISTICAL PROPERTY ESTIMATES AND FORMULAE ESTIMATES

GROUP ID NO	COMPOUND NAME	ESTIMATE	FORMULA	ESTIMATE	FORMULA	ESTIMATE	FORMULA
1470	TRIMETHYLPROPANE	11	C <sub>4</sub> H <sub>10</sub>	11	C <sub>4</sub> H <sub>10</sub>	11	C <sub>4</sub> H <sub>10</sub>
1480	TRIMETHYLAMINE	11	C <sub>3</sub> H <sub>9</sub> N	11	C <sub>3</sub> H <sub>9</sub> N	11	C <sub>3</sub> H <sub>9</sub> N
1510	VINYL ACETATE	11	C <sub>4</sub> H <sub>6</sub> O <sub>2</sub>	11	C <sub>4</sub> H <sub>6</sub> O <sub>2</sub>	11	C <sub>4</sub> H <sub>6</sub> O <sub>2</sub>
1520	VINYL CHLORIDE	6	C <sub>2</sub> H <sub>3</sub> Cl	6	C <sub>2</sub> H <sub>3</sub> Cl	6	C <sub>2</sub> H <sub>3</sub> Cl
1530	VINYLIDENE CHLORIDE	11	C <sub>2</sub> H <sub>2</sub> Cl <sub>2</sub>	11	C <sub>2</sub> H <sub>2</sub> Cl <sub>2</sub>	11	C <sub>2</sub> H <sub>2</sub> Cl <sub>2</sub>
1540	ACRYLONITRILE	11	C <sub>3</sub> H <sub>3.5</sub> N	11	C <sub>3</sub> H <sub>3.5</sub> N	11	C <sub>3</sub> H <sub>3.5</sub> N
1550	ACRYLONITRILE	11	C <sub>3</sub> H <sub>3.5</sub> N	11	C <sub>3</sub> H <sub>3.5</sub> N	11	C <sub>3</sub> H <sub>3.5</sub> N
1560	ACRYLONITRILE	11	C <sub>3</sub> H <sub>3.5</sub> N	11	C <sub>3</sub> H <sub>3.5</sub> N	11	C <sub>3</sub> H <sub>3.5</sub> N

\* ORGANIC CHEMICAL PRODUCTS DATA (21)

† G = GAS, L = LIQUID, MC = MELTING POINT

## SECTION 6

### REFERENCES

- (1) Environmental Protection Agency. VOC Fugitive Emissions in Synthetic Organic Chemicals Manufacturing Industry - Background Information for Proposed Standards. Emission Standards and Engineering Division. Research Triangle Park, North Carolina, March 1980.
- (2) Operating Manual - OVA-108, Analabs, Foxboro Analytical, North Haven, CT, D6473.
- (3) Operating Manual - TLV Sniffer, J. W. Bacharach Instrument Company, Division of Ambac Industries, Santa Clara, CA. 95050.
- (4) Delaney, B. T. Operation and Use of Portable Organic Vapor Analyzer. Exxon Research and Engineering, February 24, 1978.
- (5) Weast, R. C., ed. CRC Handbook of Chemistry and Physics, 48th Edition. The Chemical Rubber Co., Cleveland, Ohio, 1968, pp. D-57.
- (6) Mood, Graybill, and Boes, Introduction to the Theory of Statistics. Third Ed., McGraw-Hill, New York, N.Y., 1974, pp. 181.
- (7) B. R. Draper and H. Smith, Applied Regression Analysis, John Wiley & Sons, Inc., New York, 1968, pp. 407.
- (8) Dale M. Heien, "A Note on Log-Linear Regression," Journal of the American Statistical Association, 63, 1968, pp. 1034-1038.